

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111719\
 Data File : PL054348.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2019 11:52
 Operator : SG\AJ
 Sample : PB124874BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB124874BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 06:24:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.043	193.8E6	46735185	17.882	18.676
28)	SA Decachlor...	8.331	9.126	185.5E6	50557994	18.902	17.954
Target Compounds							
2)	A alpha-BHC	3.988	0.000	4283042	0	0.246	N.D. #
3)	MA gamma-BHC...	4.276	0.000	939360	0	0.060	N.D. #
7)	B delta-BHC	4.735	0.000	7355592	0	0.483	N.D. #
14)	MA Endrin	6.126	0.000	5215992	0	0.450	N.D. #
15)	B Endosulfa...	0.000	6.963	0	3538265	N.D.	1.385 #
16)	A 4,4'-DDD	6.247	0.000	5466140	0	0.614	N.D. #
18)	B Endrin al...	6.568	7.088	4359334	2059538	0.475	0.938 #
19)	B Endosulfa...	6.781	0.000	4824279	0	0.474	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL111719\
Data File : PL054348.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2019 11:52
Operator : SG\AJ
Sample : PB124874BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB124874BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 06:24:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

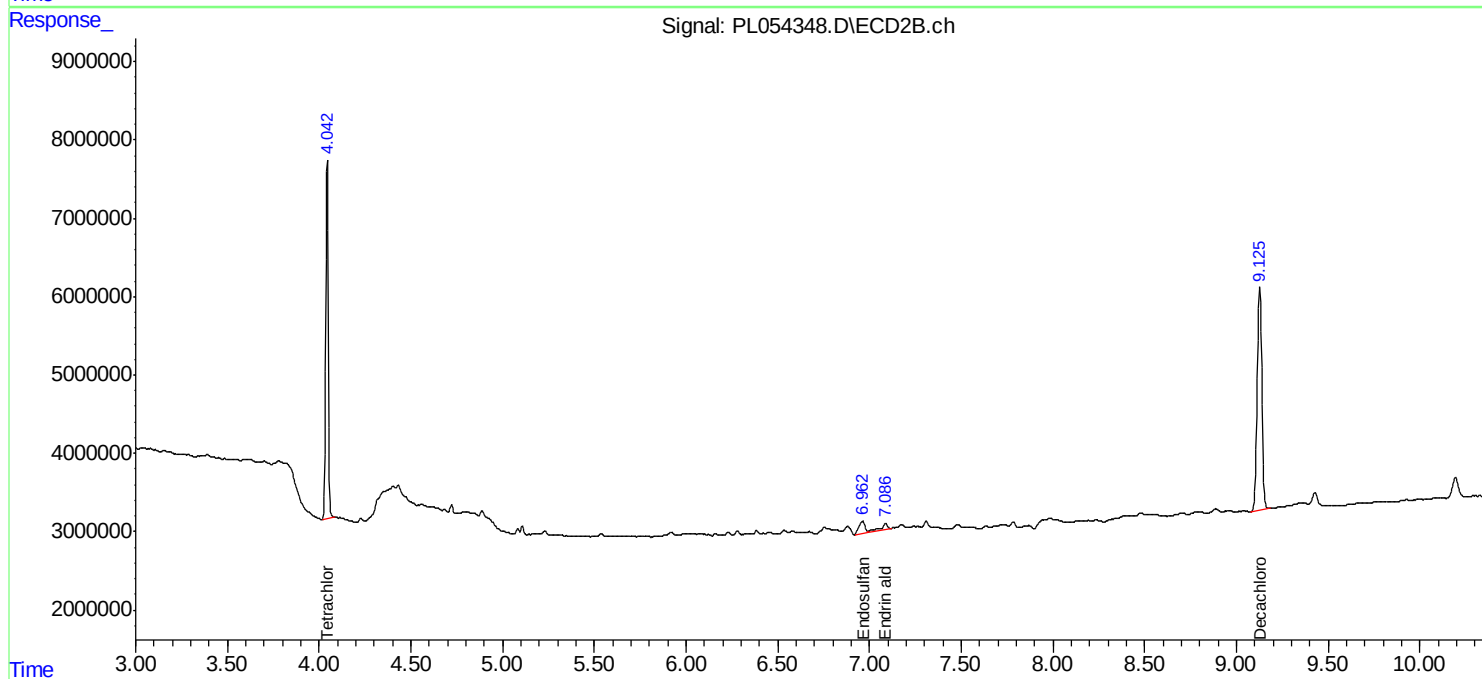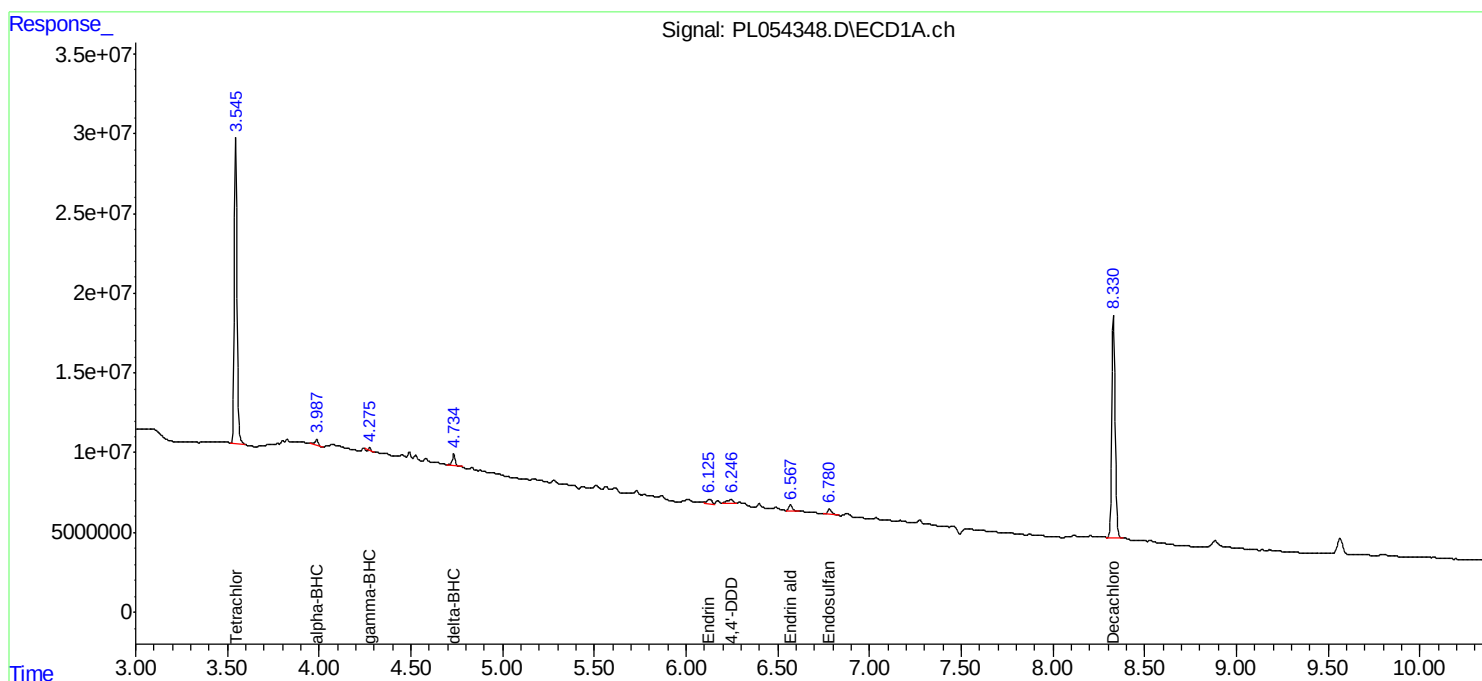


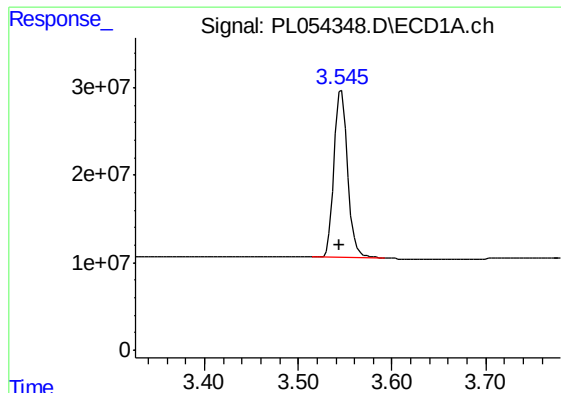

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.002 min
Response: 193829359
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB124874BL

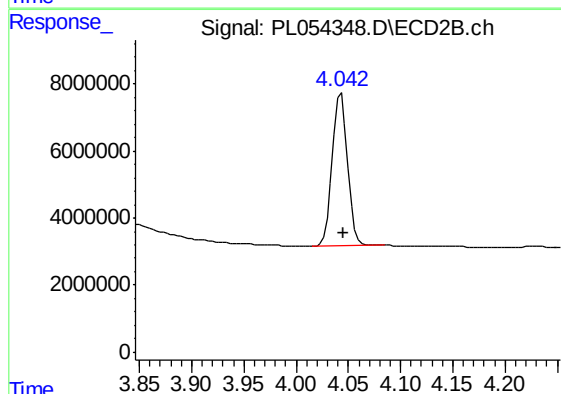


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.003 min
Response: 46735185
Conc: 18.68 ng/ml

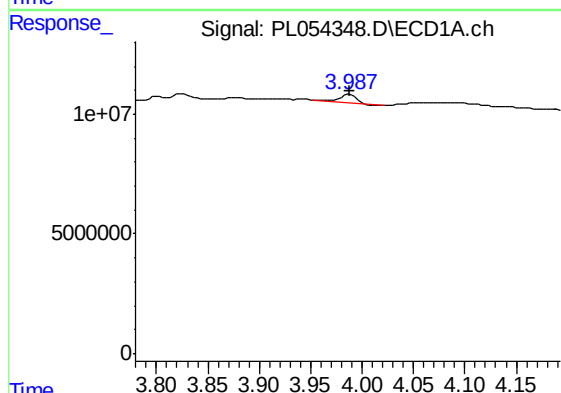


#2 alpha-BHC

R.T.: 3.988 min
Delta R.T.: 0.000 min
Response: 4283042
Conc: 0.25 ng/ml

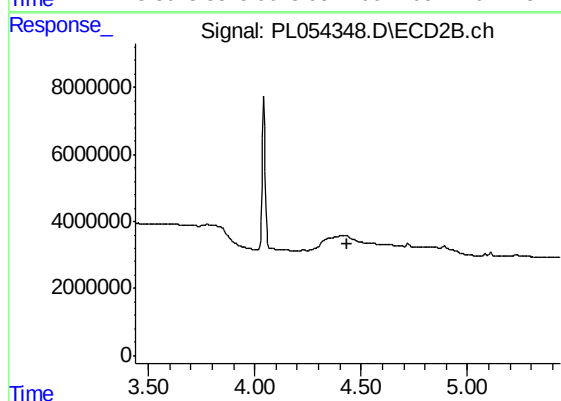

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

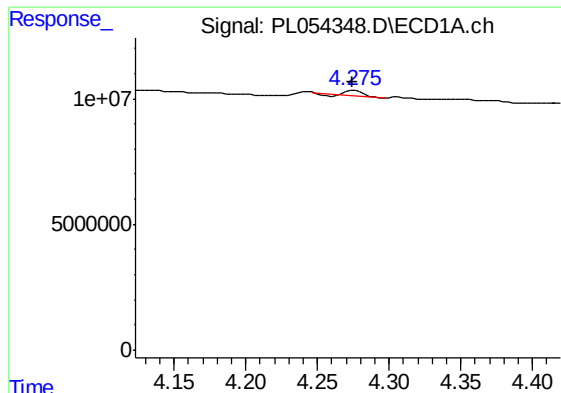

#3 gamma-BHC (Lindane)


R.T.: 4.276 min
Delta R.T.: 0.001 min
Response: 939360
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB124874BL

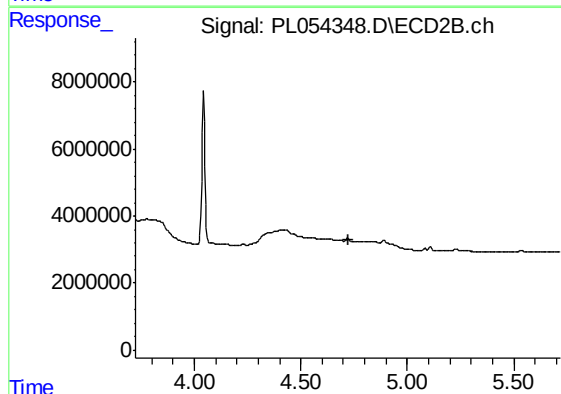


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

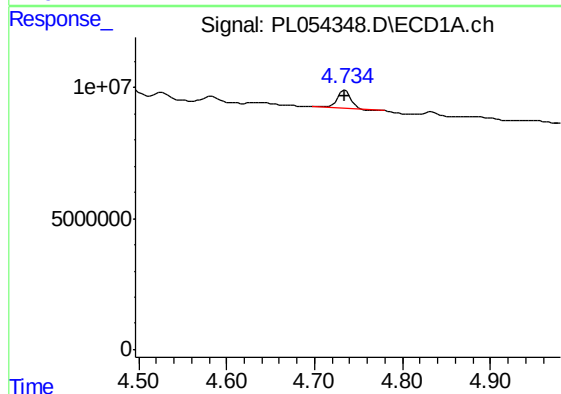


#7 delta-BHC

R.T.: 4.735 min
Delta R.T.: 0.001 min
Response: 7355592
Conc: 0.48 ng/ml

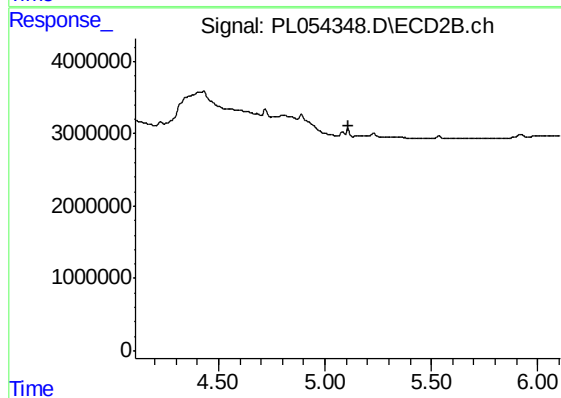

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

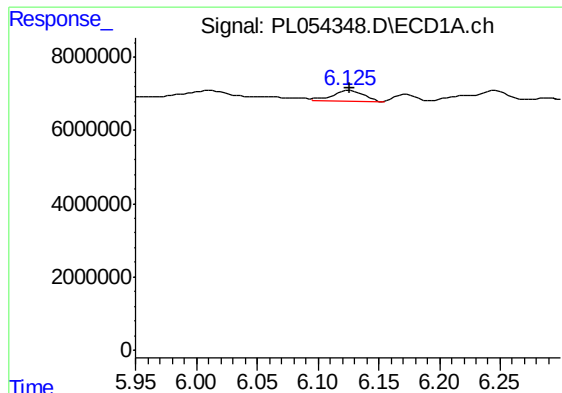

#14 Endrin


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 5215992
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB124874BL

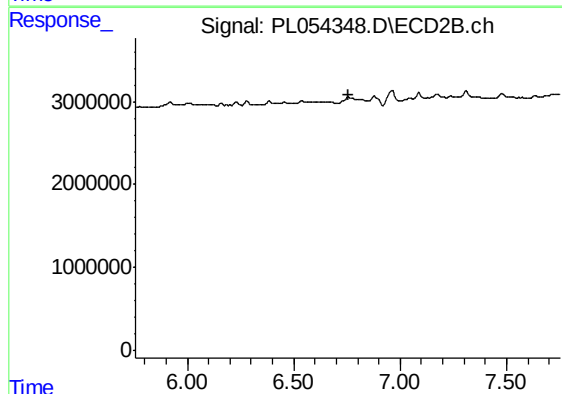


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

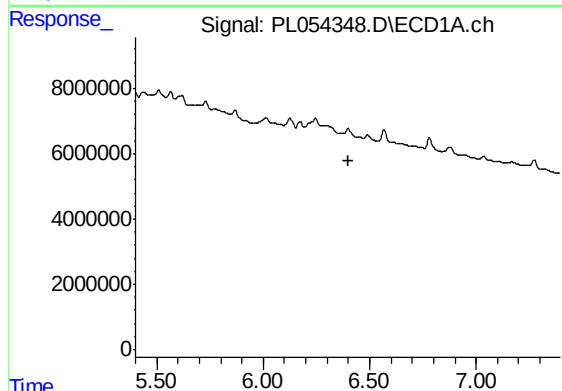


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

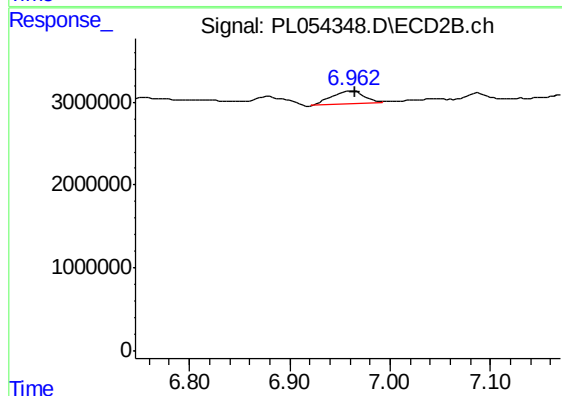

#15 Endosulfan II


R.T.: 6.963 min
Delta R.T.: -0.002 min
Response: 3538265
Conc: 1.39 ng/ml

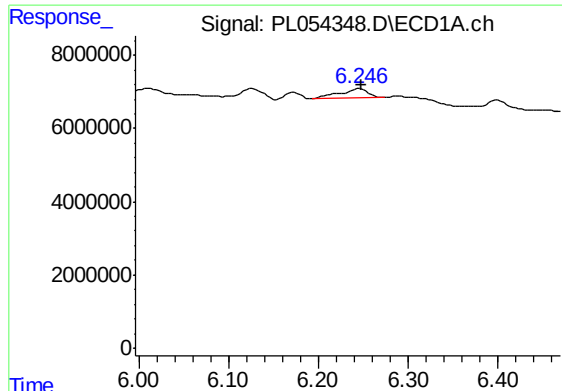

#16 4,4'-DDD


R.T.: 6.247 min
Delta R.T.: -0.001 min
Response: 5466140
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB124874BL

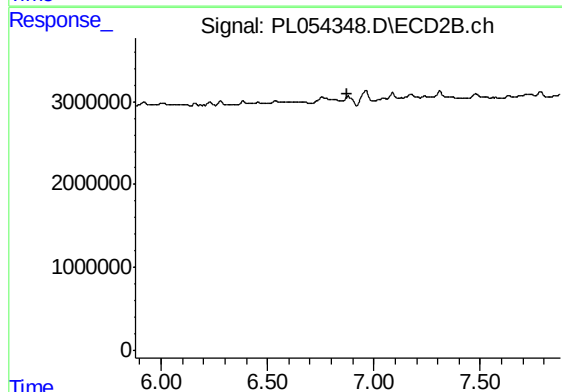


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

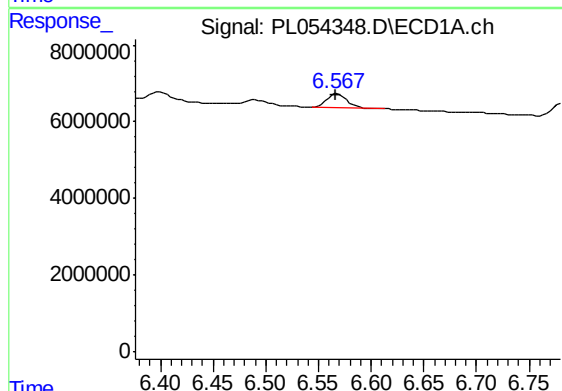


#18 Endrin aldehyde

R.T.: 6.568 min
Delta R.T.: 0.001 min
Response: 4359334
Conc: 0.48 ng/ml

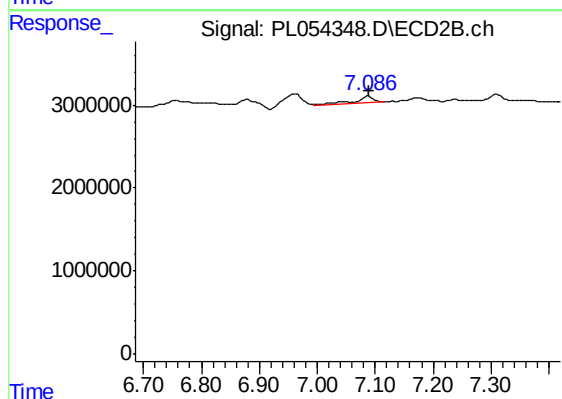

#18 Endrin aldehyde


R.T.: 7.088 min
Delta R.T.: -0.001 min
Response: 2059538
Conc: 0.94 ng/ml

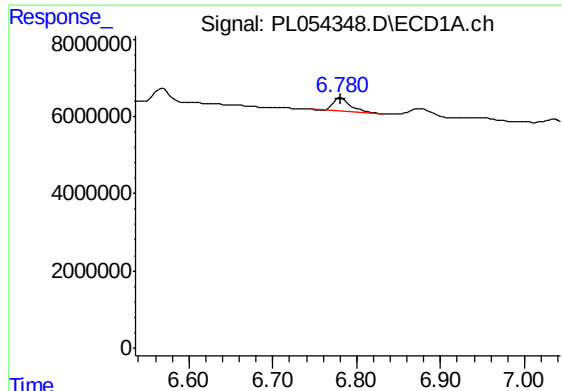

#19 Endosulfan Sulfate


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 4824279
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB124874BL

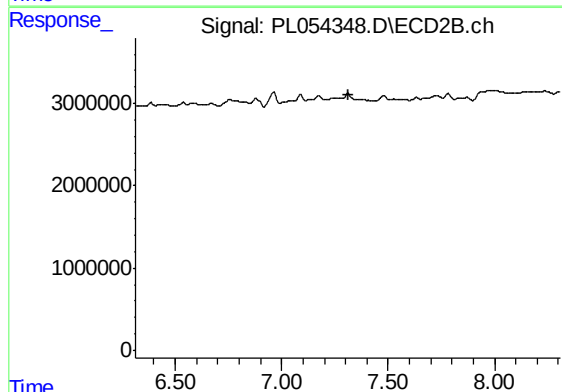


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

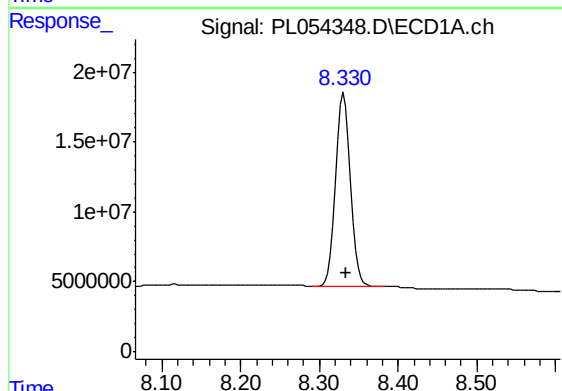

#28 Decachlorobiphenyl

R.T.: 8.331 min
Delta R.T.: -0.003 min
Response: 185455100
Conc: 18.90 ng/ml

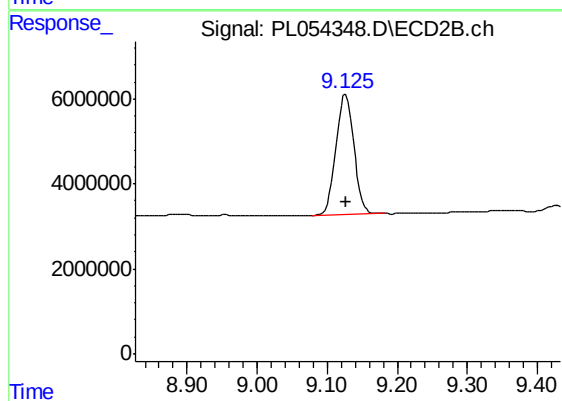

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.000 min
Response: 50557994
Conc: 17.95 ng/ml