

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112520\
 Data File : PL063225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 17:38
 Operator : DD\AJ
 Sample : L4858-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PHC-340EM-012

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:19:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	3.950	34589745	64059267	20.310	19.627
28) SA Decachlor...	8.124	8.989	37465142	47999062	20.062	20.174
Target Compounds						
9) A Endosulfan I	0.000	6.158	0	10452686	N.D.	3.096 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112520\
Data File : PL063225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 17:38
Operator : DD\AJ
Sample : L4858-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PHC-340EM-012

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:19:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

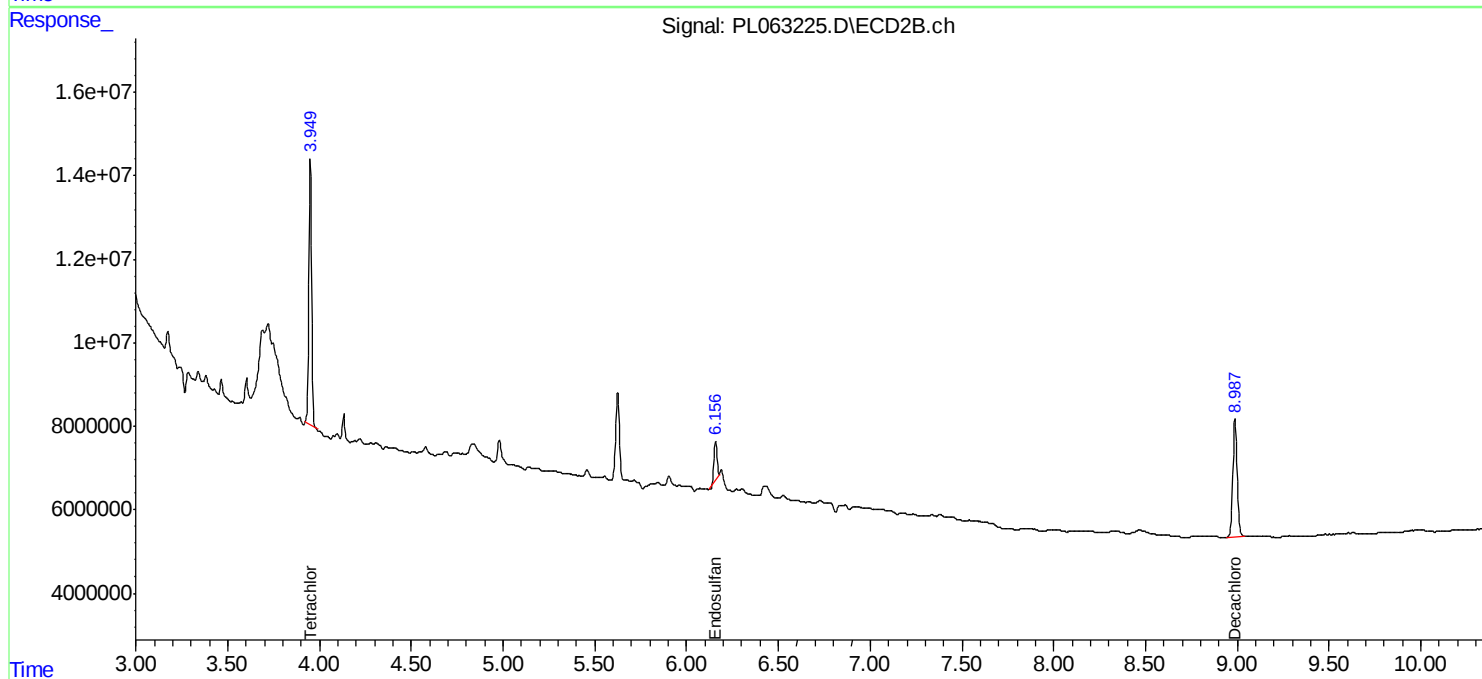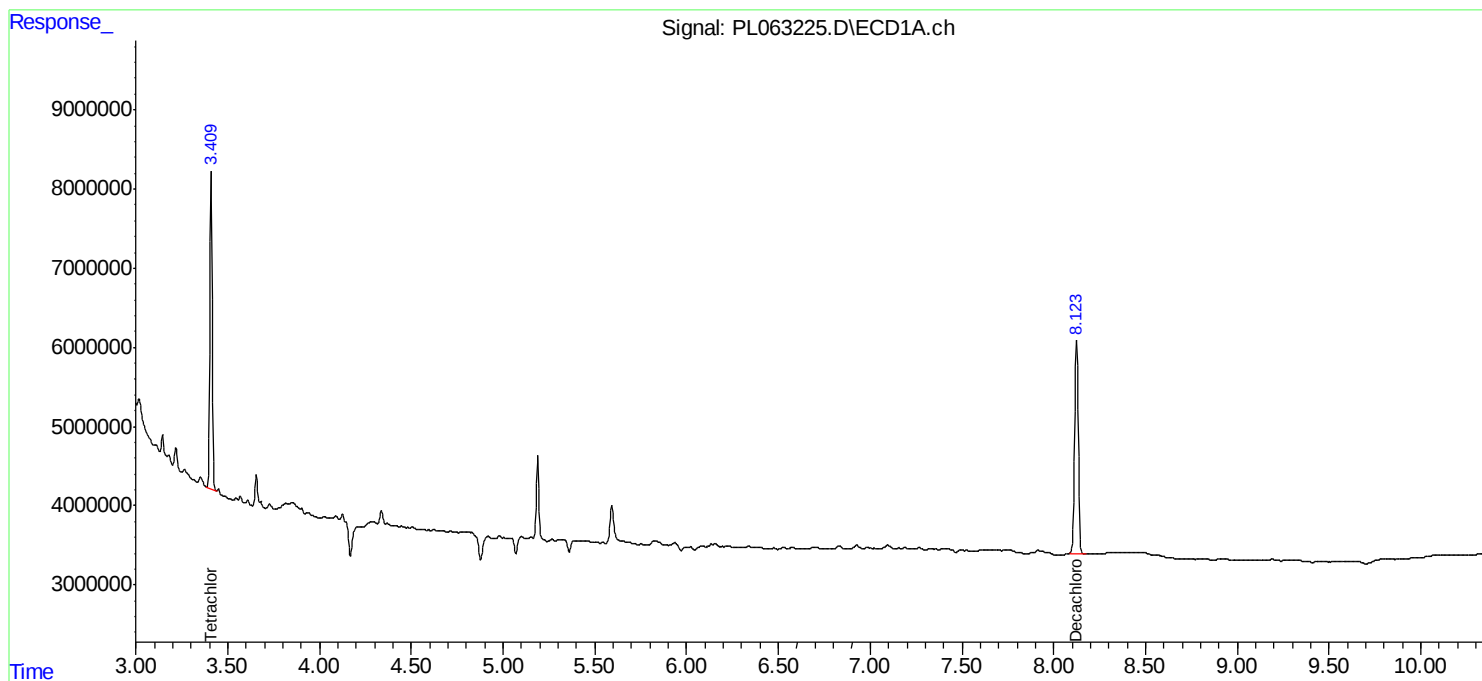


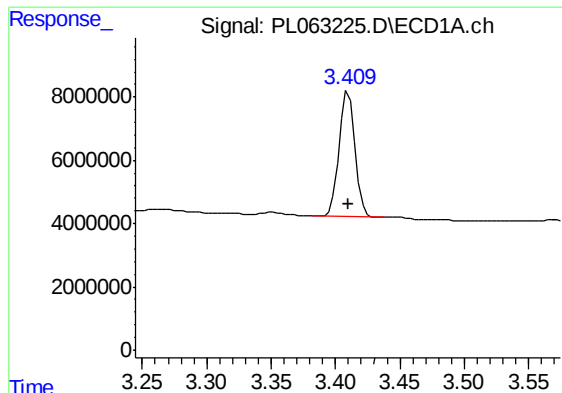

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 34589745
Conc: 20.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHC-340EM-012

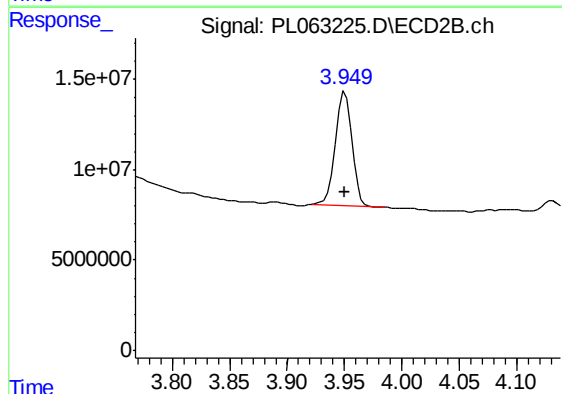


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 64059267
Conc: 19.63 ng/ml

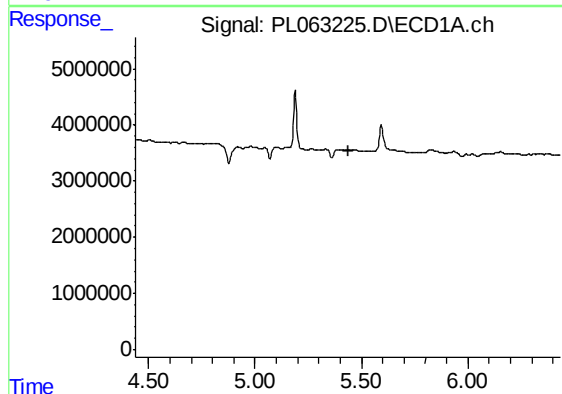


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.437 min
Response: 0
Conc: N.D.

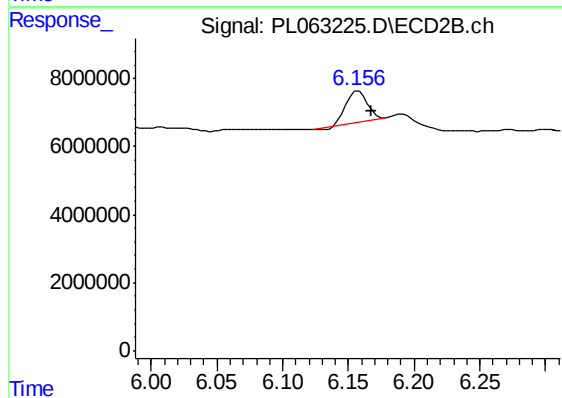

#9 Endosulfan I


R.T.: 6.158 min
Delta R.T.: -0.010 min
Response: 10452686
Conc: 3.10 ng/ml

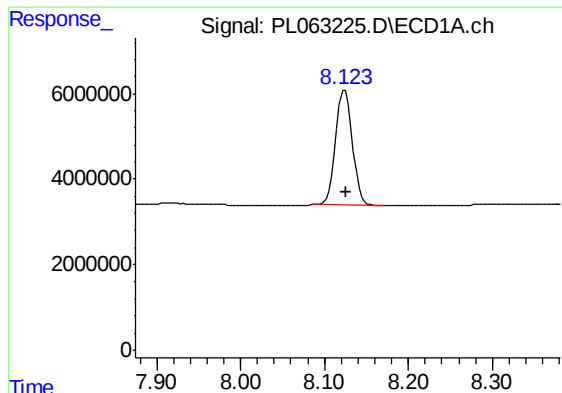

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 37465142
Conc: 20.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PHC-340EM-012

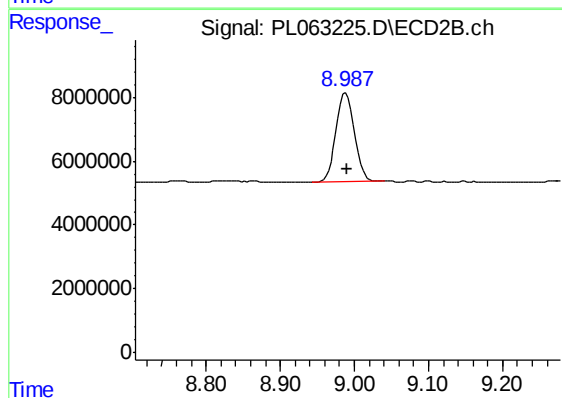

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: -0.001 min
Response: 47999062
Conc: 20.17 ng/ml