

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112520\
 Data File : PL063246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 22:37
 Operator : DD\AJ
 Sample : L4893-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R-LA-36-2-WC

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:57:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:25:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	34947737	63064676	20.520	19.323
28)	SA Decachlor...	8.125	8.989	23216647	27268192	12.432	11.461
Target Compounds							
17)	MA 4,4'-DDT	6.298	7.063	1436358	2467480	1.068m	0.966m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112520\
Data File : PL063246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 22:37
Operator : DD\AJ
Sample : L4893-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
R-LA-36-2-WC


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:25:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

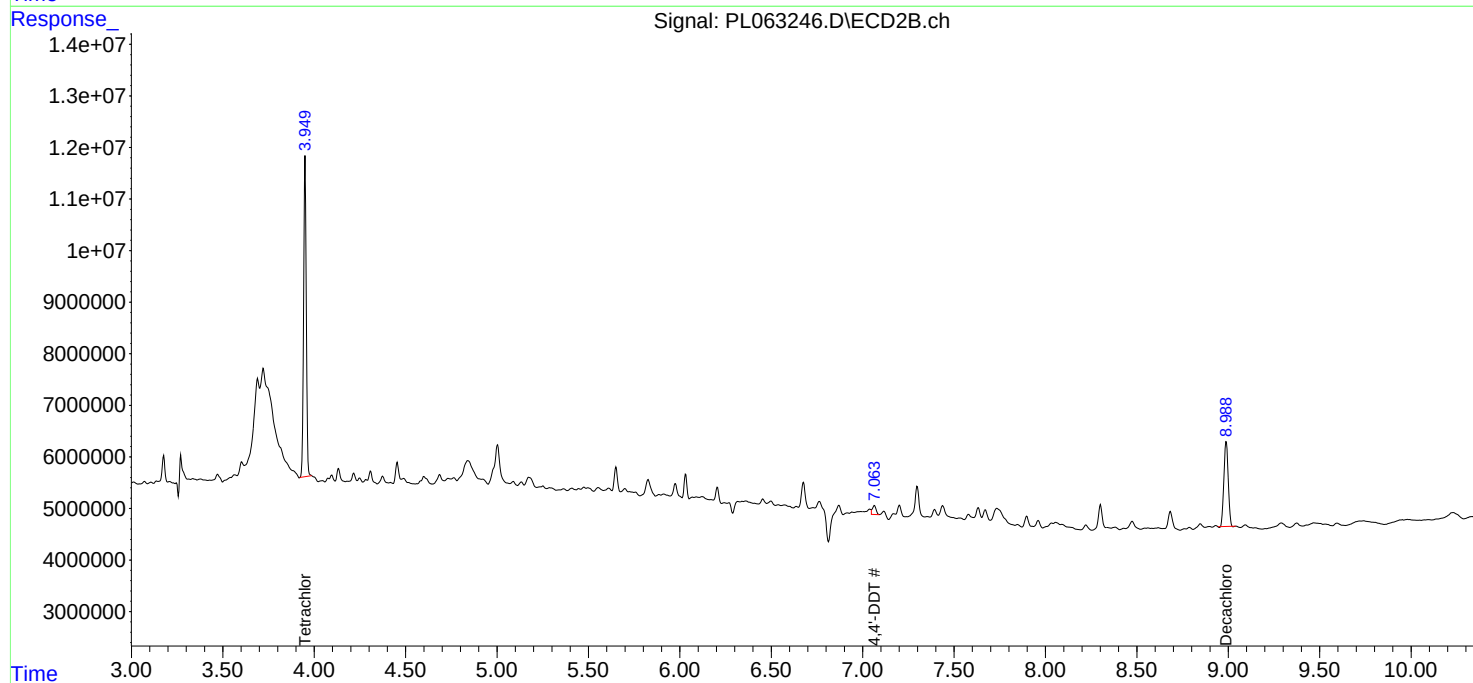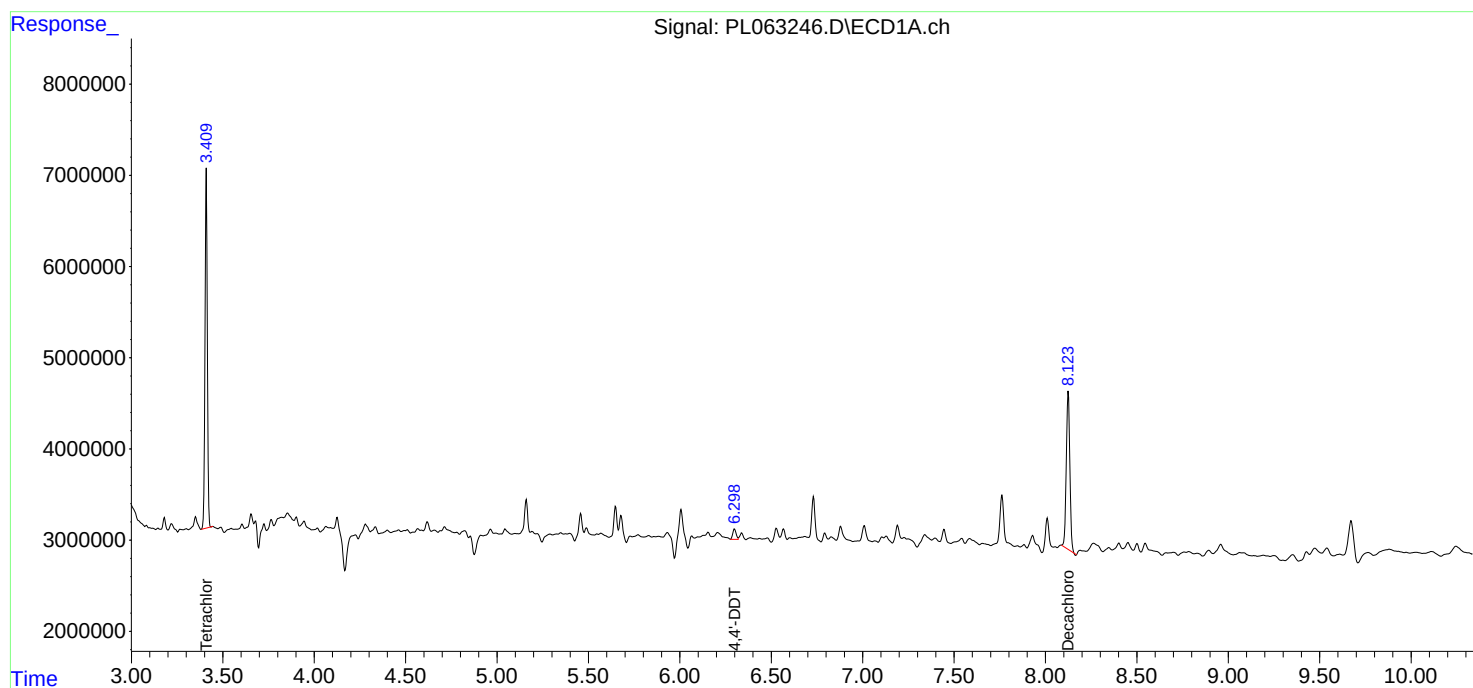

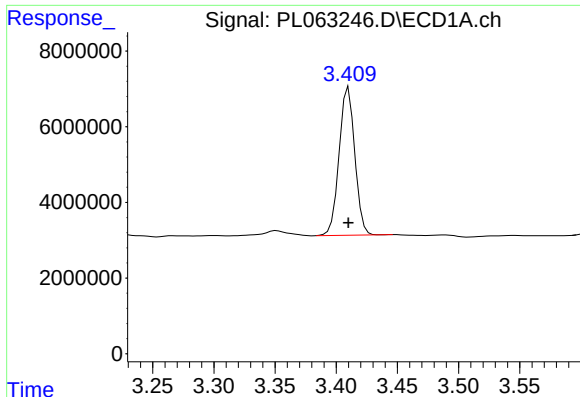


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 34947737
Conc: 20.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-LA-36-2-WC


Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:07 PM

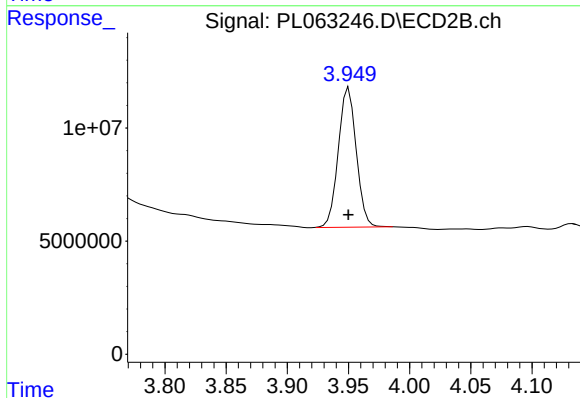


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 63064676
Conc: 19.32 ng/ml

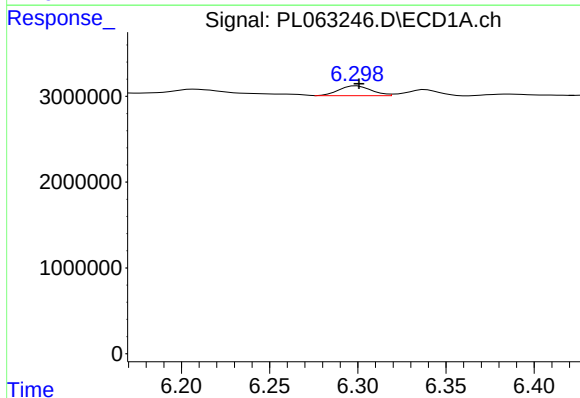


#17 4,4'-DDT

R.T.: 6.298 min
Delta R.T.: -0.003 min
Response: 1436358
Conc: 1.07 ng/ml m

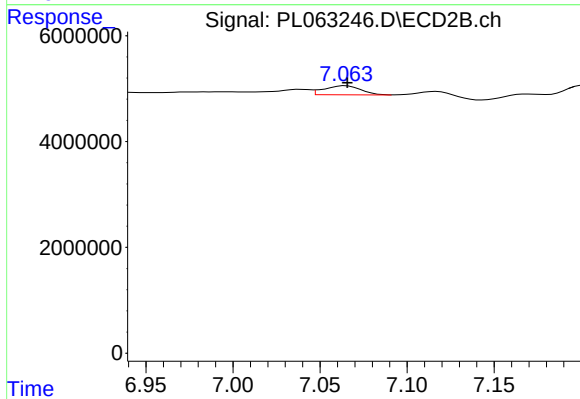

#17 4,4'-DDT

R.T.: 7.063 min
Delta R.T.: -0.002 min
Response: 2467480
Conc: 0.97 ng/ml m

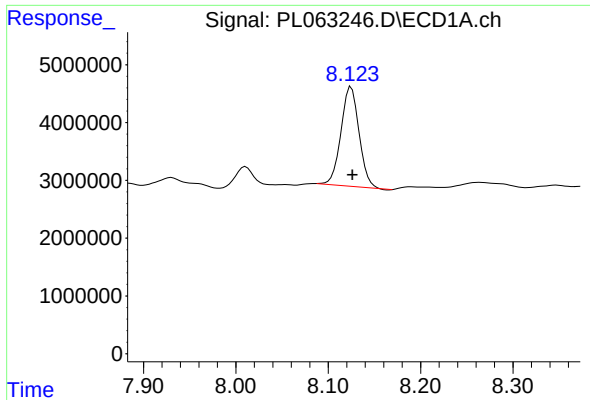


#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.001 min
Response: 23216647
Conc: 12.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-LA-36-2-WC

Manual Integrations
APPROVED

Ankita
11/27/2020 12:57:07 PM

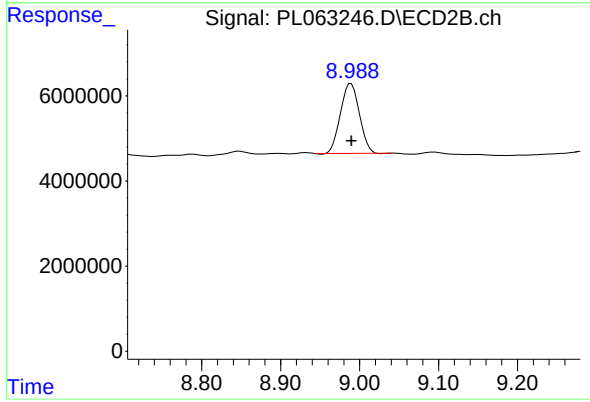

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 27268192
Conc: 11.46 ng/ml