

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112522\
 Data File : PL079439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2022 15:34
 Operator : AR\AJ
 Sample : PB149287BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 23:58:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 24 00:09:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.565	41004026	53052860	18.151	19.490
28)	SA Decachlor...	8.769	7.631	37374838	46985180	19.245	20.000
Target Compounds							
2)	A alpha-BHC	0.000	3.036	0	110262	N.D.	0.026 #
7)	B delta-BHC	4.540f	0.000	1695280	0	0.611	N.D. #
8)	B Heptachlo...	5.462	4.468	1082876	38293	0.379	0.011 #
9)	A Endosulfan I	5.858f	0.000	202352	0	0.076	N.D. #
13)	MA Dieldrin	0.000	5.088	0	961670	N.D.	0.285 #
14)	MA Endrin	0.000	5.388f	0	590359	N.D.	0.195 #
15)	B Endosulfa...	6.551f	5.630f	368988	199311	0.163	0.071 #
24)	Chlordane-2	0.000	4.087	0	1846590	N.D.	15.772 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112522\
Data File : PL079439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2022 15:34
Operator : AR\AJ
Sample : PB149287BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 23:58:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Thu Nov 24 00:09:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

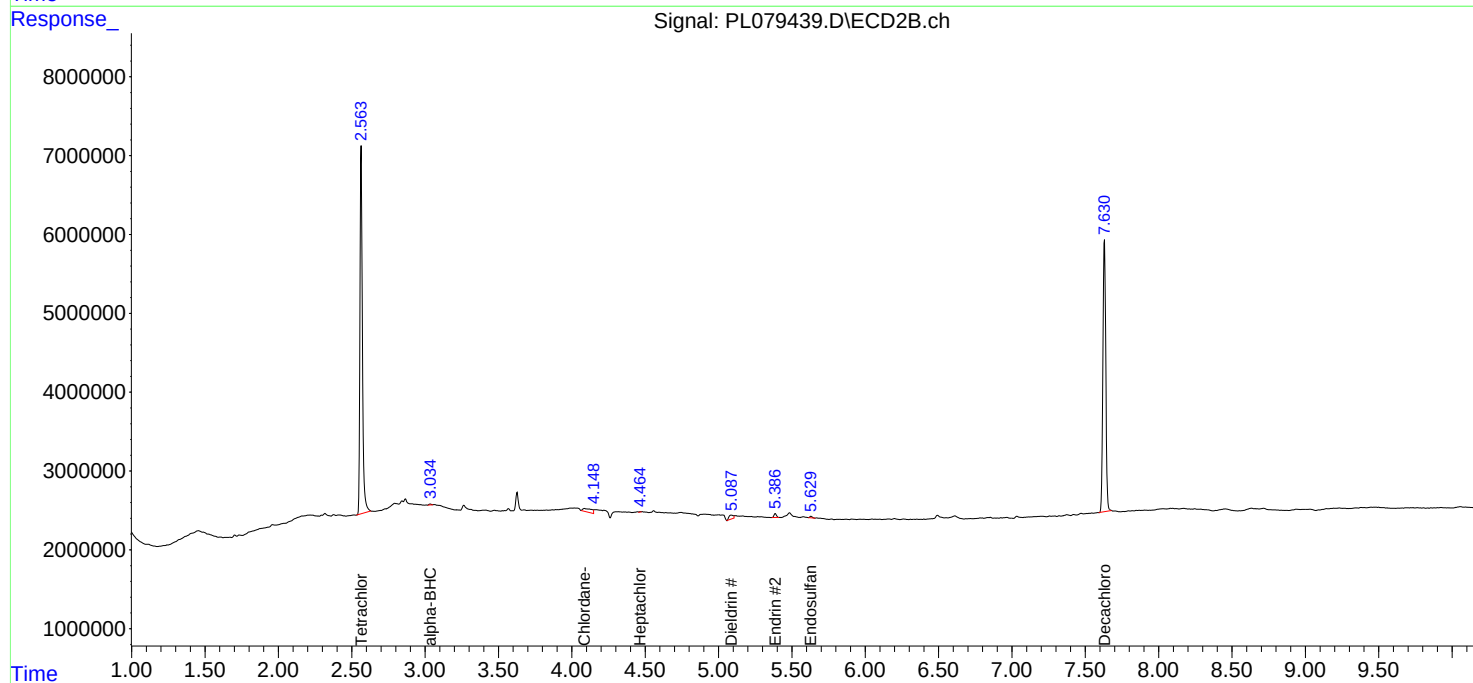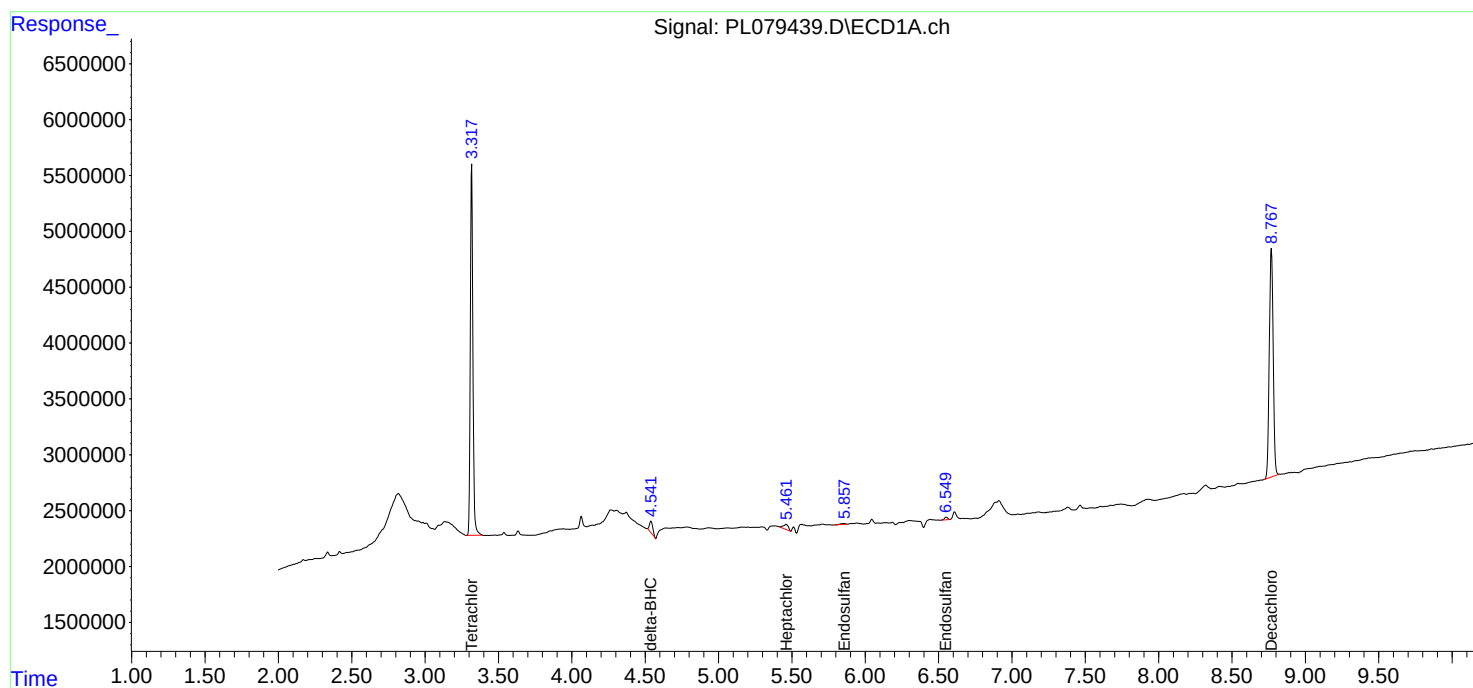


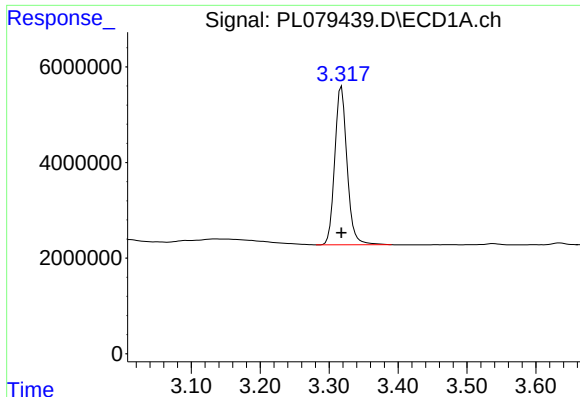

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 41004026
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

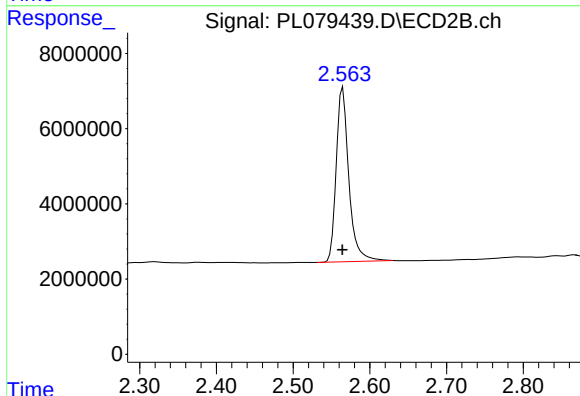


#1 Tetrachloro-m-xylene

R.T.: 2.565 min
Delta R.T.: 0.000 min
Response: 53052860
Conc: 19.49 ng/ml

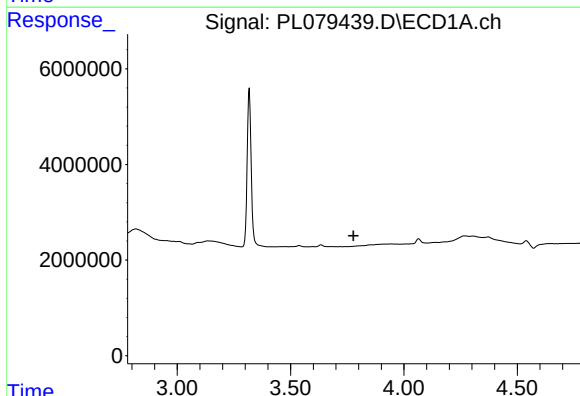


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.778 min
Response: 0
Conc: N.D.

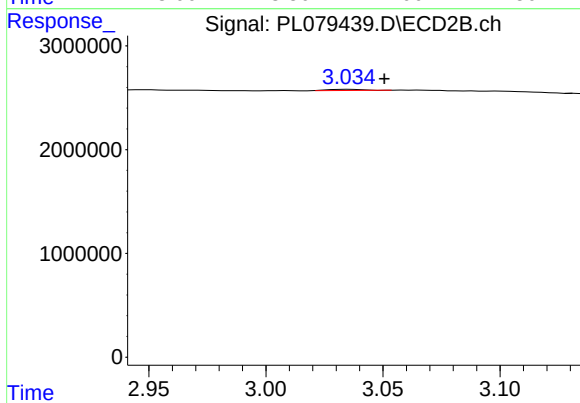

#2 alpha-BHC


R.T.: 3.036 min
Delta R.T.: -0.015 min
Response: 110262
Conc: 0.03 ng/ml

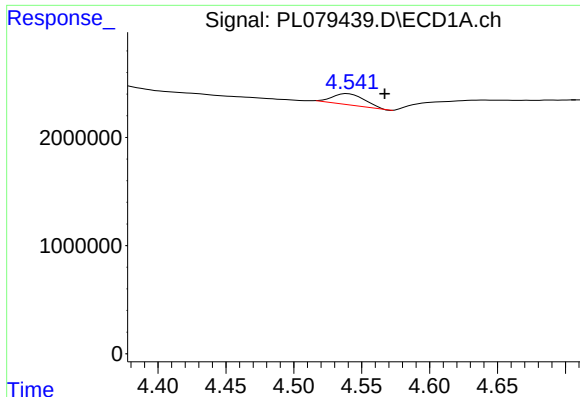

#7 delta-BHC


R.T.: 4.540 min
Delta R.T.: -0.027 min
Response: 1695280
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

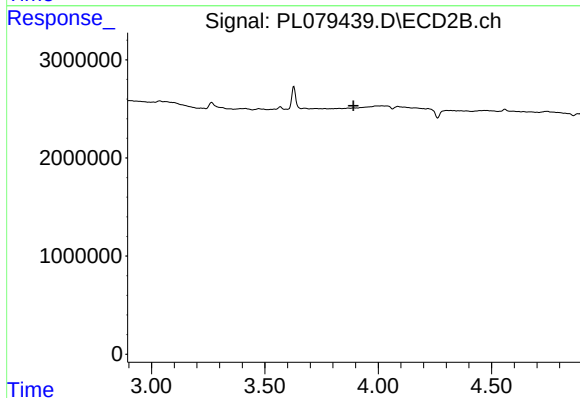


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.891 min
Response: 0
Conc: N.D.

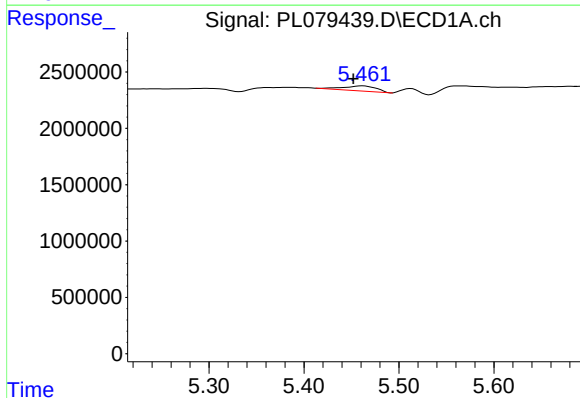


#8 Heptachlor epoxide

R.T.: 5.462 min
Delta R.T.: 0.010 min
Response: 1082876
Conc: 0.38 ng/ml

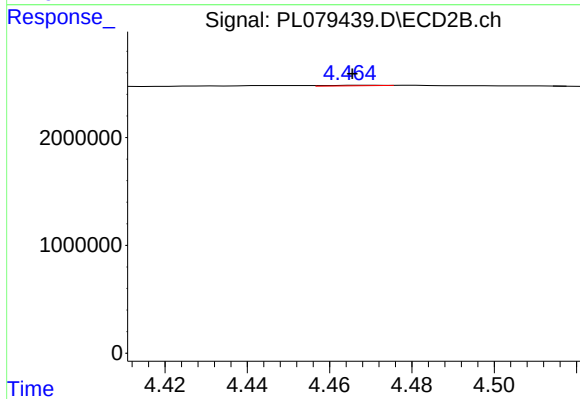

#8 Heptachlor epoxide


R.T.: 4.468 min
Delta R.T.: 0.002 min
Response: 38293
Conc: 0.01 ng/ml

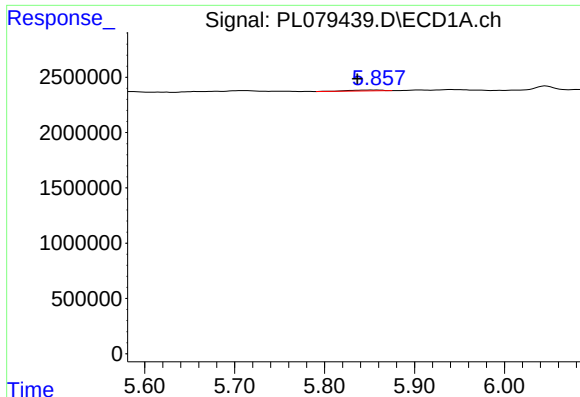

#9 Endosulfan I


R.T.: 5.858 min
Delta R.T.: 0.022 min
Response: 202352
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

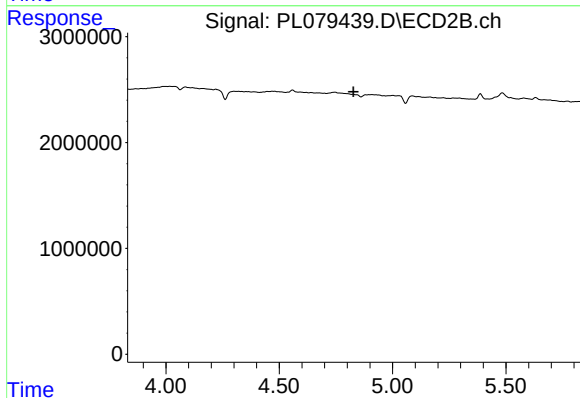


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

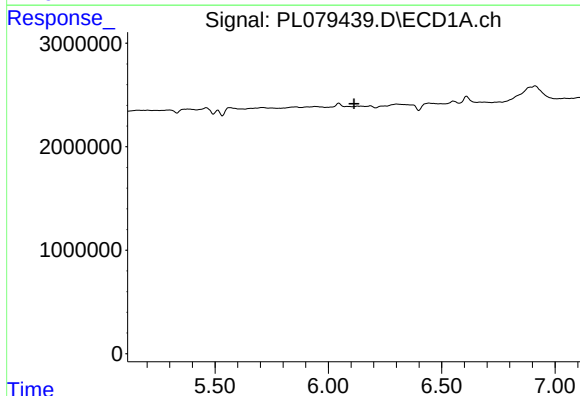


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

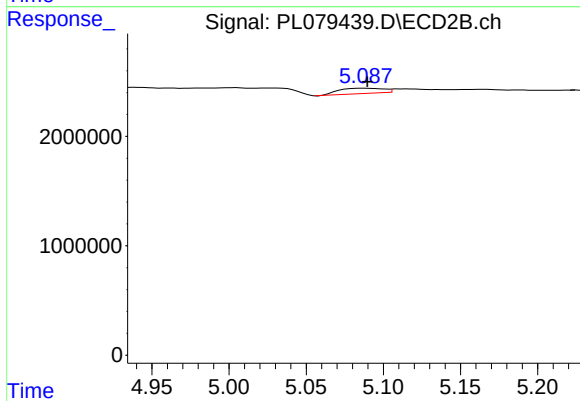

#13 Dieldrin


R.T.: 5.088 min
Delta R.T.: -0.001 min
Response: 961670
Conc: 0.29 ng/ml

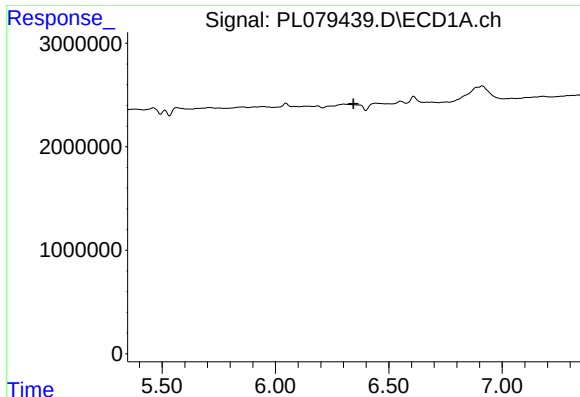

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

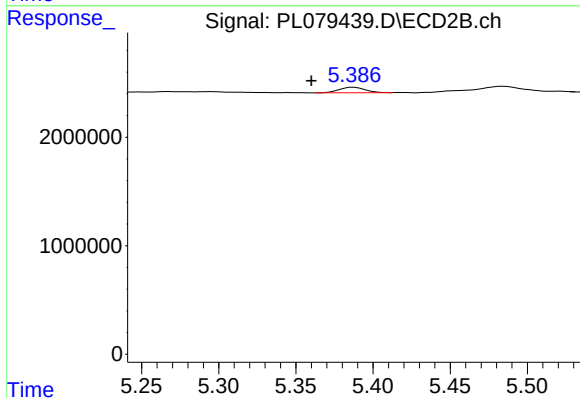


#14 Endrin

R.T.: 5.388 min
Delta R.T.: 0.027 min
Response: 590359
Conc: 0.20 ng/ml

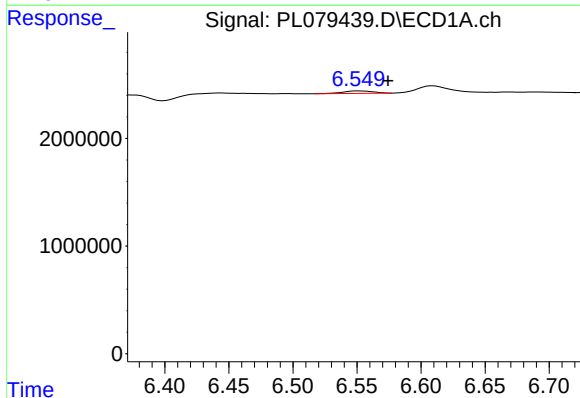


#15 Endosulfan II

R.T.: 6.551 min
Delta R.T.: -0.023 min
Response: 368988
Conc: 0.16 ng/ml

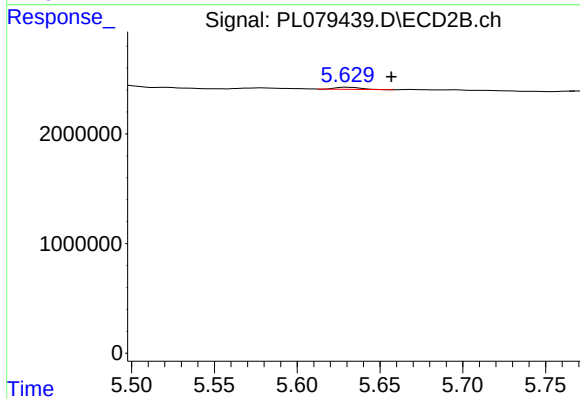

#15 Endosulfan II


R.T.: 5.630 min
Delta R.T.: -0.027 min
Response: 199311
Conc: 0.07 ng/ml

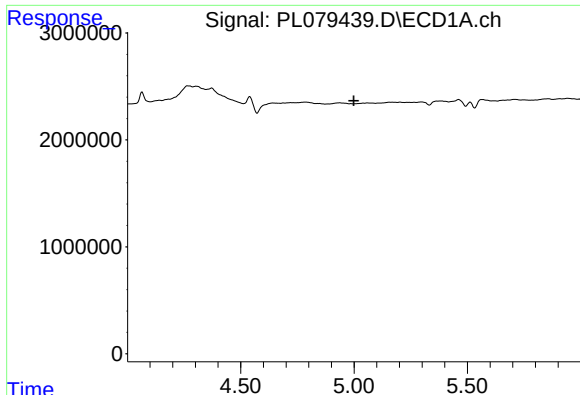

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.999 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

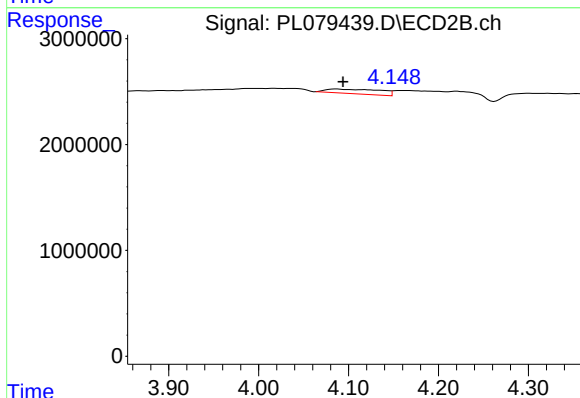


#24 Chlordane-2

R.T.: 4.087 min
Delta R.T.: -0.007 min
Response: 1846590
Conc: 15.77 ng/ml

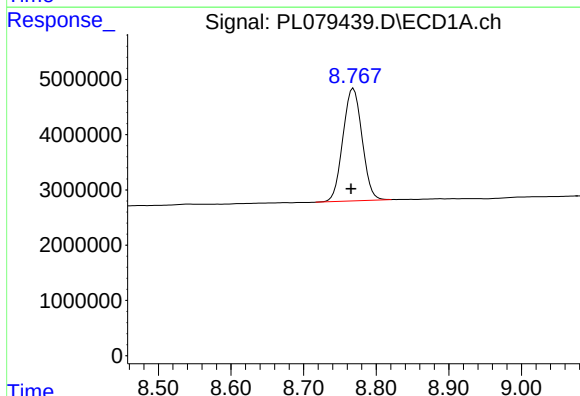

#28 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: 0.003 min
Response: 37374838
Conc: 19.24 ng/ml

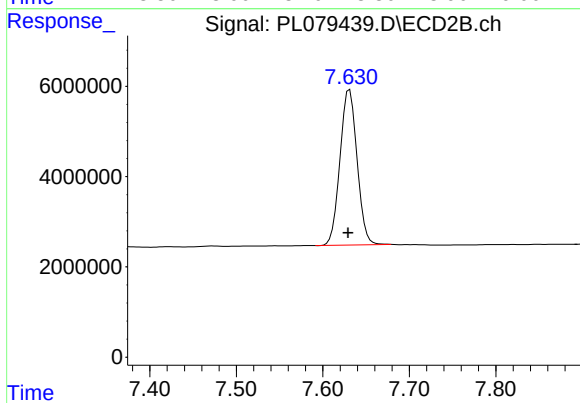

#28 Decachlorobiphenyl

R.T.: 7.631 min
Delta R.T.: 0.002 min
Response: 46985180
Conc: 20.00 ng/ml