

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
 Data File : PL071244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 13:26
 Operator : AR\AJ
 Sample : M4877-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:24:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.501	8224155	21259329	17.509	16.941
28)	SA Decachlor...	10.331	11.394	9739563	17007324	13.451	12.235
Target Compounds							
7)	B delta-BHC	0.000	7.021f	0	787513	N.D.	0.463 #
10)	B gamma-Chl...	7.310f	0.000	198649	0	0.313	N.D. #
11)	B alpha-Chl...	0.000	8.315	0	896689	N.D.	0.564 #
12)	B 4,4'-DDE	7.566	8.500	962224	2291902	1.700	1.489
17)	MA 4,4'-DDT	8.410	9.358	660603	690523	1.208	0.496 #
20)	A Methoxychlor	8.982f	0.000	397663	0	1.101	N.D. #
21)	B Endrin ke...	0.000	9.986	0	89750	N.D.	0.061 #
26)	Chlordane-4	0.000	8.315	0	896689	N.D.	3.379 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
Data File : PL071244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 13:26
Operator : AR\AJ
Sample : M4877-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:24:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

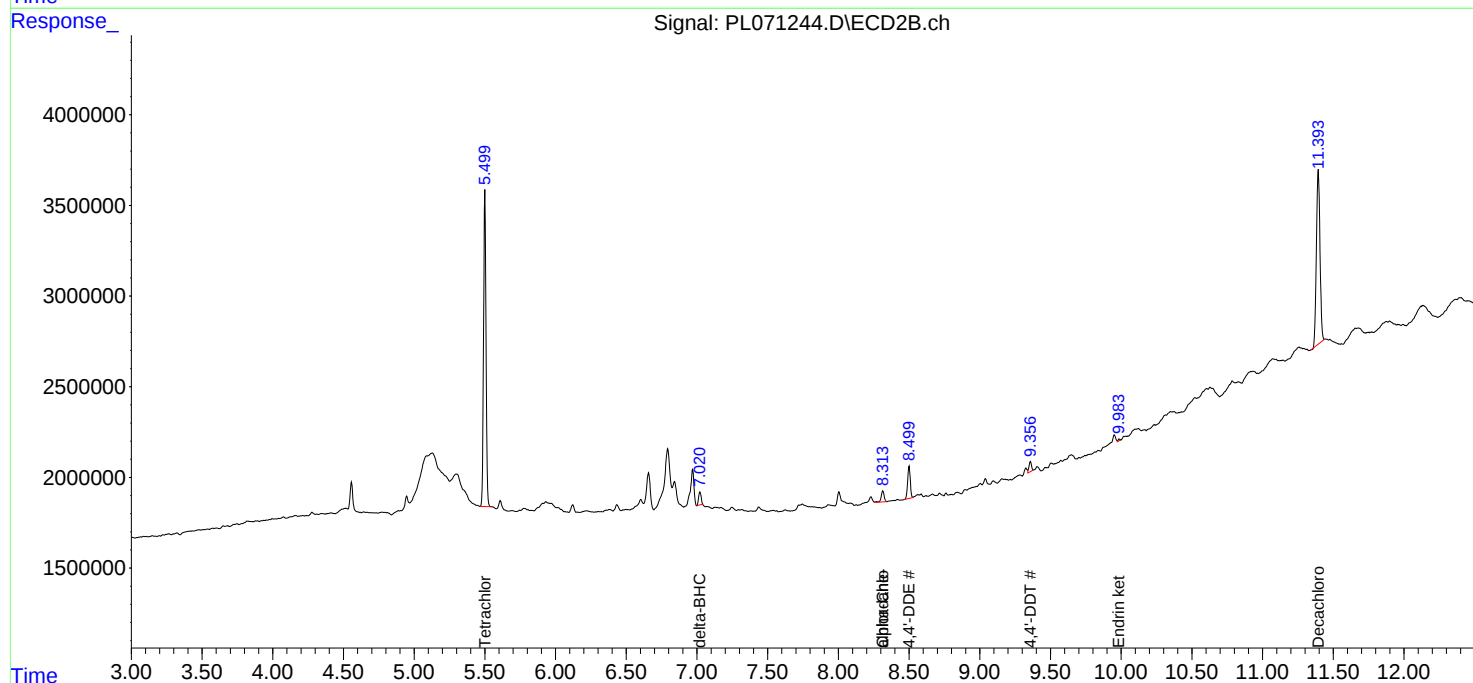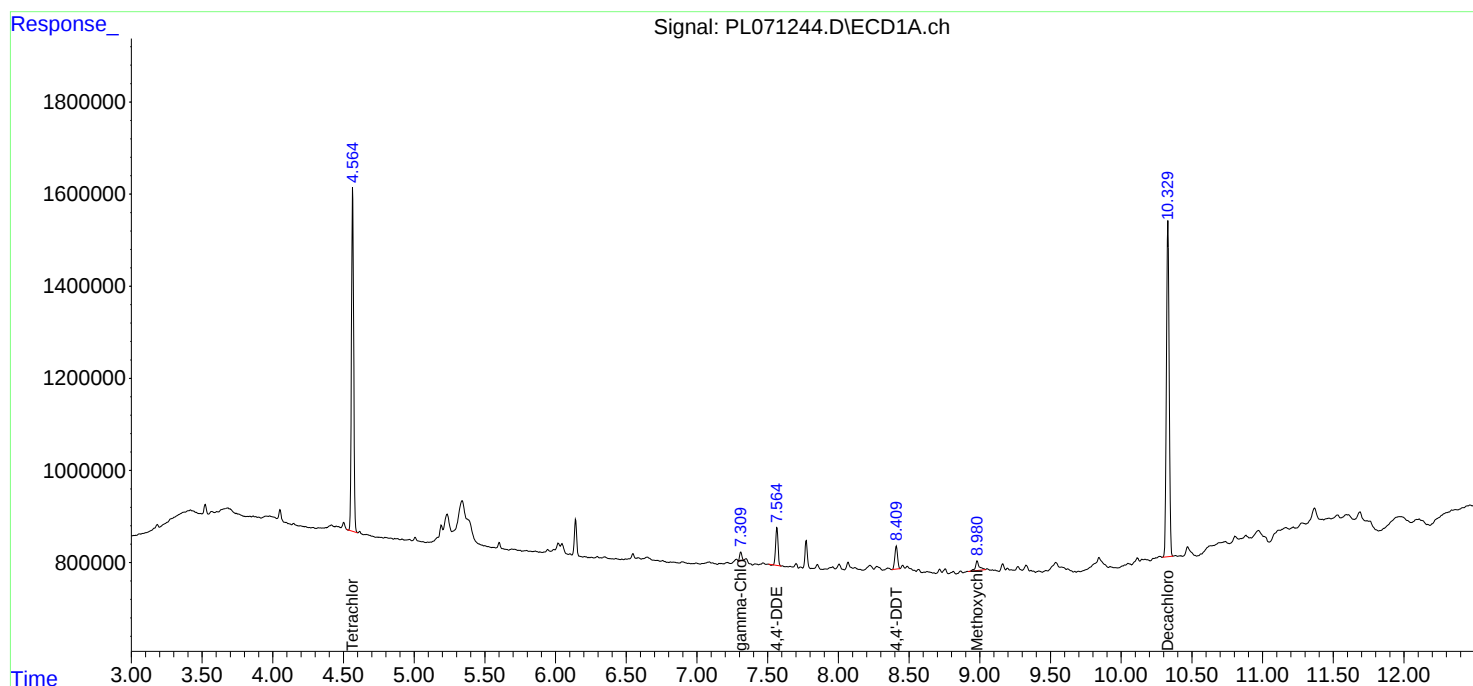


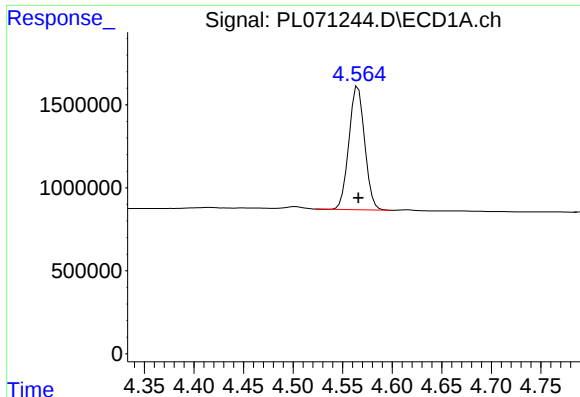

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 8224155
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

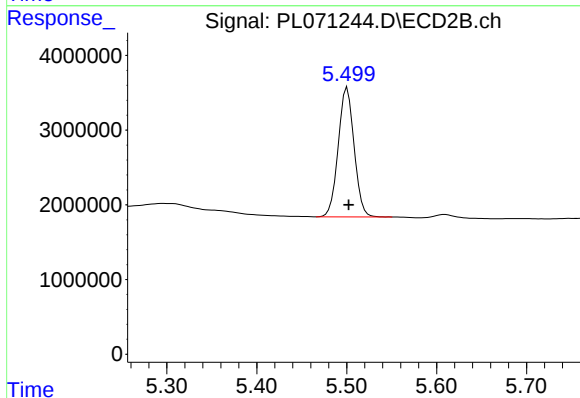


#1 Tetrachloro-m-xylene

R.T.: 5.501 min
Delta R.T.: -0.001 min
Response: 21259329
Conc: 16.94 ng/ml

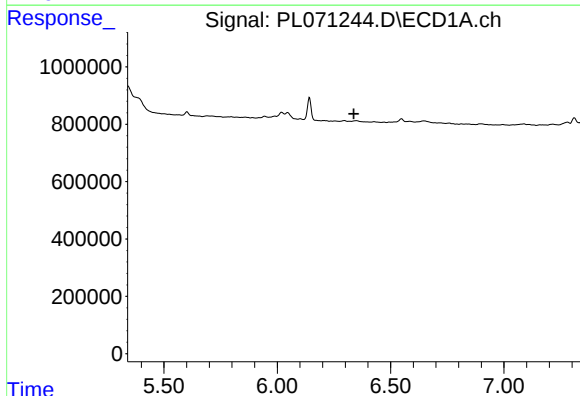


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

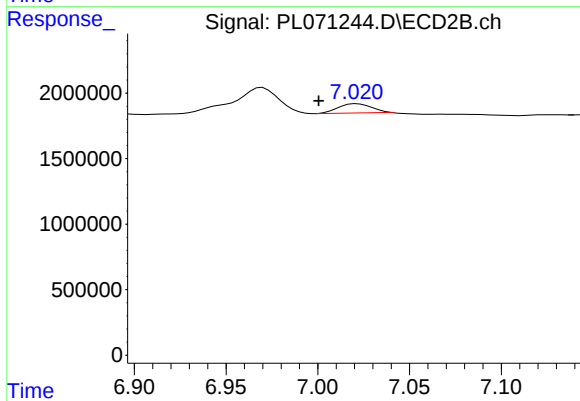

#7 delta-BHC


R.T.: 7.021 min
Delta R.T.: 0.021 min
Response: 787513
Conc: 0.46 ng/ml

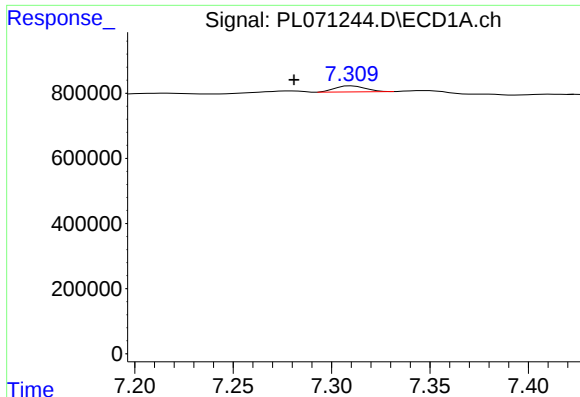

#10 gamma-Chlordane


R.T.: 7.310 min
Delta R.T.: 0.029 min
Response: 198649
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

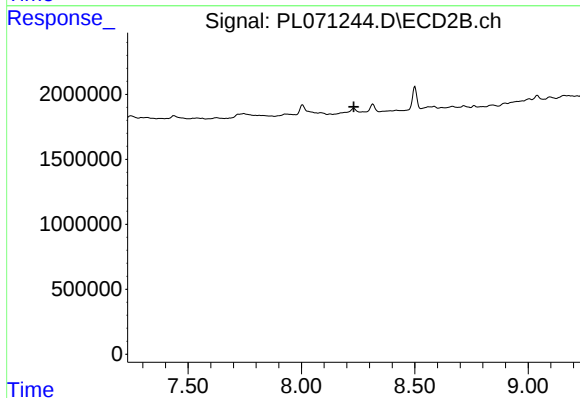


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

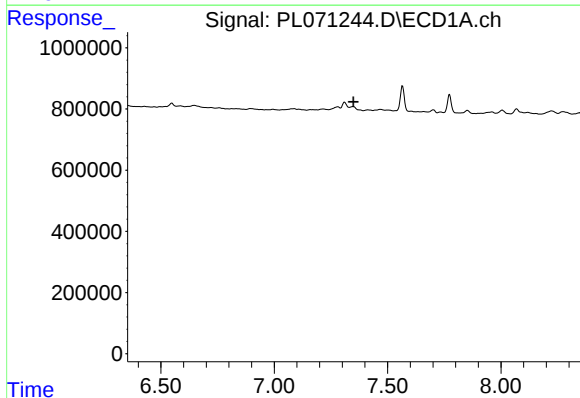


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.

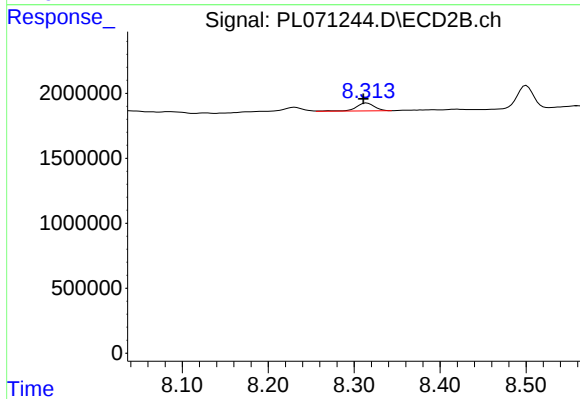

#11 alpha-Chlordane


R.T.: 8.315 min
Delta R.T.: 0.004 min
Response: 896689
Conc: 0.56 ng/ml

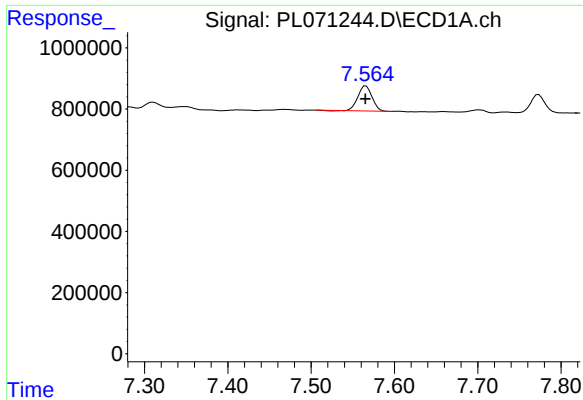

#12 4,4'-DDE


R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 962224
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

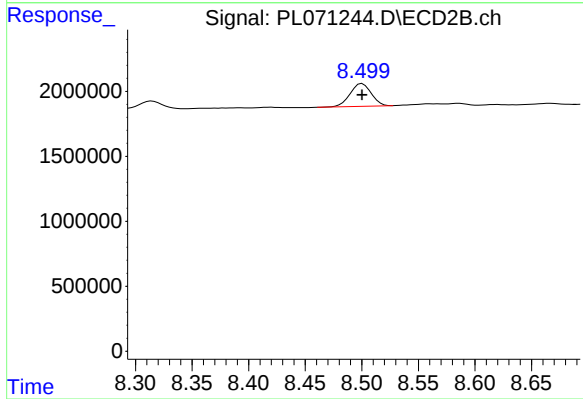


#12 4,4'-DDE

R.T.: 8.500 min
Delta R.T.: 0.000 min
Response: 2291902
Conc: 1.49 ng/ml

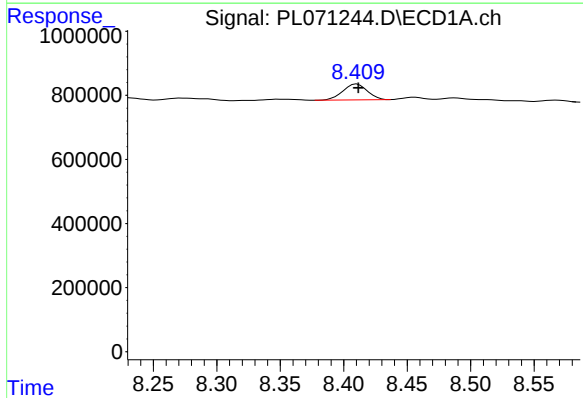


#17 4,4'-DDT

R.T.: 8.410 min
Delta R.T.: -0.001 min
Response: 660603
Conc: 1.21 ng/ml

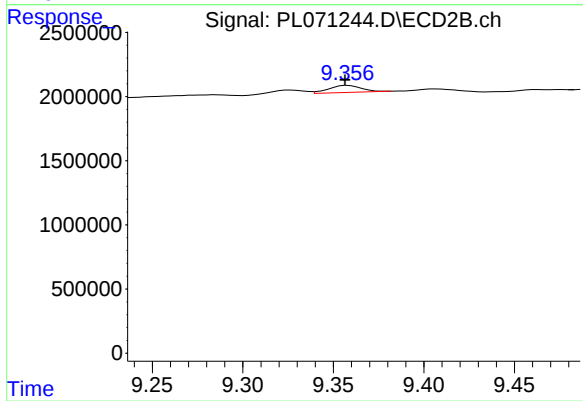

#17 4,4'-DDT


R.T.: 9.358 min
Delta R.T.: 0.002 min
Response: 690523
Conc: 0.50 ng/ml

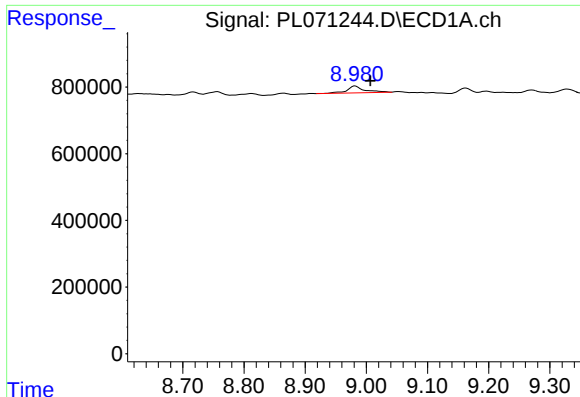

#20 Methoxychlor


R.T.: 8.982 min
Delta R.T.: -0.025 min
Response: 397663
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

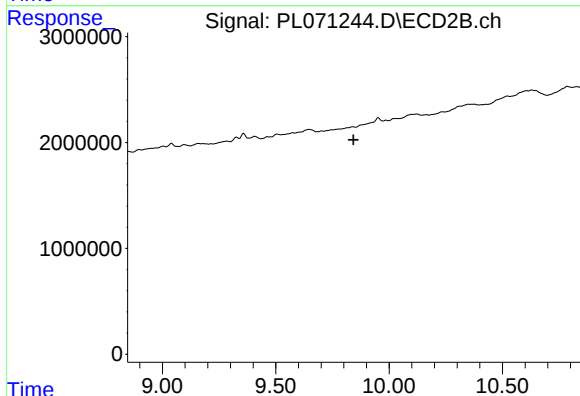


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

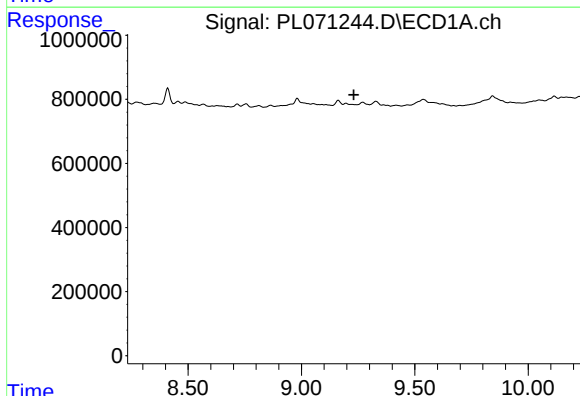


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

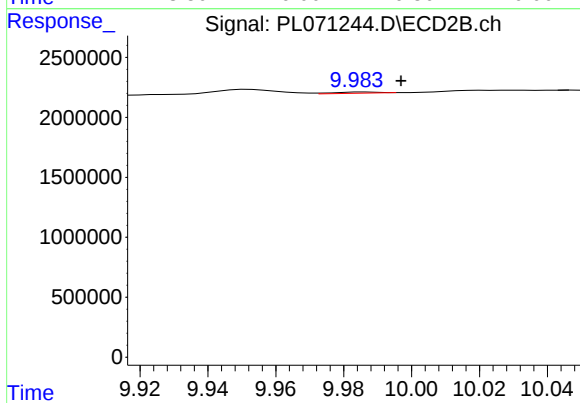

#21 Endrin ketone


R.T.: 9.986 min
Delta R.T.: -0.011 min
Response: 89750
Conc: 0.06 ng/ml

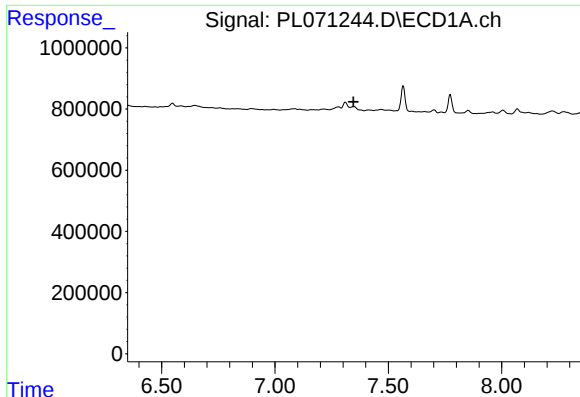

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

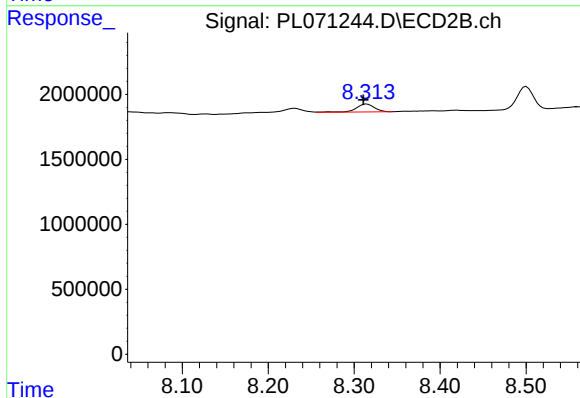


#26 Chlordane-4

R.T.: 8.315 min
Delta R.T.: 0.004 min
Response: 896689
Conc: 3.38 ng/ml

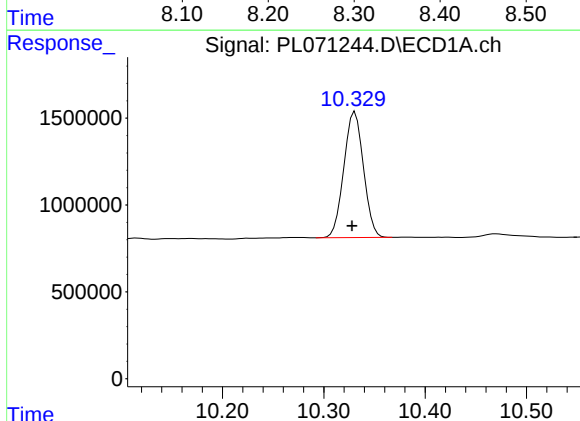

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.003 min
Response: 9739563
Conc: 13.45 ng/ml

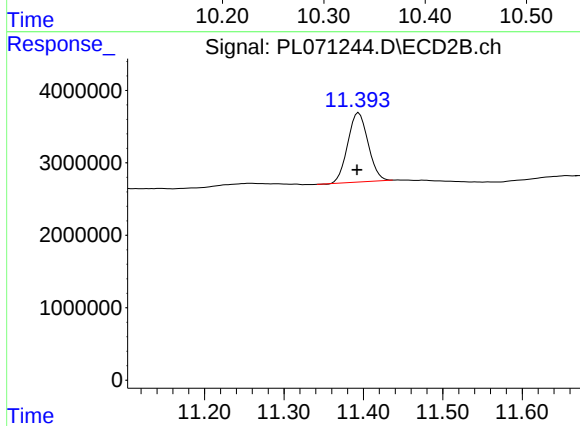

#28 Decachlorobiphenyl

R.T.: 11.394 min
Delta R.T.: 0.002 min
Response: 17007324
Conc: 12.24 ng/ml