

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
 Data File : PL071246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 14:00
 Operator : AR\AJ
 Sample : M4891-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:25:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.503	11254267	30964572	23.961	24.674
28)	SA Decachlor...	10.333	11.400	12083636	21524347	16.688	15.485
Target Compounds							
7)	B delta-BHC	0.000	7.025f	0	281663	N.D.	0.166 #
10)	B gamma-Chl...	7.283	0.000	241385	0	0.380	N.D. #
14)	MA Endrin	8.010f	0.000	164597	0	0.291	N.D. #
15)	B Endosulfa...	8.267f	0.000	128666	0	0.220	N.D. #
21)	B Endrin ke...	0.000	9.980f	0	2989315	N.D.	2.041 #
24)	Chlordane-2	6.581	0.000	122797	0	5.234	N.D. #
25)	Chlordane-3	7.283	0.000	241385	0	3.892	N.D. #
27)	Chlordane-5	8.267f	0.000	128666	0	5.390	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
Data File : PL071246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 14:00
Operator : AR\AJ
Sample : M4891-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:25:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

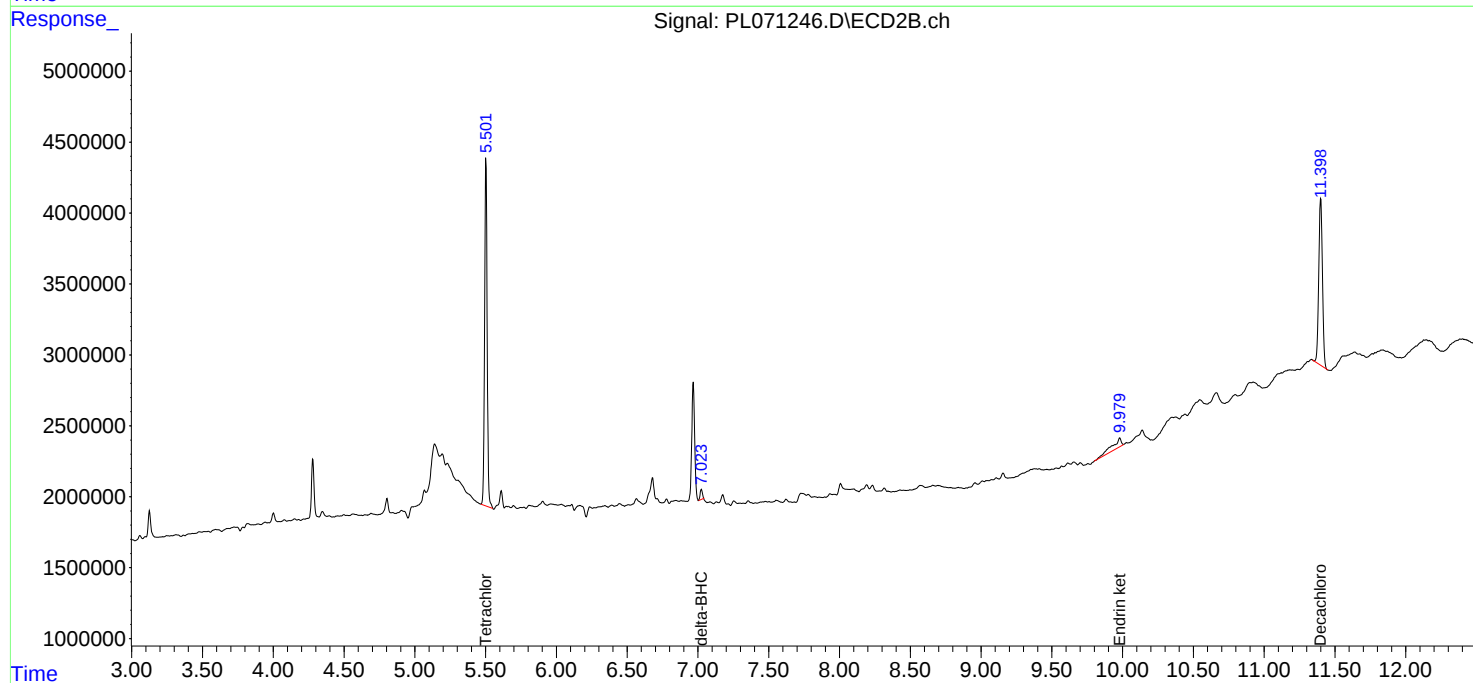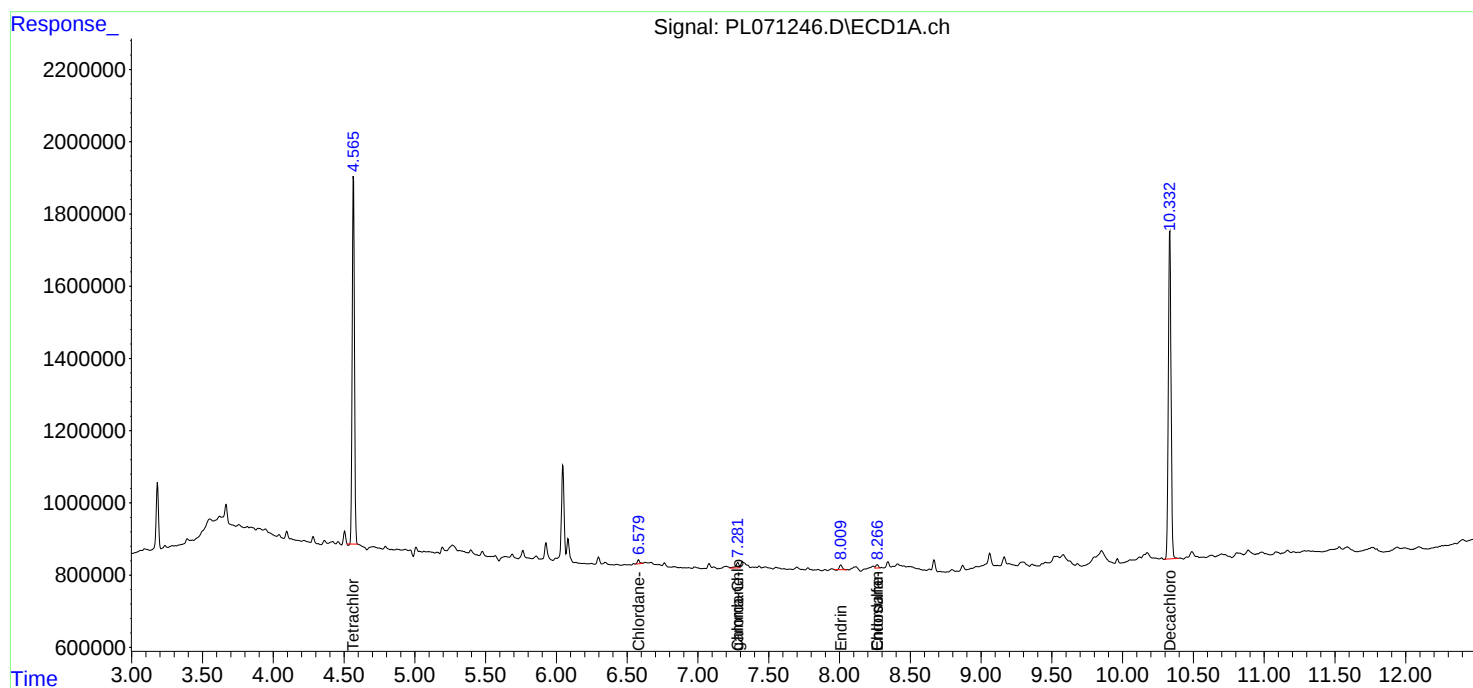


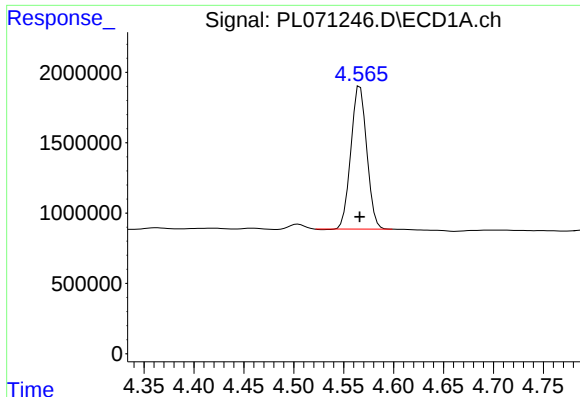

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.000 min
Response: 11254267
Conc: 23.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

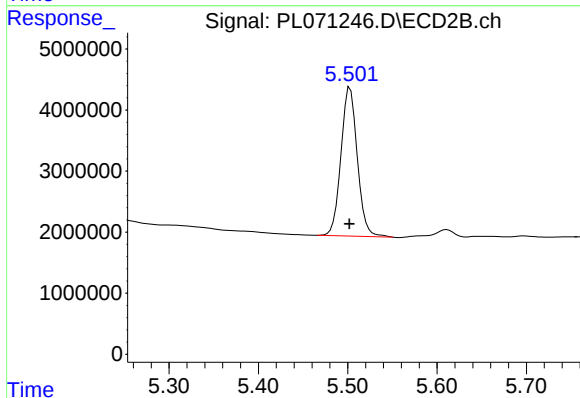


#1 Tetrachloro-m-xylene

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 30964572
Conc: 24.67 ng/ml

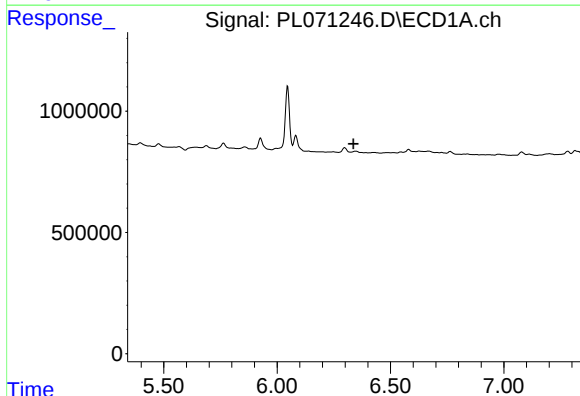


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

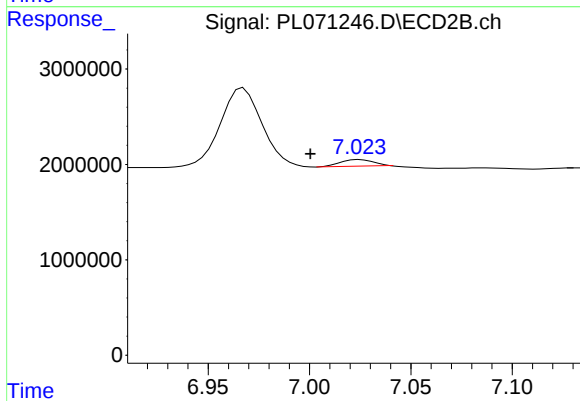

#7 delta-BHC


R.T.: 7.025 min
Delta R.T.: 0.024 min
Response: 281663
Conc: 0.17 ng/ml

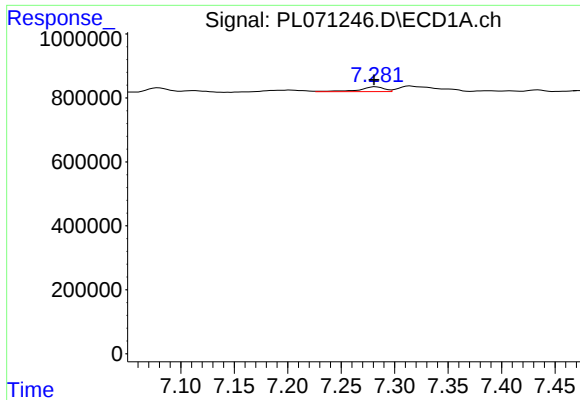

#10 gamma-Chlordane


R.T.: 7.283 min
Delta R.T.: 0.002 min
Response: 241385
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

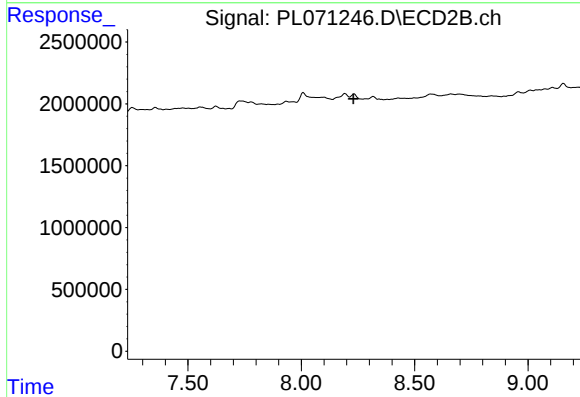


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

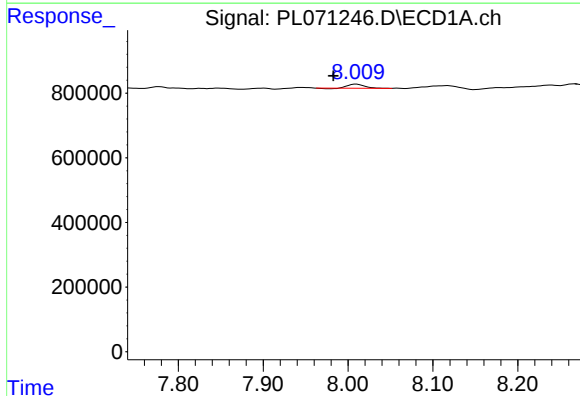


#14 Endrin

R.T.: 8.010 min
Delta R.T.: 0.027 min
Response: 164597
Conc: 0.29 ng/ml



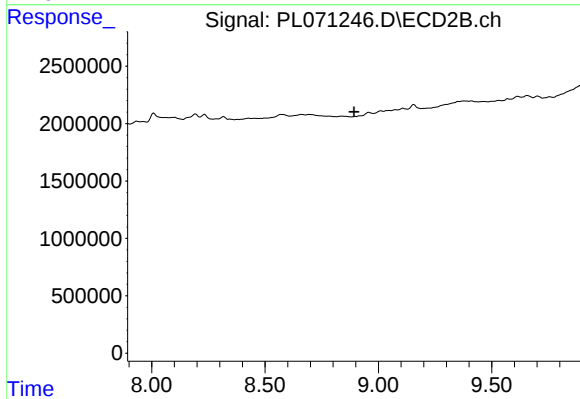



#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

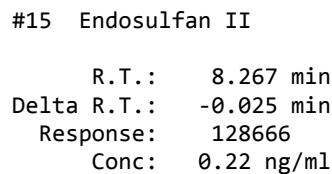

Instrument :
ECD_L
ClientSampleId :

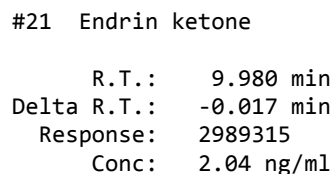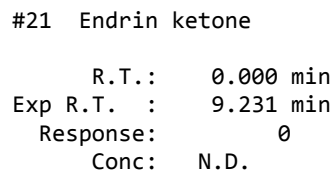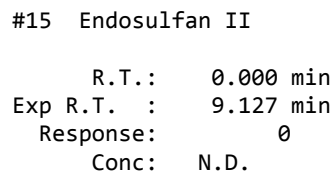


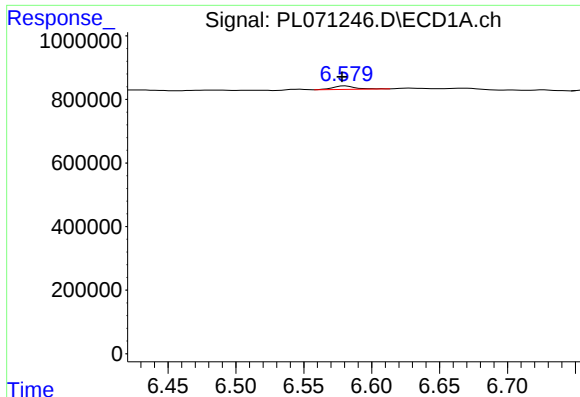

#24 Chlordane-2


R.T.: 6.581 min
Delta R.T.: 0.003 min
Response: 122797
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

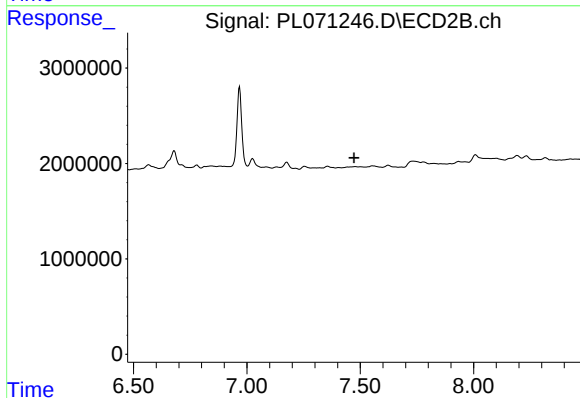


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.472 min
Response: 0
Conc: N.D.

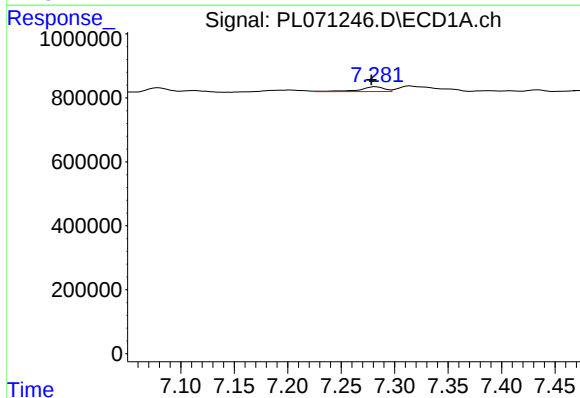

#25 Chlordane-3

R.T.: 7.283 min
Delta R.T.: 0.004 min
Response: 241385
Conc: 3.89 ng/ml

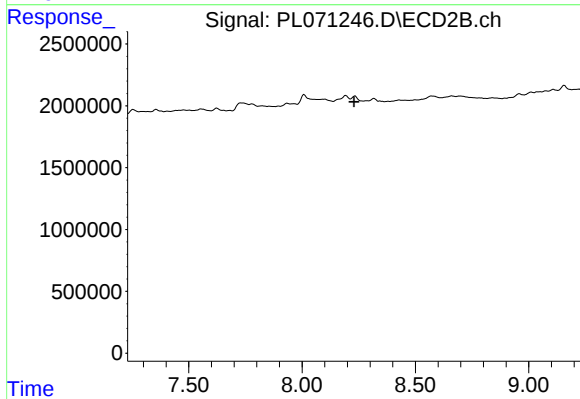

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

