

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
 Data File : PL071247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 14:16
 Operator : AR\AJ
 Sample : M4891-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:25:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.567	5.503	11377155	31161582	24.222	24.831
28)	SA Decachlor...	10.331	11.396	13968151	24278129	19.291	17.466
Target Compounds							
10)	B gamma-Chl...	7.282	0.000	271808	0	0.428	N.D. #
14)	MA Endrin	8.008f	0.000	183899	0	0.325	N.D. #
15)	B Endosulfa...	8.267f	9.154f	220965	1399671	0.378	1.039 #
25)	Chlordane-3	7.282	0.000	271808	0	4.383	N.D. #
27)	Chlordane-5	8.267f	0.000	220965	0	9.257	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
Data File : PL071247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 14:16
Operator : AR\AJ
Sample : M4891-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:25:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

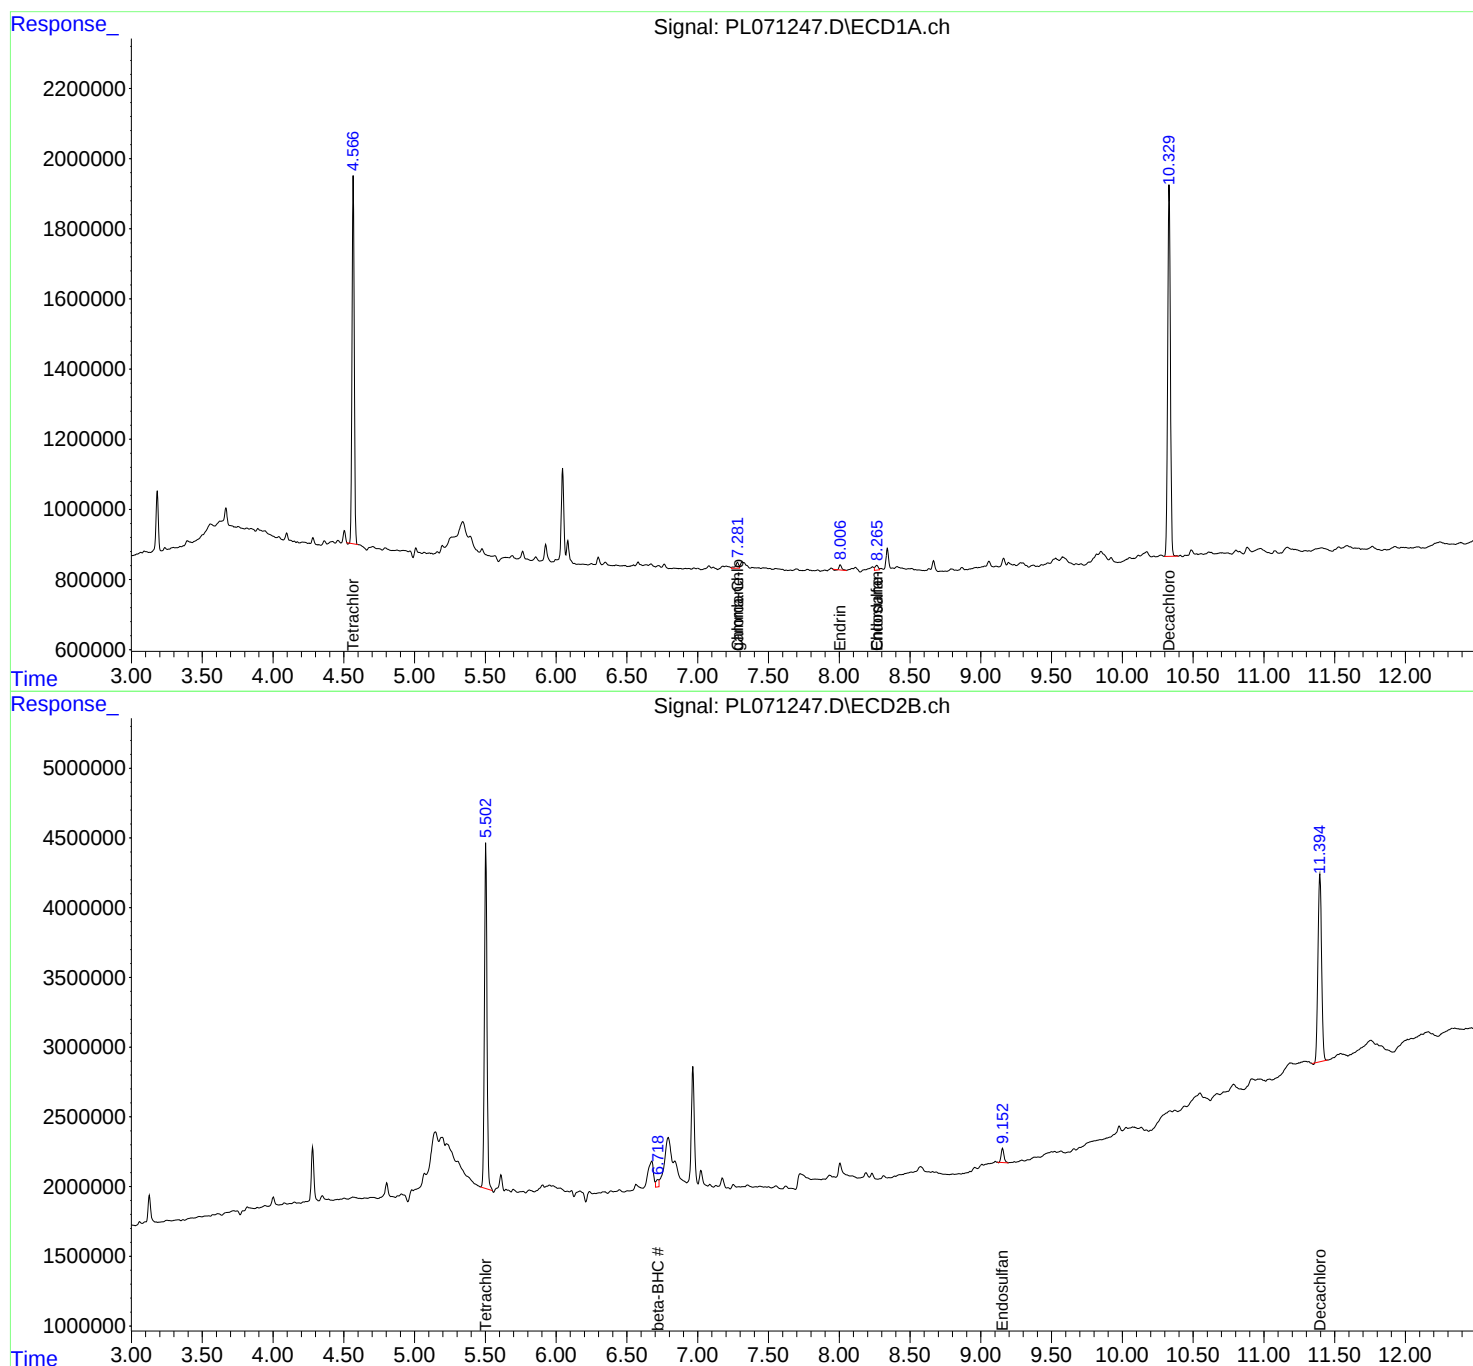


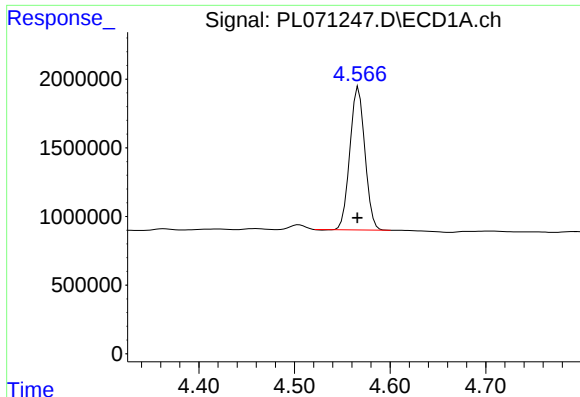

#1 Tetrachloro-m-xylene


R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 11377155
Conc: 24.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

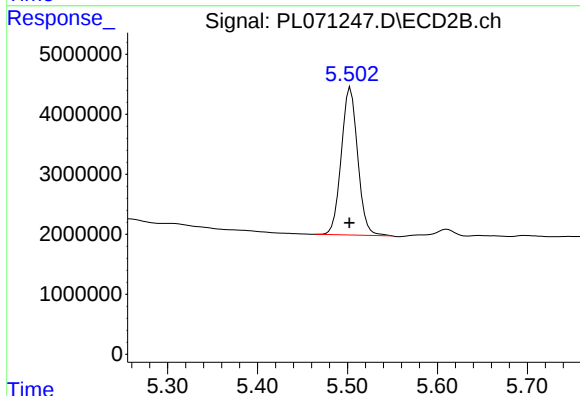


#1 Tetrachloro-m-xylene

R.T.: 5.503 min
Delta R.T.: 0.001 min
Response: 31161582
Conc: 24.83 ng/ml

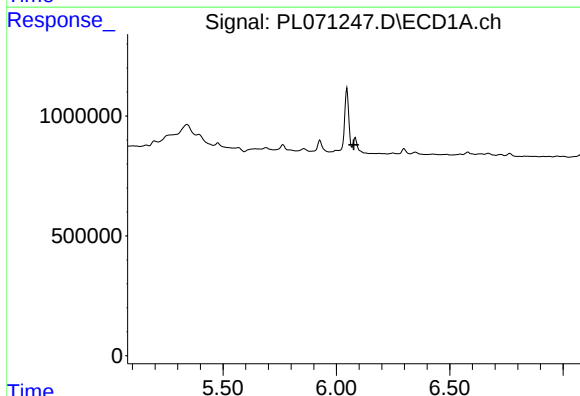


#6 beta-BHC

R.T.: 6.083 min
Delta R.T.: 0.006 min
Response: -1267539
Conc: N.D.

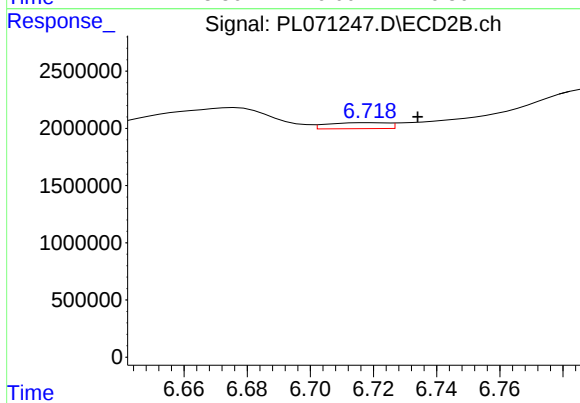

#6 beta-BHC


R.T.: 6.719 min
Delta R.T.: -0.015 min
Response: 694909
Conc: 0.79 ng/ml

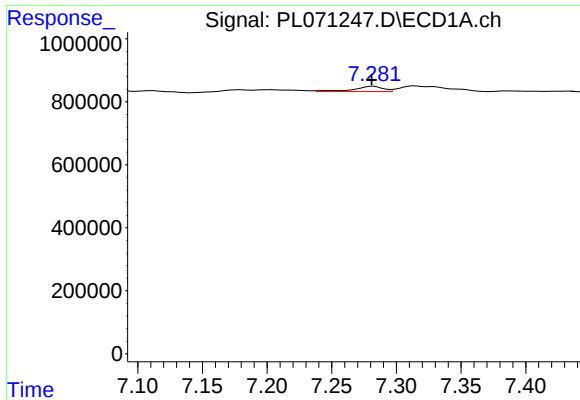

#10 gamma-Chlordane


R.T.: 7.282 min
Delta R.T.: 0.001 min
Response: 271808
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

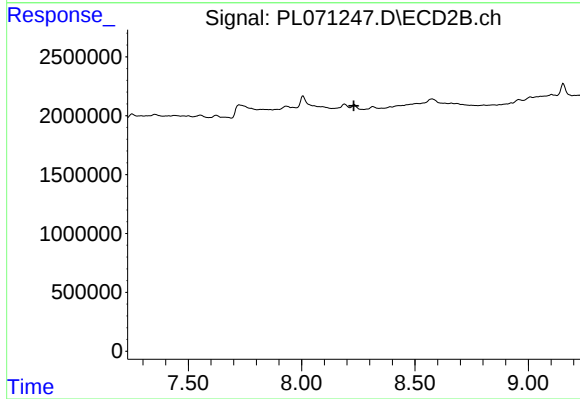


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.230 min
Response: 0
Conc: N.D.

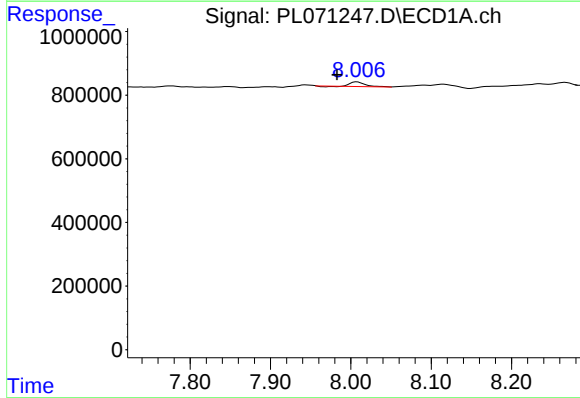


#14 Endrin

R.T.: 8.008 min
Delta R.T.: 0.025 min
Response: 183899
Conc: 0.33 ng/ml

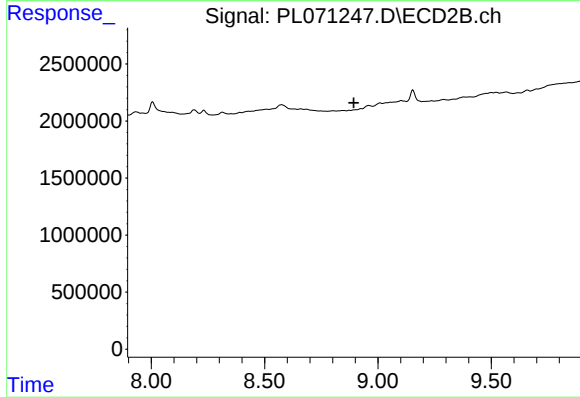

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

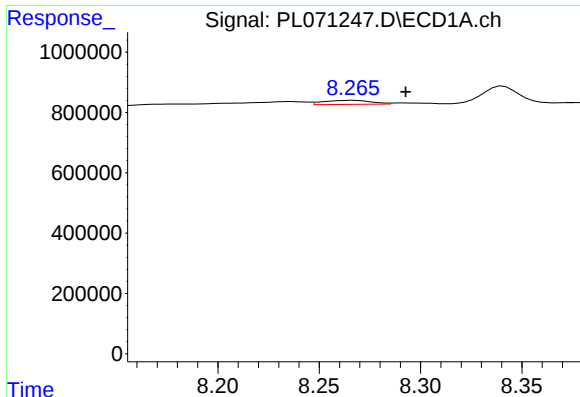

#15 Endosulfan II


R.T.: 8.267 min
Delta R.T.: -0.026 min
Response: 220965
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

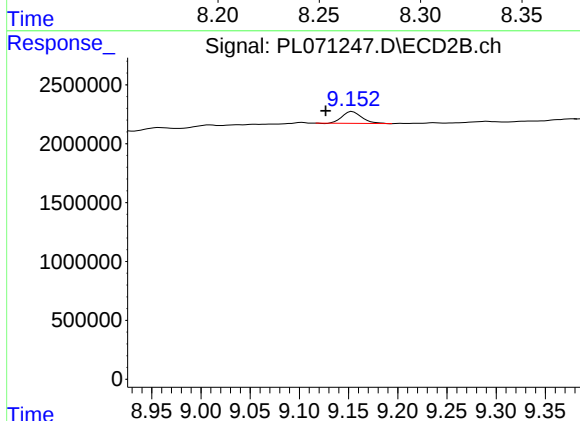


#15 Endosulfan II

R.T.: 9.154 min
Delta R.T.: 0.027 min
Response: 1399671
Conc: 1.04 ng/ml

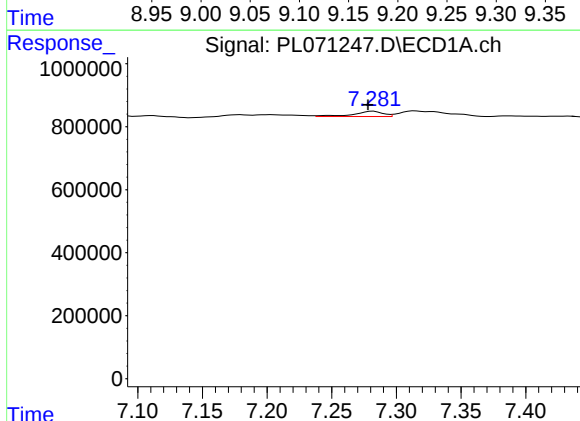


#25 Chlordane-3

R.T.: 7.282 min
Delta R.T.: 0.004 min
Response: 271808
Conc: 4.38 ng/ml

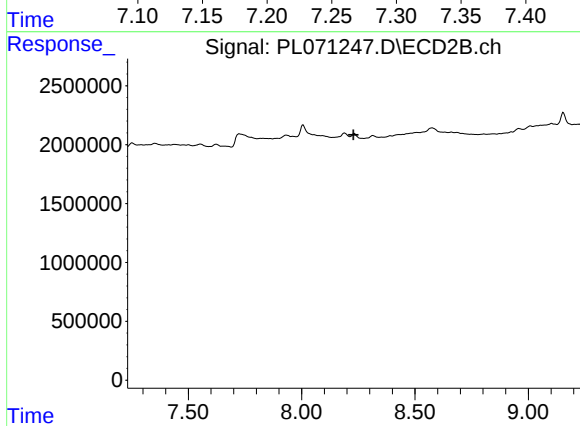

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

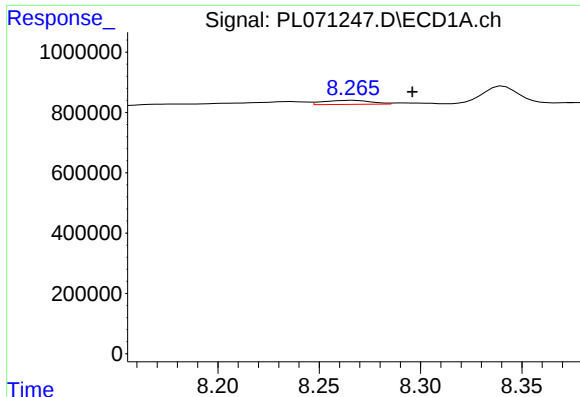

#27 Chlordane-5


R.T.: 8.267 min
Delta R.T.: -0.029 min
Response: 220965
Conc: 9.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

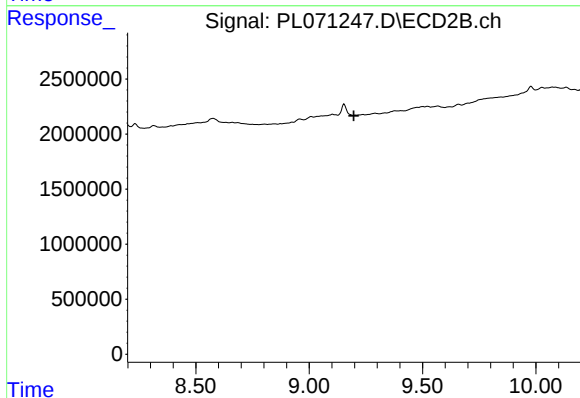


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

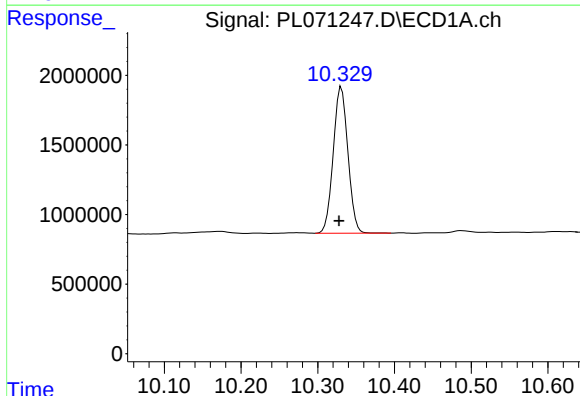

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.003 min
Response: 13968151
Conc: 19.29 ng/ml

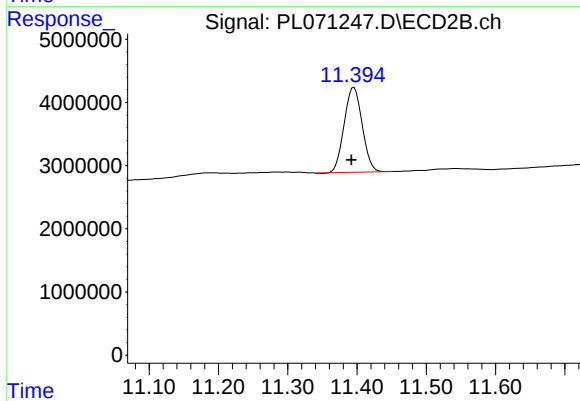

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.004 min
Response: 24278129
Conc: 17.47 ng/ml