

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
 Data File : PL071251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 15:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:26:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.500	10631597	28204107	22.635	22.475
28)	SA Decachlor...	10.330	11.396	13077538	25410296	18.061	18.281
Target Compounds							
2)	A alpha-BHC	5.251f	6.057f	153127	712115	0.234	0.385 #
3)	MA gamma-BHC...	5.706	0.000	406334	0	0.636	N.D. #
7)	B delta-BHC	0.000	7.020f	0	1850367	N.D.	1.088 #
14)	MA Endrin	8.007f	0.000	289870	0	0.513	N.D. #
15)	B Endosulfa...	8.270f	0.000	175111	0	0.300	N.D. #
20)	A Methoxychlor	8.985f	0.000	394878	0	1.093	N.D. #
21)	B Endrin ke...	0.000	10.022f	0	1343101	N.D.	0.917 #
27)	Chlordane-5	8.270f	0.000	175111	0	7.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
Data File : PL071251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 15:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:26:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

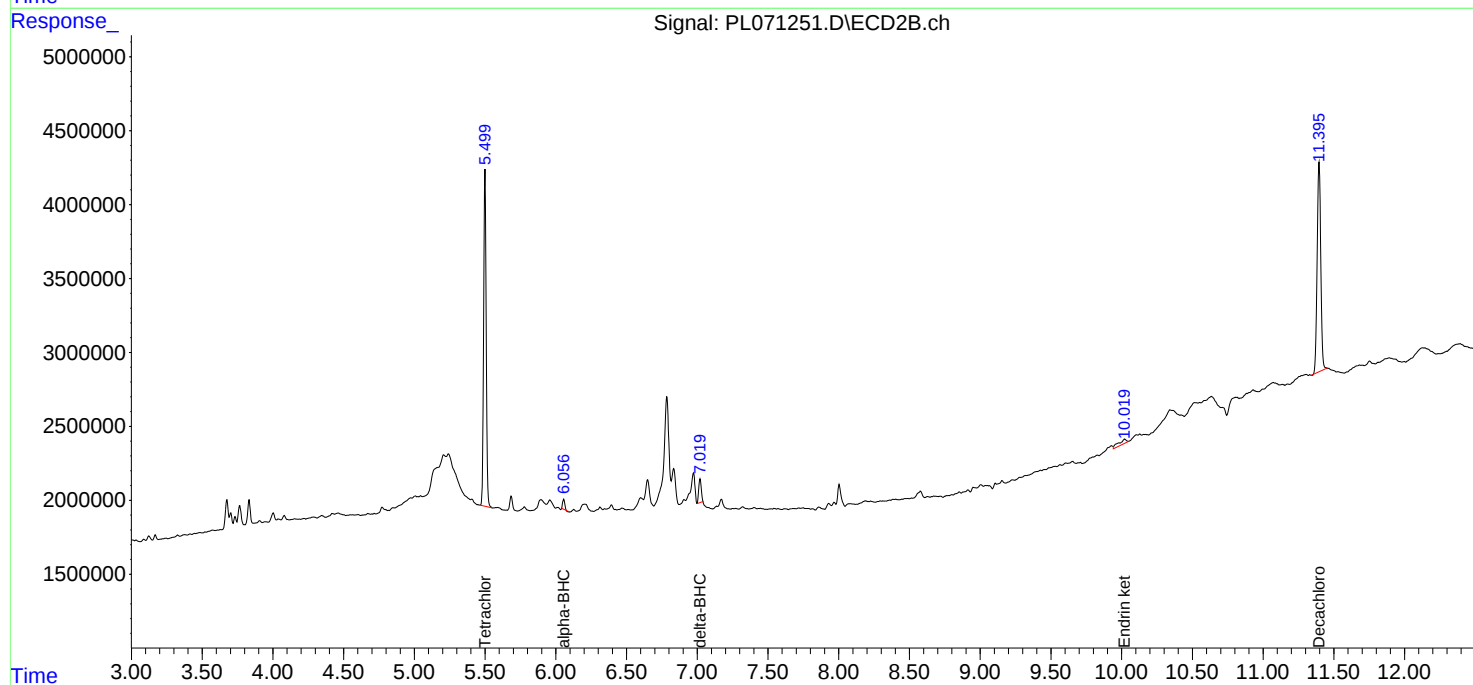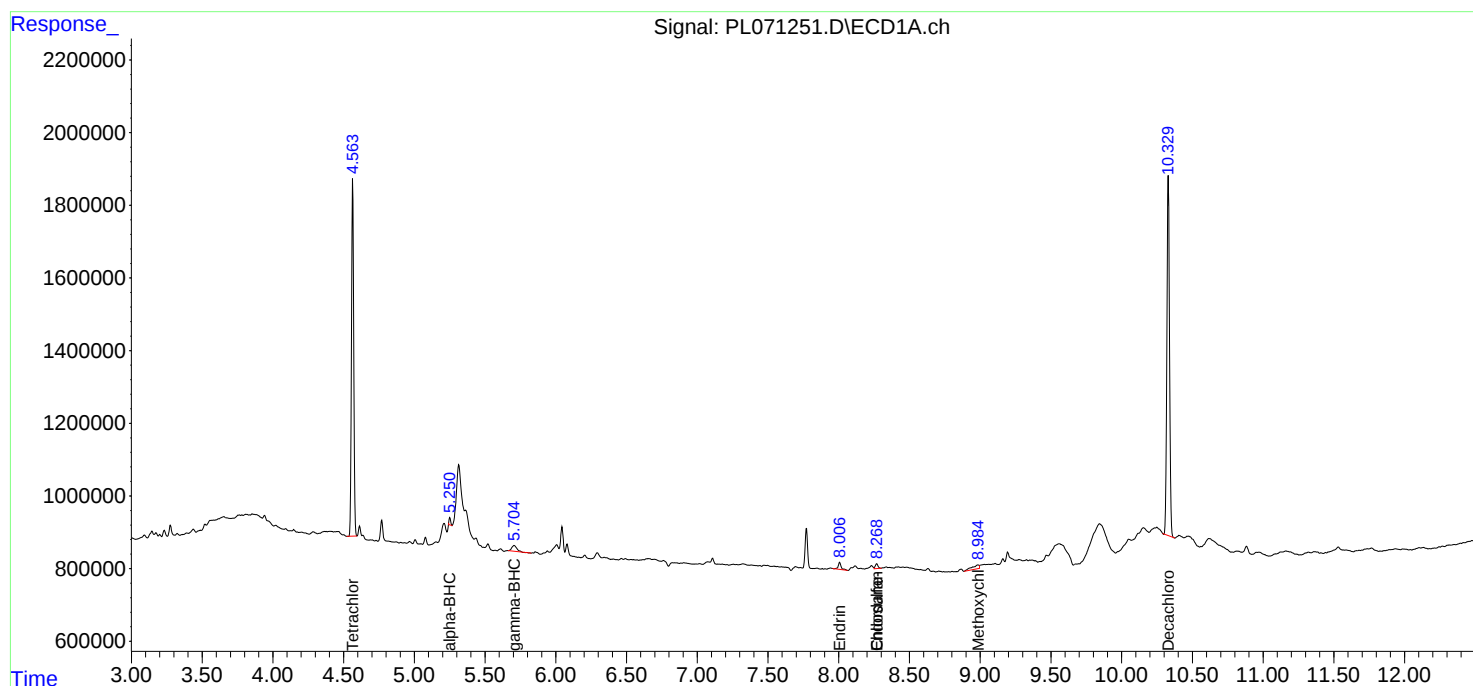


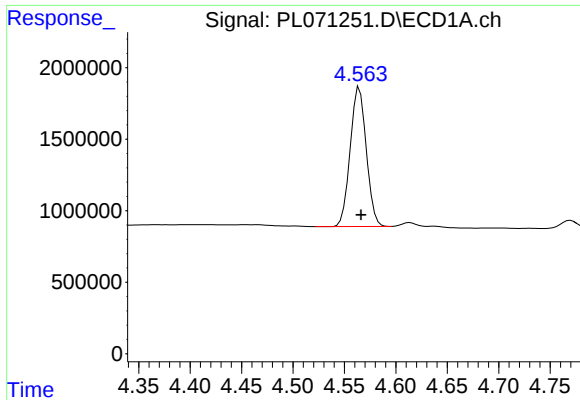

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: -0.001 min
Response: 10631597
Conc: 22.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

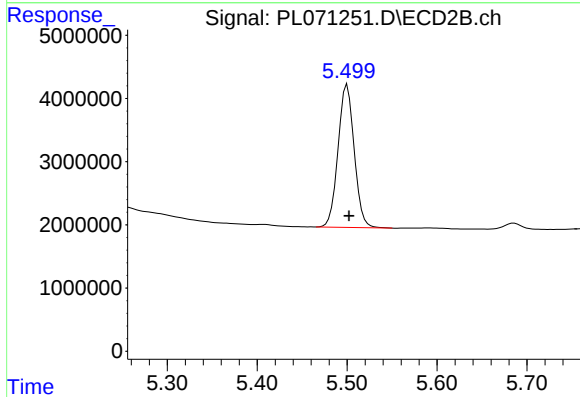


#1 Tetrachloro-m-xylene

R.T.: 5.500 min
Delta R.T.: -0.002 min
Response: 28204107
Conc: 22.47 ng/ml

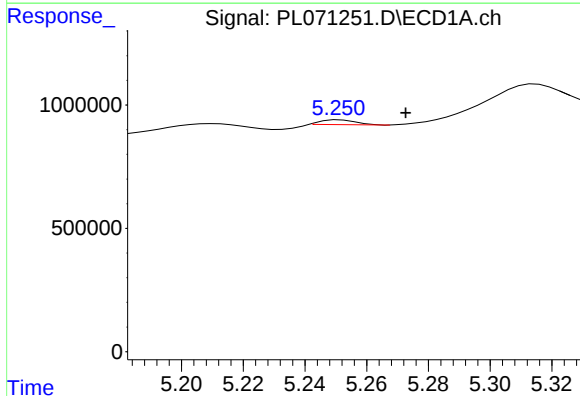


#2 alpha-BHC

R.T.: 5.251 min
Delta R.T.: -0.021 min
Response: 153127
Conc: 0.23 ng/ml

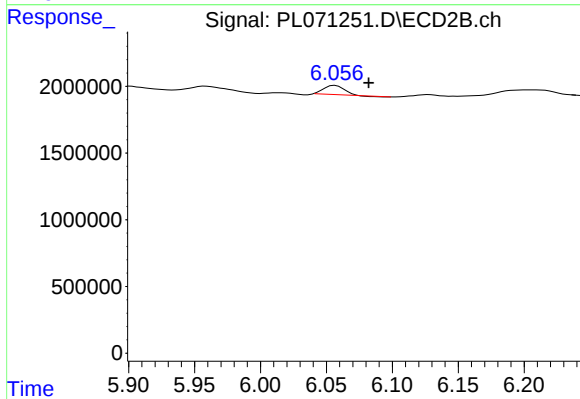

#2 alpha-BHC


R.T.: 6.057 min
Delta R.T.: -0.025 min
Response: 712115
Conc: 0.38 ng/ml

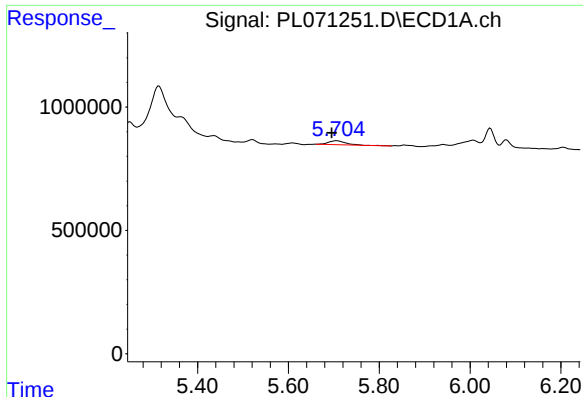

#3 gamma-BHC (Lindane)


R.T.: 5.706 min
Delta R.T.: 0.011 min
Response: 406334
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

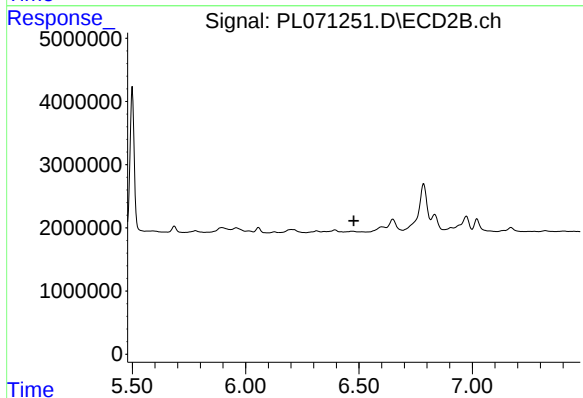


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

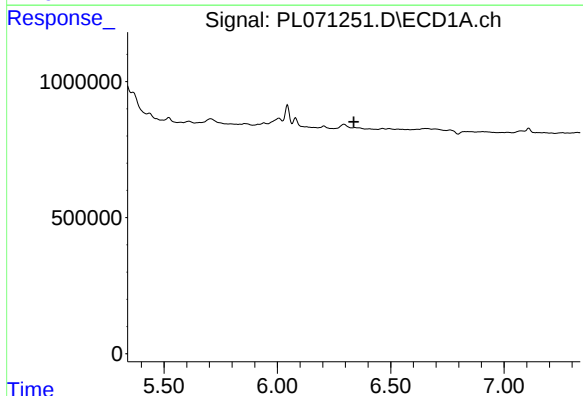


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

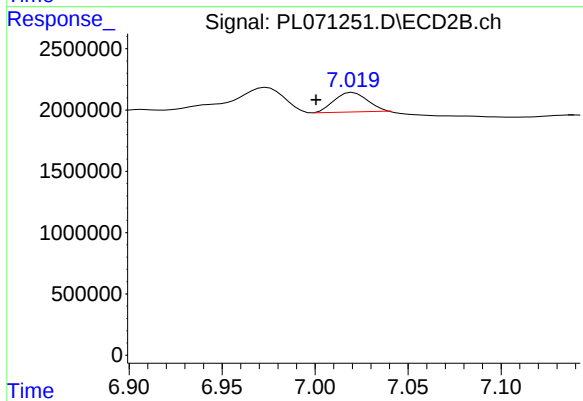

#7 delta-BHC


R.T.: 7.020 min
Delta R.T.: 0.020 min
Response: 1850367
Conc: 1.09 ng/ml

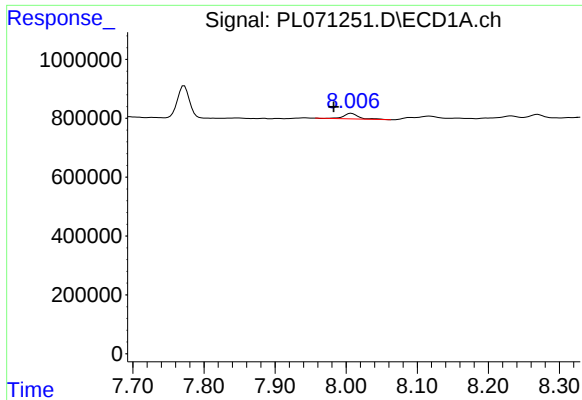

#14 Endrin


R.T.: 8.007 min
Delta R.T.: 0.024 min
Response: 289870
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

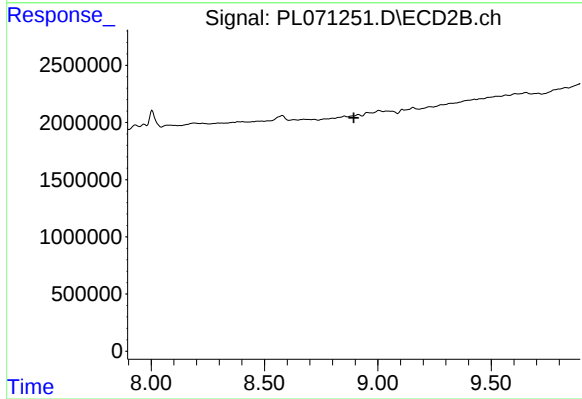


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

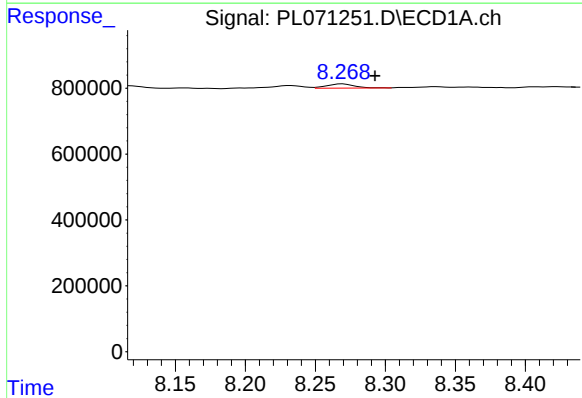


#15 Endosulfan II

R.T.: 8.270 min
Delta R.T.: -0.023 min
Response: 175111
Conc: 0.30 ng/ml

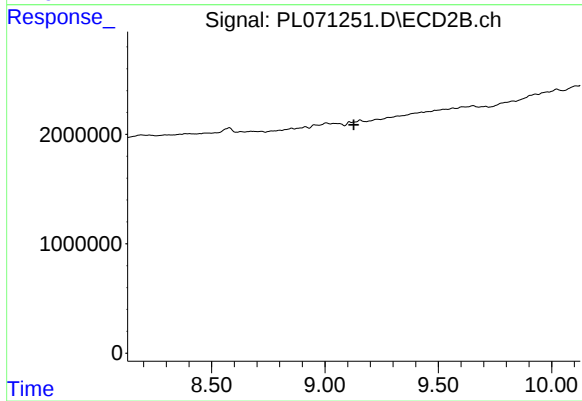

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.127 min
Response: 0
Conc: N.D.

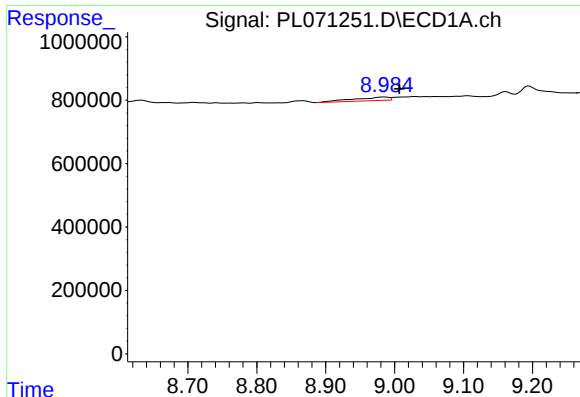

#20 Methoxychlor


R.T.: 8.985 min
Delta R.T.: -0.022 min
Response: 394878
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

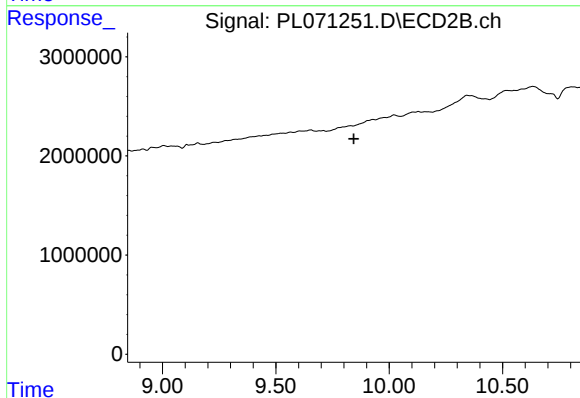


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.843 min
Response: 0
Conc: N.D.

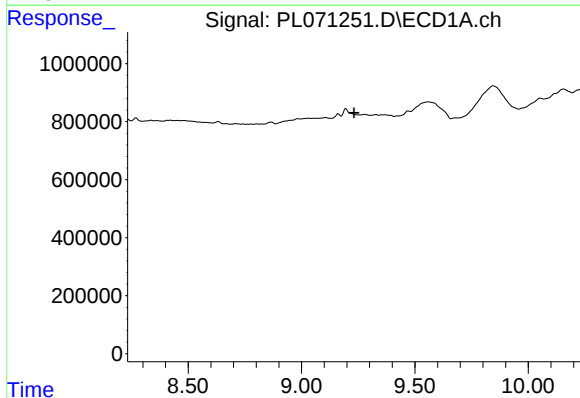


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.

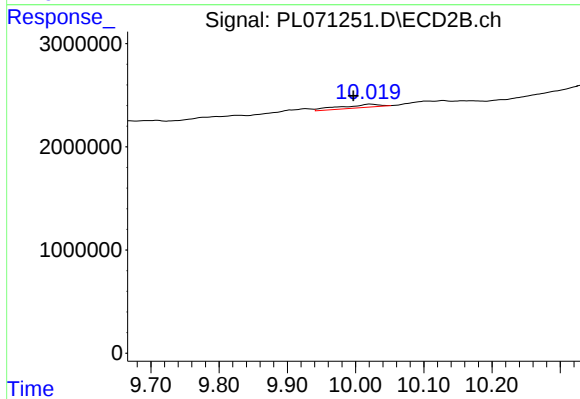

#21 Endrin ketone


R.T.: 10.022 min
Delta R.T.: 0.025 min
Response: 1343101
Conc: 0.92 ng/ml

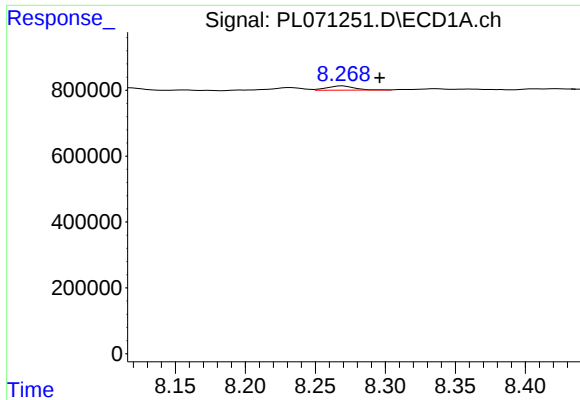

#27 Chlordane-5


R.T.: 8.270 min
Delta R.T.: -0.026 min
Response: 175111
Conc: 7.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

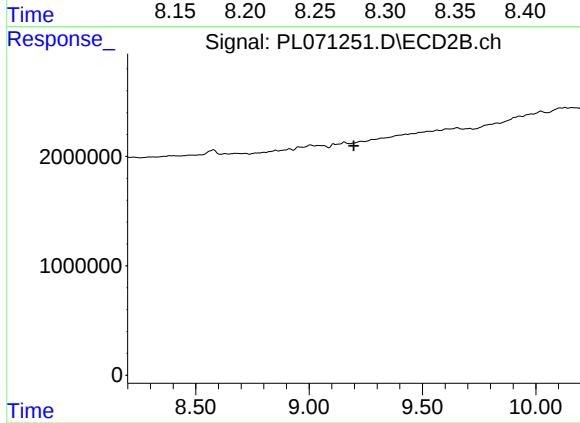


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.197 min
Response: 0
Conc: N.D.

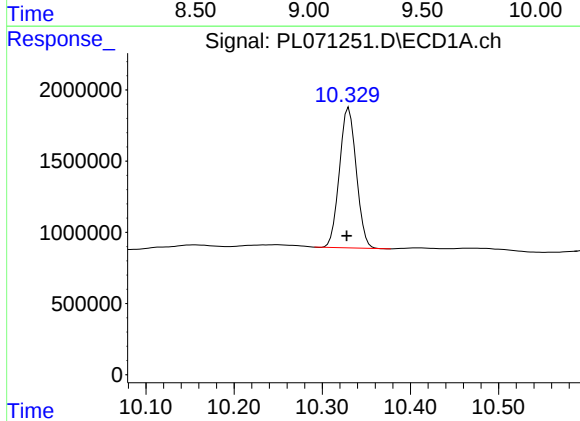

#28 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.002 min
Response: 13077538
Conc: 18.06 ng/ml

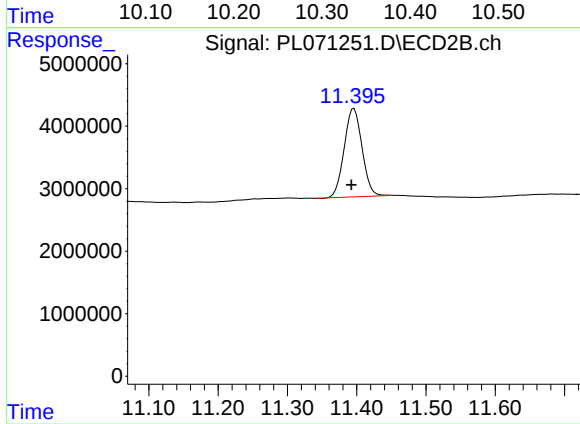

#28 Decachlorobiphenyl

R.T.: 11.396 min
Delta R.T.: 0.004 min
Response: 25410296
Conc: 18.28 ng/ml