

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
 Data File : PL071246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2021 14:00
 Operator : AR\AJ
 Sample : M4891-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MINEBROOK-1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 03:25:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 16:26:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.566	5.503	11254267	30964572	23.961	24.674
28)	SA Decachlor...	10.333	11.400	12083636	21524347	16.688	15.485

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120221\
Data File : PL071246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2021 14:00
Operator : AR\AJ
Sample : M4891-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MINEBROOK-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 03:25:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 16:26:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

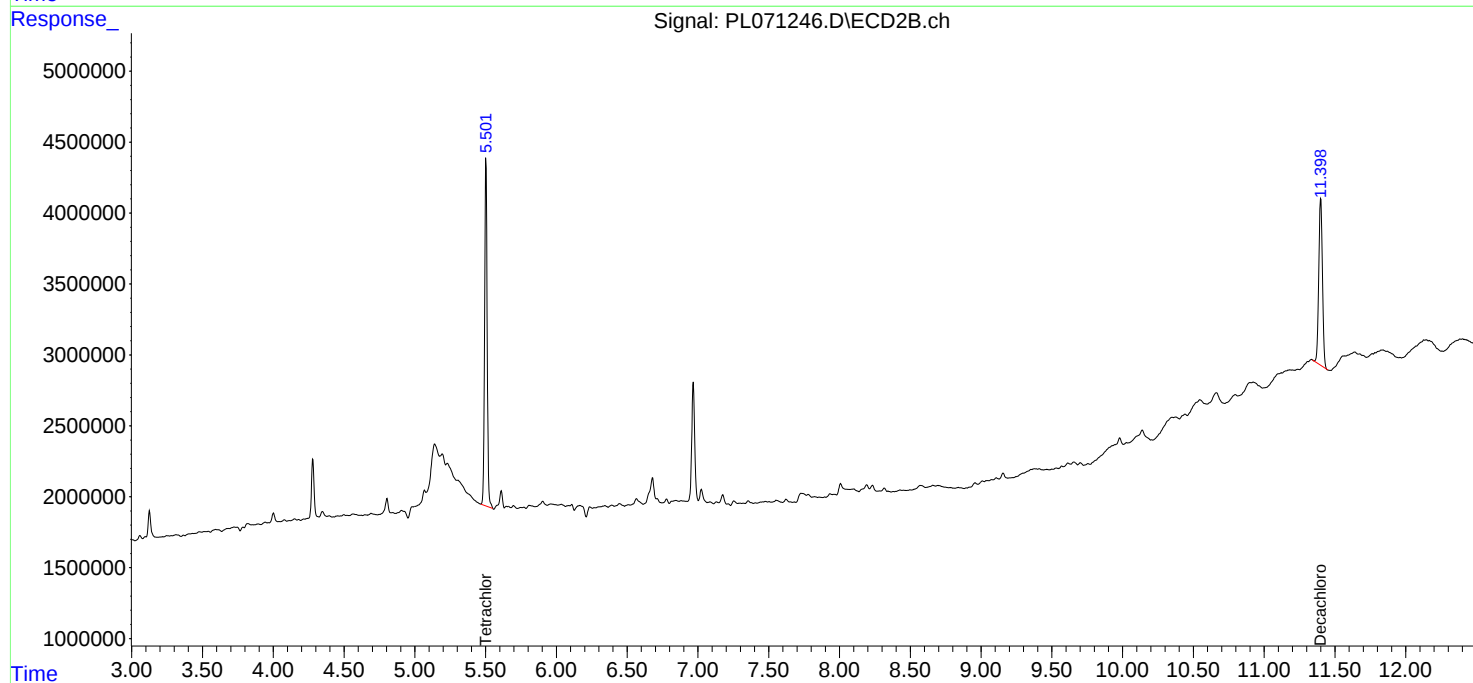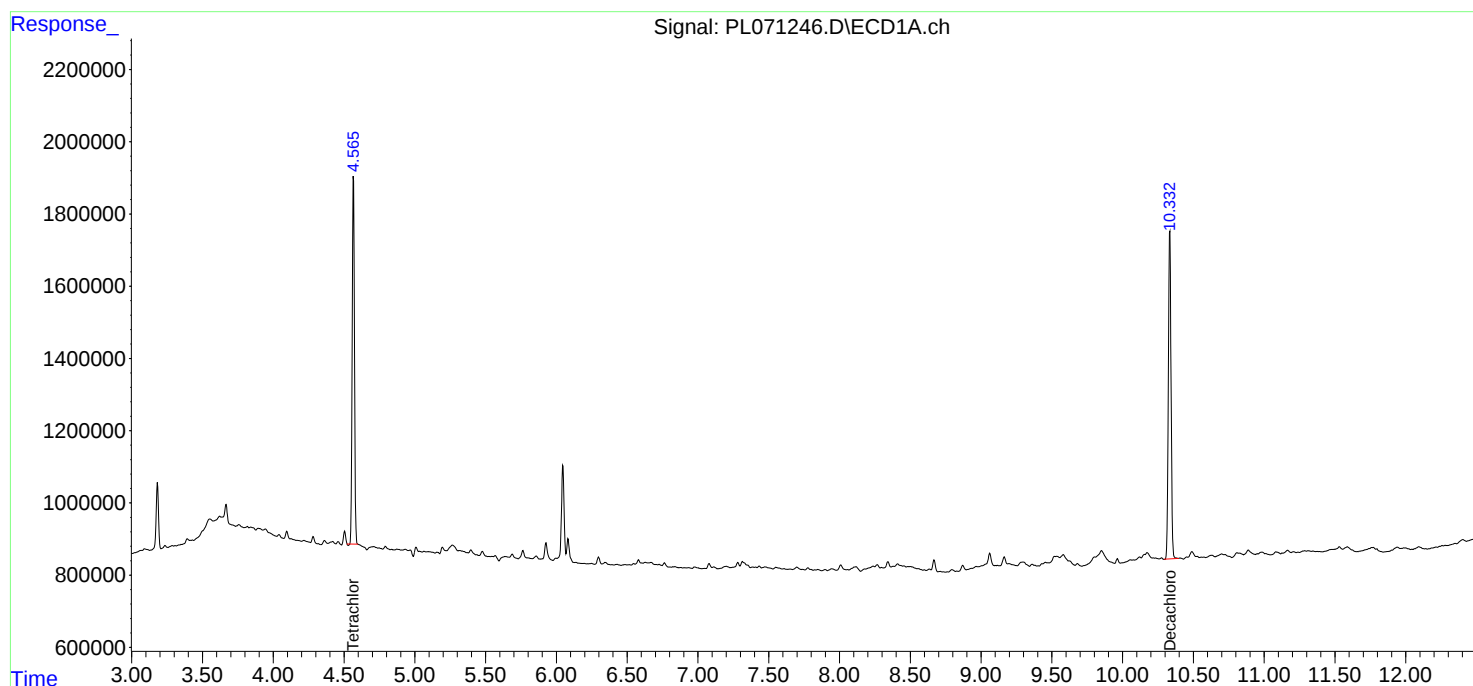


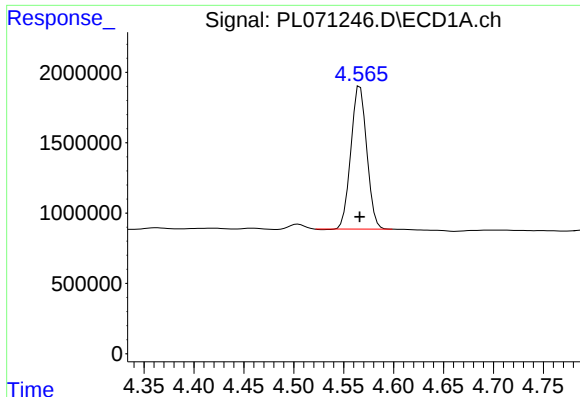

#1 Tetrachloro-m-xylene


R.T.: 4.566 min
Delta R.T.: 0.000 min
Response: 11254267
Conc: 23.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
MINEBROOK-1-COMP

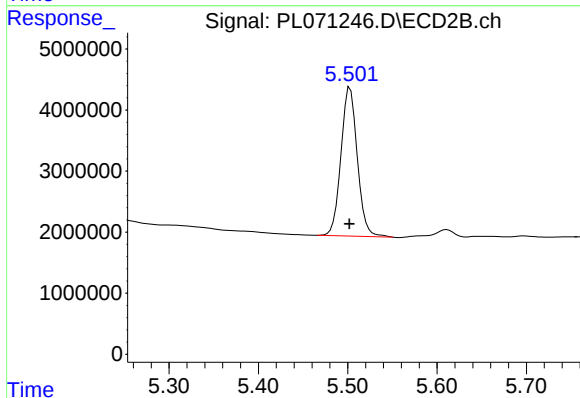


#1 Tetrachloro-m-xylene

R.T.: 5.503 min
Delta R.T.: 0.000 min
Response: 30964572
Conc: 24.67 ng/ml

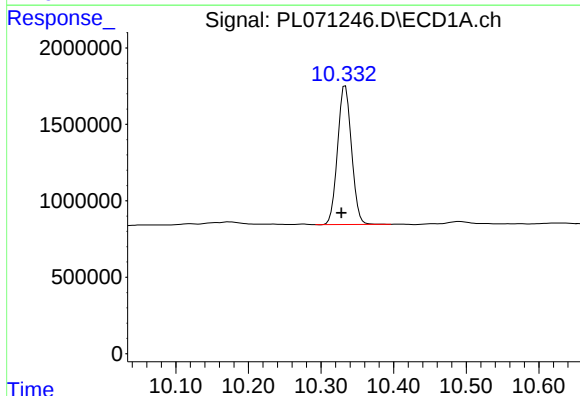

#28 Decachlorobiphenyl

R.T.: 10.333 min
Delta R.T.: 0.006 min
Response: 12083636
Conc: 16.69 ng/ml

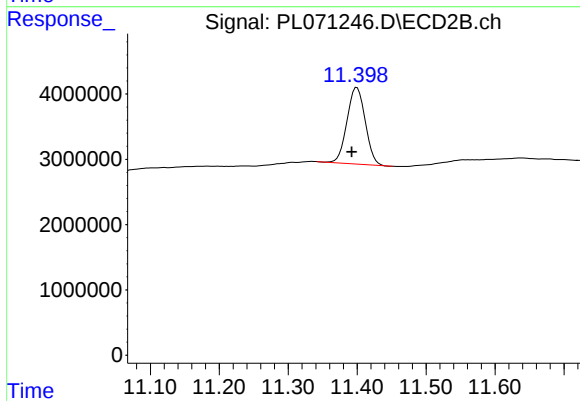

#28 Decachlorobiphenyl

R.T.: 11.400 min
Delta R.T.: 0.008 min
Response: 21524347
Conc: 15.49 ng/ml