

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 19:20
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:54:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 00:54:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	101.7E6	165.8E6	50.000	50.000
28)	SA Decachlor...	8.128	8.992	102.5E6	132.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.268	4.937	27694234	58386639	500.000	500.000
24)	Chlordane-2	4.764	5.404	30448858	65057050	500.000	500.000
25)	Chlordane-3	5.328	6.048	85898062	233.4E6	500.000	500.000
26)	Chlordane-4	5.385	6.122	73275424	276.3E6	500.000	500.000
27)	Chlordane-5	6.213	6.924	31765298	45467624	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 19:20
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:54:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 00:54:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

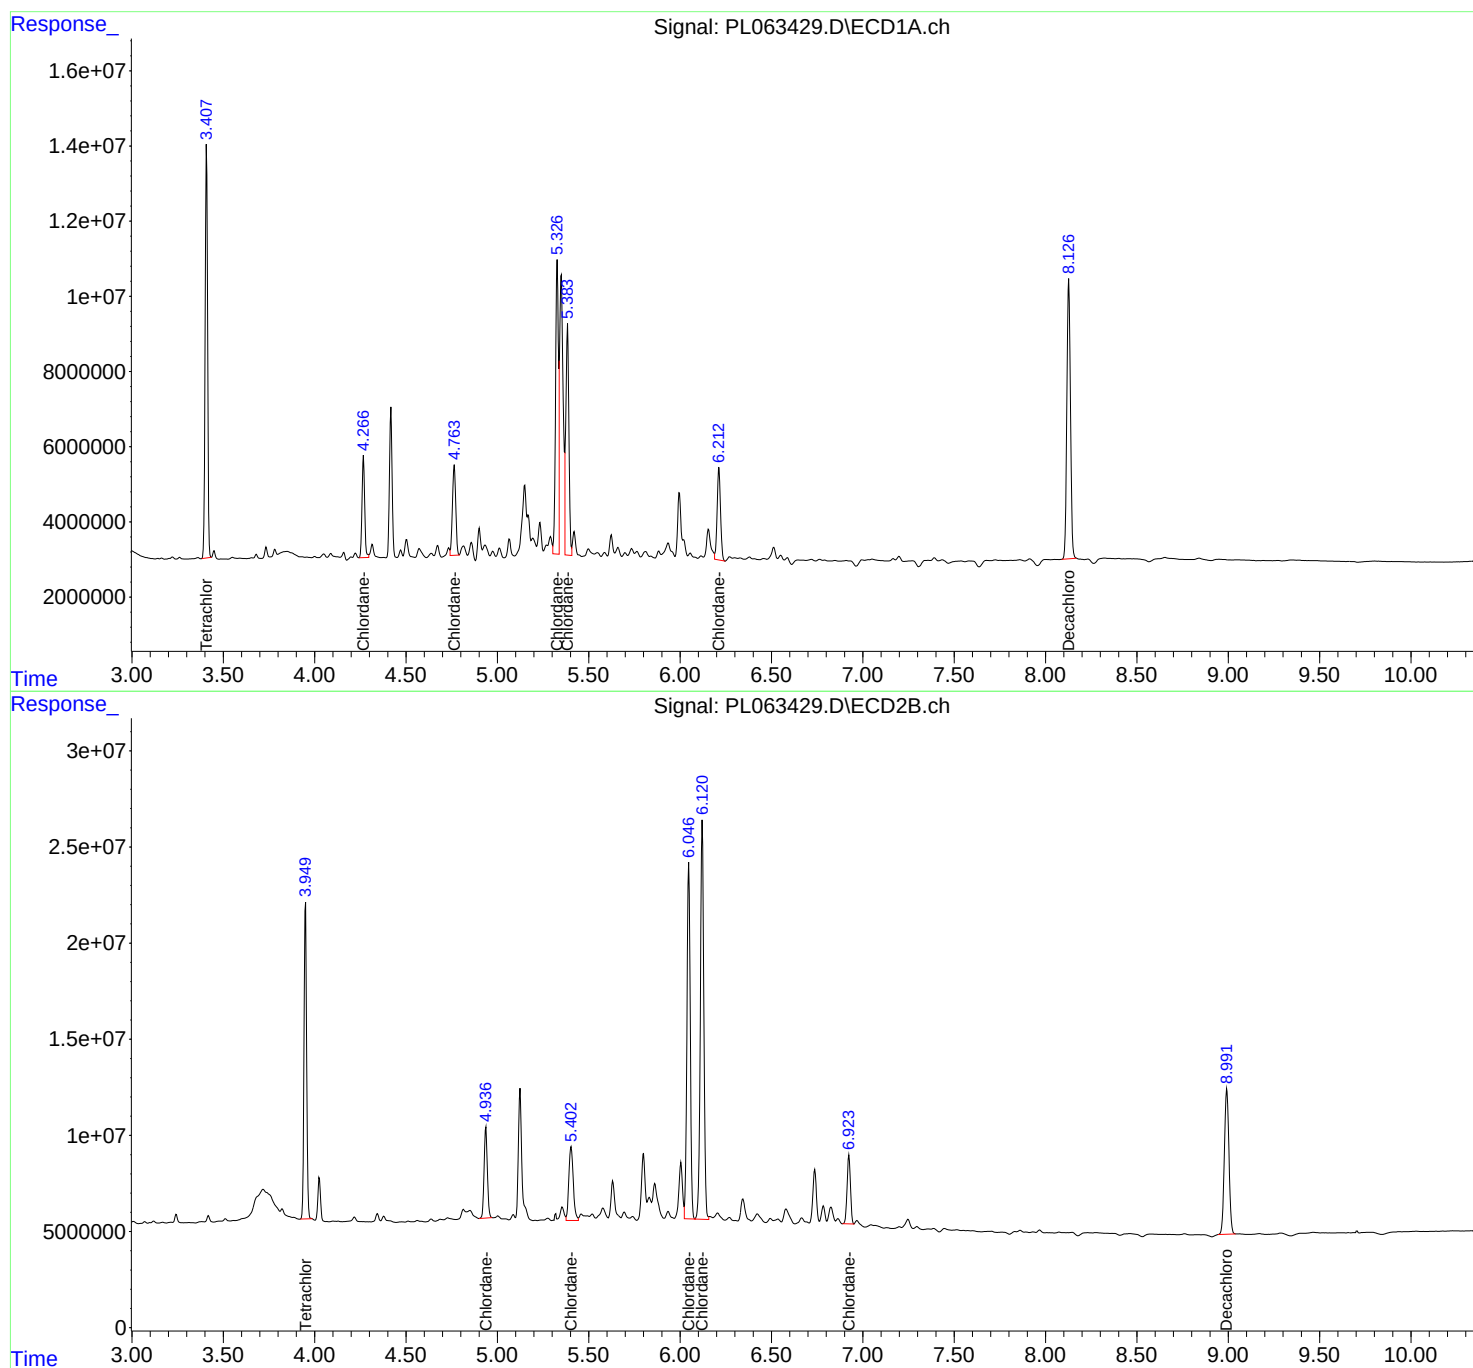


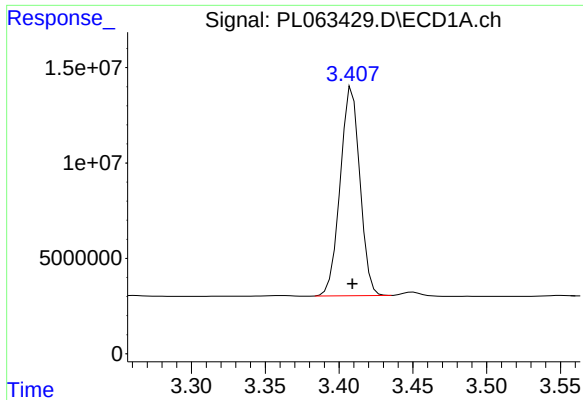

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 101653052
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

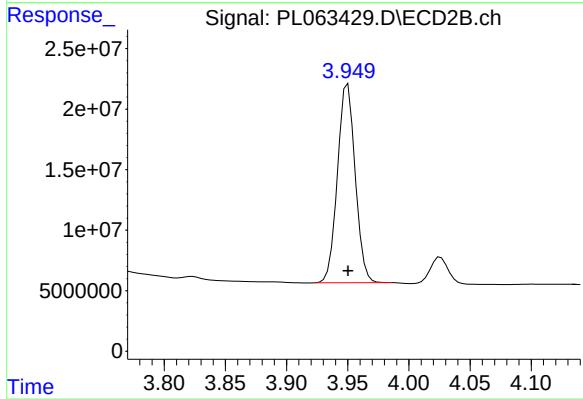


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 165838492
Conc: 50.00 ng/ml

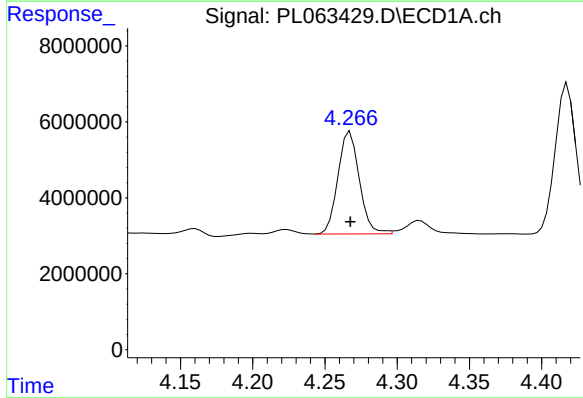


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 27694234
Conc: 500.00 ng/ml

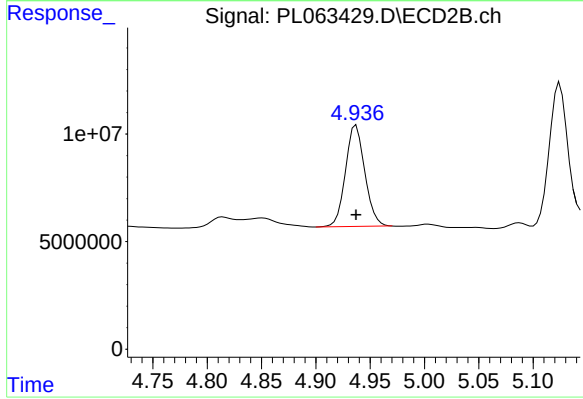

#23 Chlordane-1


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 58386639
Conc: 500.00 ng/ml

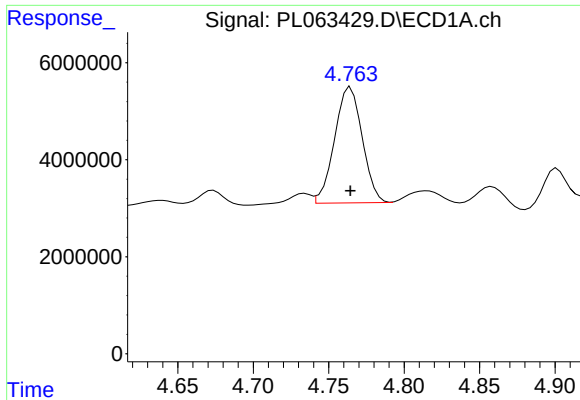

#24 Chlordane-2


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 30448858
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

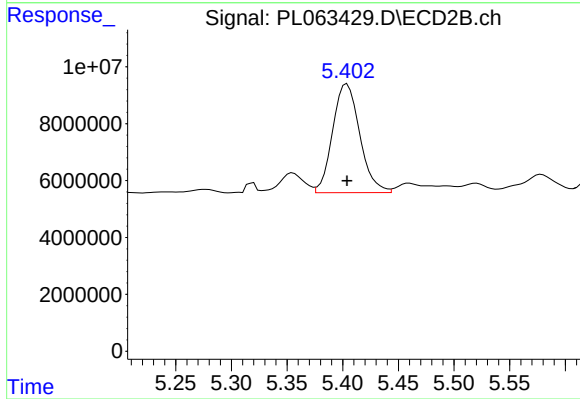


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 65057050
Conc: 500.00 ng/ml

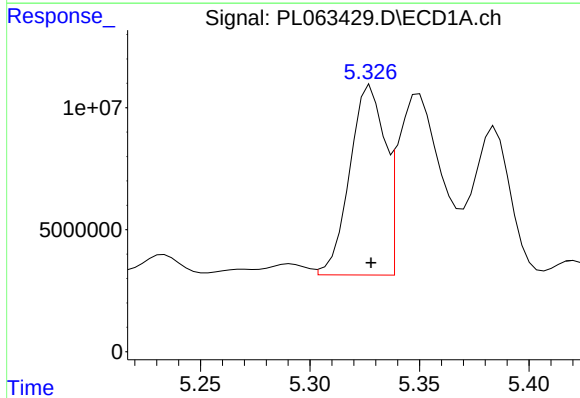


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 85898062
Conc: 500.00 ng/ml

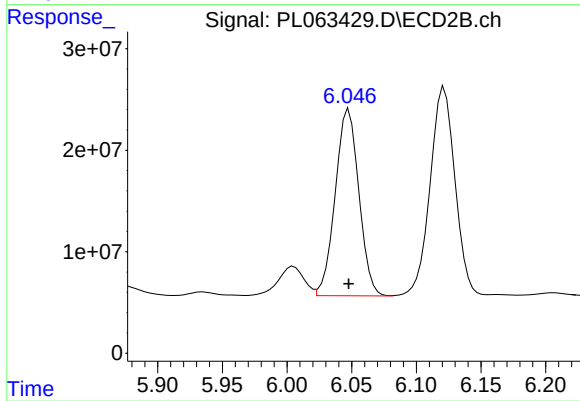

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 233415452
Conc: 500.00 ng/ml

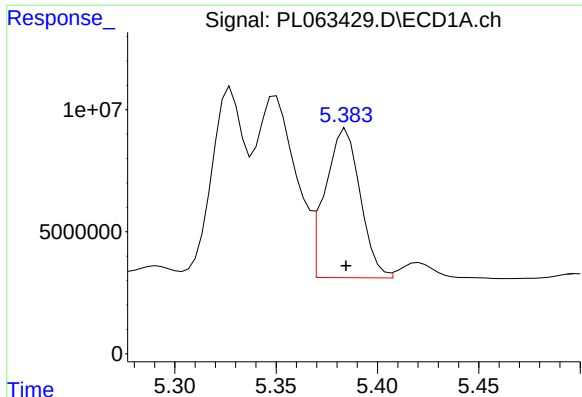

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 73275424
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

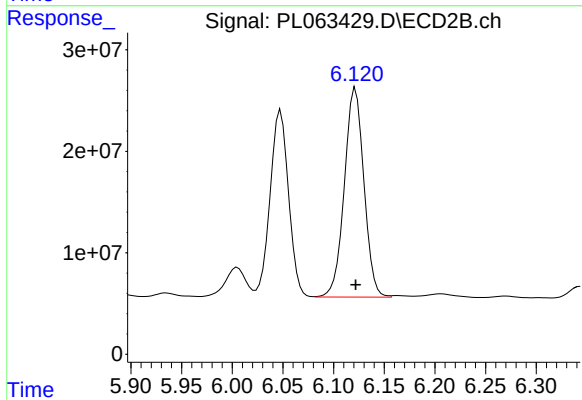


#26 Chlordane-4

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 276330610
Conc: 500.00 ng/ml

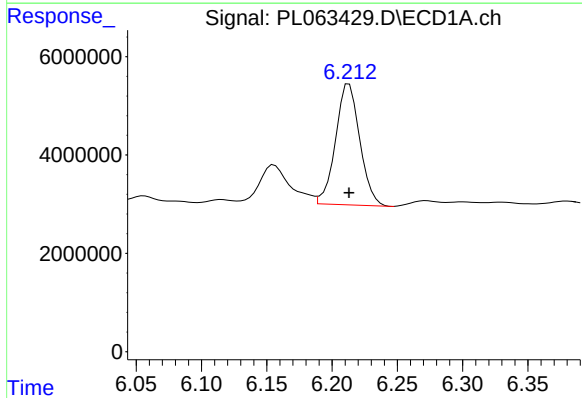


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 31765298
Conc: 500.00 ng/ml

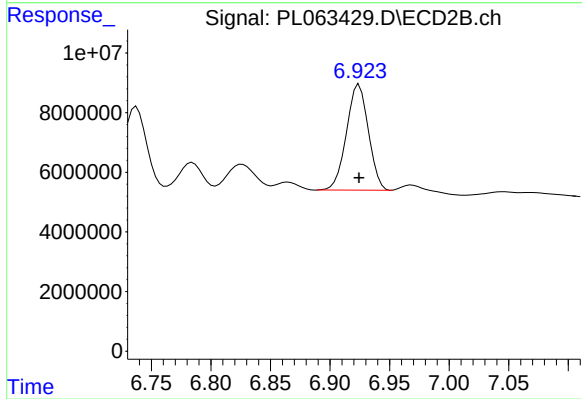

#27 Chlordane-5


R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 45467624
Conc: 500.00 ng/ml

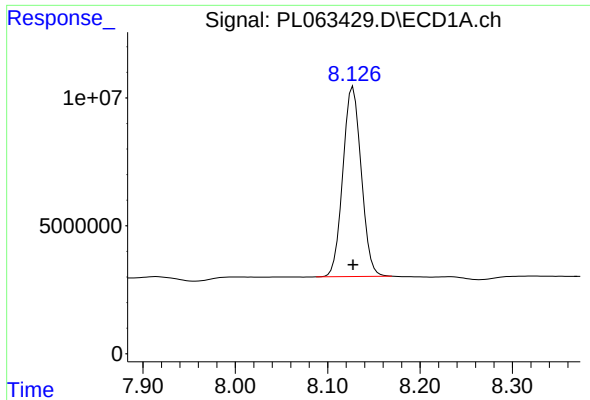

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 102501357
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

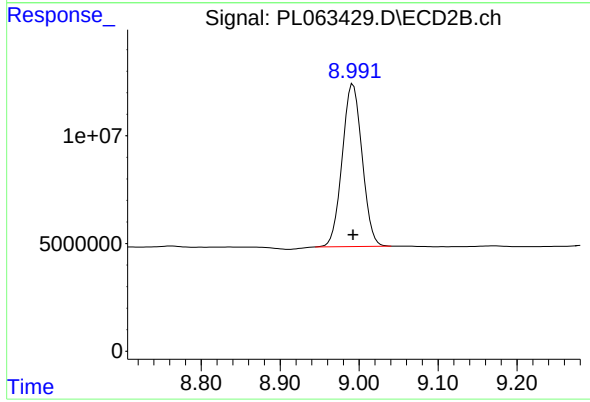

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 132095064
Conc: 50.00 ng/ml