

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 19:48
 Operator : DD\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:55:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 00:54:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.967f	10513490	16649114	5.171	5.020
28)	SA Decachlor...	8.128	9.009f	12335451	14625016	6.017	5.536
Target Compounds							
23)	Chlordane-1	4.268	4.954f	2764435	5131541	49.910	43.944
24)	Chlordane-2	4.764	5.420f	3419060	6534391	56.144	50.220
25)	Chlordane-3	5.327	6.065f	8738965	23681215	50.868	50.728
26)	Chlordane-4	5.384	6.139f	7356239	28741392	50.196	52.005
27)	Chlordane-5	6.214	6.941f	3166237	4956779	49.838	54.509


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 19:48
Operator : DD\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:55:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 00:54:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

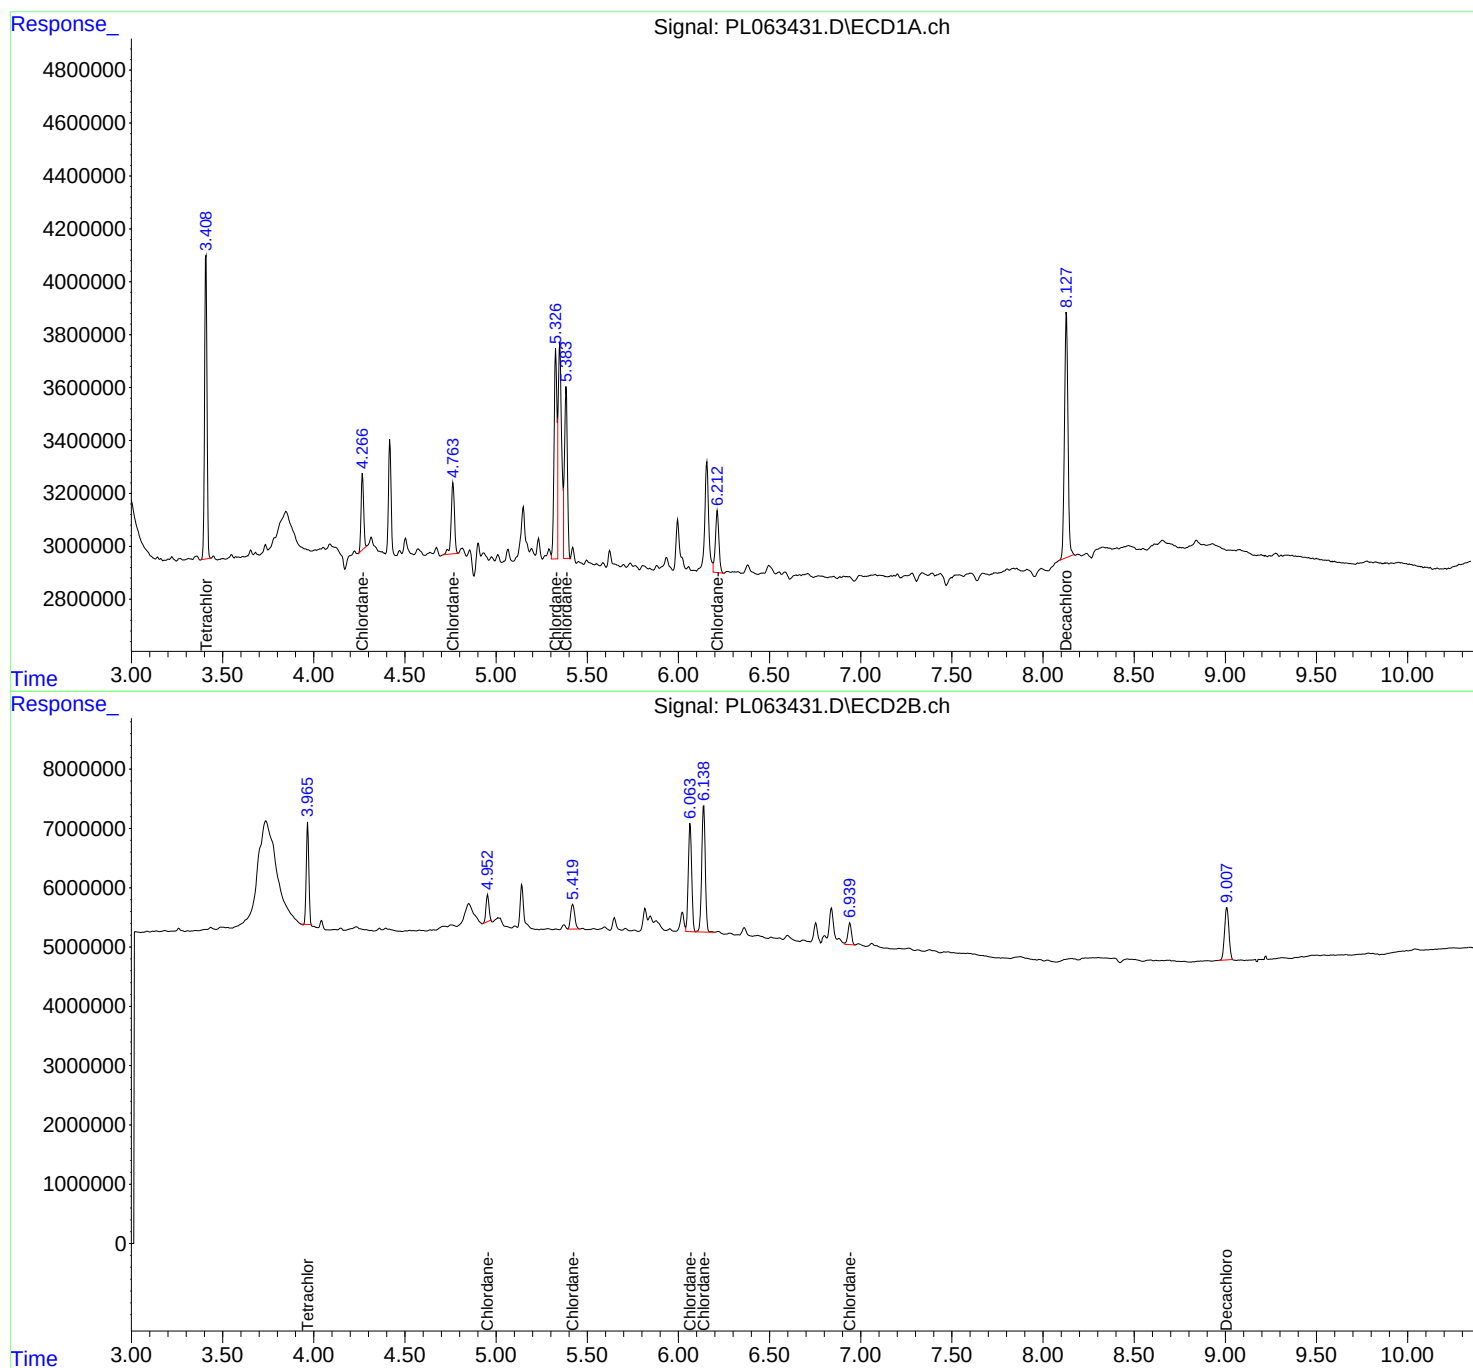


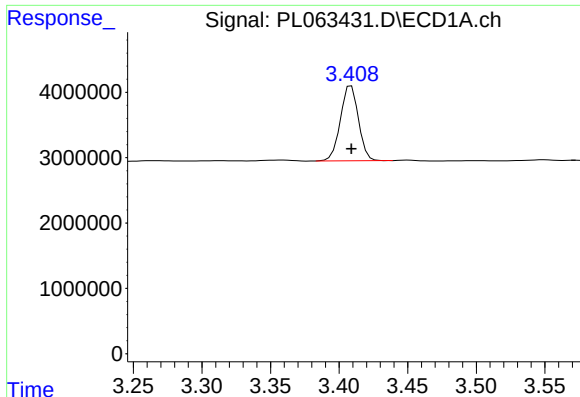

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 10513490
Conc: 5.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

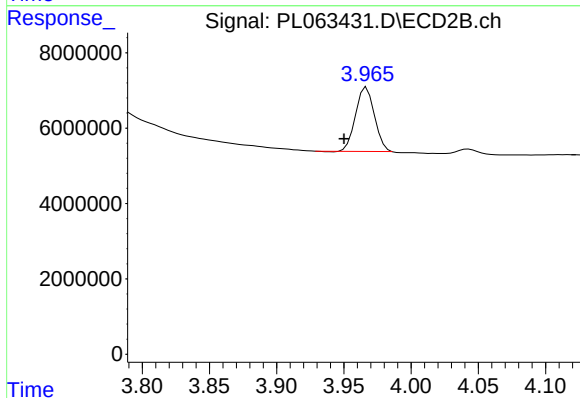


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.017 min
Response: 16649114
Conc: 5.02 ng/ml

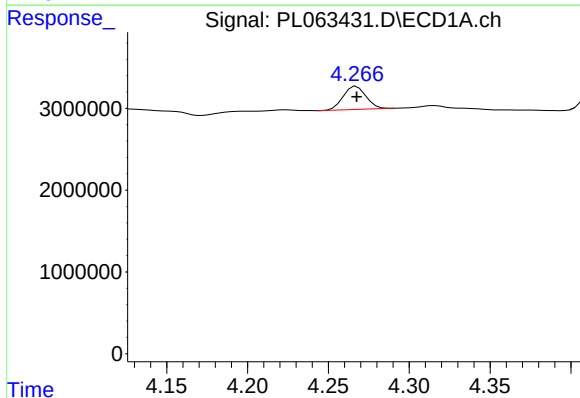


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 2764435
Conc: 49.91 ng/ml

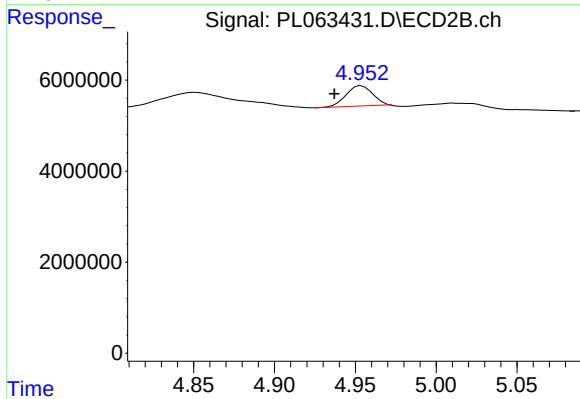

#23 Chlordane-1


R.T.: 4.954 min
Delta R.T.: 0.017 min
Response: 5131541
Conc: 43.94 ng/ml

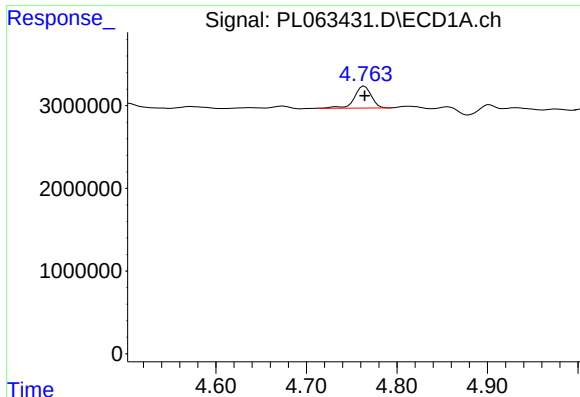

#24 Chlordane-2


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 3419060
Conc: 56.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

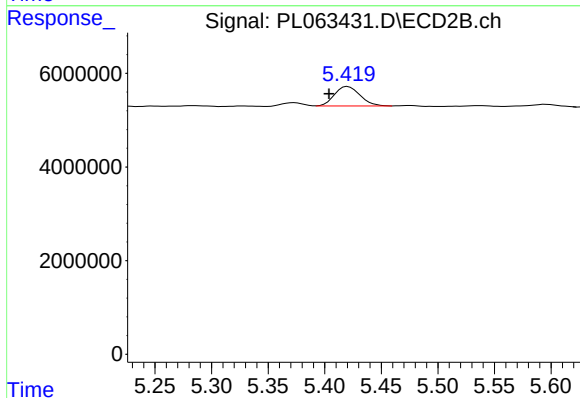


#24 Chlordane-2

R.T.: 5.420 min
Delta R.T.: 0.017 min
Response: 6534391
Conc: 50.22 ng/ml

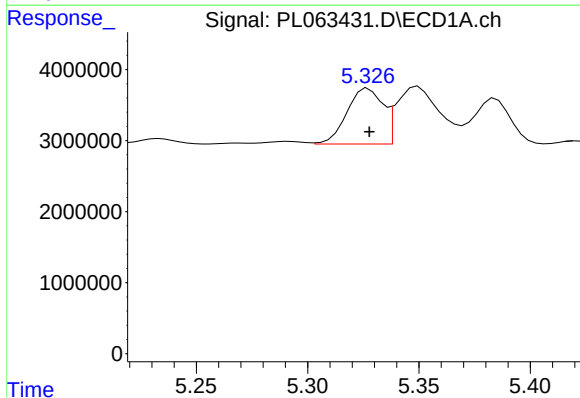


#25 Chlordane-3

R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 8738965
Conc: 50.87 ng/ml

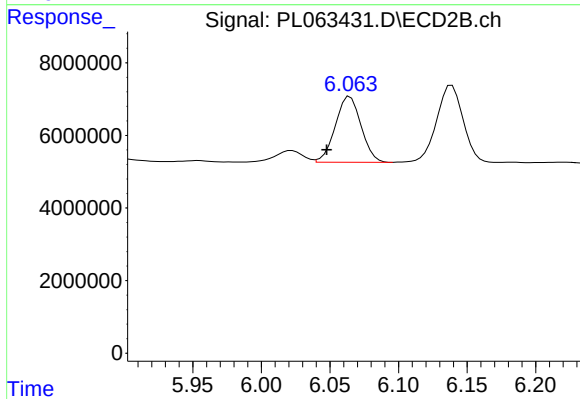

#25 Chlordane-3


R.T.: 6.065 min
Delta R.T.: 0.017 min
Response: 23681215
Conc: 50.73 ng/ml

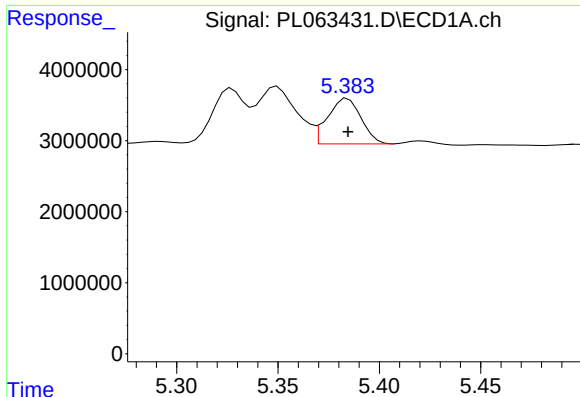

#26 Chlordane-4


R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 7356239
Conc: 50.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

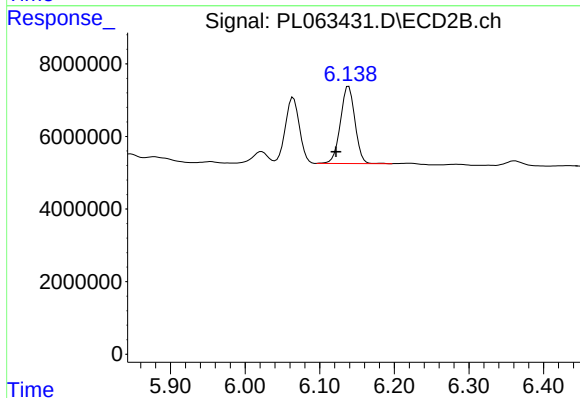


#26 Chlordane-4

R.T.: 6.139 min
Delta R.T.: 0.017 min
Response: 28741392
Conc: 52.01 ng/ml

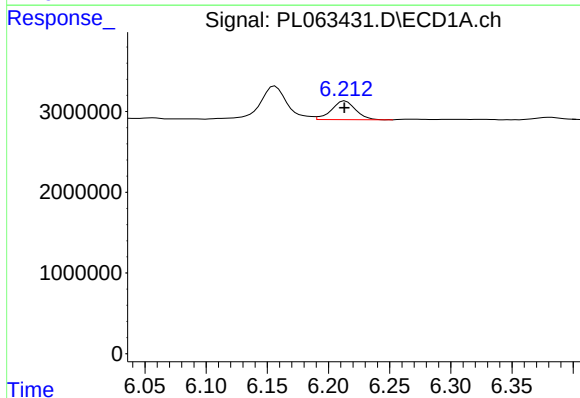


#27 Chlordane-5

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 3166237
Conc: 49.84 ng/ml

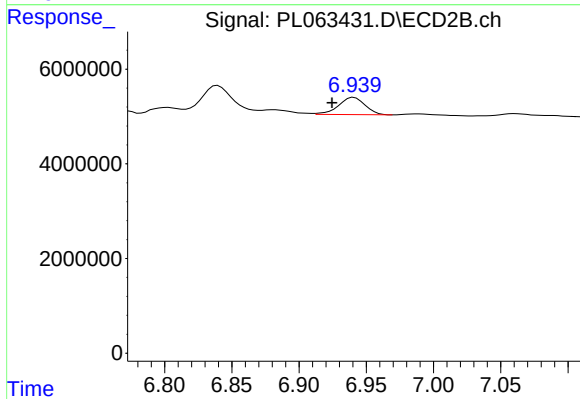

#27 Chlordane-5


R.T.: 6.941 min
Delta R.T.: 0.016 min
Response: 4956779
Conc: 54.51 ng/ml

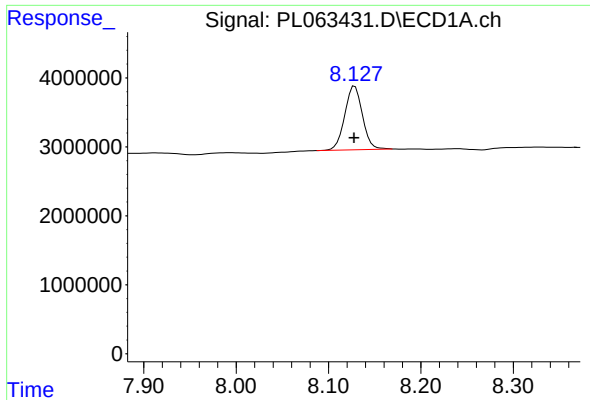

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 12335451
Conc: 6.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

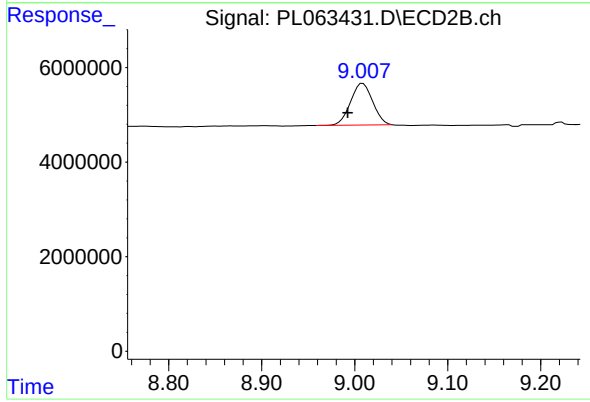

#28 Decachlorobiphenyl

R.T.: 9.009 min
Delta R.T.: 0.016 min
Response: 14625016
Conc: 5.54 ng/ml