

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 17:26
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 14:15:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 10:28:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	32536492	55888045	19.120	17.832
28)	SA Decachlor...	8.128	8.993	38173651	48177752	18.955	19.131
Target Compounds							
9)	A Endosulfan I	5.437	6.169	16427346	34309713	9.412	10.280
10)	B gamma-Chl...	5.327	6.048	15621332	27070291	8.398	7.627
12)	B 4,4'-DDE	5.550	6.279	28886082	52651191	17.007	15.033
13)	MA Dieldrin	5.678	6.426	31123791	59563518	17.096	17.338
19)	B Endosulfa...	6.585	7.201	30370855	47228716	17.710	16.978
20)	A Methoxychlor	6.845	7.528	81209788	134.8E6	91.265	96.619
21)	B Endrin ke...	7.070	7.670	61998159	49798259	31.049	17.073 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 17:26
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 14:15:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 10:28:14 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

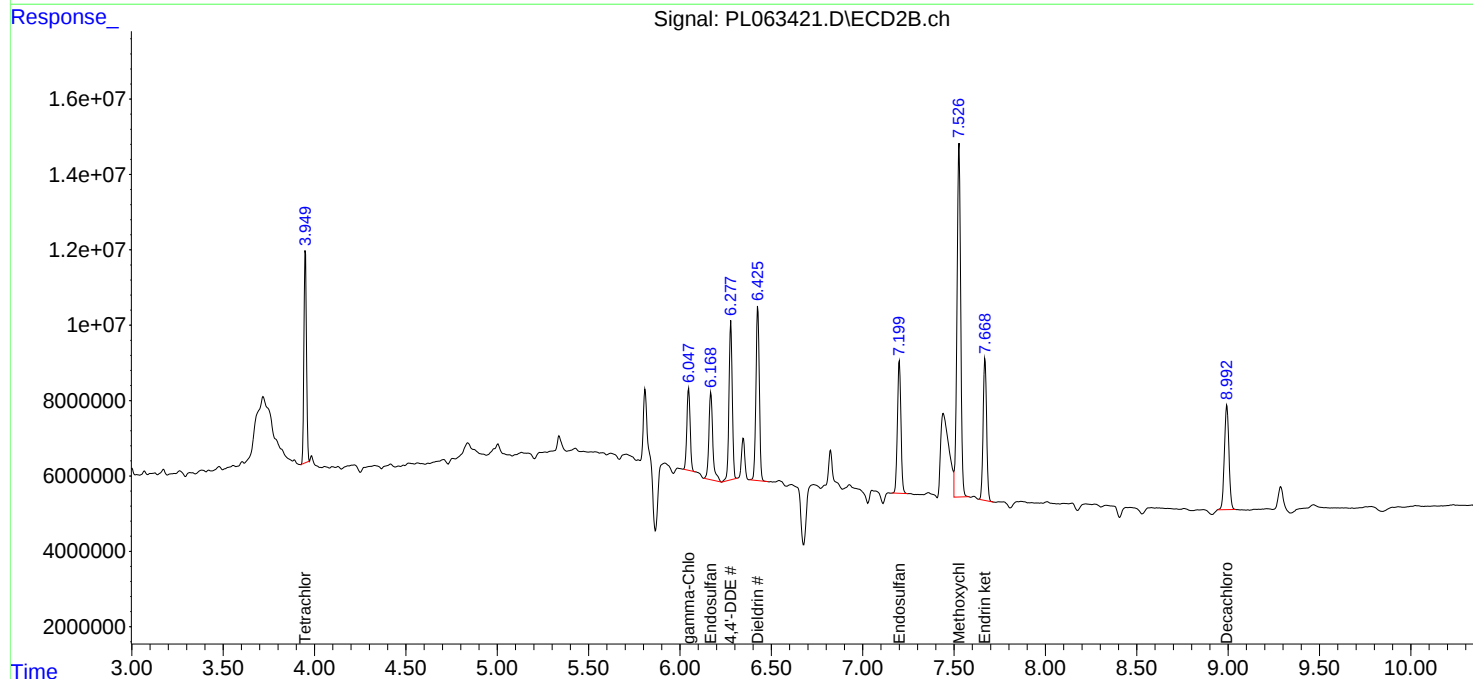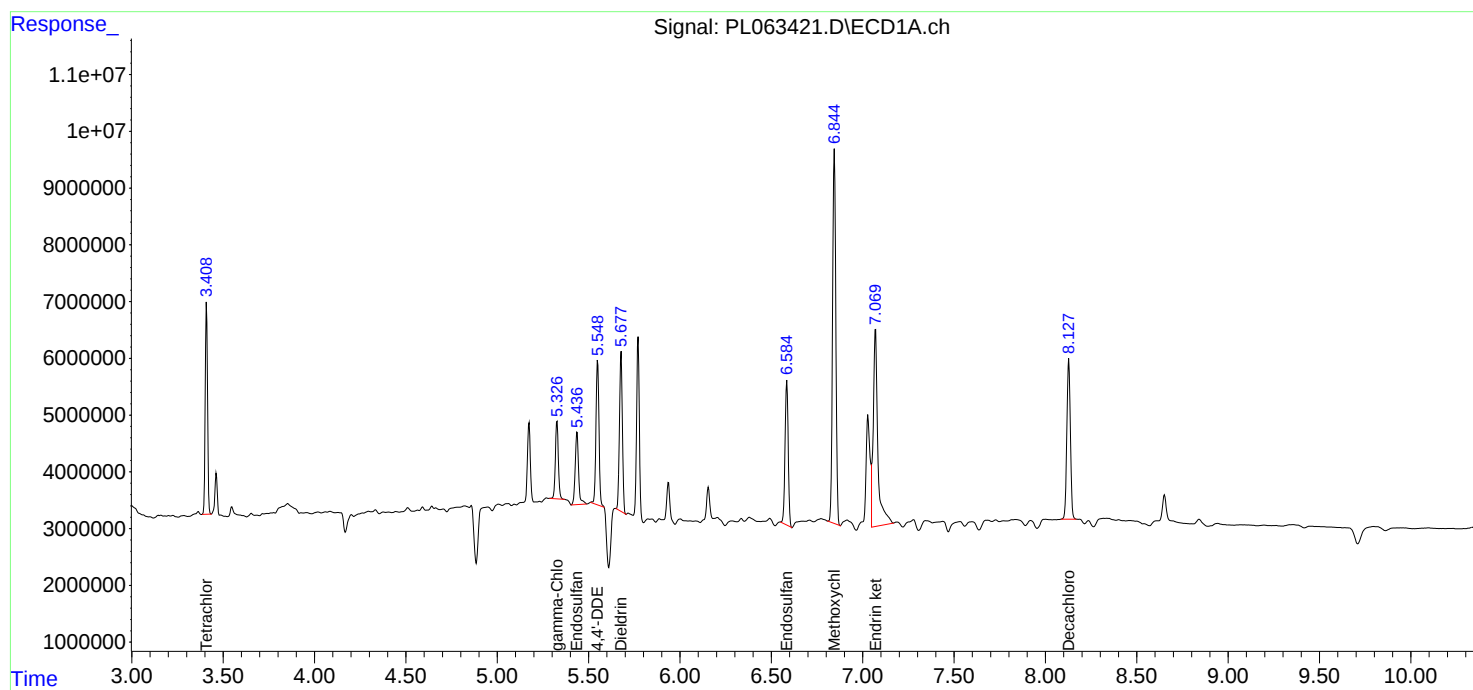


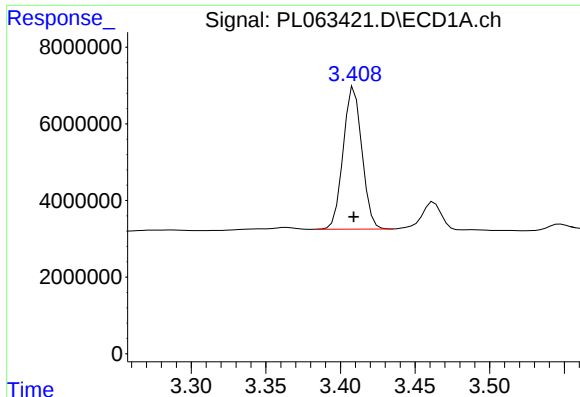

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 32536492
Conc: 19.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

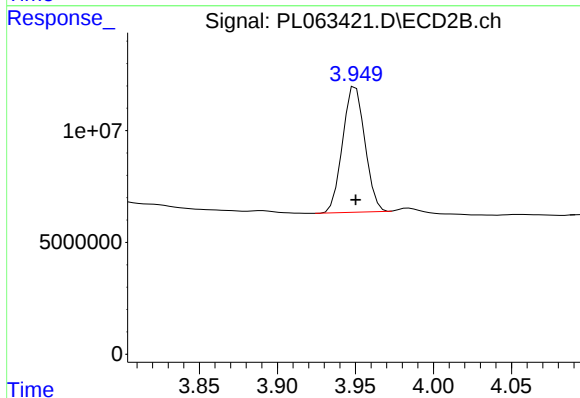


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 55888045
Conc: 17.83 ng/ml

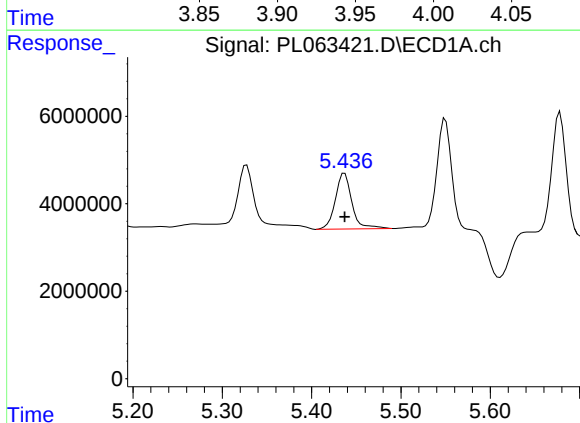


#9 Endosulfan I

R.T.: 5.437 min
Delta R.T.: 0.000 min
Response: 16427346
Conc: 9.41 ng/ml

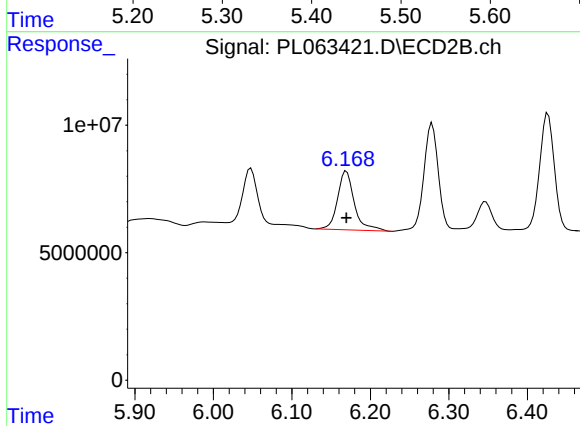

#9 Endosulfan I


R.T.: 6.169 min
Delta R.T.: 0.000 min
Response: 34309713
Conc: 10.28 ng/ml

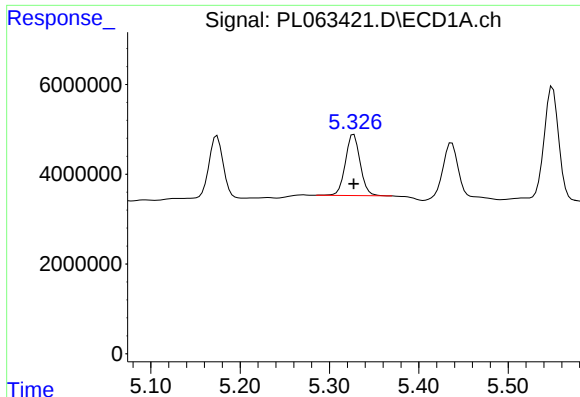

#10 gamma-Chlordane


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 15621332
Conc: 8.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

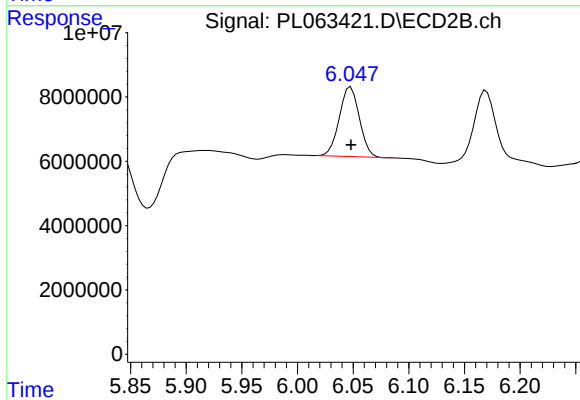


#10 gamma-Chlordane

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 27070291
Conc: 7.63 ng/ml

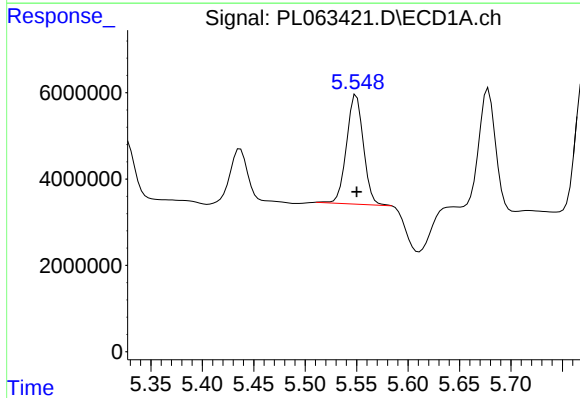


#12 4,4'-DDE

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 28886082
Conc: 17.01 ng/ml

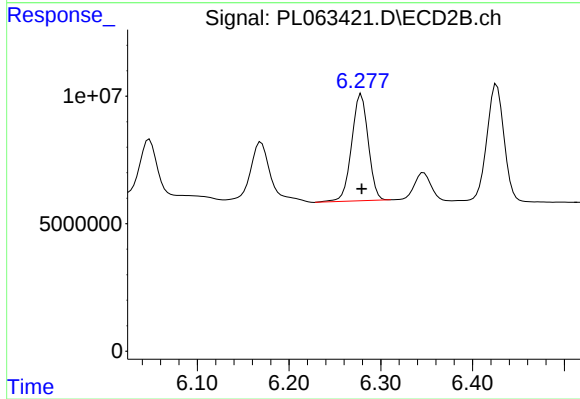

#12 4,4'-DDE


R.T.: 6.279 min
Delta R.T.: 0.000 min
Response: 52651191
Conc: 15.03 ng/ml

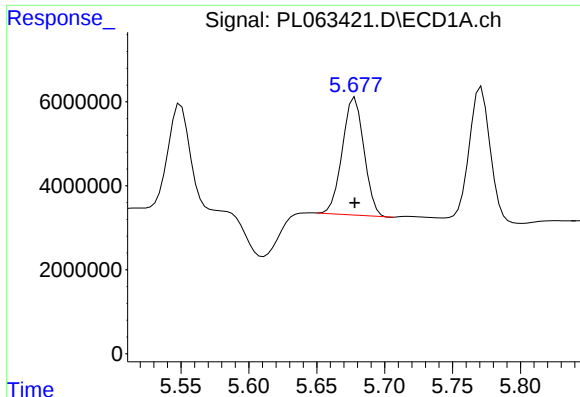

#13 Dieldrin


R.T.: 5.678 min
Delta R.T.: 0.000 min
Response: 31123791
Conc: 17.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

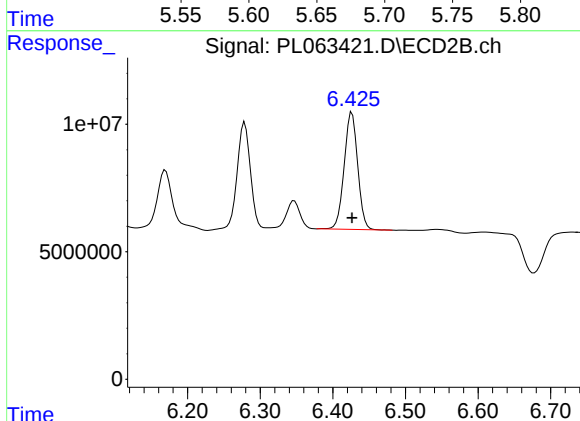


#13 Dieldrin

R.T.: 6.426 min
Delta R.T.: 0.000 min
Response: 59563518
Conc: 17.34 ng/ml

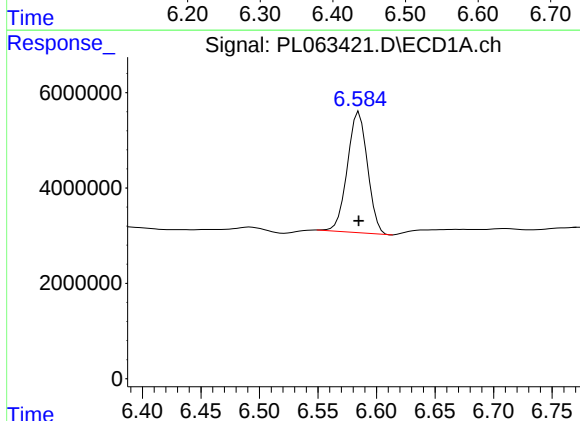


#19 Endosulfan Sulfate

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 30370855
Conc: 17.71 ng/ml

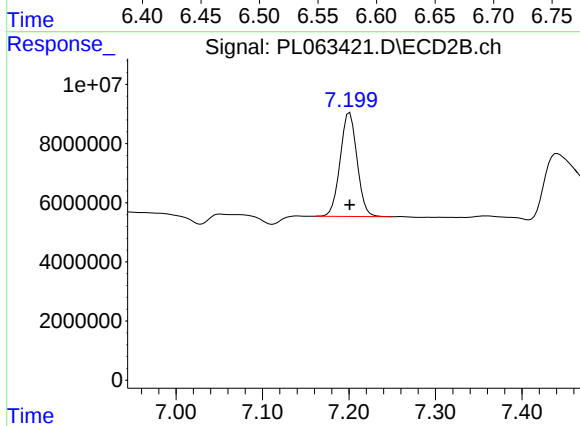

#19 Endosulfan Sulfate


R.T.: 7.201 min
Delta R.T.: 0.000 min
Response: 47228716
Conc: 16.98 ng/ml

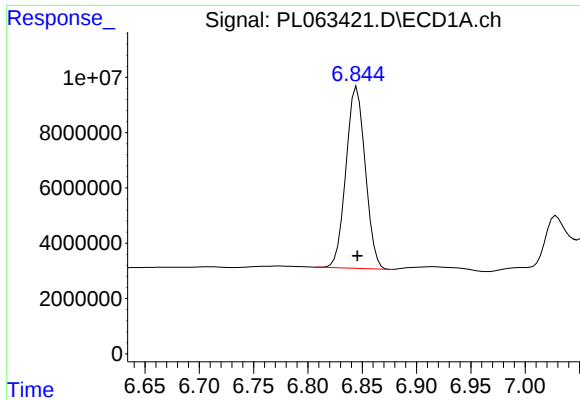

#20 Methoxychlor


R.T.: 6.845 min
Delta R.T.: 0.000 min
Response: 81209788
Conc: 91.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

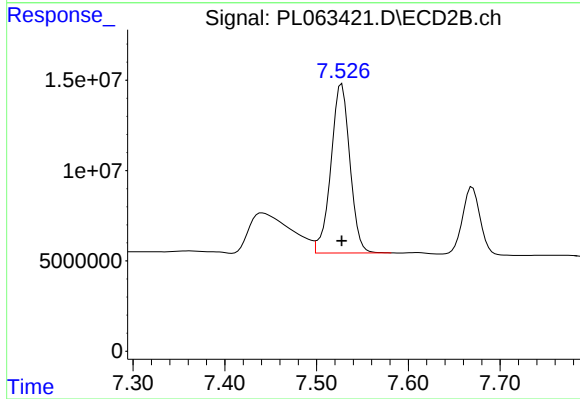


#20 Methoxychlor

R.T.: 7.528 min
Delta R.T.: 0.000 min
Response: 134750813
Conc: 96.62 ng/ml

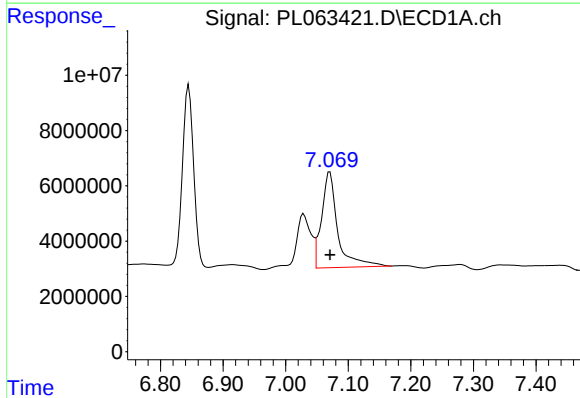


#21 Endrin ketone

R.T.: 7.070 min
Delta R.T.: 0.000 min
Response: 61998159
Conc: 31.05 ng/ml

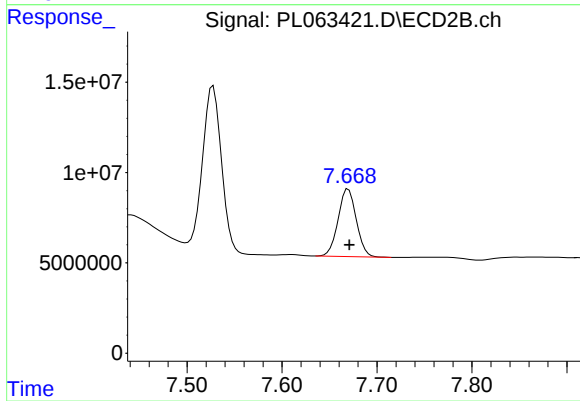

#21 Endrin ketone


R.T.: 7.670 min
Delta R.T.: 0.000 min
Response: 49798259
Conc: 17.07 ng/ml

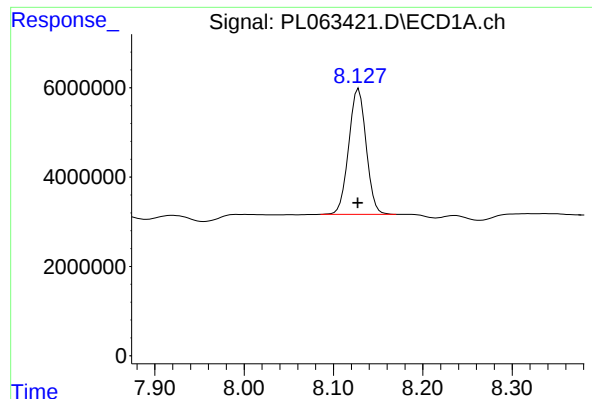

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 38173651
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

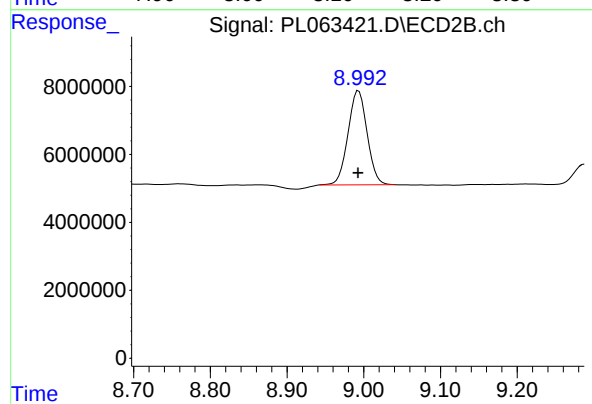

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 48177752
Conc: 19.13 ng/ml