

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 18:51
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:54:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 00:54:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.950	204.6E6	333.7E6	100.660	100.606
28)	SA Decachlor...	8.128	8.992	191.2E6	246.4E6	93.286	93.274
Target Compounds							
23)	Chlordane-1	4.268	4.938	53581483	118.0E6	967.376	1010.285
24)	Chlordane-2	4.763	5.404	57845640	126.9E6	949.882m	975.381
25)	Chlordane-3	5.328	6.048	172.3E6	473.4E6	1003.207	1014.072
26)	Chlordane-4	5.385	6.123	144.2E6	557.5E6	983.678	1008.693
27)	Chlordane-5	6.214	6.925	60355354	93343041	950.020	1026.478



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 18:51
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:54:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 00:54:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

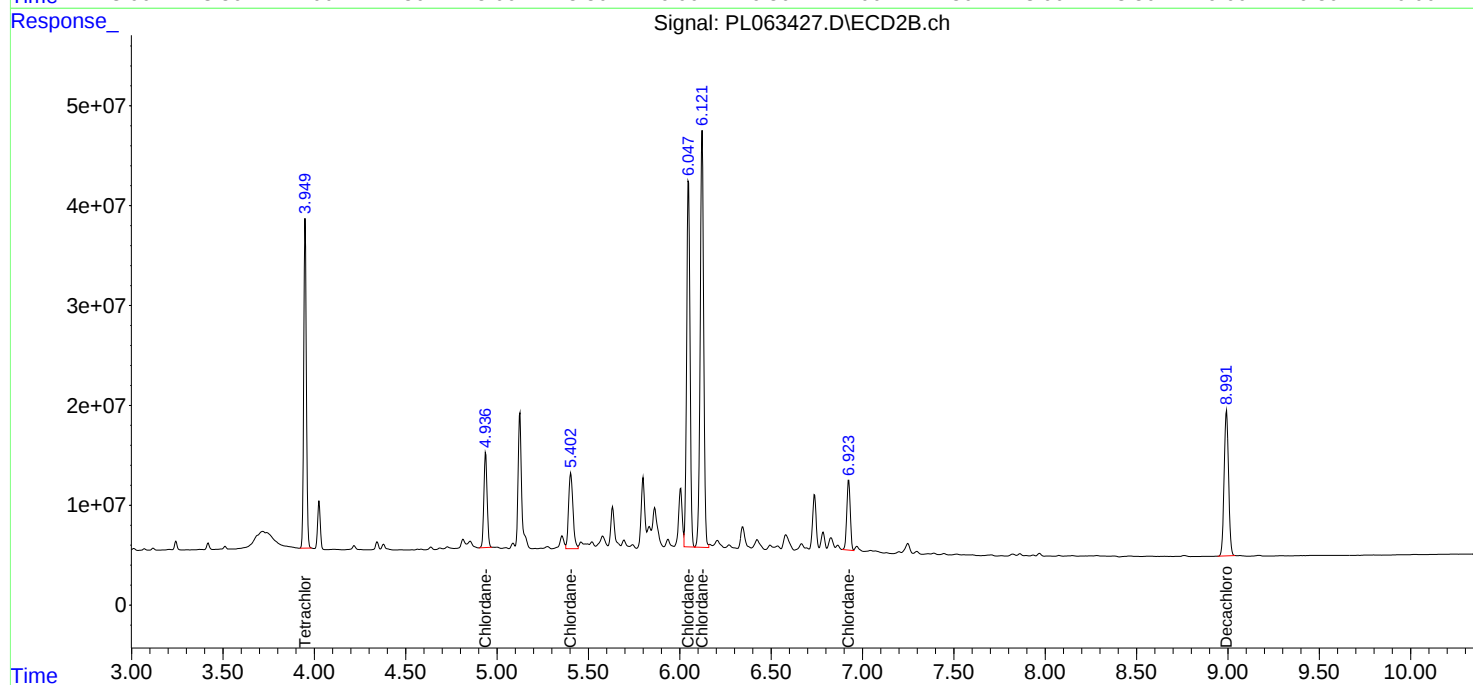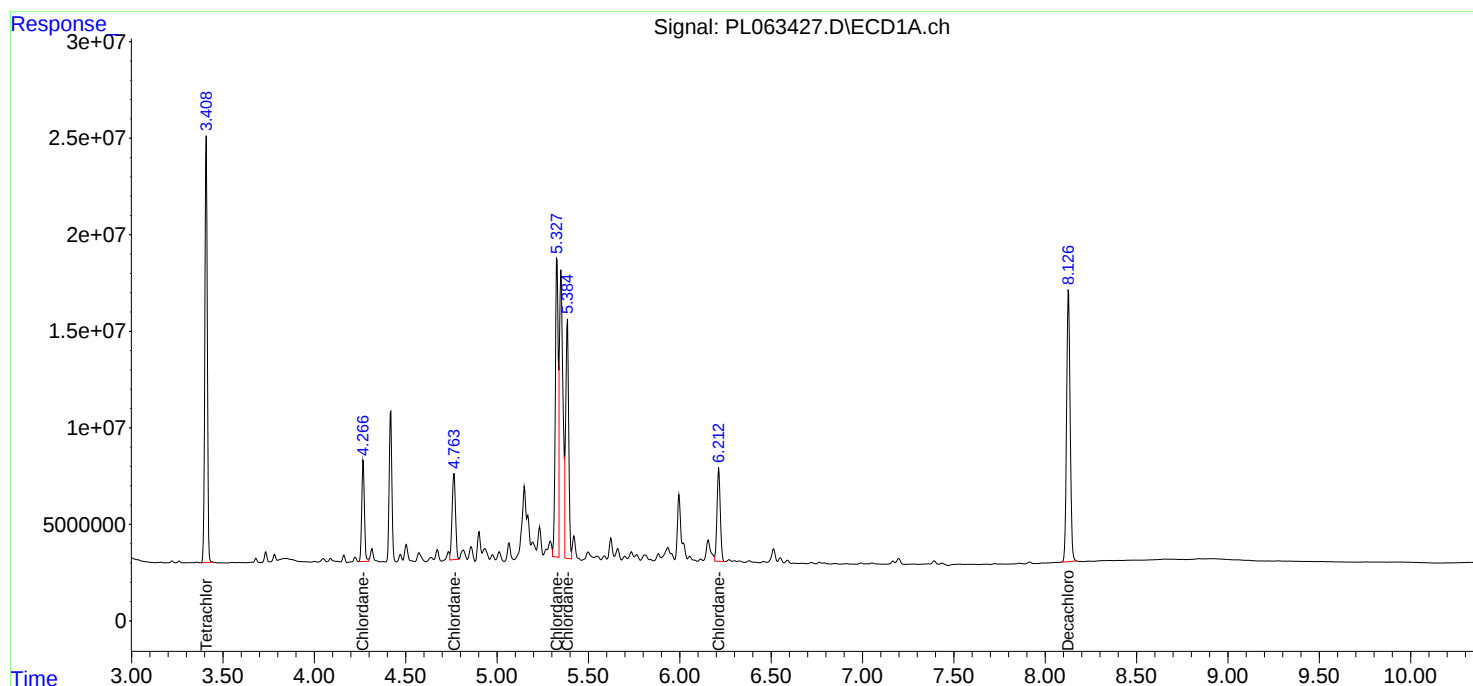


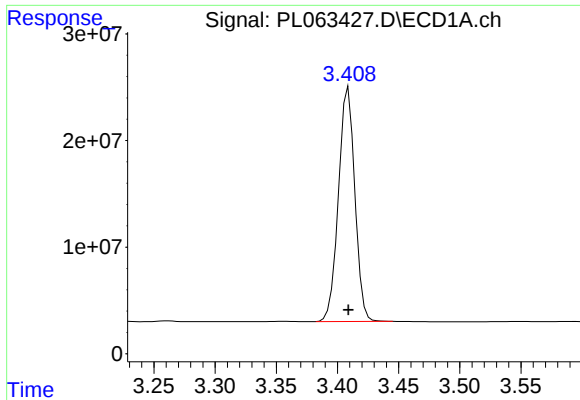

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 204648589
Conc: 100.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

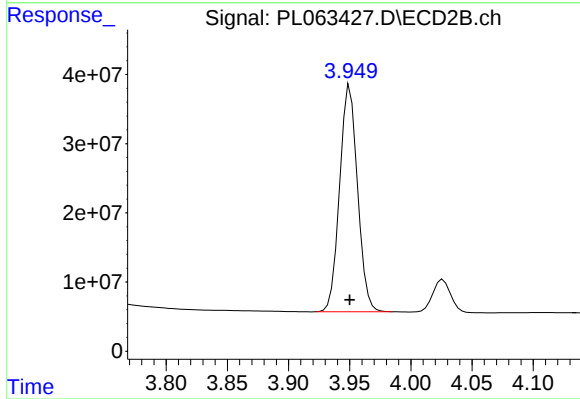


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 333686437
Conc: 100.61 ng/ml

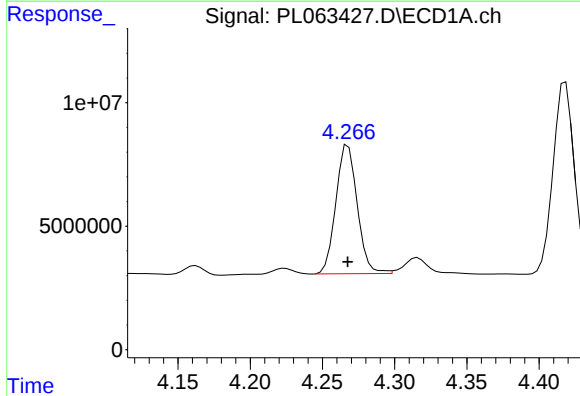


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 53581483
Conc: 967.38 ng/ml

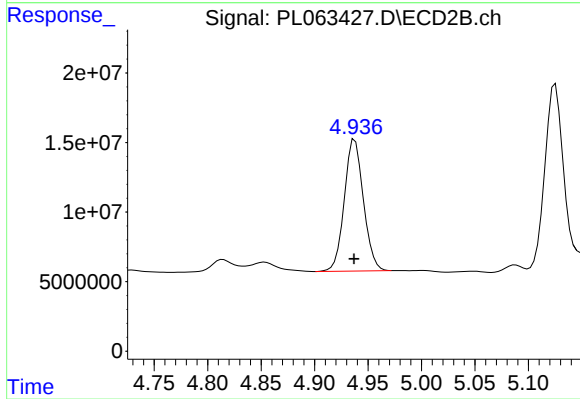

#23 Chlordane-1


R.T.: 4.938 min
Delta R.T.: 0.000 min
Response: 117974282
Conc: 1010.28 ng/ml

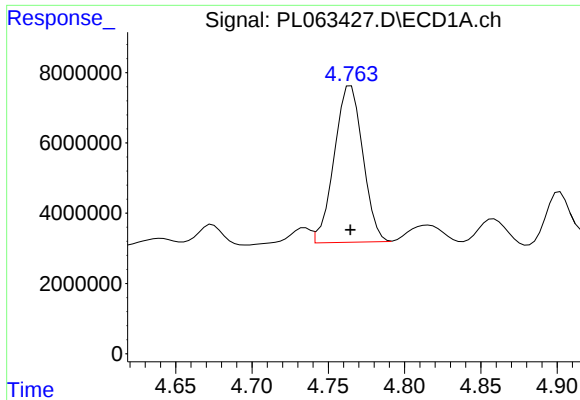

#24 Chlordane-2


R.T.: 4.763 min
Delta R.T.: -0.001 min
Response: 57845640
Conc: 949.88 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

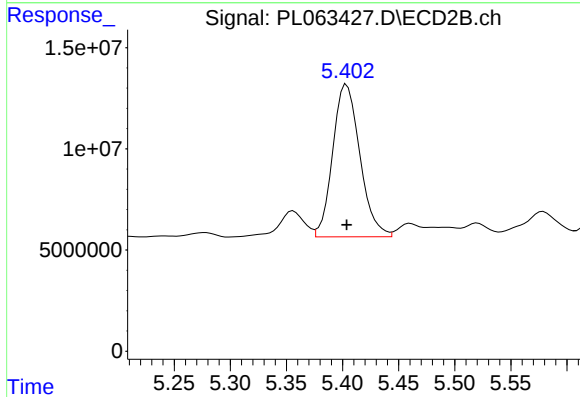


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 126910792
Conc: 975.38 ng/ml

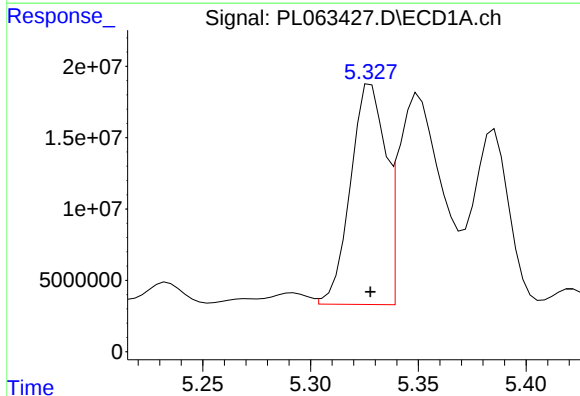


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 172346994
Conc: 1003.21 ng/ml

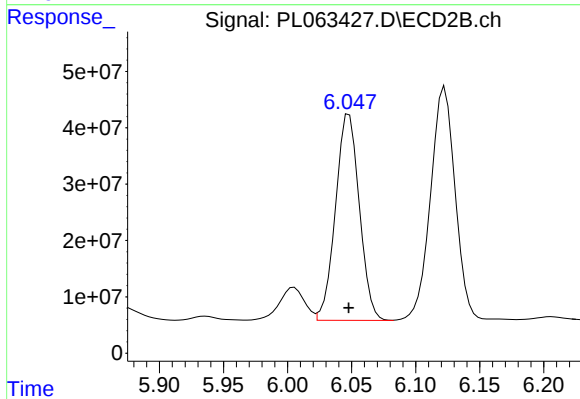

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 473400183
Conc: 1014.07 ng/ml

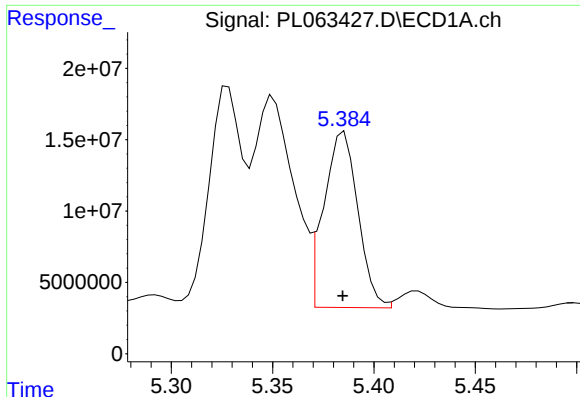

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 144158818
Conc: 983.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

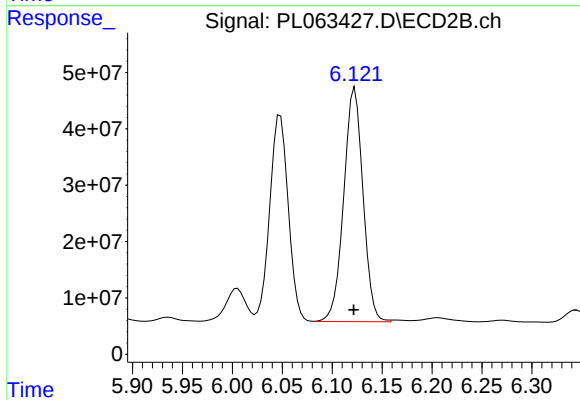


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: 0.001 min
Response: 557465534
Conc: 1008.69 ng/ml

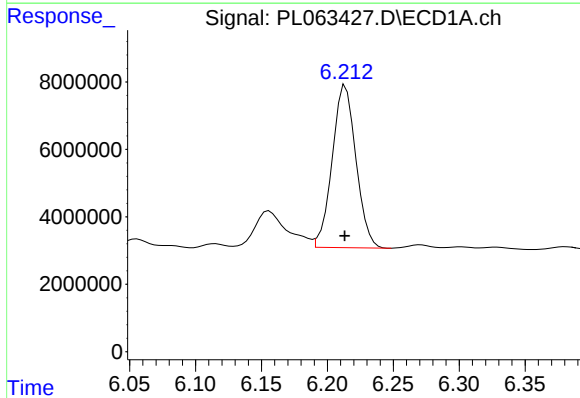


#27 Chlordane-5

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 60355354
Conc: 950.02 ng/ml

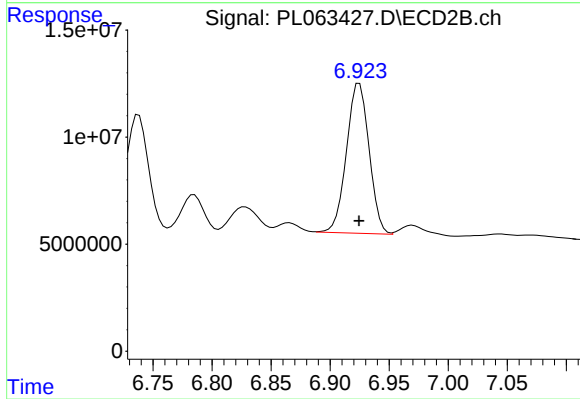

#27 Chlordane-5


R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 93343041
Conc: 1026.48 ng/ml

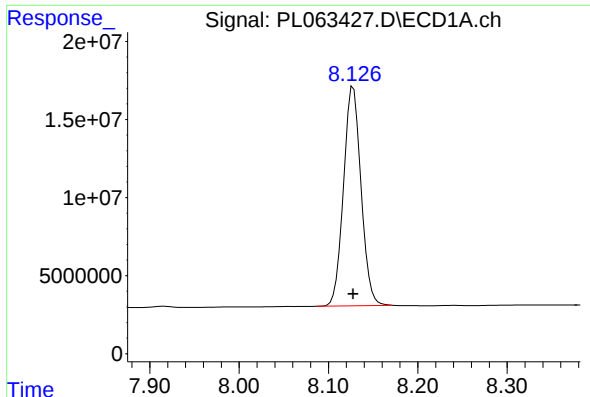

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.000 min
Response: 191239277
Conc: 93.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

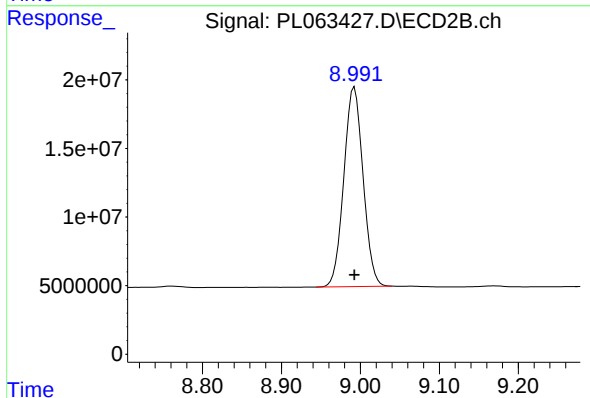

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 246421274
Conc: 93.27 ng/ml