

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 19:06
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:54:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 00:54:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.951	155.2E6	253.6E6	76.359	76.450
28)	SA Decachlor...	8.127	8.992	149.7E6	193.0E6	73.037	73.067
Target Compounds							
23)	Chlordane-1	4.268	4.938	41376908	89172590	747.031	763.639
24)	Chlordane-2	4.765	5.404	44991247	97642982	738.800	750.441
25)	Chlordane-3	5.328	6.049	130.8E6	358.9E6	761.327	768.728
26)	Chlordane-4	5.385	6.123	109.5E6	424.6E6	747.034	768.193
27)	Chlordane-5	6.214	6.925	46351506	71207773	729.593	783.060



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 19:06
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:54:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 00:54:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

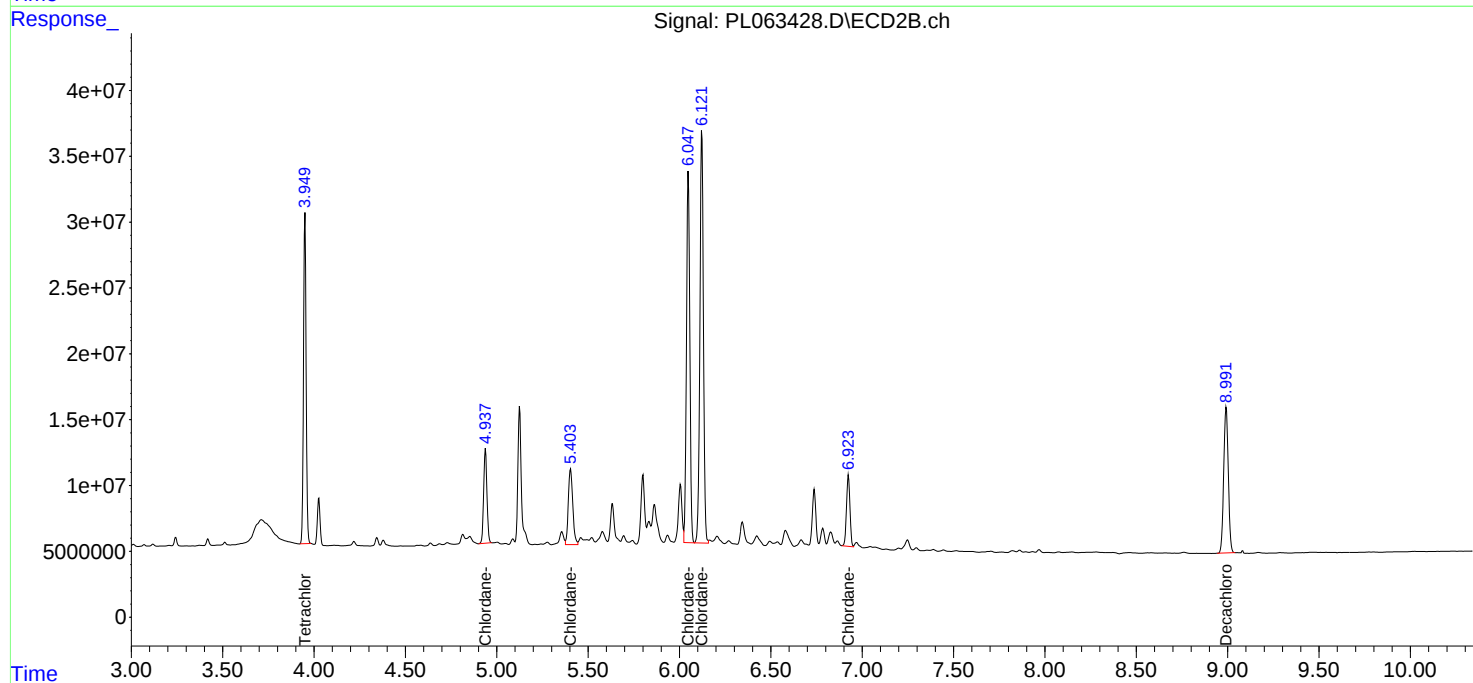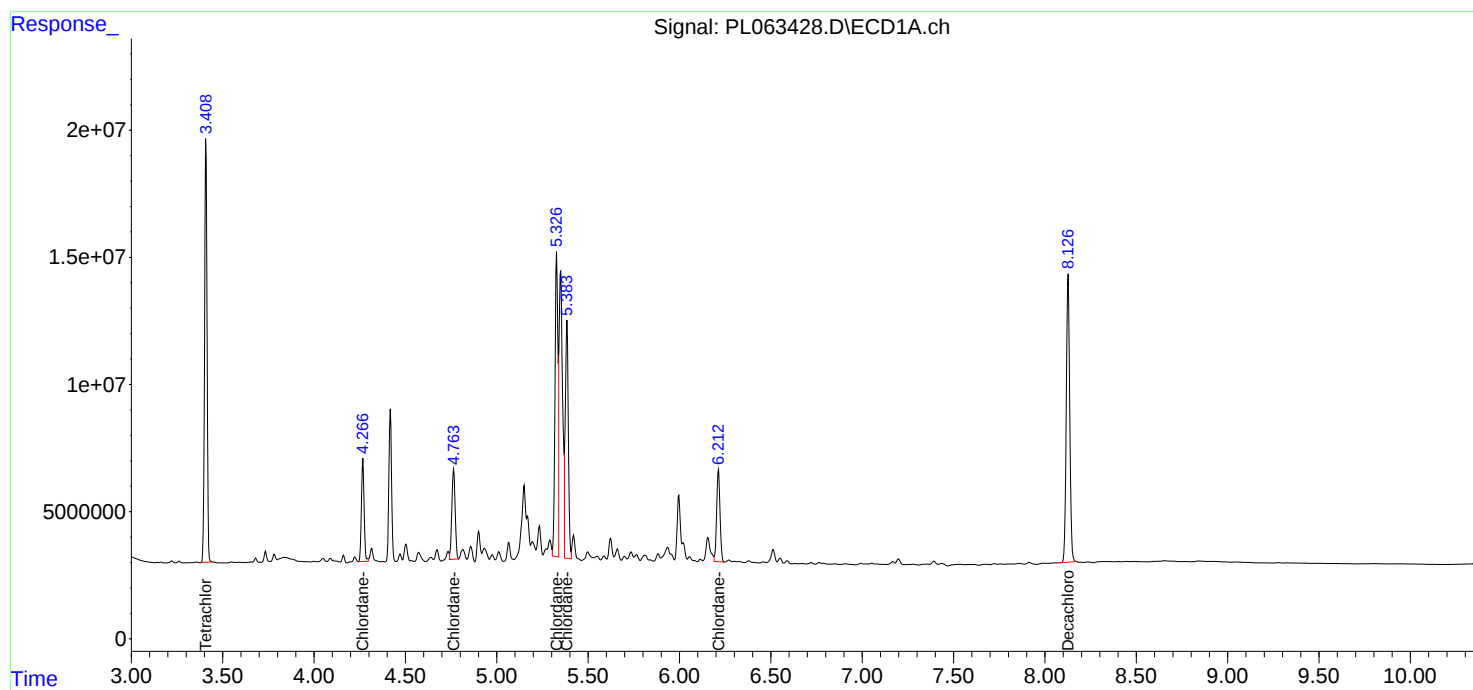


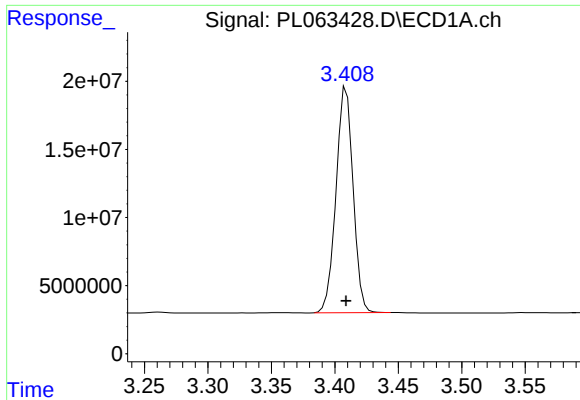

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 155242676
Conc: 76.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

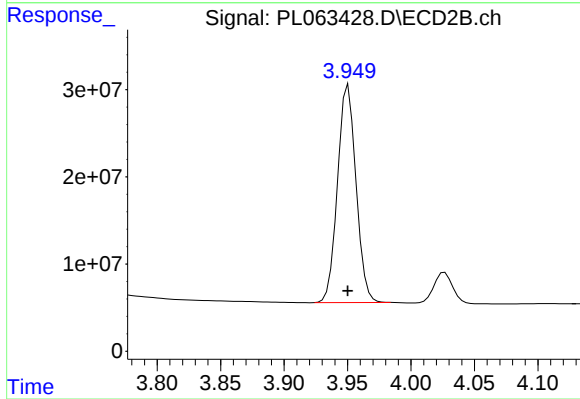


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 253568108
Conc: 76.45 ng/ml

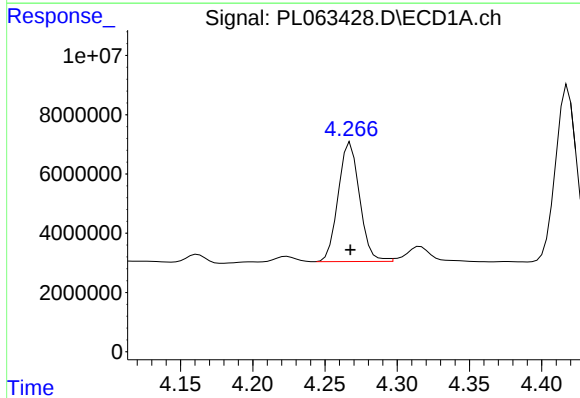


#23 Chlordane-1

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 41376908
Conc: 747.03 ng/ml

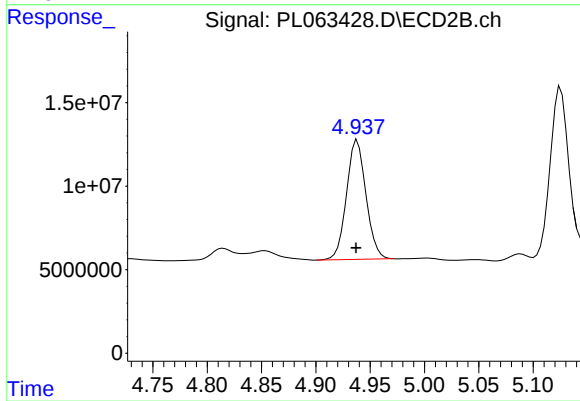

#23 Chlordane-1


R.T.: 4.938 min
Delta R.T.: 0.001 min
Response: 89172590
Conc: 763.64 ng/ml

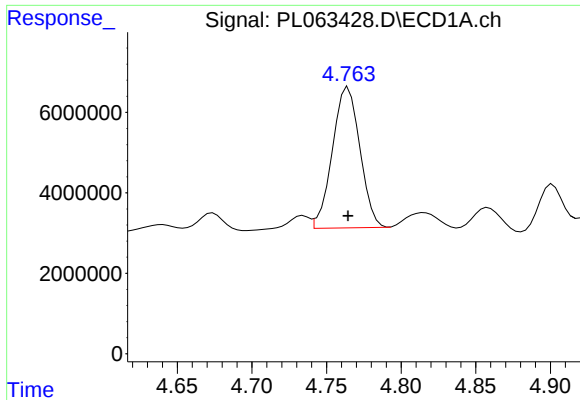

#24 Chlordane-2


R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 44991247
Conc: 738.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

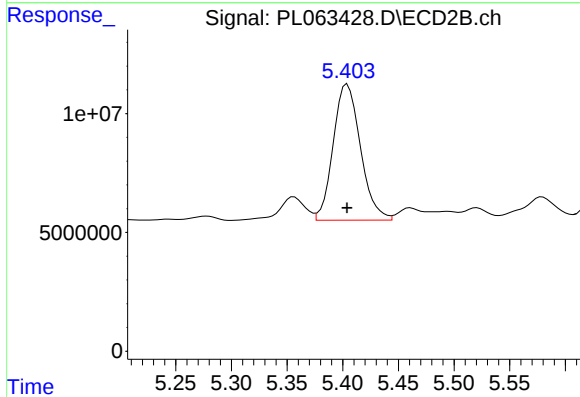


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 97642982
Conc: 750.44 ng/ml

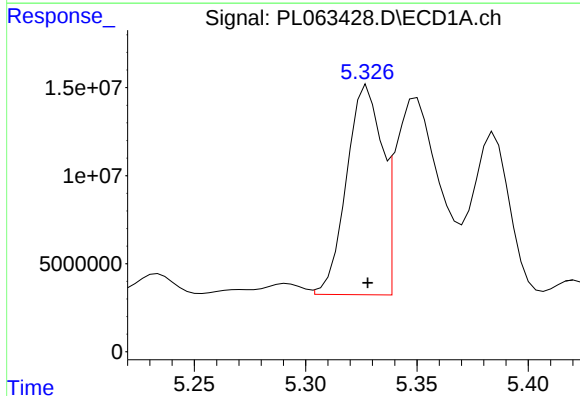


#25 Chlordane-3

R.T.: 5.328 min
Delta R.T.: 0.000 min
Response: 130793054
Conc: 761.33 ng/ml

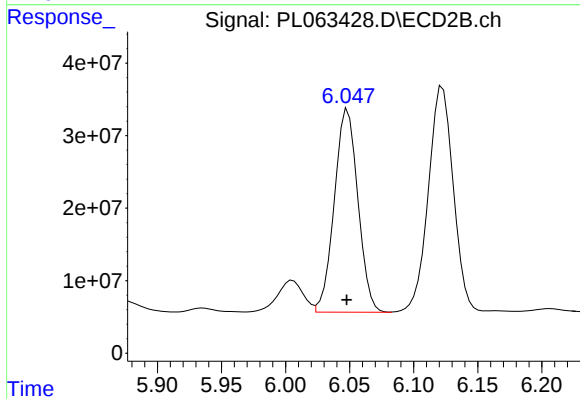

#25 Chlordane-3


R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 358866124
Conc: 768.73 ng/ml

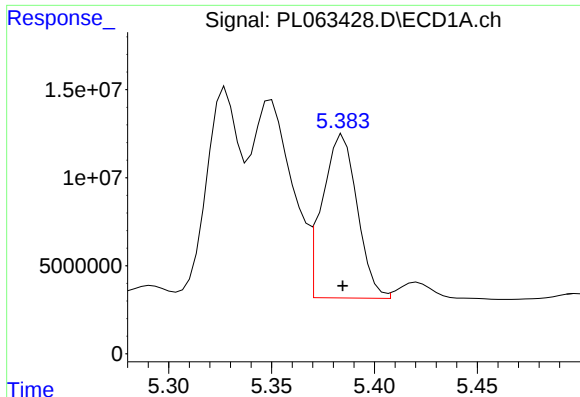

#26 Chlordane-4


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 109478464
Conc: 747.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

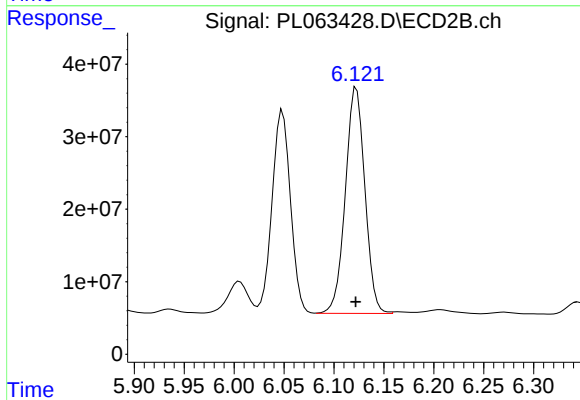


#26 Chlordane-4

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 424550696
Conc: 768.19 ng/ml

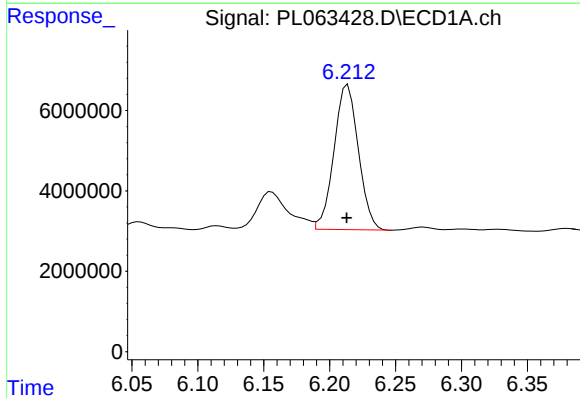


#27 Chlordane-5

R.T.: 6.214 min
Delta R.T.: 0.000 min
Response: 46351506
Conc: 729.59 ng/ml

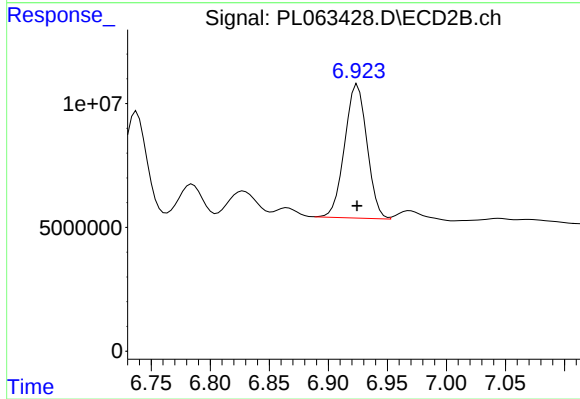

#27 Chlordane-5


R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 71207773
Conc: 783.06 ng/ml

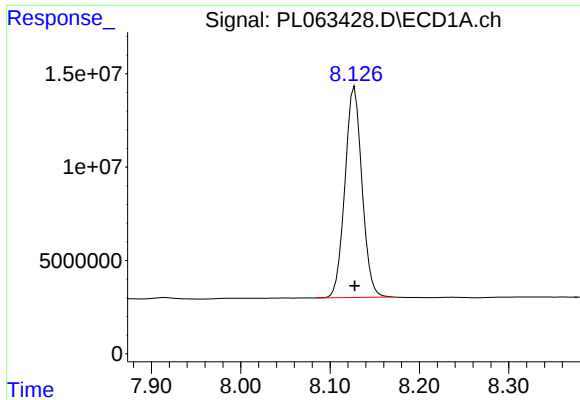

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 149728213
Conc: 73.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

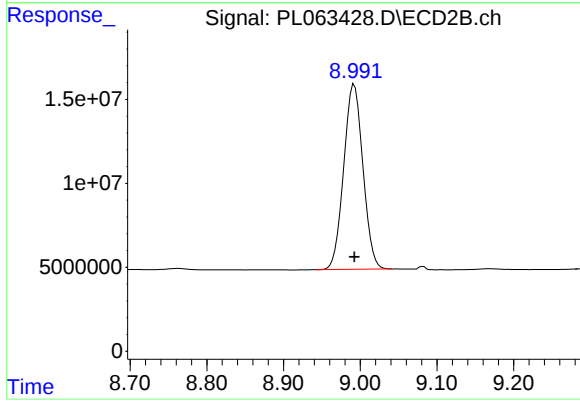

#28 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 193035675
Conc: 73.07 ng/ml