

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
 Data File : PL063438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 21:28
 Operator : DD\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL121020CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:49:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 10 01:46:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.409	3.951	101.2E6	167.4E6	59.452	53.421
28)	SA Decachlor...	8.127	8.993	103.1E6	130.4E6	51.201	51.780
Target Compounds							
23)	Chlordane-1	4.267	4.937	27384785	58338338	500.588	511.628
24)	Chlordane-2	4.764	5.404	30656138	65193134	492.937	506.306
25)	Chlordane-3	5.327	6.048	85115823	232.7E6	493.205	494.084
26)	Chlordane-4	5.384	6.122	72265311	278.7E6	493.777	497.251
27)	Chlordane-5	6.213	6.925	30271542	45407816	486.252	485.256



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121020\
Data File : PL063438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 21:28
Operator : DD\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL121020CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:49:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121020.M
Quant Title : GC Extractables
QLast Update : Thu Dec 10 01:46:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

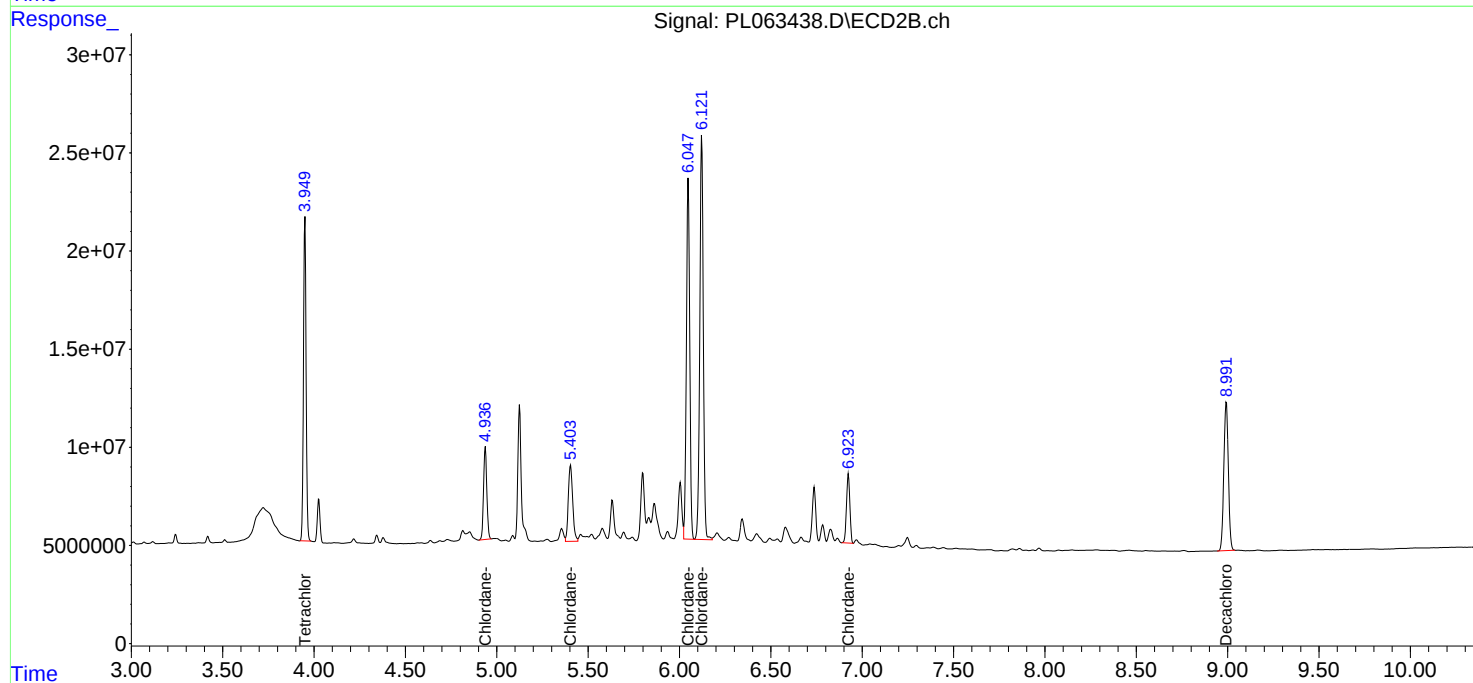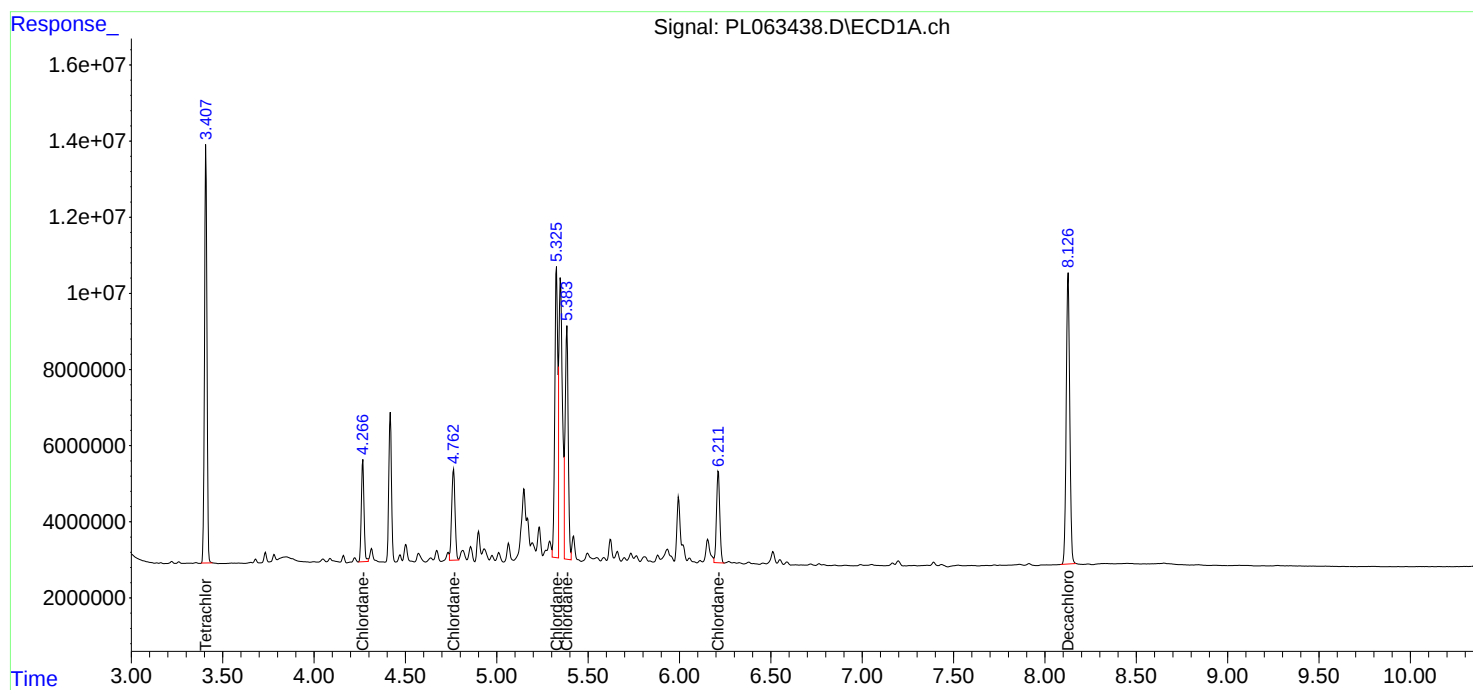


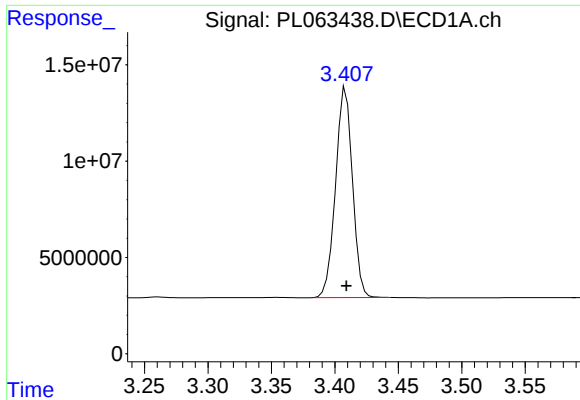

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 101169691
Conc: 59.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121020CHLOR

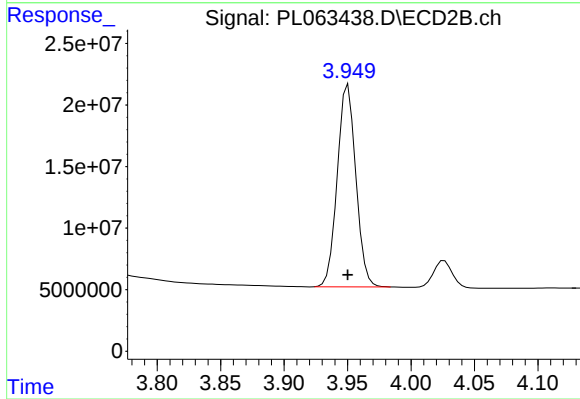


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 167430522
Conc: 53.42 ng/ml

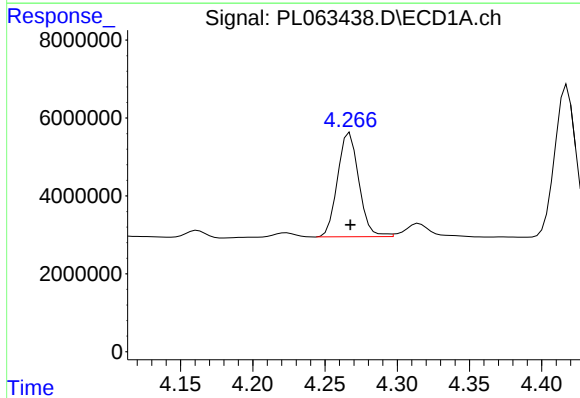


#23 Chlordane-1

R.T.: 4.267 min
Delta R.T.: 0.000 min
Response: 27384785
Conc: 500.59 ng/ml

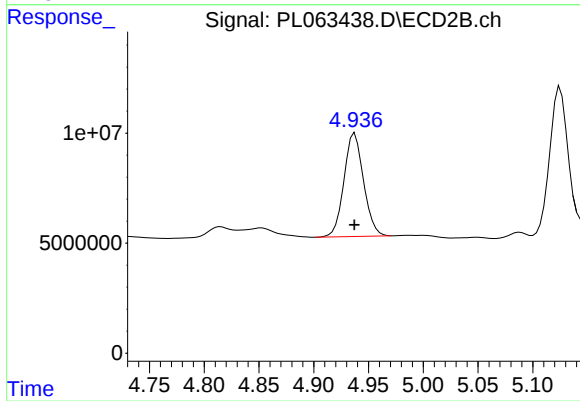

#23 Chlordane-1


R.T.: 4.937 min
Delta R.T.: 0.000 min
Response: 58338338
Conc: 511.63 ng/ml

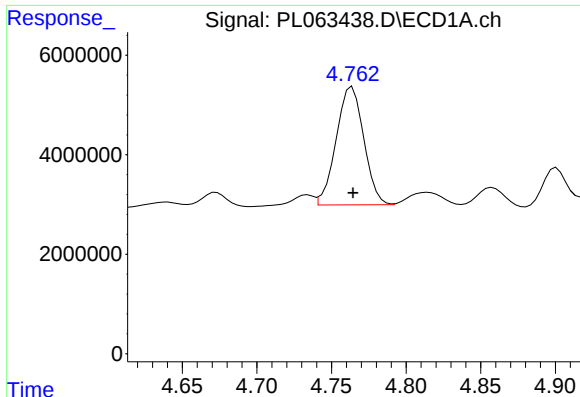

#24 Chlordane-2


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 30656138
Conc: 492.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121020CHLOR

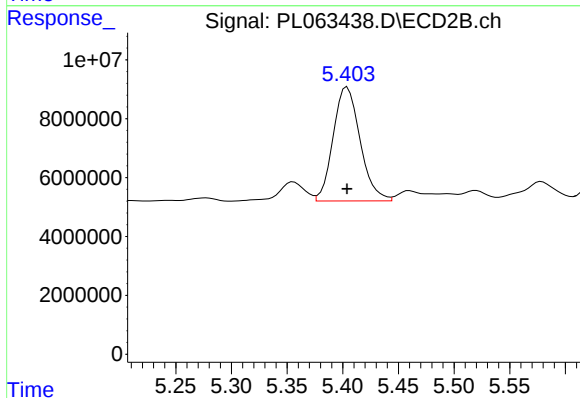


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 65193134
Conc: 506.31 ng/ml

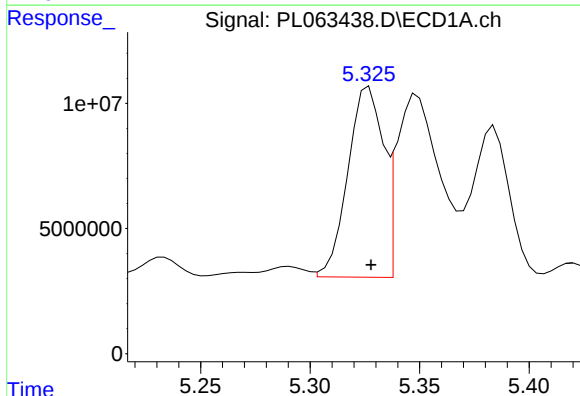


#25 Chlordane-3

R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 85115823
Conc: 493.20 ng/ml

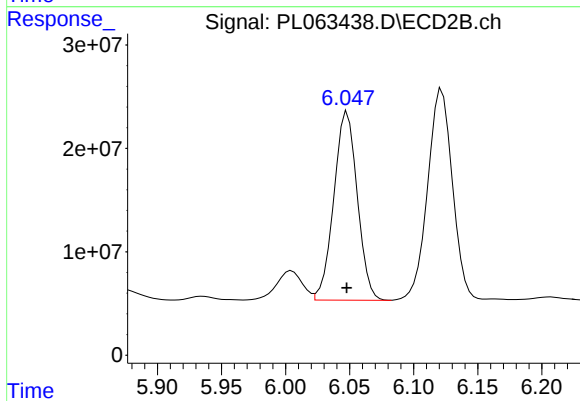

#25 Chlordane-3


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 232701010
Conc: 494.08 ng/ml

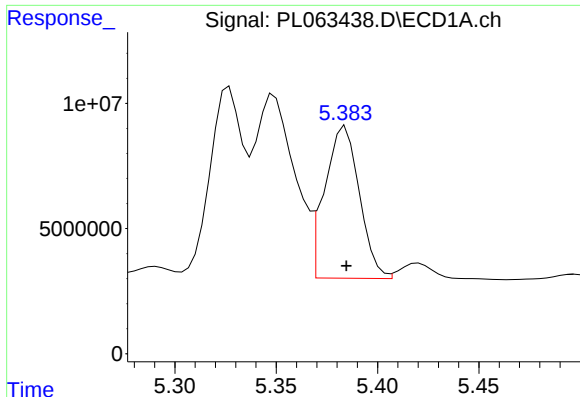

#26 Chlordane-4


R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 72265311
Conc: 493.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121020CHLOR

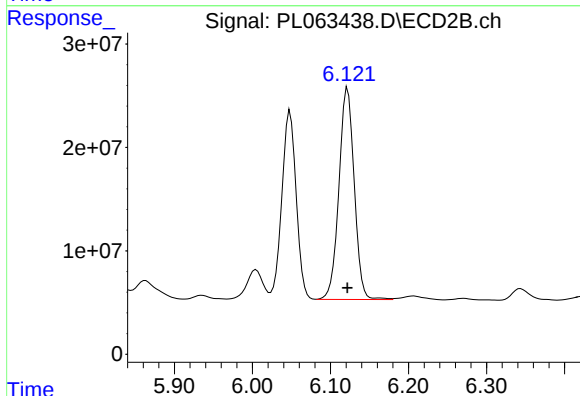


#26 Chlordane-4

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 278699066
Conc: 497.25 ng/ml

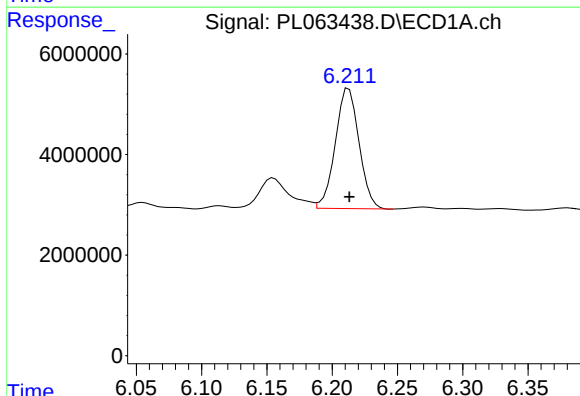


#27 Chlordane-5

R.T.: 6.213 min
Delta R.T.: 0.000 min
Response: 30271542
Conc: 486.25 ng/ml

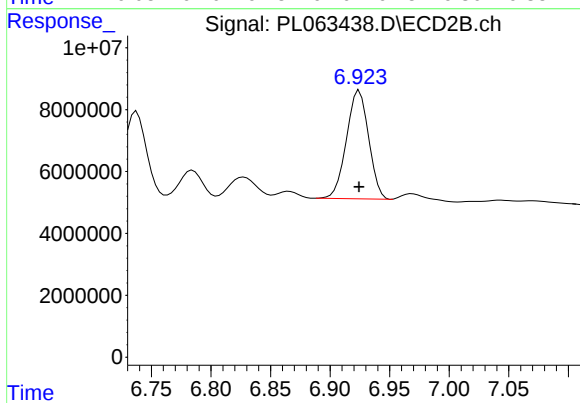

#27 Chlordane-5


R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 45407816
Conc: 485.26 ng/ml

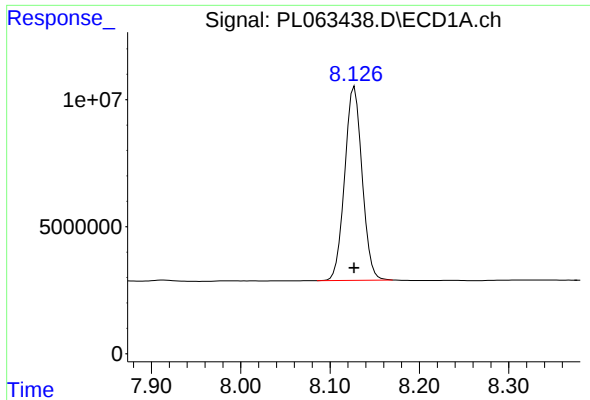

#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 103112067
Conc: 51.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL121020CHLOR

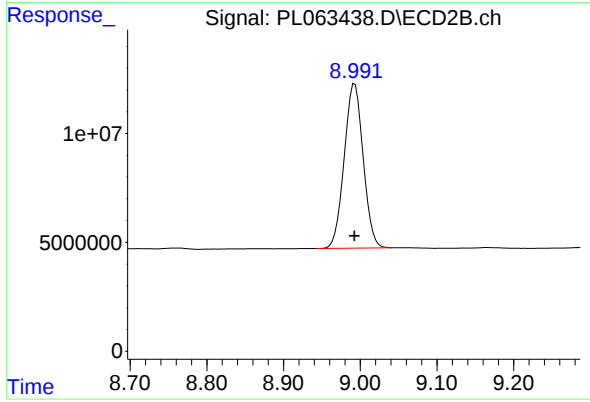

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 130398478
Conc: 51.78 ng/ml