

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121521\
 Data File : PL071466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2021 18:33
 Operator : AR\AJ
 Sample : M5089-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MS-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 00:37:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.560	5.496	9026827	23843392	19.044	20.014
28) SA Decachlor...	10.318	11.384	11767898	19774885	17.712	18.201
Target Compounds						
12) B 4,4'-DDE	7.556	8.489	354220	963891	0.649	0.809m
13) MA Dieldrin	7.692	8.648	1664633	777866	2.843m	0.640 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121521\
Data File : PL071466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2021 18:33
Operator : AR\AJ
Sample : M5089-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MS-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 00:37:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

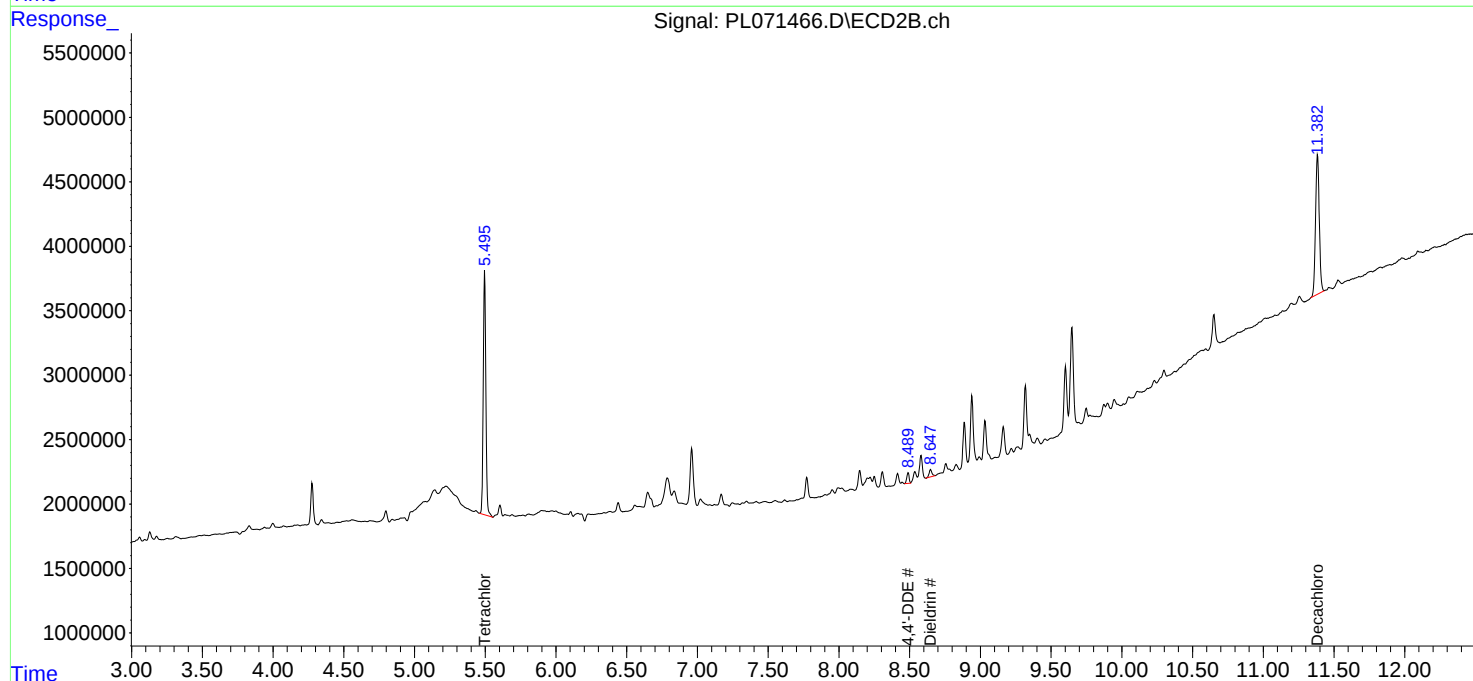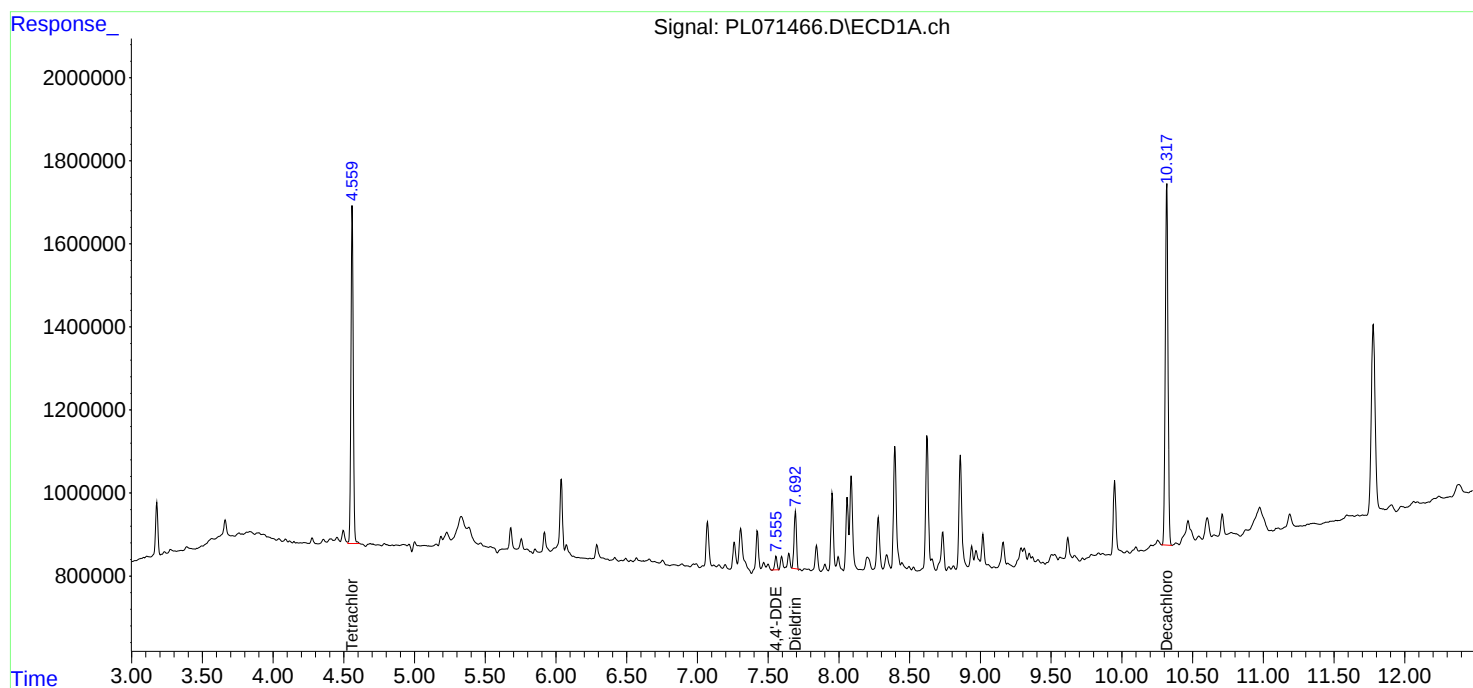


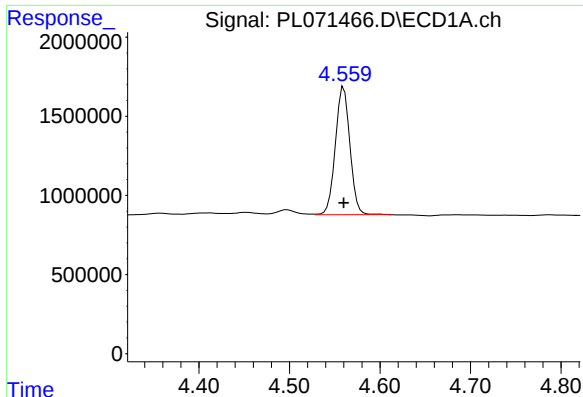

#1 Tetrachloro-m-xylene


R.T.: 4.560 min
Delta R.T.: 0.000 min
Response: 9026827
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-2

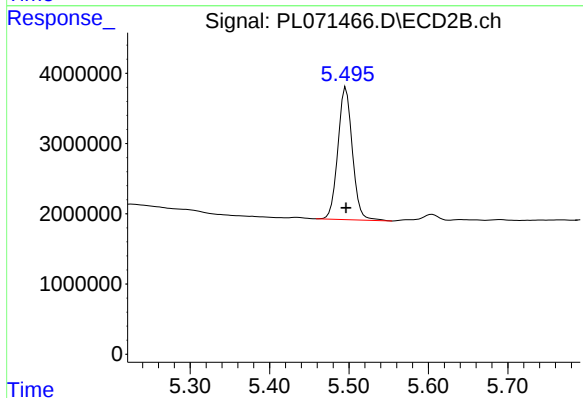


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: 0.000 min
Response: 23843392
Conc: 20.01 ng/ml

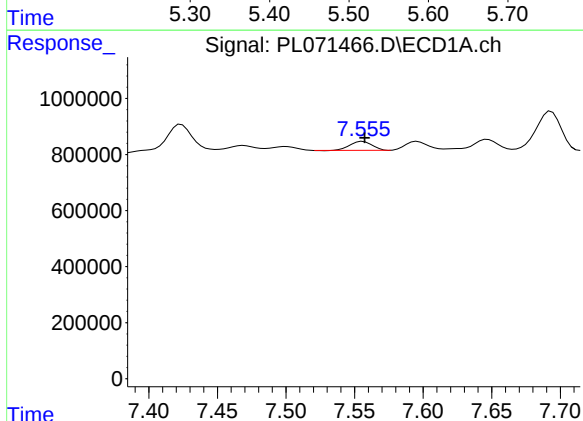


#12 4,4'-DDE

R.T.: 7.556 min
Delta R.T.: -0.001 min
Response: 354220
Conc: 0.65 ng/ml

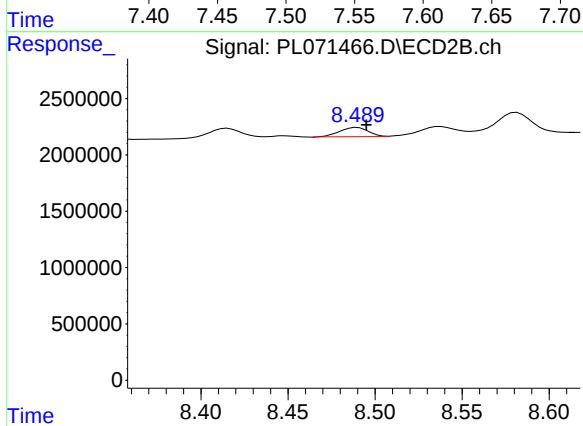

#12 4,4'-DDE


R.T.: 8.489 min
Delta R.T.: -0.006 min
Response: 963891
Conc: 0.81 ng/ml m

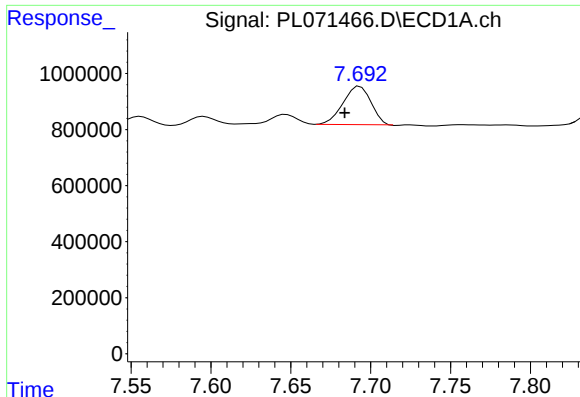

#13 Dieldrin


R.T.: 7.692 min
Delta R.T.: 0.008 min
Response: 1664633
Conc: 2.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-2

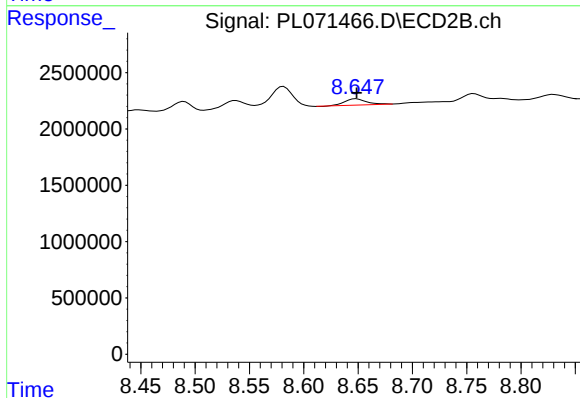


#13 Dieldrin

R.T.: 8.648 min
Delta R.T.: 0.000 min
Response: 777866
Conc: 0.64 ng/ml

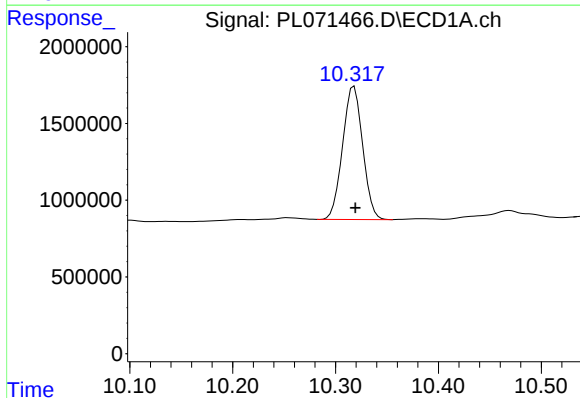

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.001 min
Response: 11767898
Conc: 17.71 ng/ml

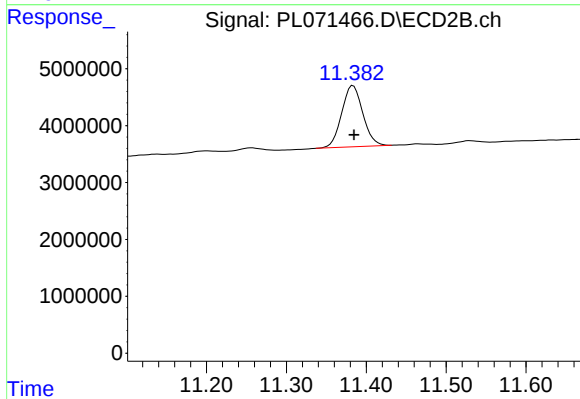

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.001 min
Response: 19774885
Conc: 18.20 ng/ml