

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121521\
 Data File : PL071469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2021 19:23
 Operator : AR\AJ
 Sample : M5089-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MS-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/16/2021
 Supervised By :Ankita Jodhani 12/16/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 00:38:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 14:29:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.495	9224928	24472378	19.462m	20.542m
28)	SA Decachlor...	10.318	11.384	12937356	25289688	19.472	23.277

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121521\
Data File : PL071469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2021 19:23
Operator : AR\AJ
Sample : M5089-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MS-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/16/2021
Supervised By : Ankita Jodhani 12/16/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 00:38:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 14:29:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

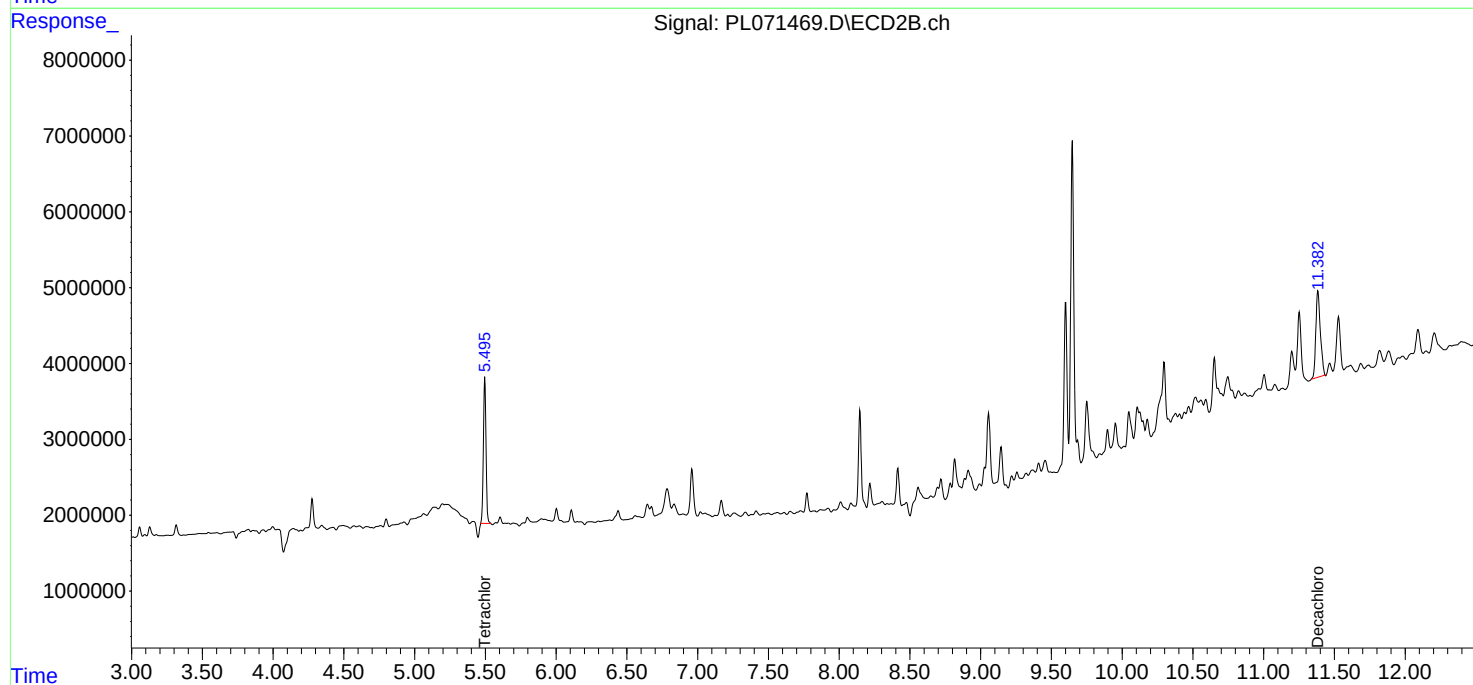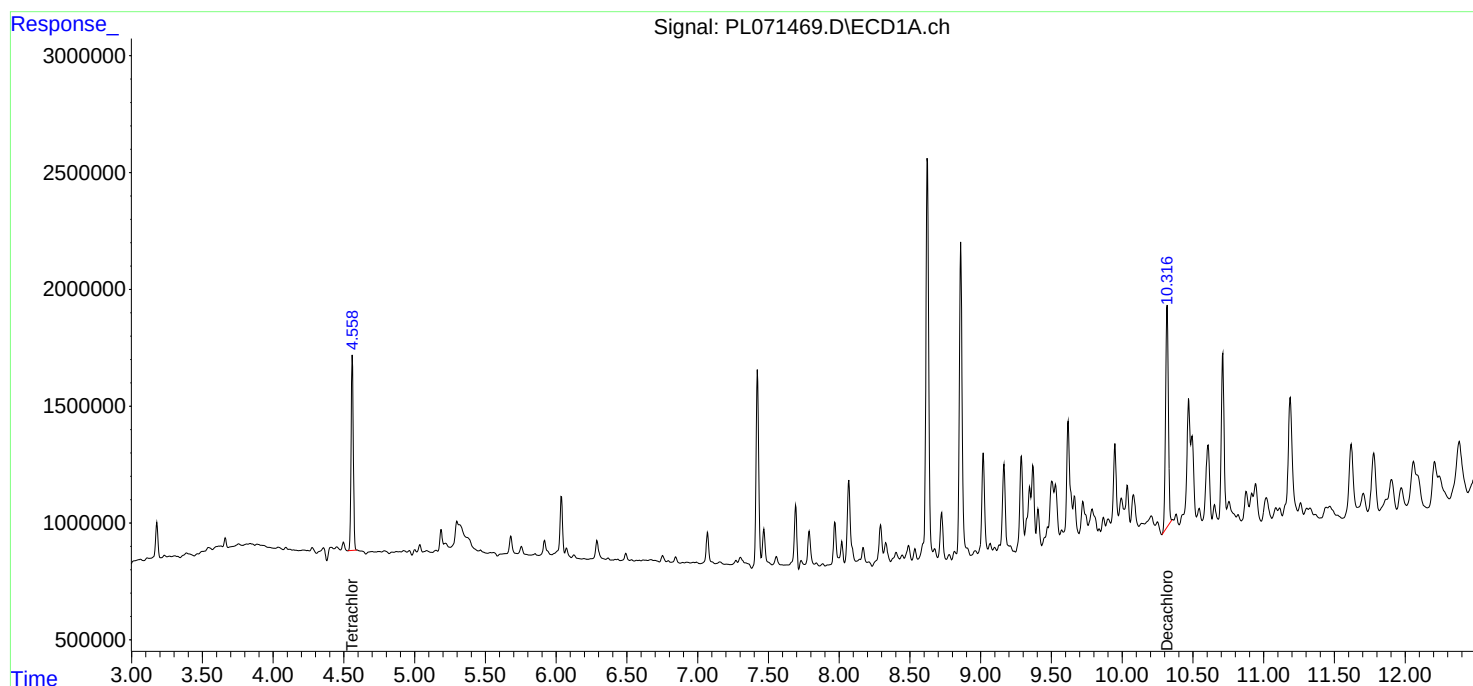

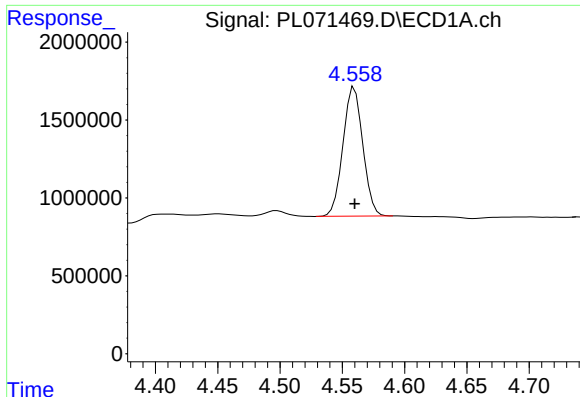


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: -0.002 min
Response: 9224928
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
MS-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/16/2021
Supervised By :Ankita Jodhani 12/16/2021

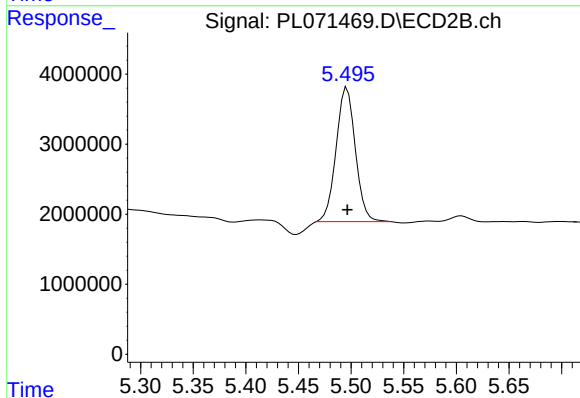


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: -0.002 min
Response: 24472378
Conc: 20.54 ng/ml m

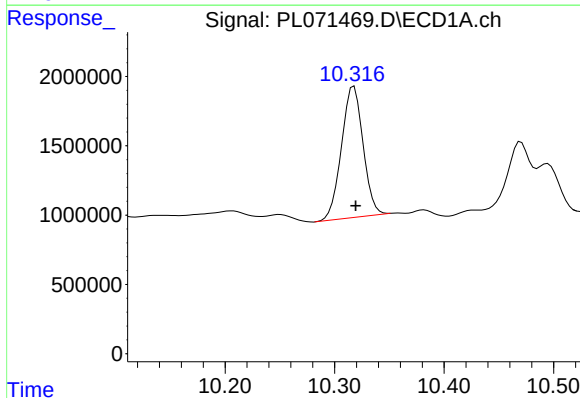

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.002 min
Response: 12937356
Conc: 19.47 ng/ml

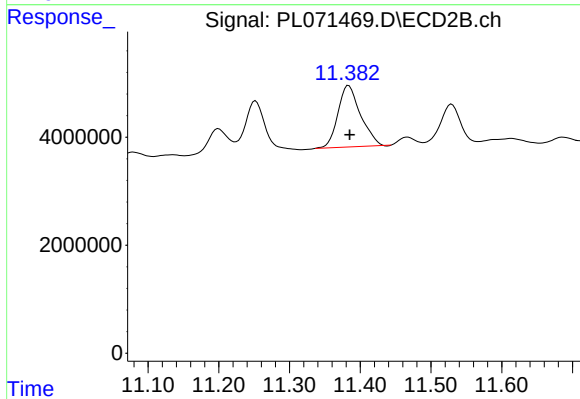

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.001 min
Response: 25289688
Conc: 23.28 ng/ml