

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010120\
 Data File : P0065172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2019 18:04
 Operator : AJ/MA
 Sample : K6460-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GW-6

Manual Integrations
 APPROVED

mohammad
 1/2/2020 4:21:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 02:07:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.454	428316	589852	20.307m	23.349m
2) SA Decachlor...	9.701	8.368	319904	533493	10.483	13.863m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010120\
Data File : PO065172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2019 18:04
Operator : AJ/MA
Sample : K6460-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GW-6


Manual Integrations
APPROVED

mohammad
1/2/2020 4:21:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 02:07:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

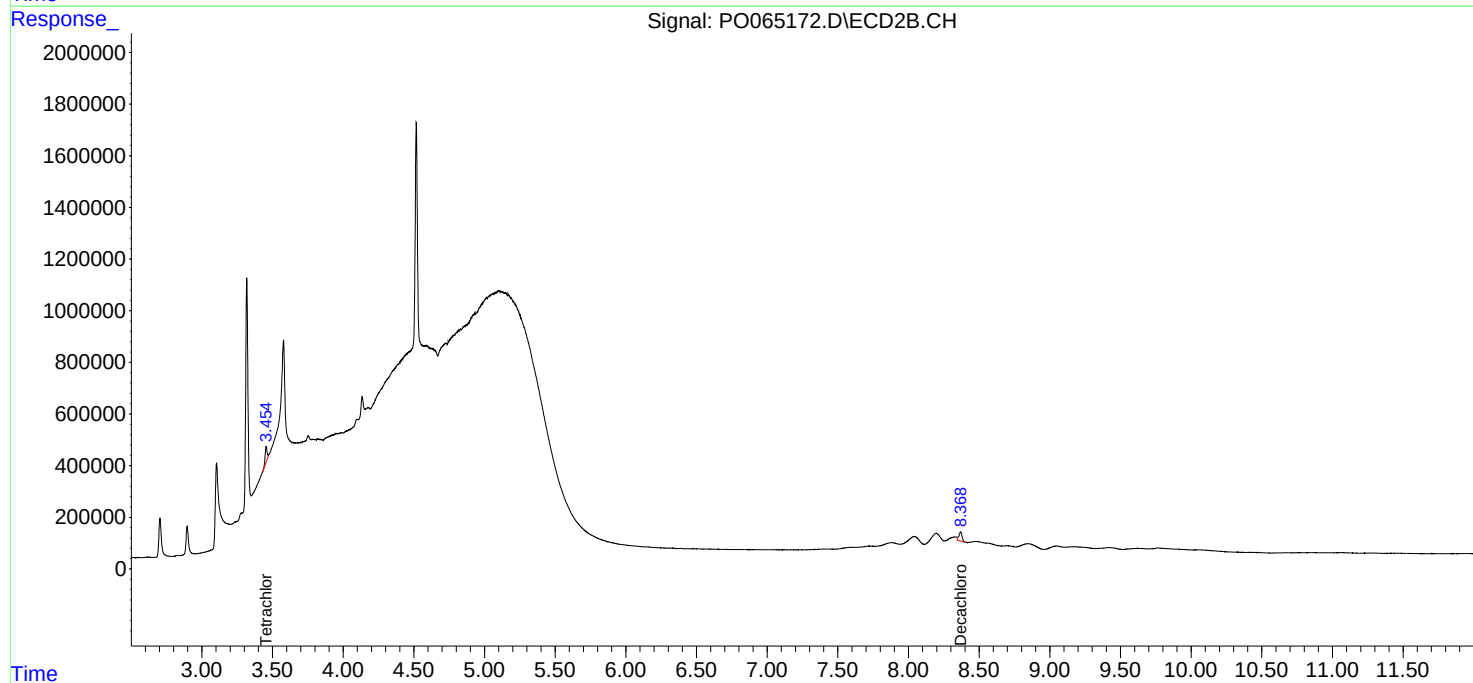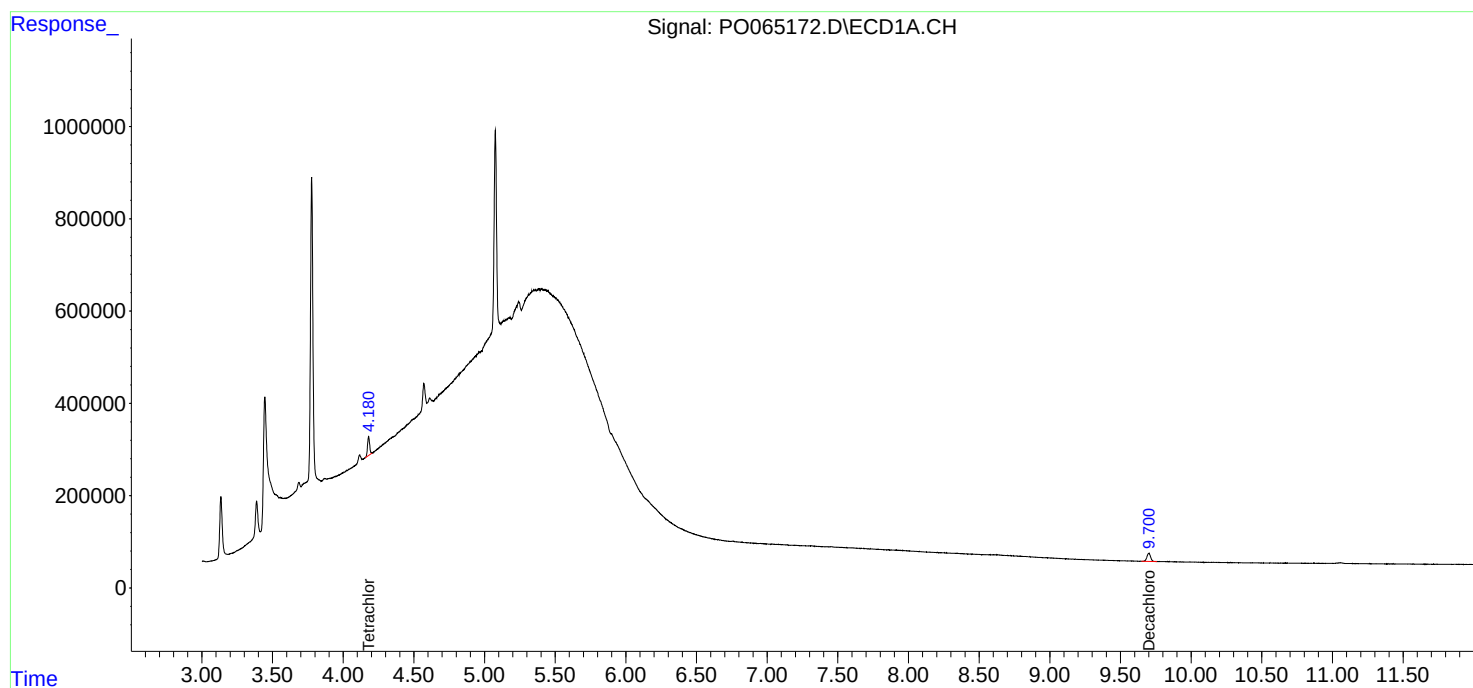

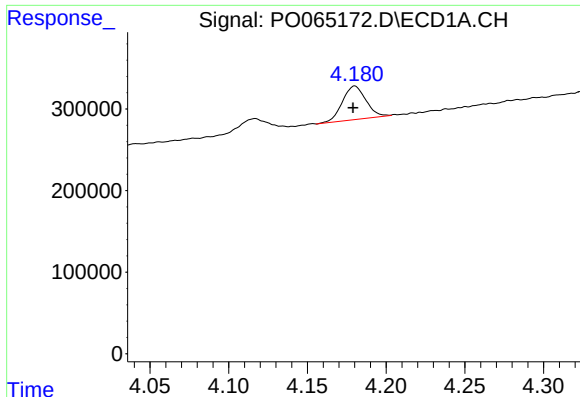


#1 Tetrachloro-m-xylene

R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 428316
Conc: 20.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
GW-6


Manual Integrations
APPROVED

mohammad
1/2/2020 4:21:28 PM

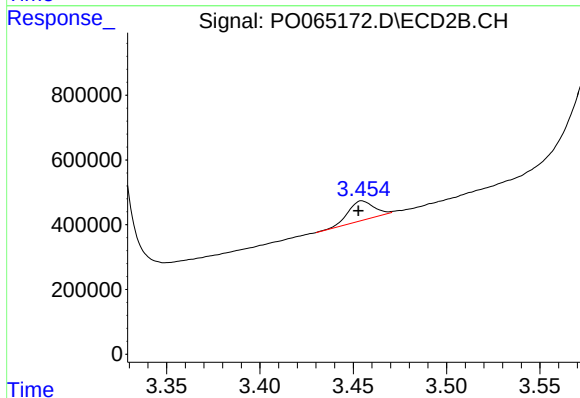


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.001 min
Response: 589852
Conc: 23.35 ng/ml m

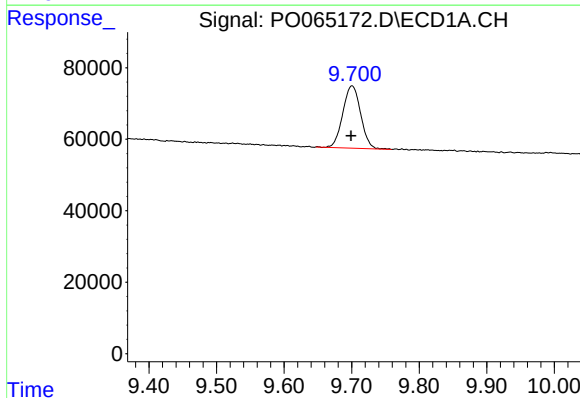

#2 Decachlorobiphenyl

R.T.: 9.701 min
Delta R.T.: 0.002 min
Response: 319904
Conc: 10.48 ng/ml

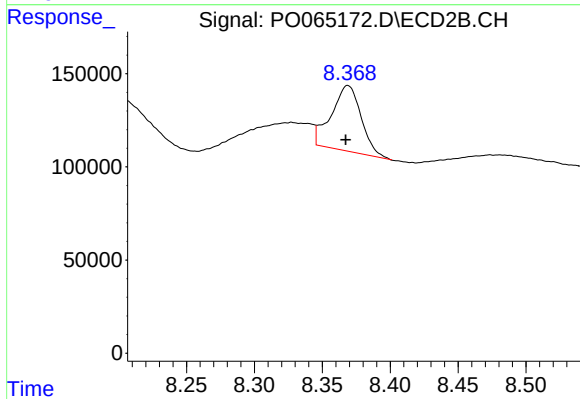

#2 Decachlorobiphenyl

R.T.: 8.368 min
Delta R.T.: 0.000 min
Response: 533493
Conc: 13.86 ng/ml m