

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010120\
 Data File : P0065188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Dec 2019 23:05
 Operator : AJ/MA
 Sample : K6471-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-123019-0-2-COMP-B8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 02:13:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.178	3.451	383620	469023	18.188	18.566
2) SA Decachlor...	9.697	8.367	503717	594078	16.506	15.437

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010120\
Data File : P0065188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Dec 2019 23:05
Operator : AJ/MA
Sample : K6471-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 02:13:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

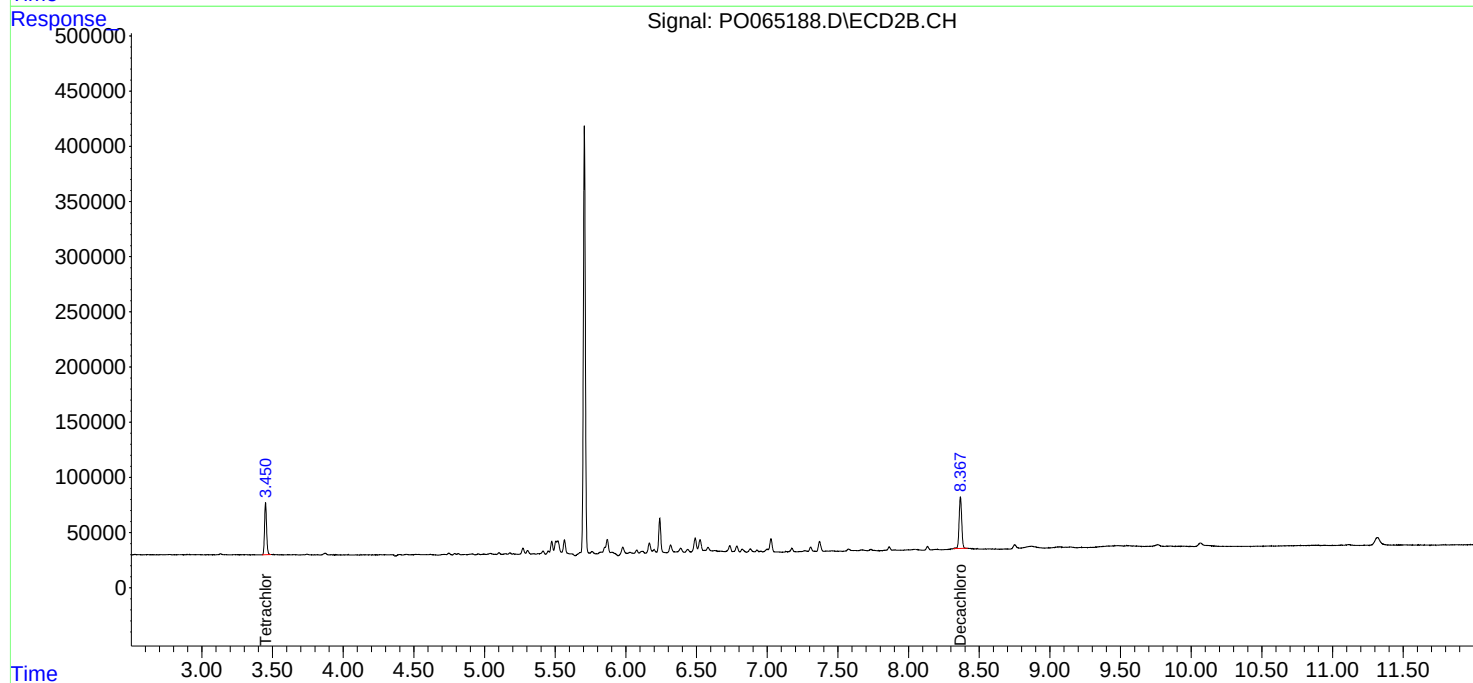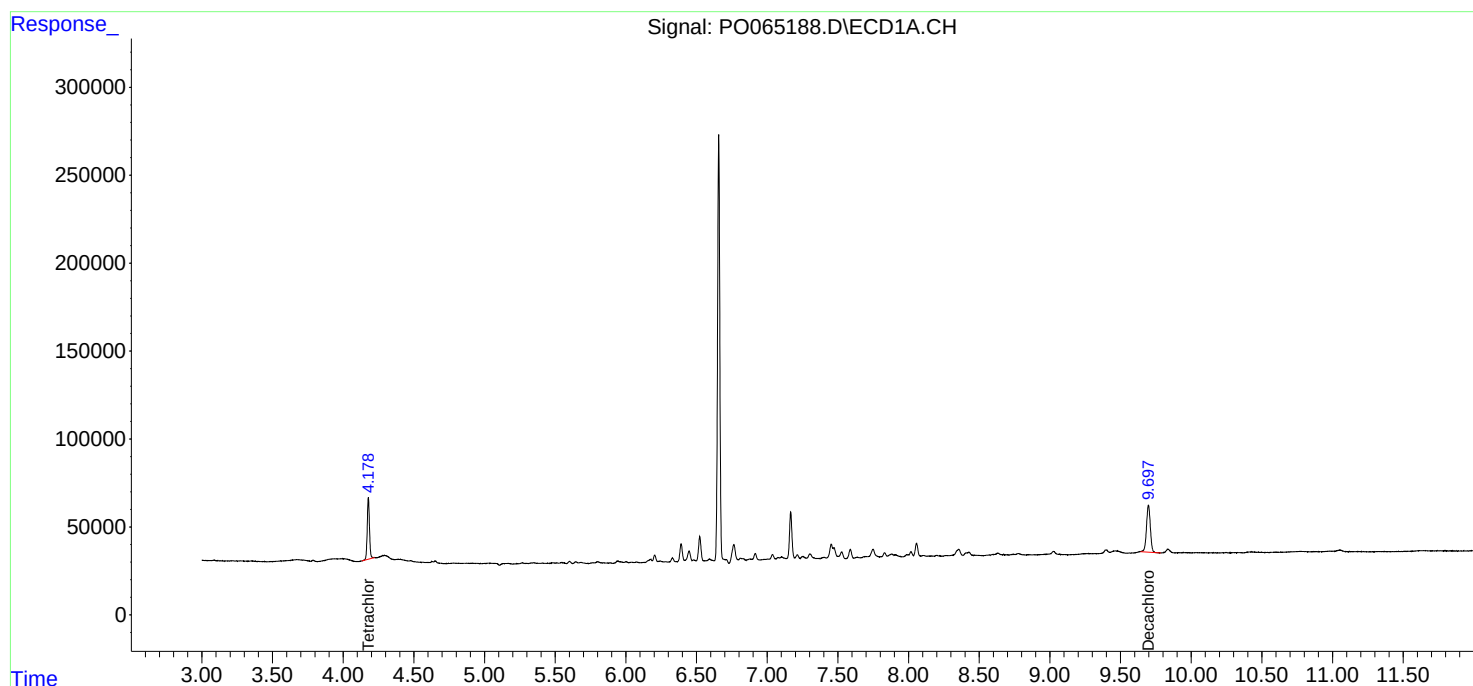


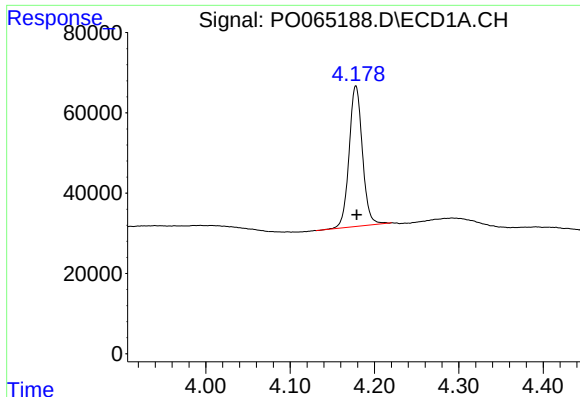

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: -0.001 min
Response: 383620
Conc: 18.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B8

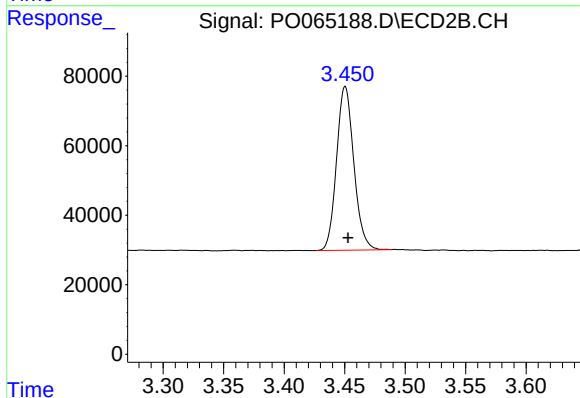


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: -0.002 min
Response: 469023
Conc: 18.57 ng/ml

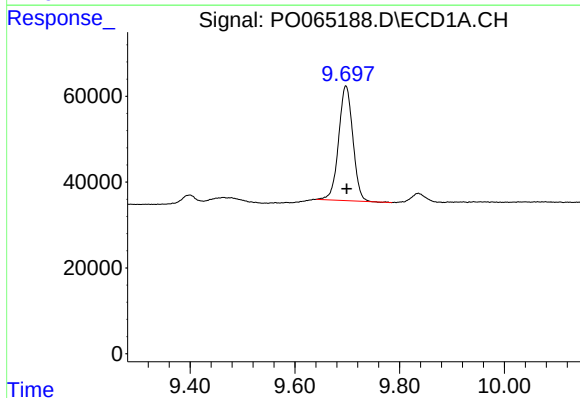

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: -0.002 min
Response: 503717
Conc: 16.51 ng/ml

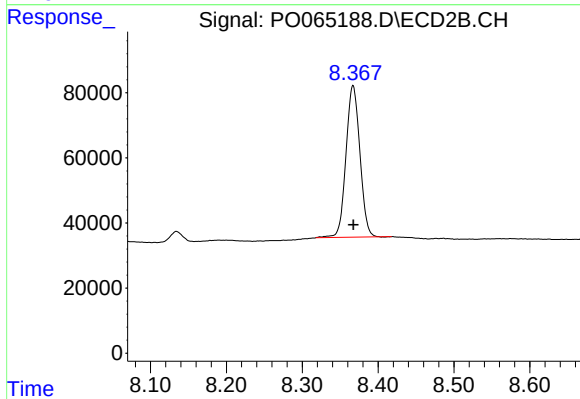

#2 Decachlorobiphenyl

R.T.: 8.367 min
Delta R.T.: 0.000 min
Response: 594078
Conc: 15.44 ng/ml