

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0010120\  
 Data File : P0065190.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 31 Dec 2019 23:39  
 Operator : AJ/MA  
 Sample : K6471-10  
 Misc :  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 MC-123019-0-2-COMP-B2

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 01 02:13:48 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0123119.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Dec 31 07:42:34 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|-------|-------|--------|--------|--------|--------|
| -----                       |       |       |        |        |        |        |
| System Monitoring Compounds |       |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.178 | 3.451 | 487334 | 674145 | 23.105 | 26.685 |
| 2) SA Decachlor...          | 9.698 | 8.367 | 551154 | 682157 | 18.061 | 17.726 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO010120\  
Data File : PO065190.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 31 Dec 2019 23:39  
Operator : AJ/MA  
Sample : K6471-10  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
MC-123019-0-2-COMP-B2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 01 02:13:48 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO123119.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Dec 31 07:42:34 2019  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

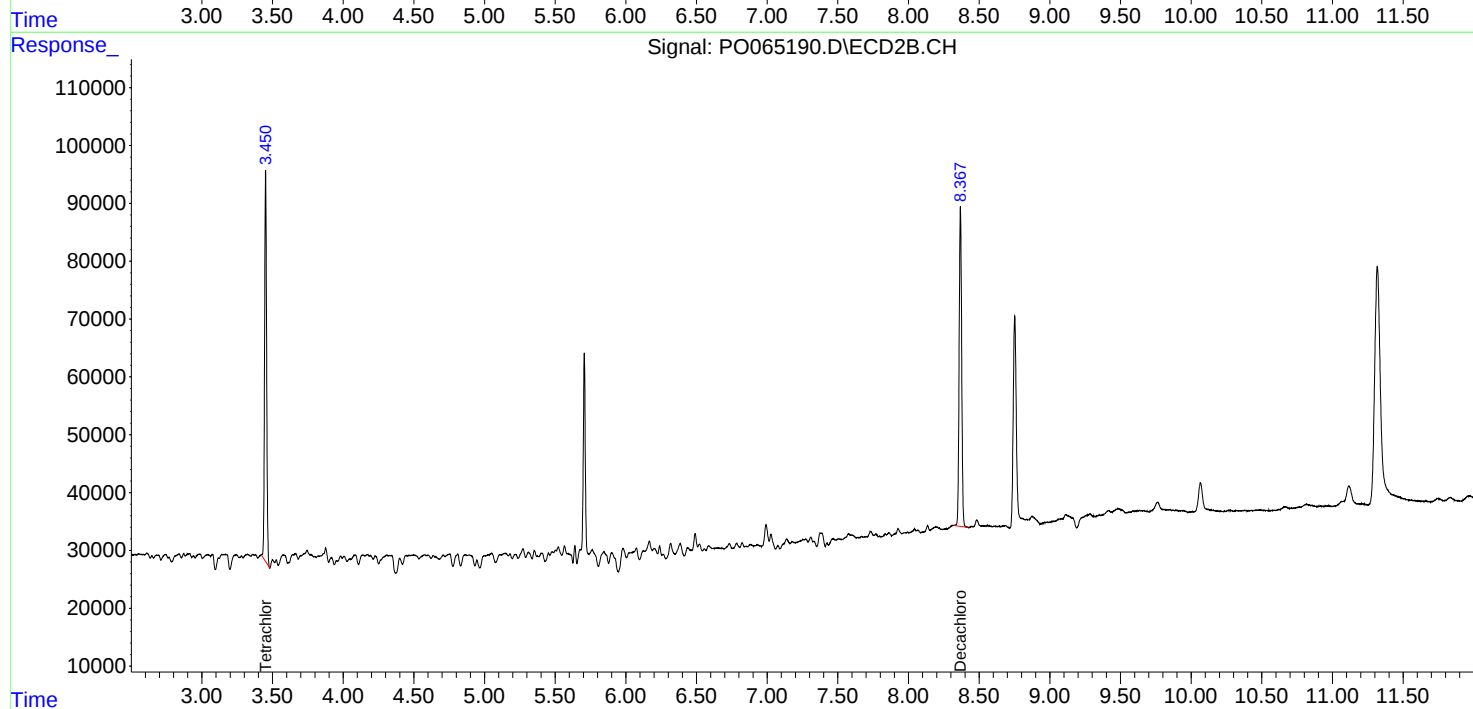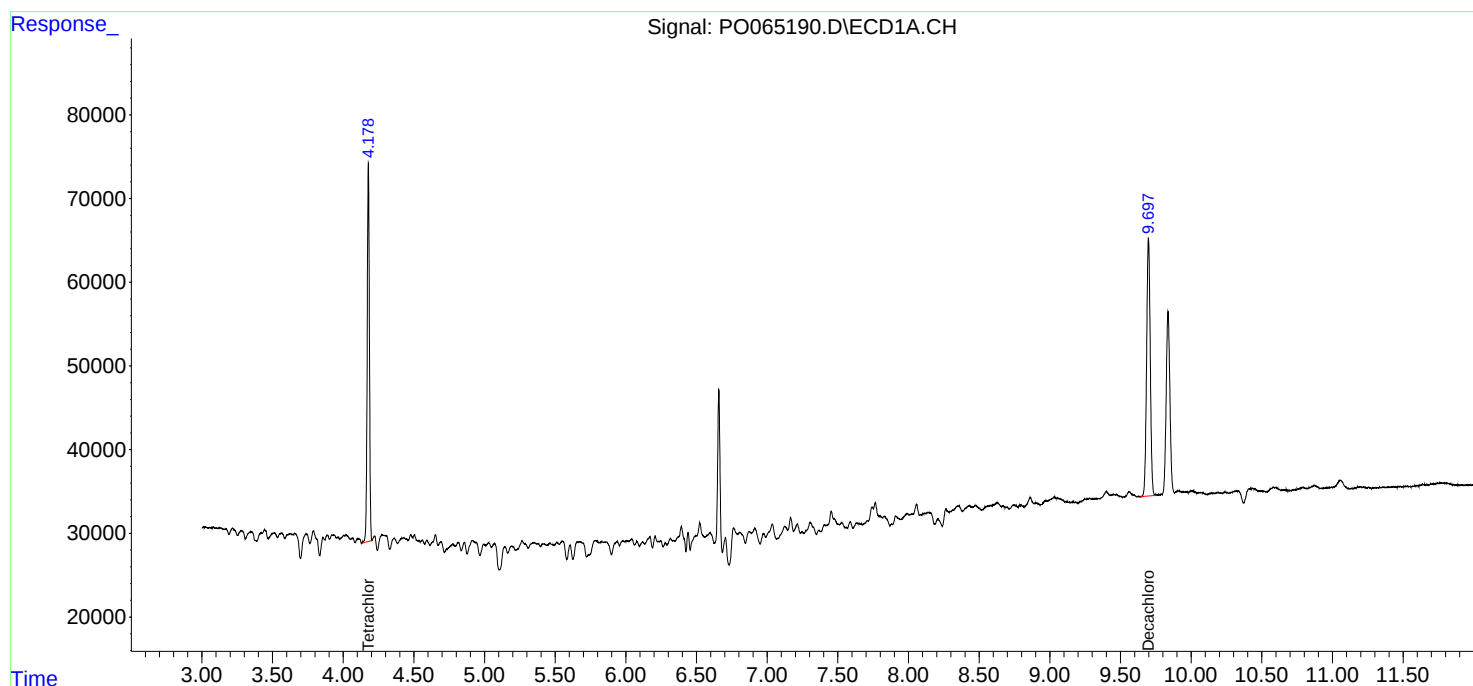


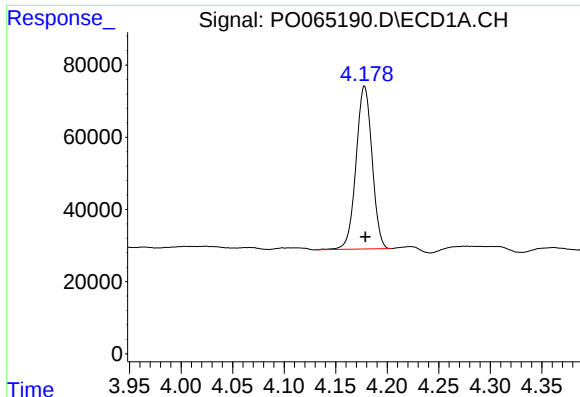

#1 Tetrachloro-m-xylene


R.T.: 4.178 min  
Delta R.T.: -0.001 min  
Response: 487334  
Conc: 23.11 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
MC-123019-0-2-COMP-B2

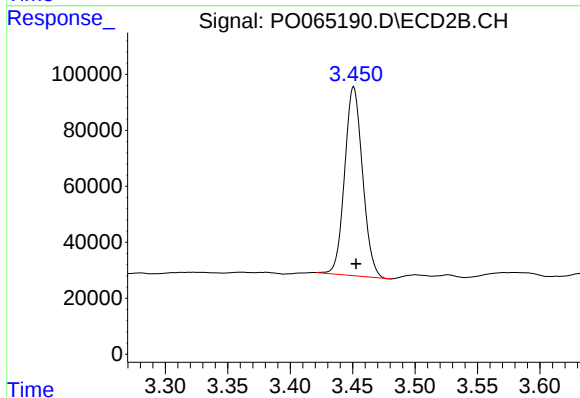


#1 Tetrachloro-m-xylene

R.T.: 3.451 min  
Delta R.T.: -0.002 min  
Response: 674145  
Conc: 26.69 ng/ml

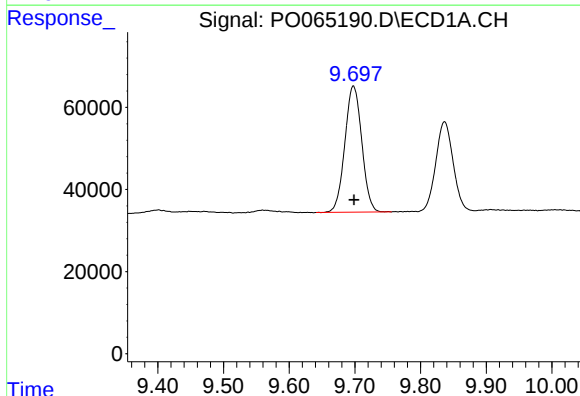

#2 Decachlorobiphenyl

R.T.: 9.698 min  
Delta R.T.: -0.001 min  
Response: 551154  
Conc: 18.06 ng/ml

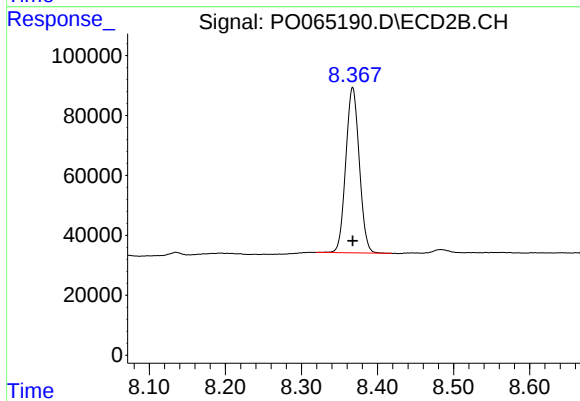

#2 Decachlorobiphenyl

R.T.: 8.367 min  
Delta R.T.: 0.000 min  
Response: 682157  
Conc: 17.73 ng/ml