

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065258.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2020 00:09
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:10:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.166	3.440	592282	698846	28.081	27.663
2)	SA Decachlor...	9.676	8.352	634596	761603	20.795	19.790
Target Compounds							
9)	L2 AR-1221-2	0.000	3.733	0	8378	N.D.	37.413 #
20)	L4 AR-1242-5	6.190	5.258	43741	38023	58.204	35.547 #
24)	L5 AR-1248-4	6.190	0.000	43741	0	33.778	N.D. #
25)	L5 AR-1248-5	6.190	0.000	43741	0	35.047	N.D. #
26)	L6 AR-1254-1	6.190	5.258	43741	38023	33.618	16.263 #
27)	L6 AR-1254-2	6.430	5.508	34220	77805	16.152	36.498 #
32)	L7 AR-1260-2	0.000	6.185	0	12448	N.D.	4.080 #
45)	L9 AR-1268-5	0.000	8.160	0	473	N.D.	0.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010220\
Data File : PO065258.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2020 00:09
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:10:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

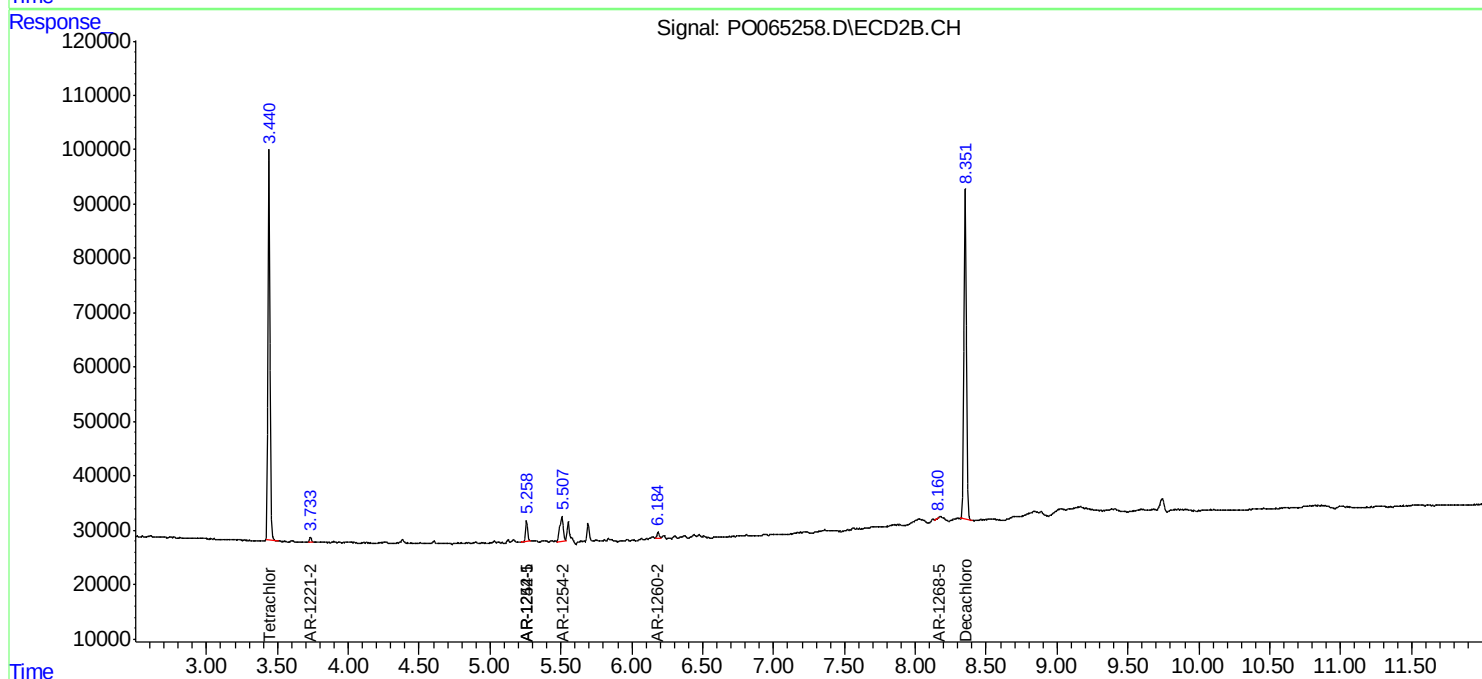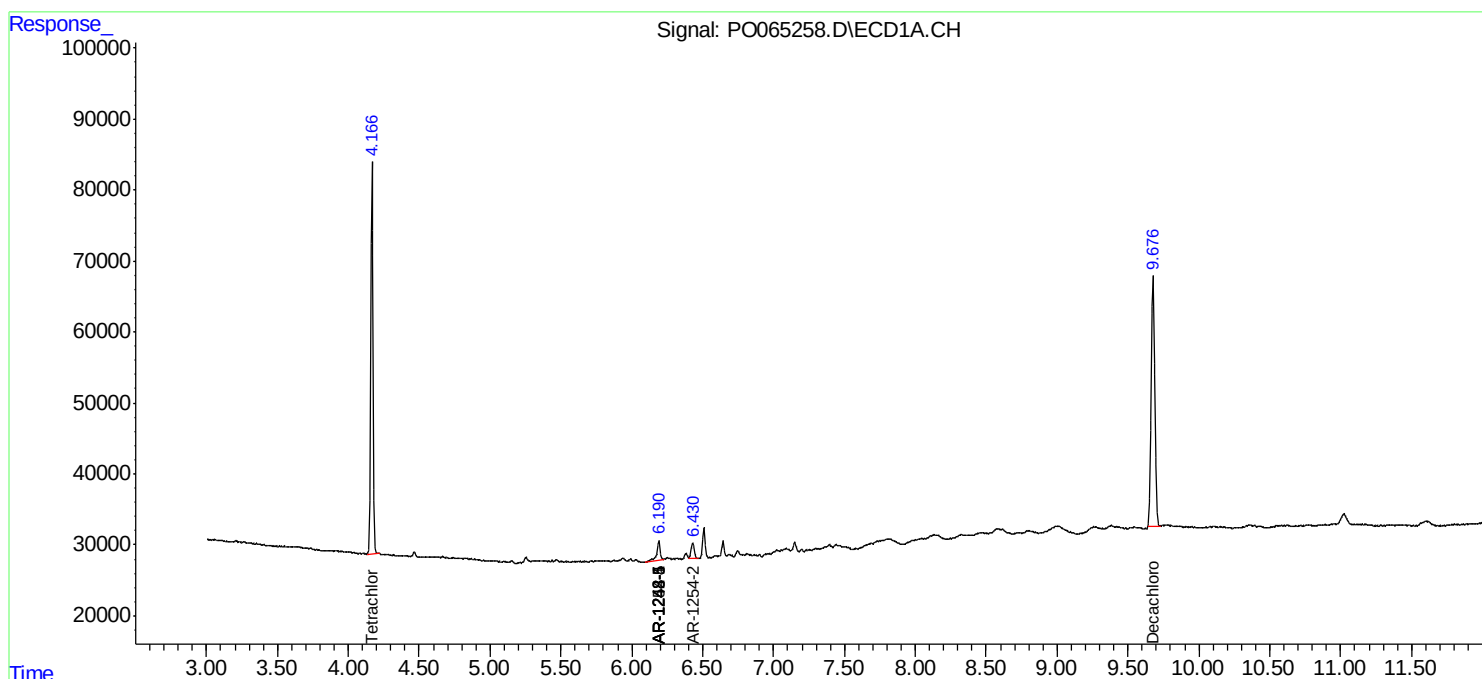


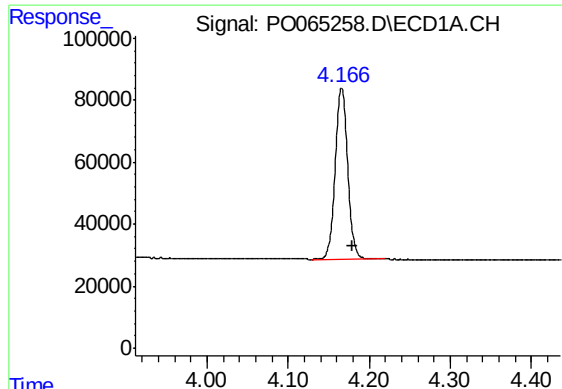

#1 Tetrachloro-m-xylene


R.T.: 4.166 min
Delta R.T.: -0.013 min
Response: 592282
Conc: 28.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

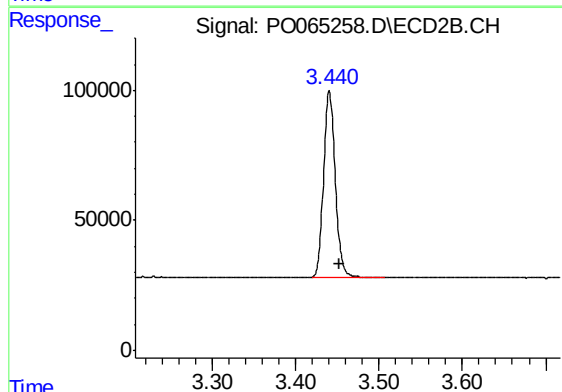


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: -0.012 min
Response: 698846
Conc: 27.66 ng/ml

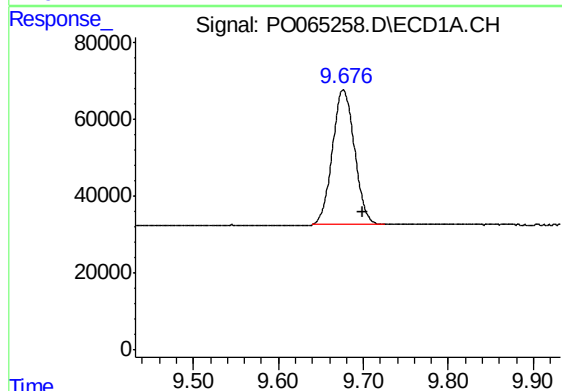


#2 Decachlorobiphenyl

R.T.: 9.676 min
Delta R.T.: -0.023 min
Response: 634596
Conc: 20.79 ng/ml

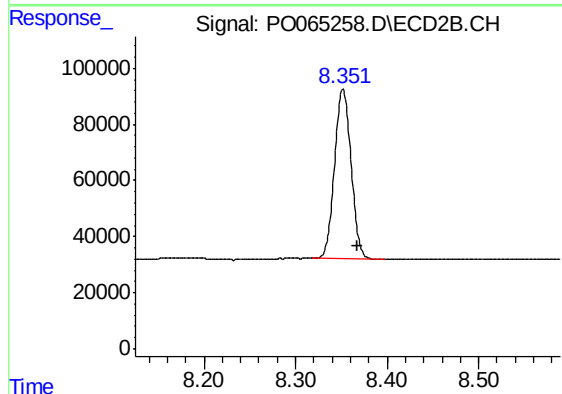

#2 Decachlorobiphenyl


R.T.: 8.352 min
Delta R.T.: -0.016 min
Response: 761603
Conc: 19.79 ng/ml

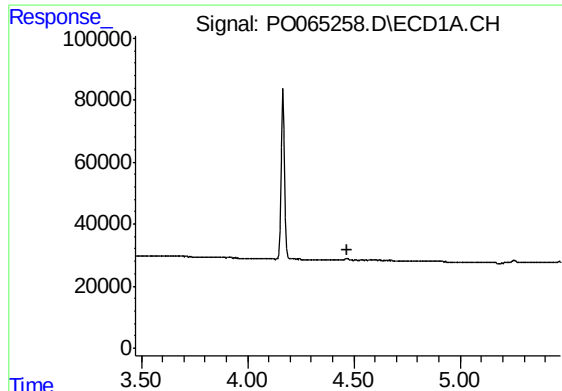

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

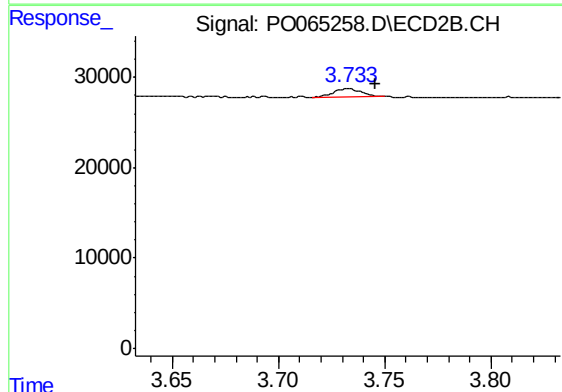


#9 AR-1221-2

R.T.: 3.733 min
Delta R.T.: -0.013 min
Response: 8378
Conc: 37.41 ng/ml

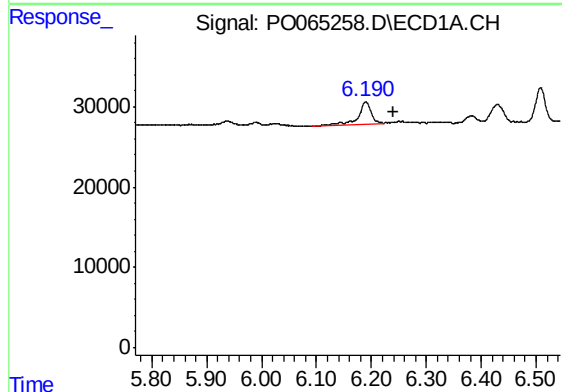


#20 AR-1242-5

R.T.: 6.190 min
Delta R.T.: -0.050 min
Response: 43741
Conc: 58.20 ng/ml

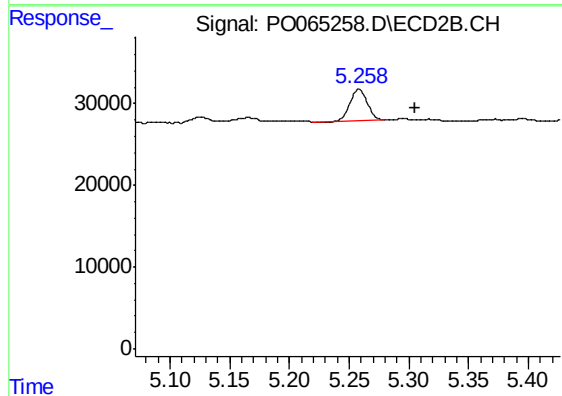

#20 AR-1242-5


R.T.: 5.258 min
Delta R.T.: -0.047 min
Response: 38023
Conc: 35.55 ng/ml

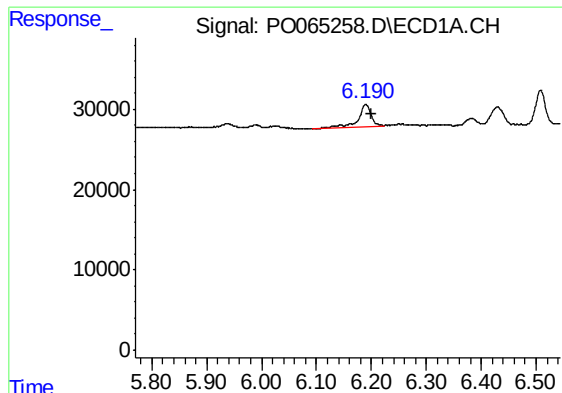

#24 AR-1248-4


R.T.: 6.190 min
Delta R.T.: -0.011 min
Response: 43741
Conc: 33.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

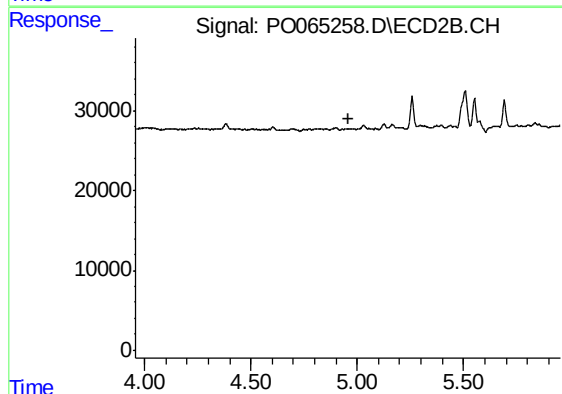


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 4.957 min
Response: 0
Conc: N.D.

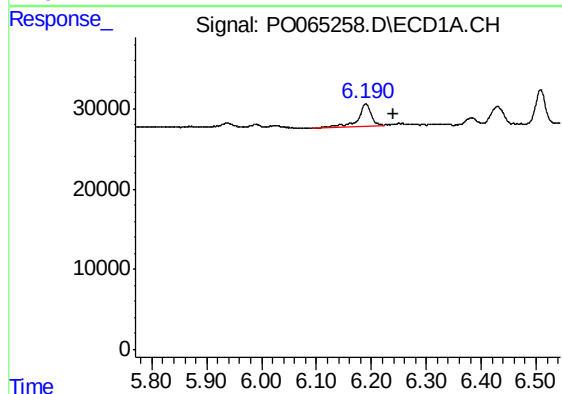


#25 AR-1248-5

R.T.: 6.190 min
Delta R.T.: -0.049 min
Response: 43741
Conc: 35.05 ng/ml

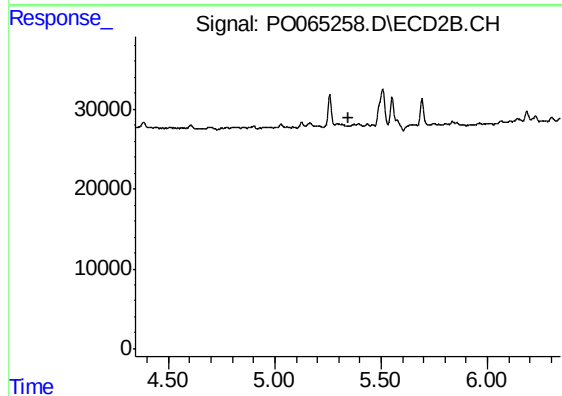

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.344 min
Response: 0
Conc: N.D.

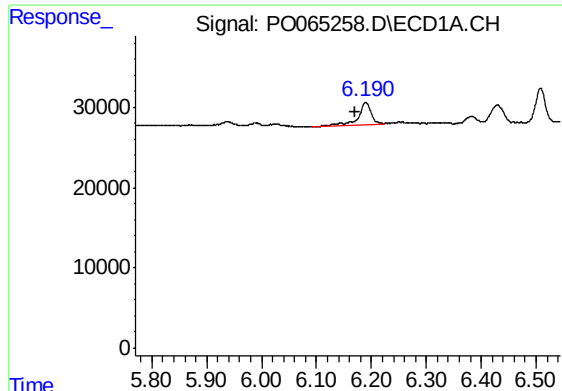

#26 AR-1254-1


R.T.: 6.190 min
Delta R.T.: 0.020 min
Response: 43741
Conc: 33.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

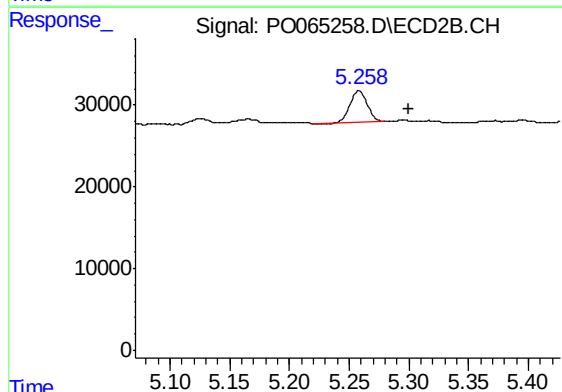


#26 AR-1254-1

R.T.: 5.258 min
Delta R.T.: -0.042 min
Response: 38023
Conc: 16.26 ng/ml

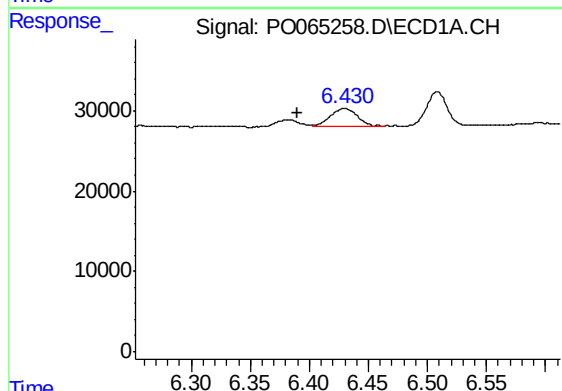


#27 AR-1254-2

R.T.: 6.430 min
Delta R.T.: 0.040 min
Response: 34220
Conc: 16.15 ng/ml

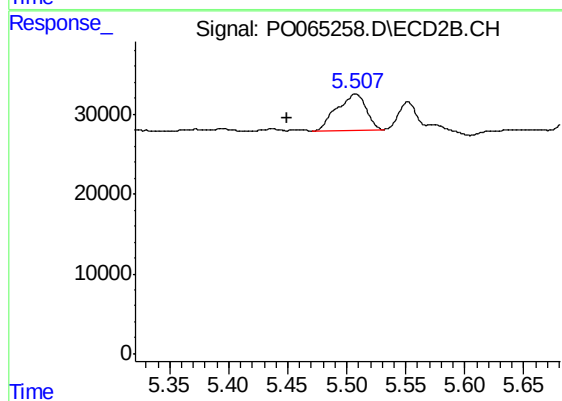

#27 AR-1254-2


R.T.: 5.508 min
Delta R.T.: 0.058 min
Response: 77805
Conc: 36.50 ng/ml

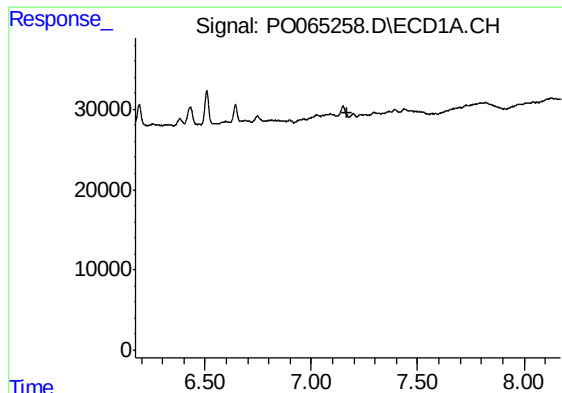

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

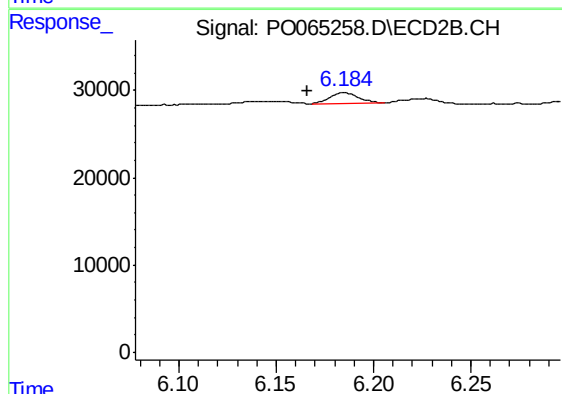


#32 AR-1260-2

R.T.: 6.185 min
Delta R.T.: 0.019 min
Response: 12448
Conc: 4.08 ng/ml

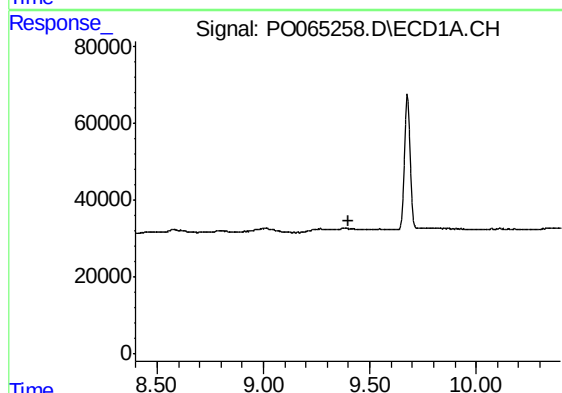

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.397 min
Response: 0
Conc: N.D.

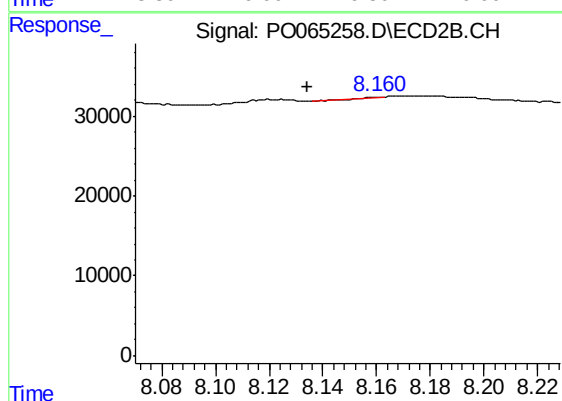

#45 AR-1268-5

R.T.: 8.160 min
Delta R.T.: 0.026 min
Response: 473
Conc: 0.03 ng/ml