

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065217.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2020 11:23
 Operator : AJ/MA
 Sample : K6471-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-123019-0-2-COMP-B1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 13:43:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.177	3.450	686053	834638	32.527	33.038
2)	SA Decachlor...	9.693	8.362	648966	781200	21.266	20.299

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010220\
Data File : PO065217.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2020 11:23
Operator : AJ/MA
Sample : K6471-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 13:43:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

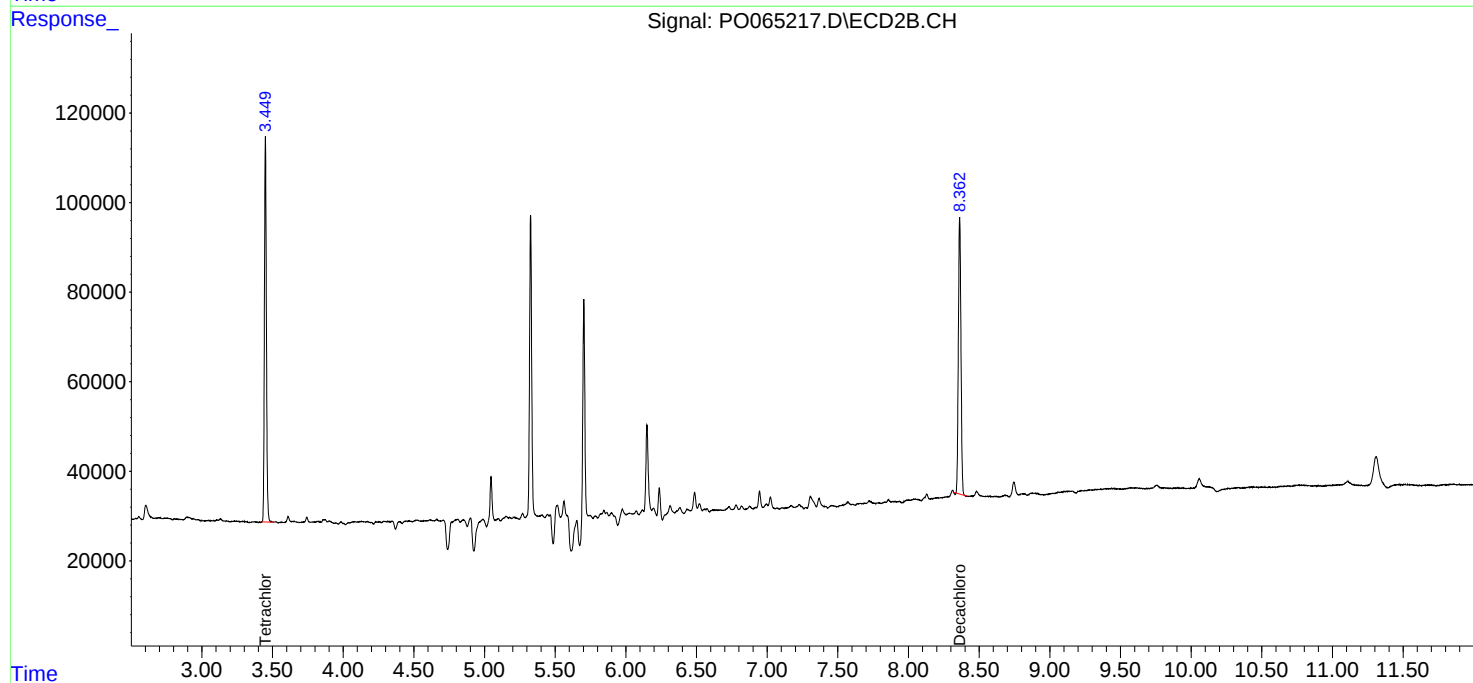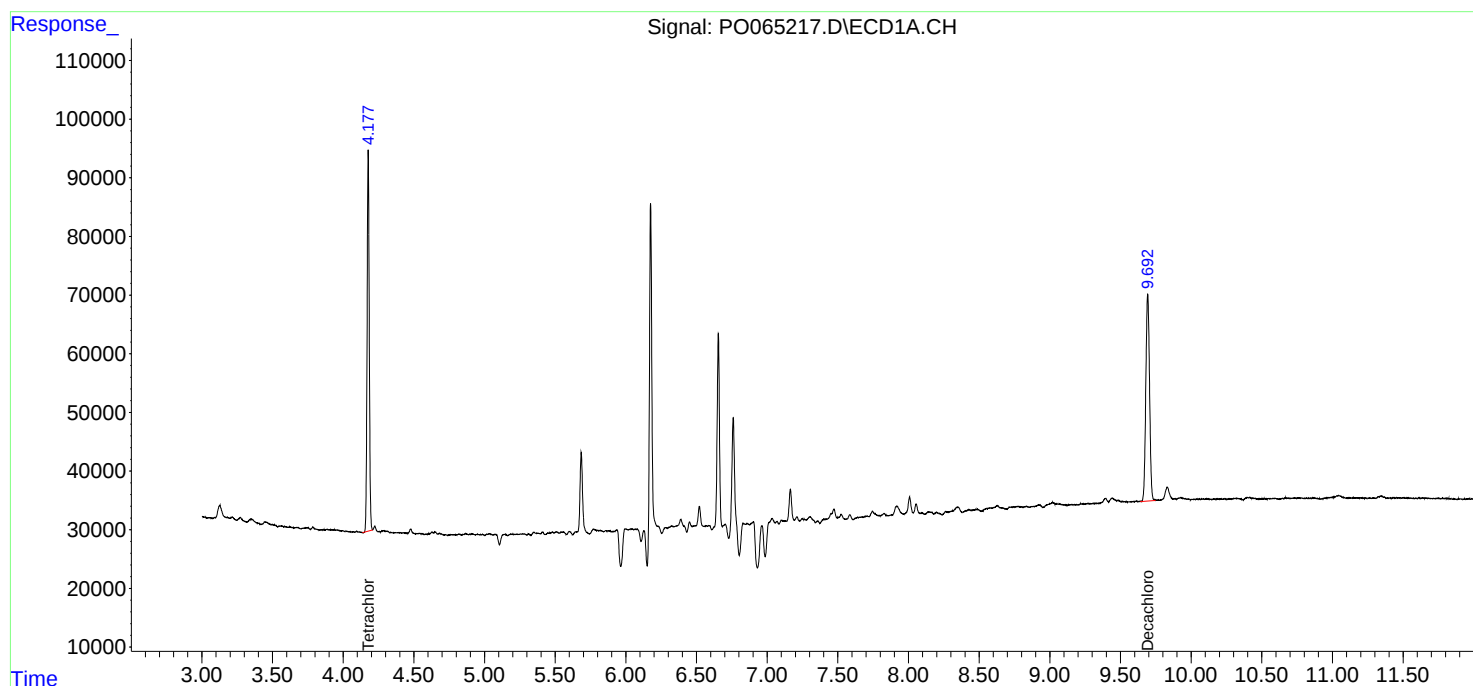


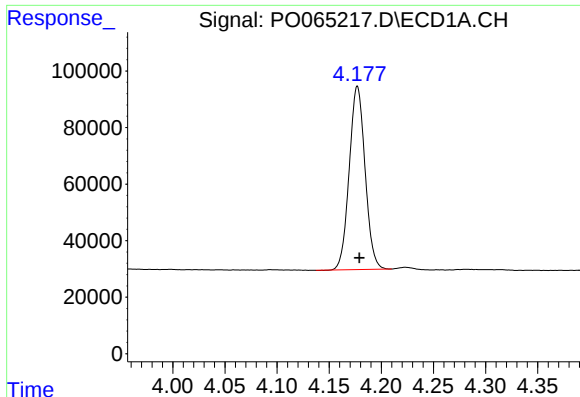

#1 Tetrachloro-m-xylene


R.T.: 4.177 min
Delta R.T.: -0.002 min
Response: 686053
Conc: 32.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B1

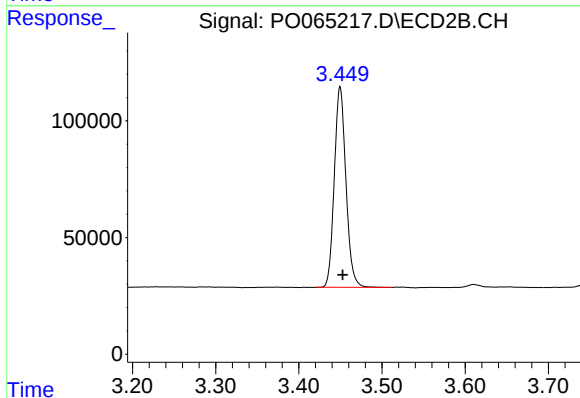


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: -0.003 min
Response: 834638
Conc: 33.04 ng/ml

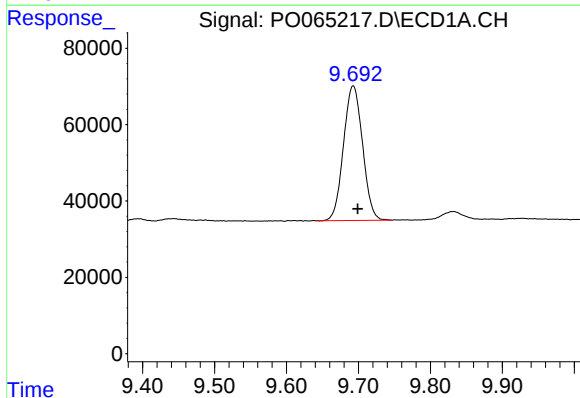

#2 Decachlorobiphenyl

R.T.: 9.693 min
Delta R.T.: -0.006 min
Response: 648966
Conc: 21.27 ng/ml

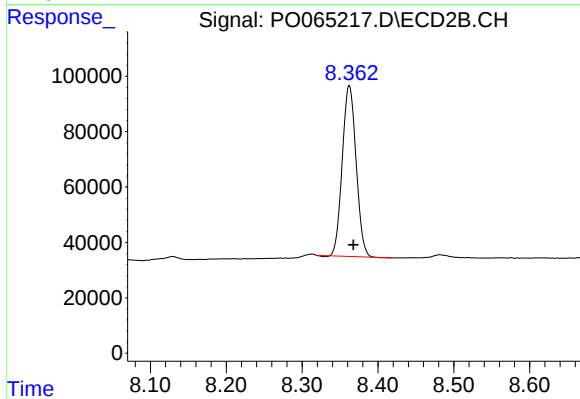

#2 Decachlorobiphenyl

R.T.: 8.362 min
Delta R.T.: -0.005 min
Response: 781200
Conc: 20.30 ng/ml