

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065220.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2020 12:13
 Operator : AJ/MA
 Sample : K6471-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-123019-0-2-COMP-B1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 13:07:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.176	3.450	677112	808013	32.103	31.984
2) SA Decachlor...	9.692	8.362	623237	754771	20.423	19.612

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010220\
Data File : PO065220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2020 12:13
Operator : AJ/MA
Sample : K6471-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 13:07:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

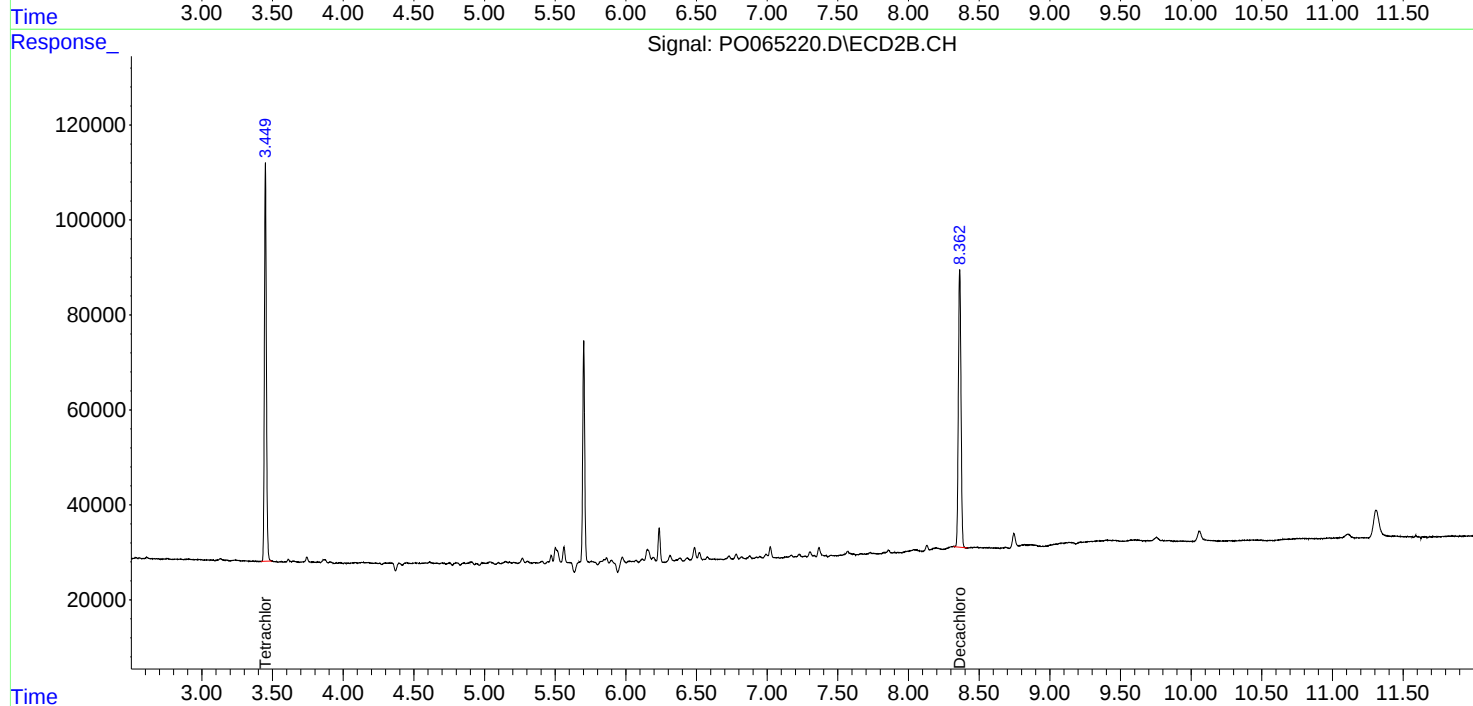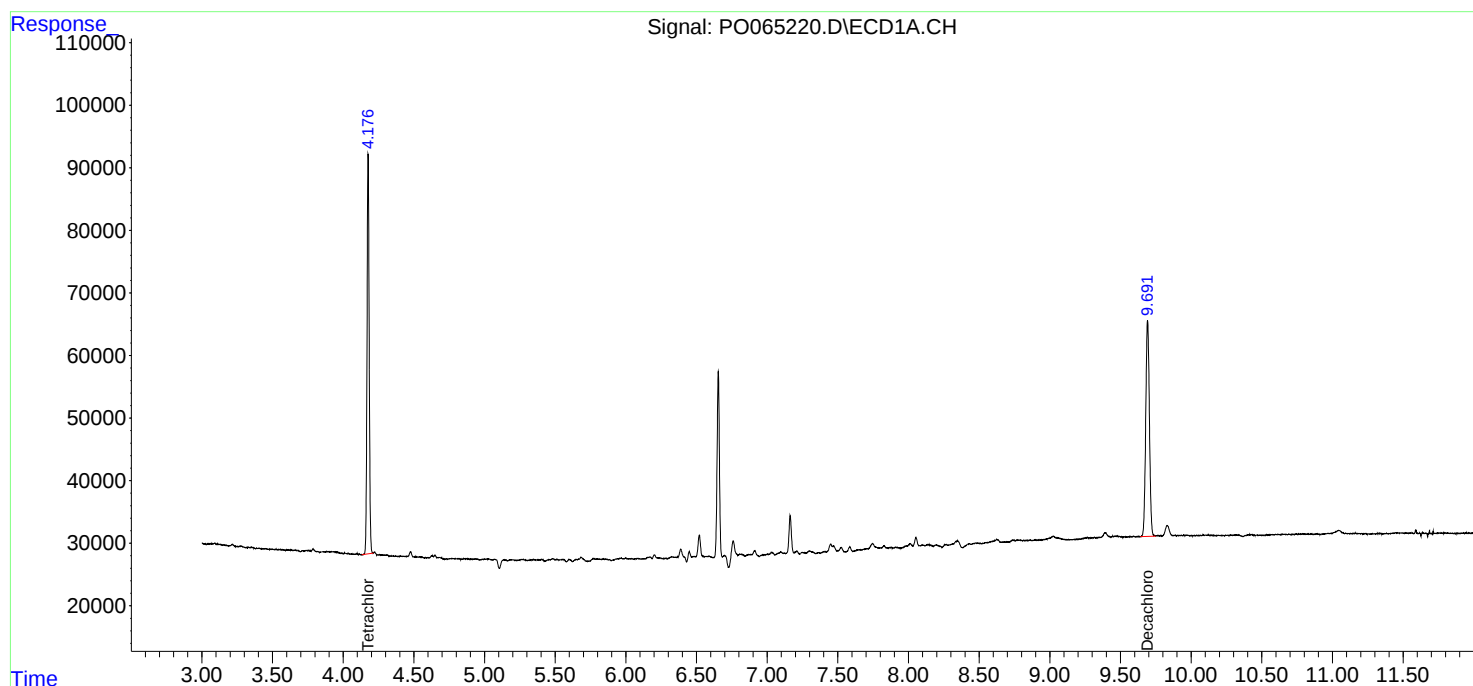


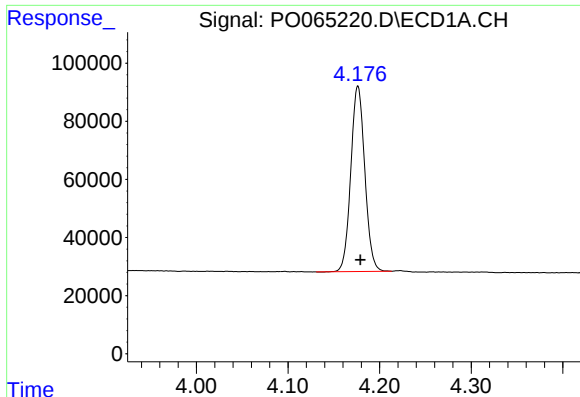

#1 Tetrachloro-m-xylene


R.T.: 4.176 min
Delta R.T.: -0.003 min
Response: 677112
Conc: 32.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MC-123019-0-2-COMP-B1

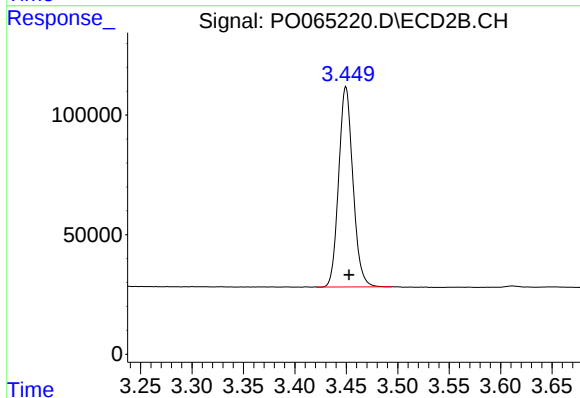


#1 Tetrachloro-m-xylene

R.T.: 3.450 min
Delta R.T.: -0.003 min
Response: 808013
Conc: 31.98 ng/ml

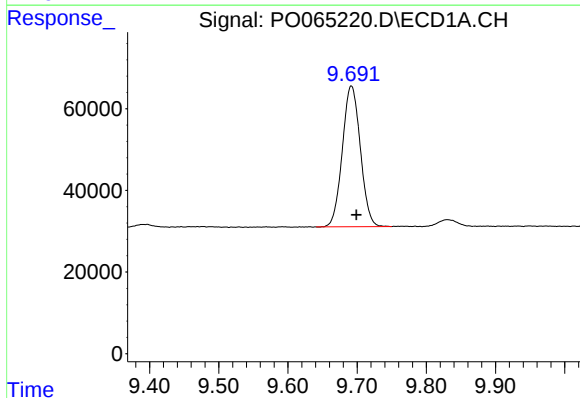

#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: -0.007 min
Response: 623237
Conc: 20.42 ng/ml

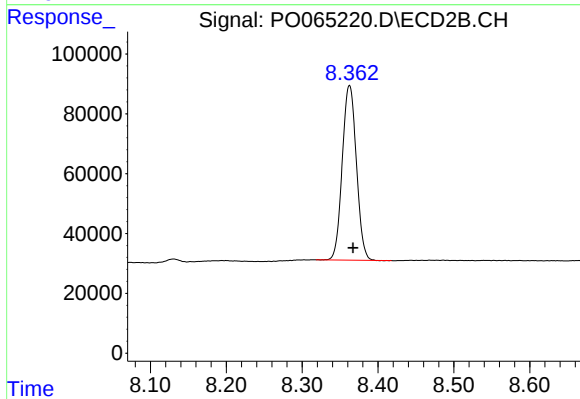

#2 Decachlorobiphenyl

R.T.: 8.362 min
Delta R.T.: -0.005 min
Response: 754771
Conc: 19.61 ng/ml