

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2020 13:36
 Operator : AJ/MA
 Sample : K6480-01 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-16

Manual Integrations
 APPROVED

mohammad
 1/3/2020 10:15:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 14:06:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.169	3.448	303234	200175	14.377m	7.924m#
2) SA Decachlor...	9.695	8.363	188086	145052	6.163	3.769m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010220\
Data File : PO065225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2020 13:36
Operator : AJ/MA
Sample : K6480-01 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-16


Manual Integrations
APPROVED

mohammad
1/3/2020 10:15:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 14:06:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

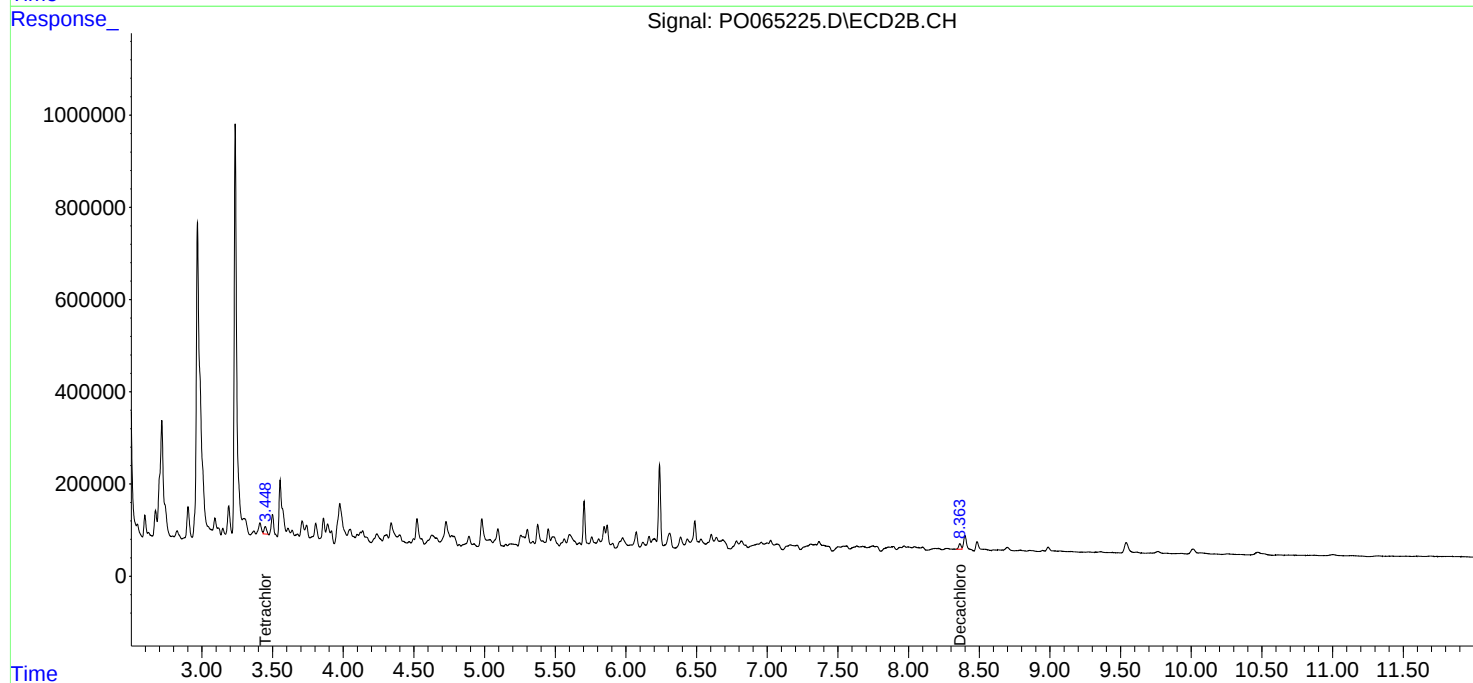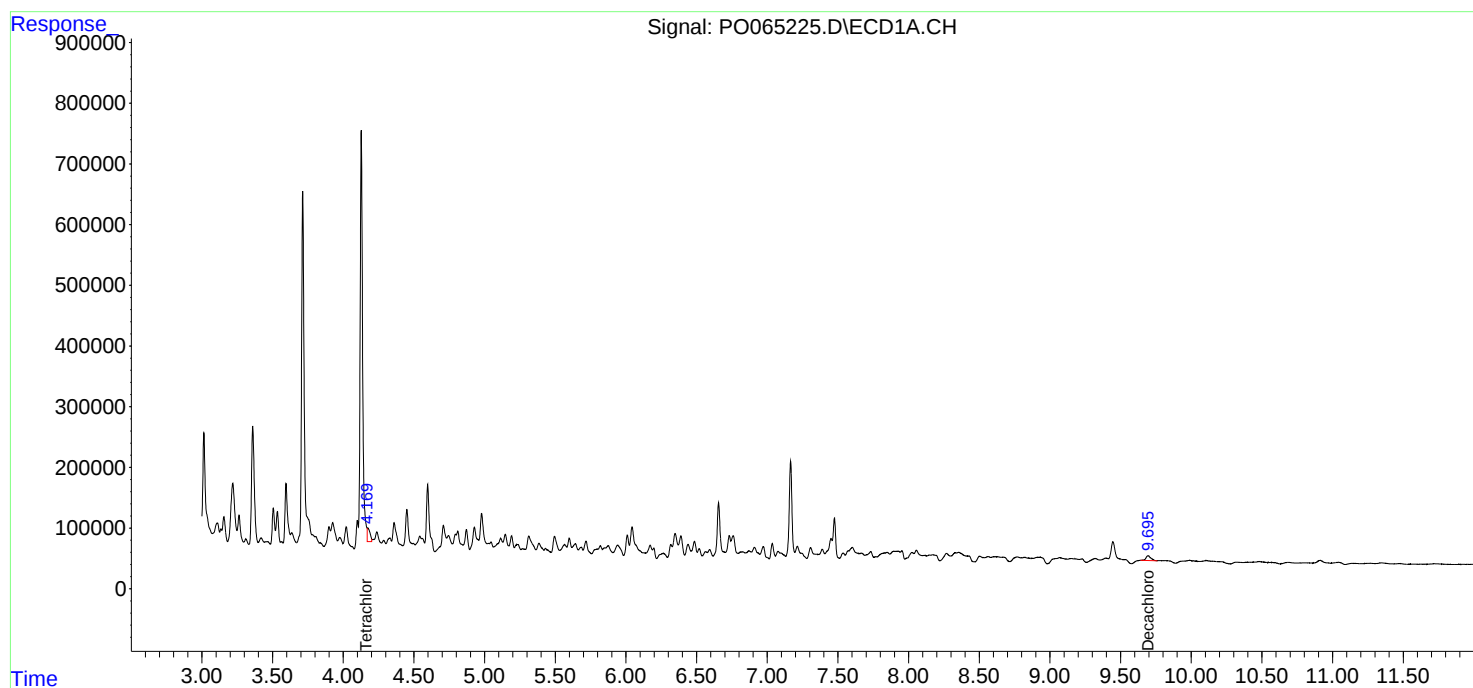

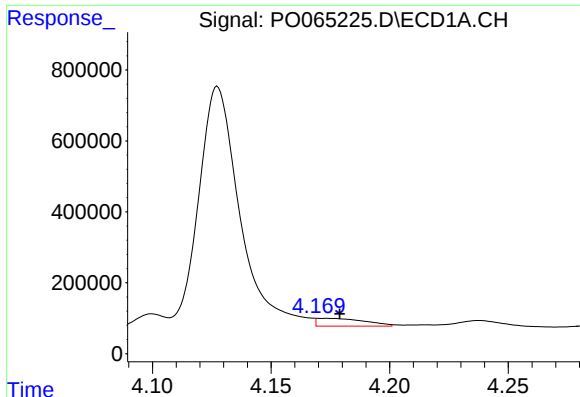


#1 Tetrachloro-m-xylene

R.T.: 4.169 min
Delta R.T.: -0.010 min
Response: 303234
Conc: 14.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-16


Manual Integrations
APPROVED

mohammad
1/3/2020 10:15:10 AM

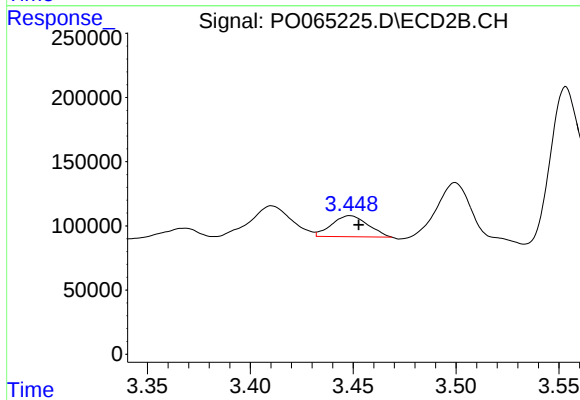


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: -0.005 min
Response: 200175
Conc: 7.92 ng/ml m

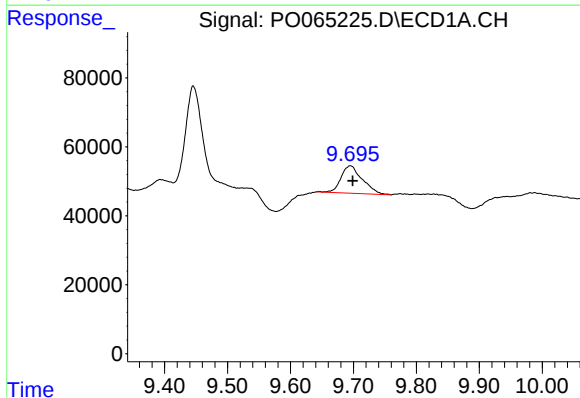

#2 Decachlorobiphenyl

R.T.: 9.695 min
Delta R.T.: -0.004 min
Response: 188086
Conc: 6.16 ng/ml

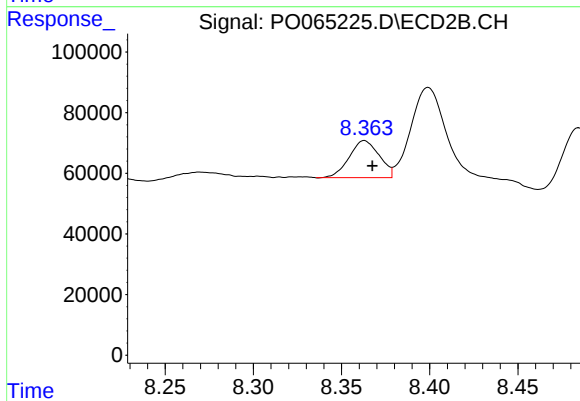

#2 Decachlorobiphenyl

R.T.: 8.363 min
Delta R.T.: -0.005 min
Response: 145052
Conc: 3.77 ng/ml m