

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065229.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2020 14:43
 Operator : AJ/MA
 Sample : K6484-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40121

Manual Integrations
 APPROVED

mohammad
 1/3/2020 10:15:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 14:57:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.177	3.451	787934	1159893	37.357m	45.913
2) SA Decachlor...	9.693	8.364	425421	484842	13.940	12.598

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
Data File : P0065229.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2020 14:43
Operator : AJ/MA
Sample : K6484-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40121


Manual Integrations
APPROVED

mohammad
1/3/2020 10:15:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 14:57:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

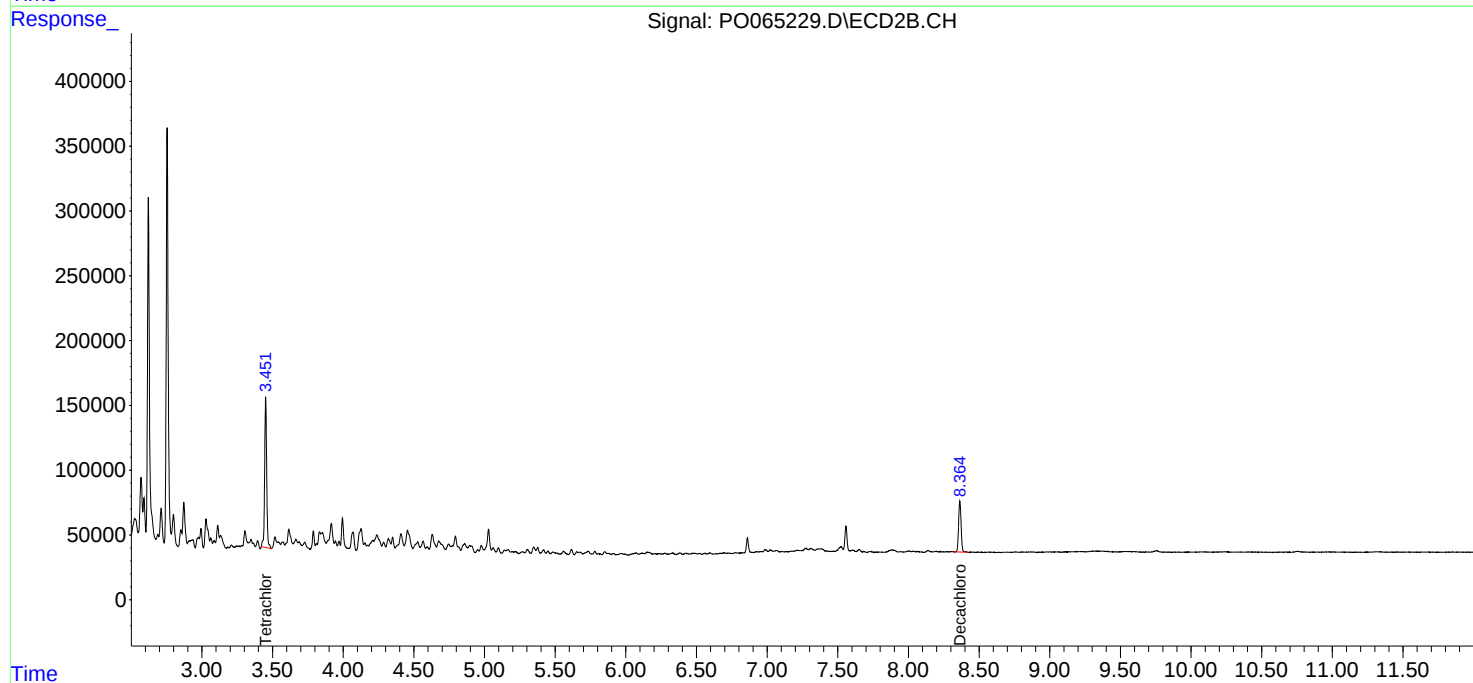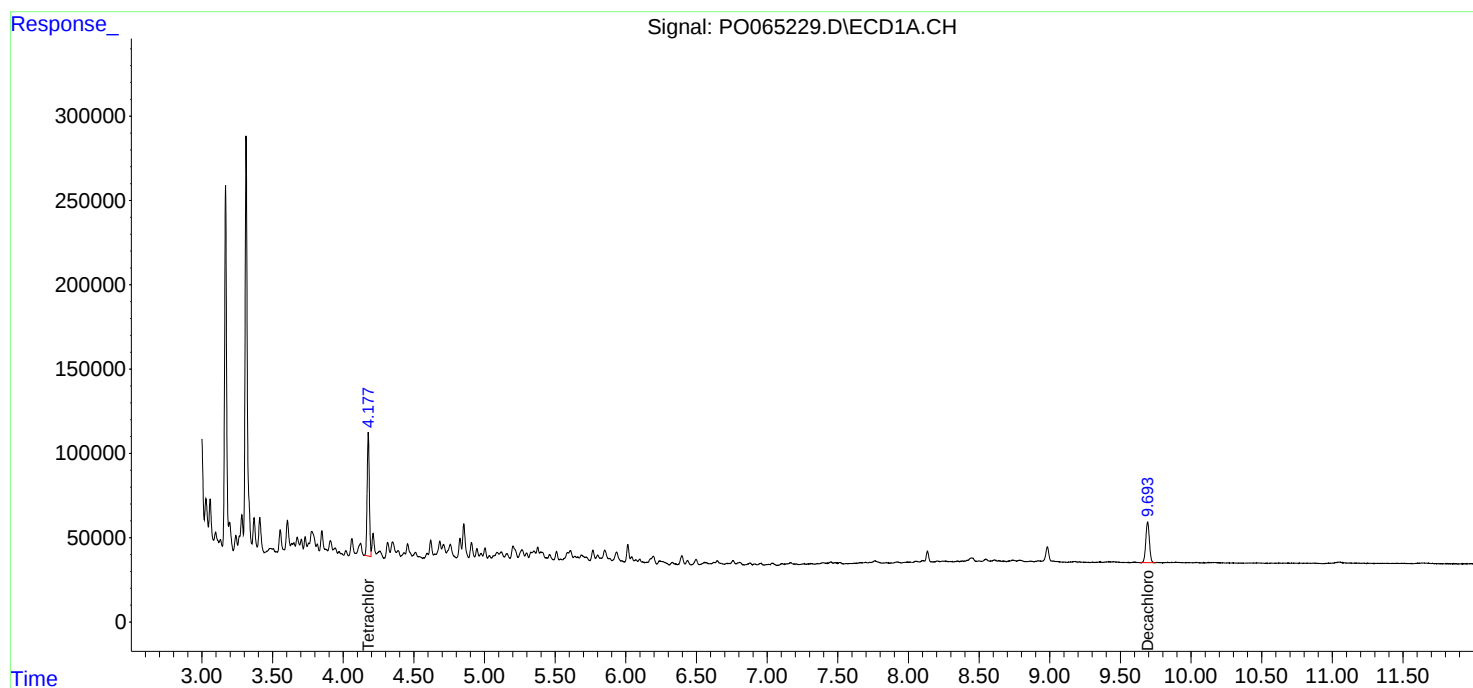

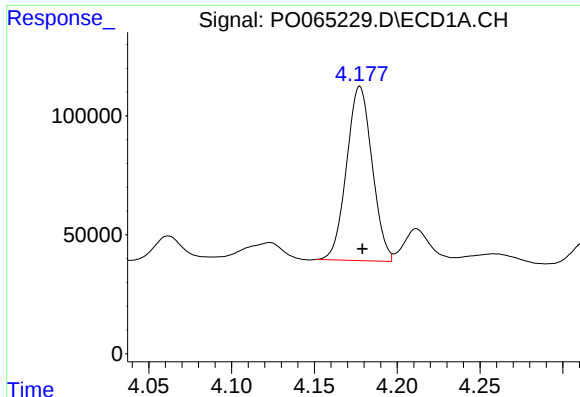

#1 Tetrachloro-m-xylene

R.T.: 4.177 min

Delta R.T.: -0.002 min


Response: 787934

Conc: 37.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40121

Manual Integrations
APPROVED

mohammad
1/3/2020 10:15:18 AM

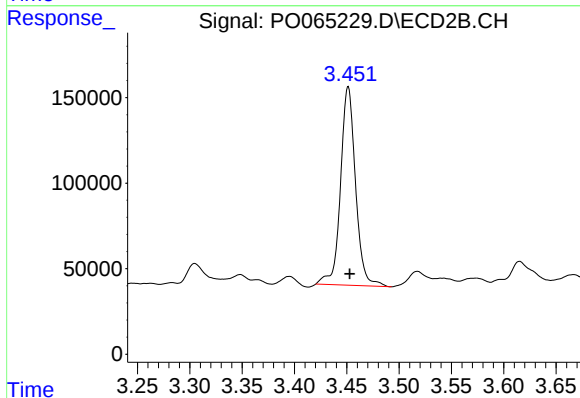


#1 Tetrachloro-m-xylene

R.T.: 3.451 min

Delta R.T.: -0.001 min

Response: 1159893

Conc: 45.91 ng/ml

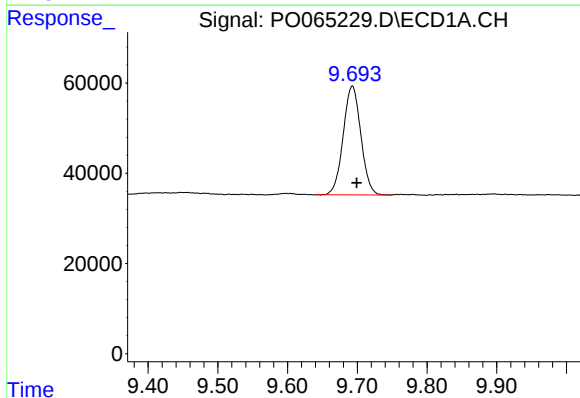


#2 Decachlorobiphenyl

R.T.: 9.693 min

Delta R.T.: -0.006 min

Response: 425421

Conc: 13.94 ng/ml

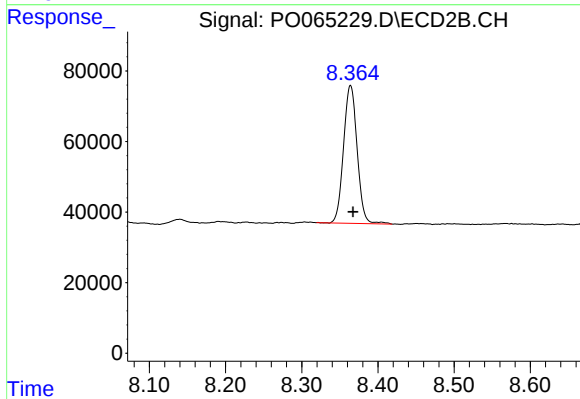

#2 Decachlorobiphenyl

R.T.: 8.364 min

Delta R.T.: -0.003 min

Response: 484842

Conc: 12.60 ng/ml