

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010220\
 Data File : P0065249.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2020 21:38
 Operator : AJ/MA
 Sample : K6482-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-123119-2-5-COMP-B6

Manual Integrations
 APPROVED

mohammad
 1/3/2020 10:16:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 22:26:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.166	3.441	634639	816420	30.089m	32.317
2) SA Decachlor...	9.676	8.353	635372	744804	20.820	19.353

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010220\
Data File : PO065249.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2020 21:38
Operator : AJ/MA
Sample : K6482-04
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MC-123119-2-5-COMP-B6


Manual Integrations
APPROVED

mohammad
1/3/2020 10:16:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 22:26:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

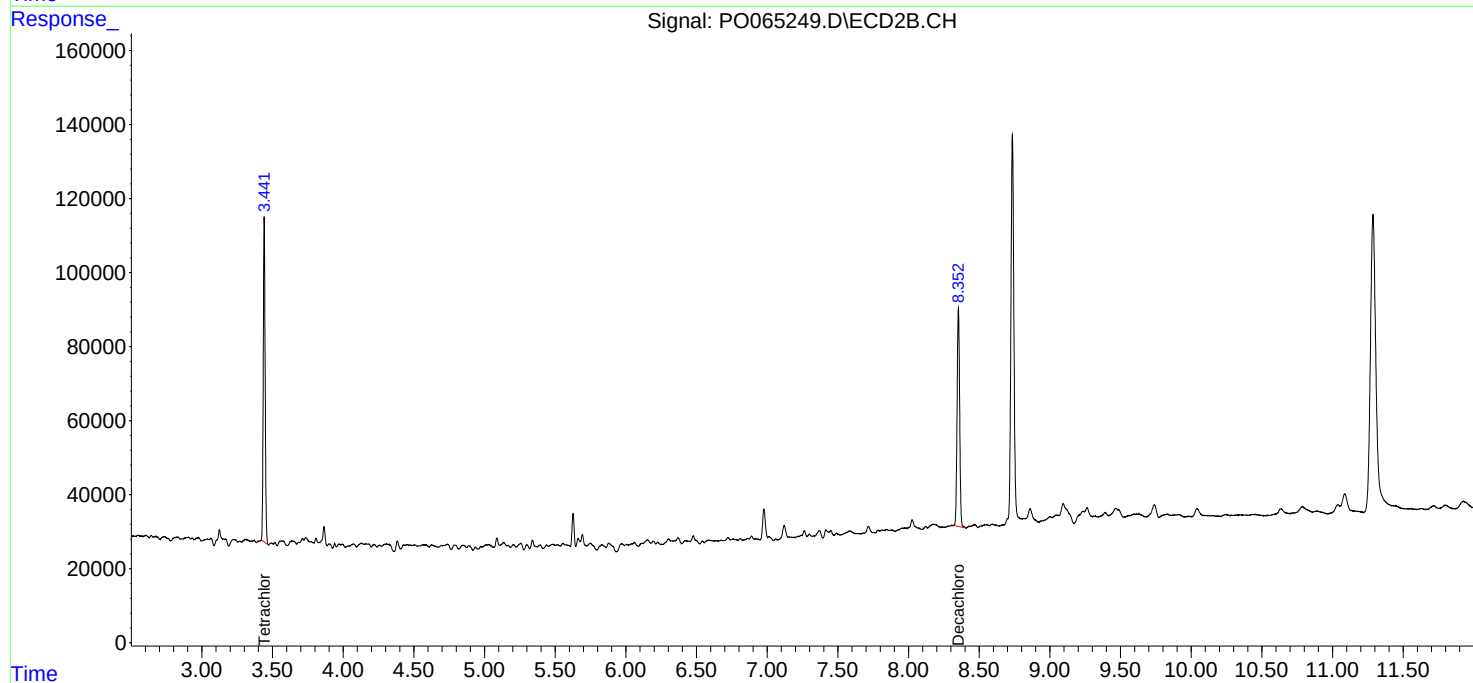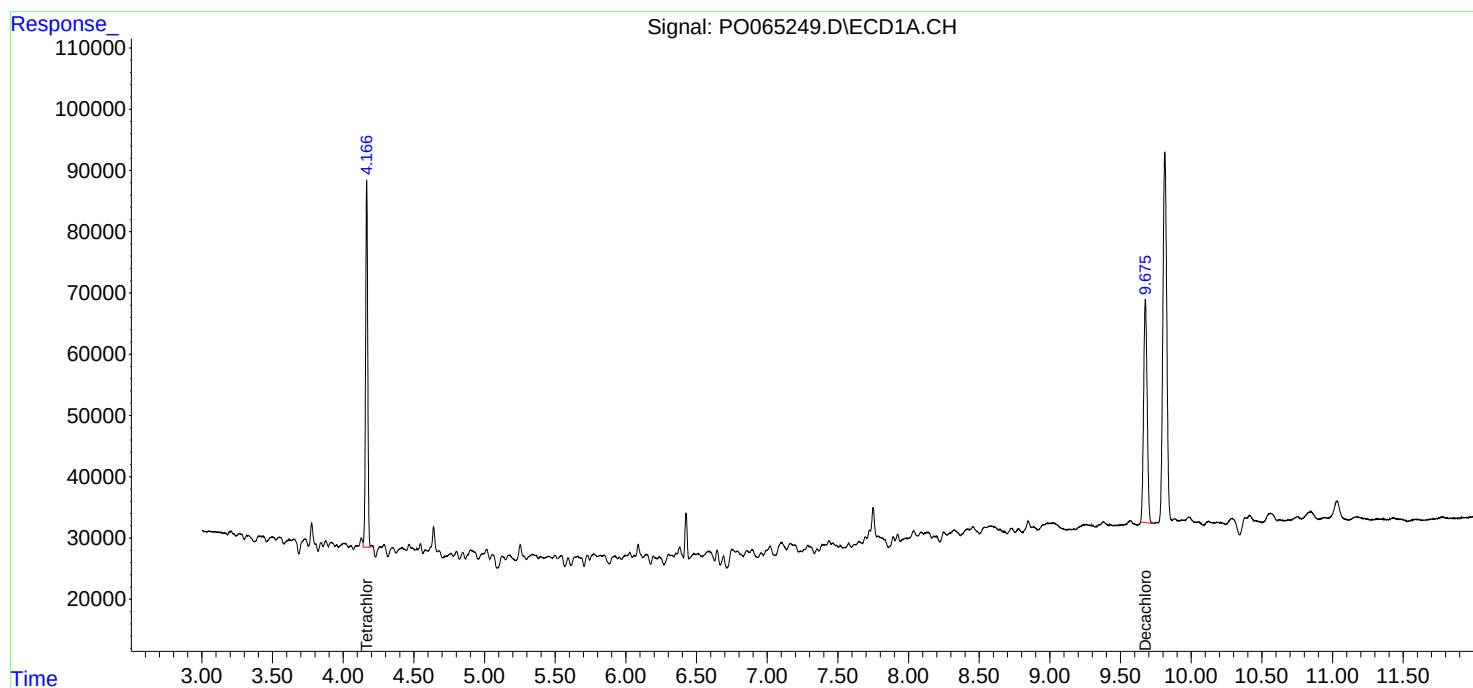

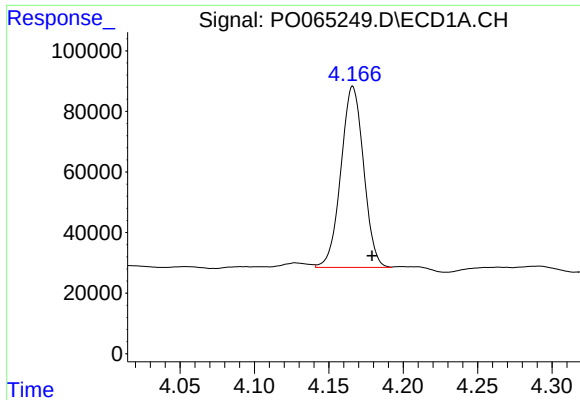


#1 Tetrachloro-m-xylene

R.T.: 4.166 min
Delta R.T.: -0.013 min
Response: 634639
Conc: 30.09 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MC-123119-2-5-COMP-B6


Manual Integrations
APPROVED

mohammad
1/3/2020 10:16:03 AM

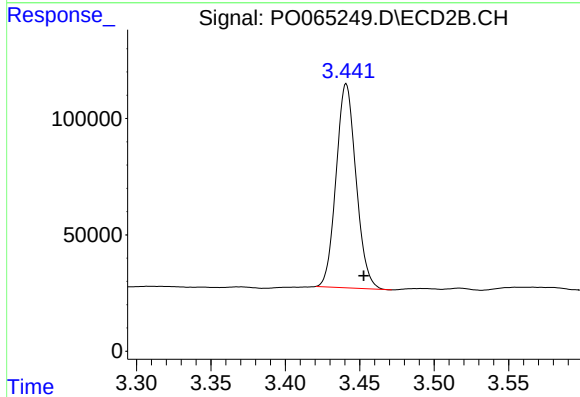


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: -0.012 min
Response: 816420
Conc: 32.32 ng/ml

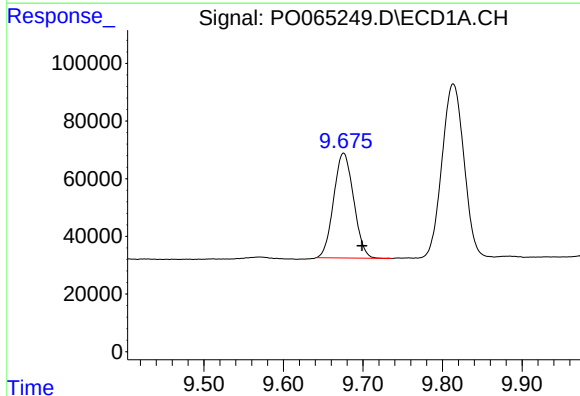

#2 Decachlorobiphenyl

R.T.: 9.676 min
Delta R.T.: -0.023 min
Response: 635372
Conc: 20.82 ng/ml

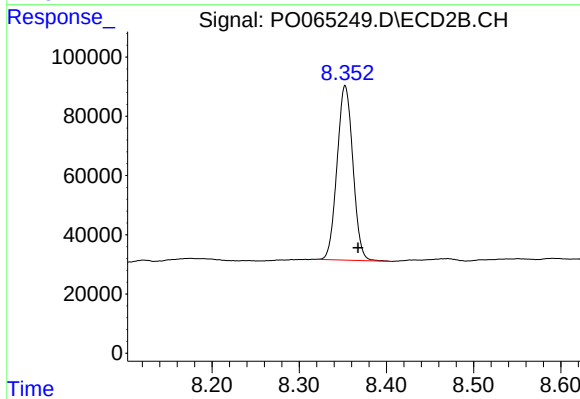

#2 Decachlorobiphenyl

R.T.: 8.353 min
Delta R.T.: -0.015 min
Response: 744804
Conc: 19.35 ng/ml