

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
 Data File : P0053148.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2019 15:18
 Operator : SM/SJ
 Sample : J6498-06RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1218-S-AB-6RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:15:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.188	3.213	11133807	1756701	8.509	7.829
2) SA Decachlor...	9.663	7.864	5554557	1818519	7.010	7.074

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
Data File : P0053148.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 15:18
Operator : SM/SJ
Sample : J6498-06RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-AB-6RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:15:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

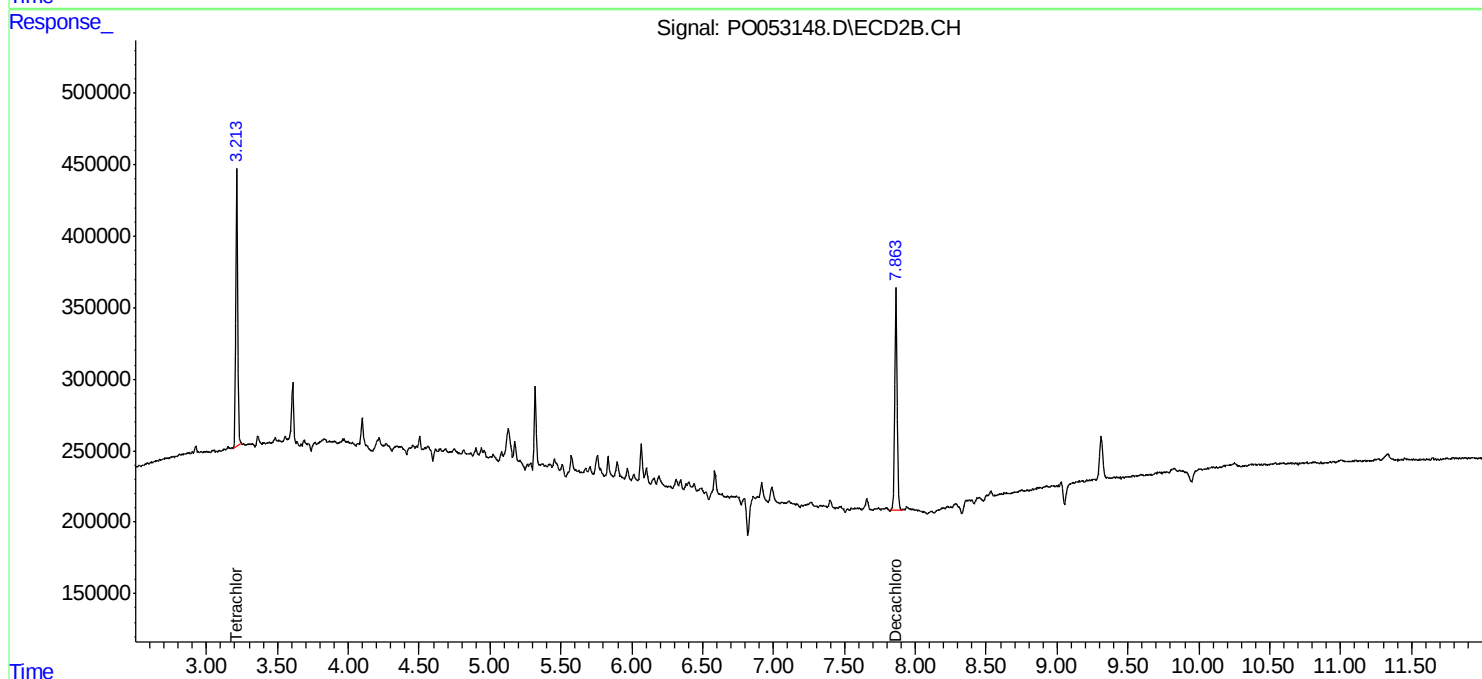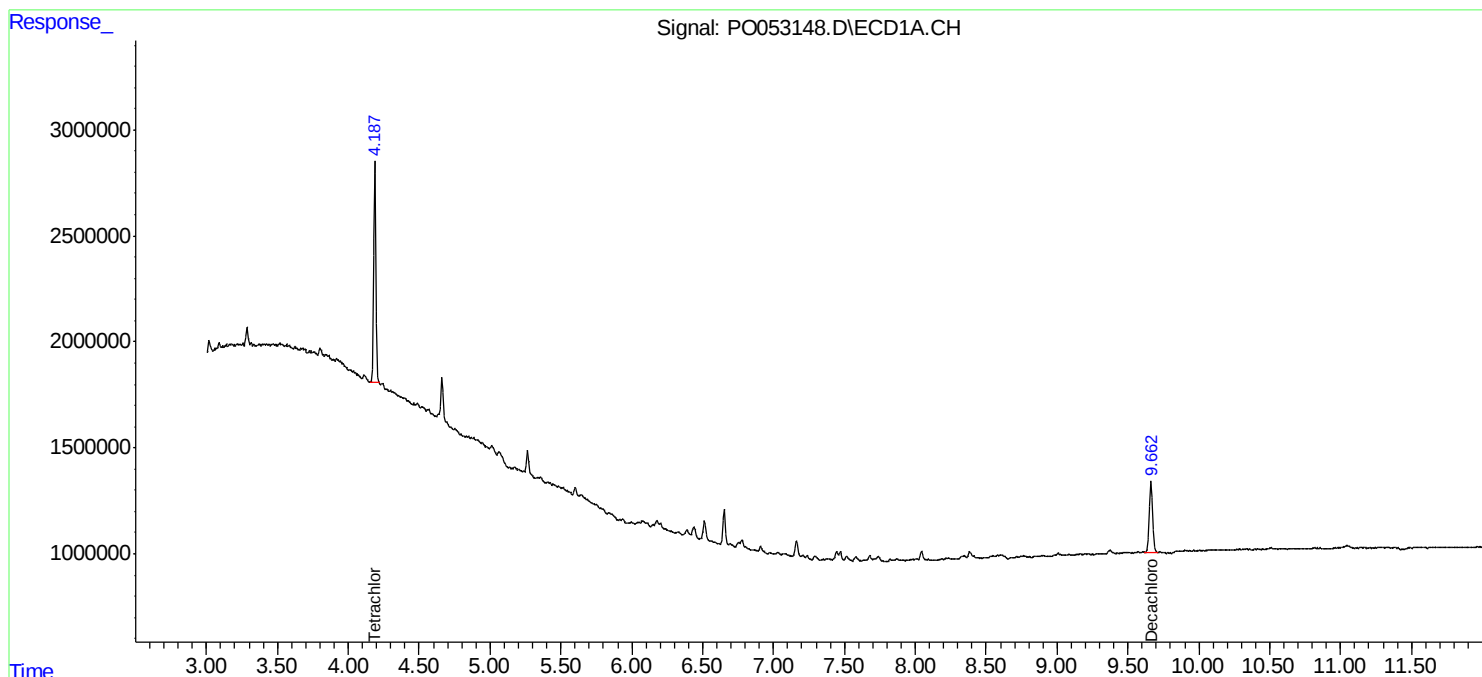


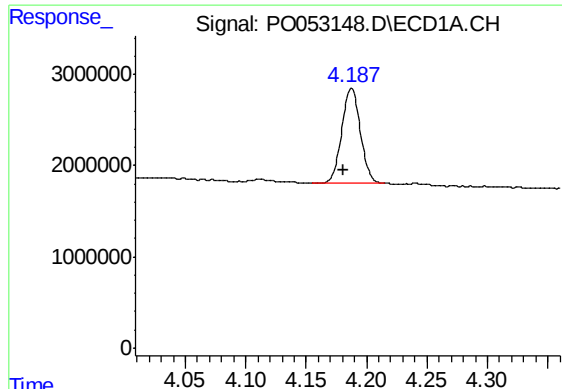

#1 Tetrachloro-m-xylene


R.T.: 4.188 min
Delta R.T.: 0.007 min
Response: 11133807
Conc: 8.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-AB-6RE

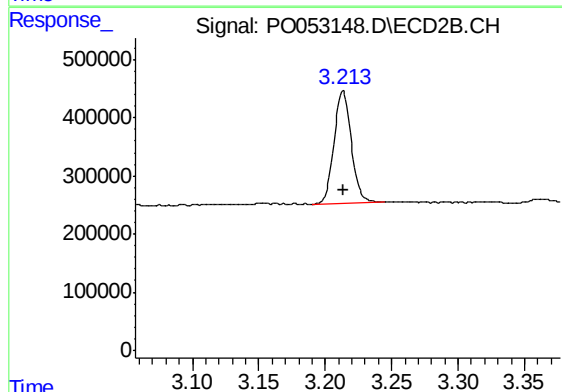


#1 Tetrachloro-m-xylene

R.T.: 3.213 min
Delta R.T.: 0.000 min
Response: 1756701
Conc: 7.83 ng/ml

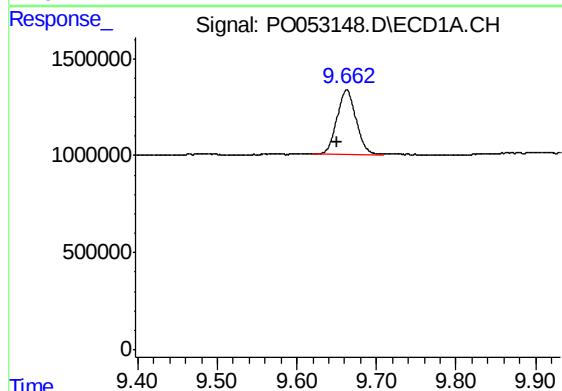

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: 0.012 min
Response: 5554557
Conc: 7.01 ng/ml

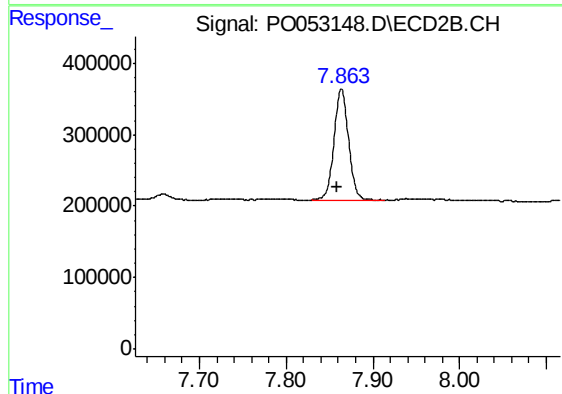

#2 Decachlorobiphenyl

R.T.: 7.864 min
Delta R.T.: 0.005 min
Response: 1818519
Conc: 7.07 ng/ml