

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
Data File : P0053157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 17:50
Operator : SM/SJ
Sample : K1002-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-05-010219-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:19:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.181	3.214	26281047	4538458	20.086	20.226
2) SA Decachlor...	9.652	7.860	8677858	2218197	10.952	8.629

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
Data File : P0053157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 17:50
Operator : SM/SJ
Sample : K1002-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-05-010219-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:19:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

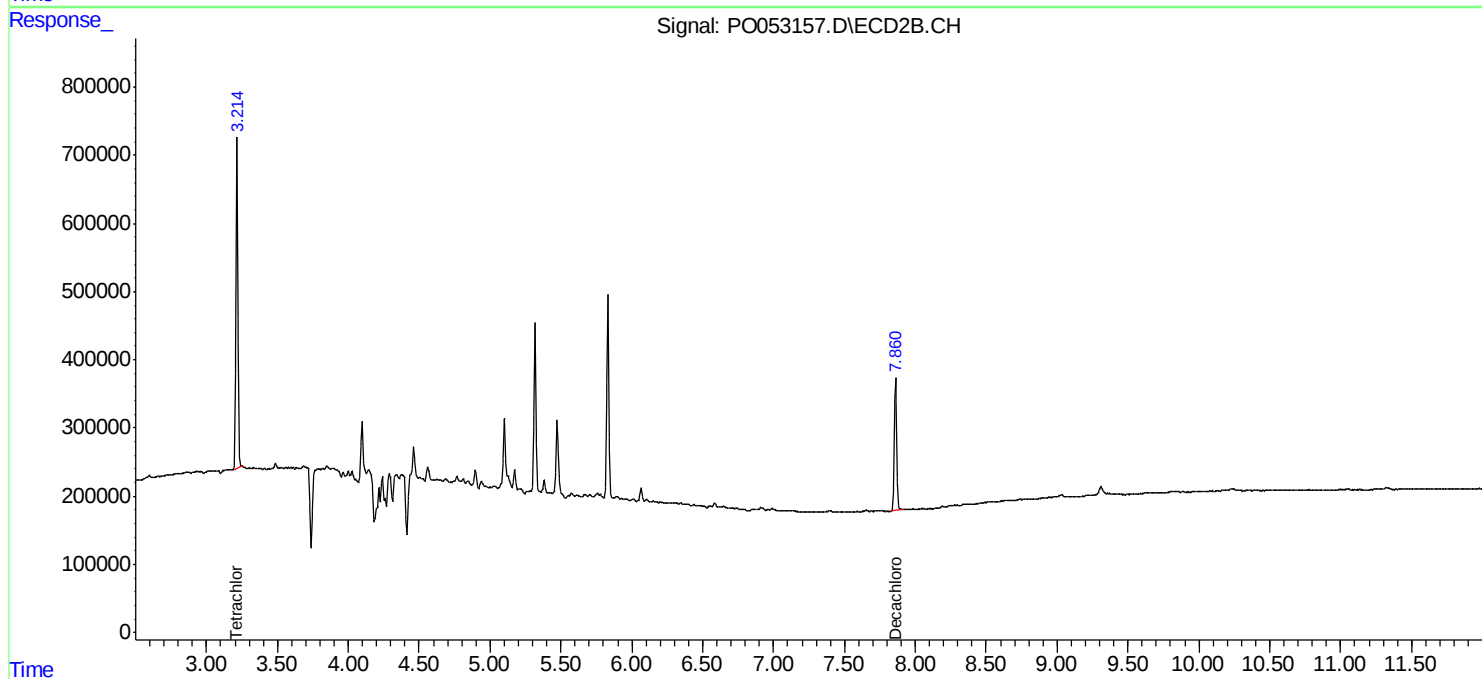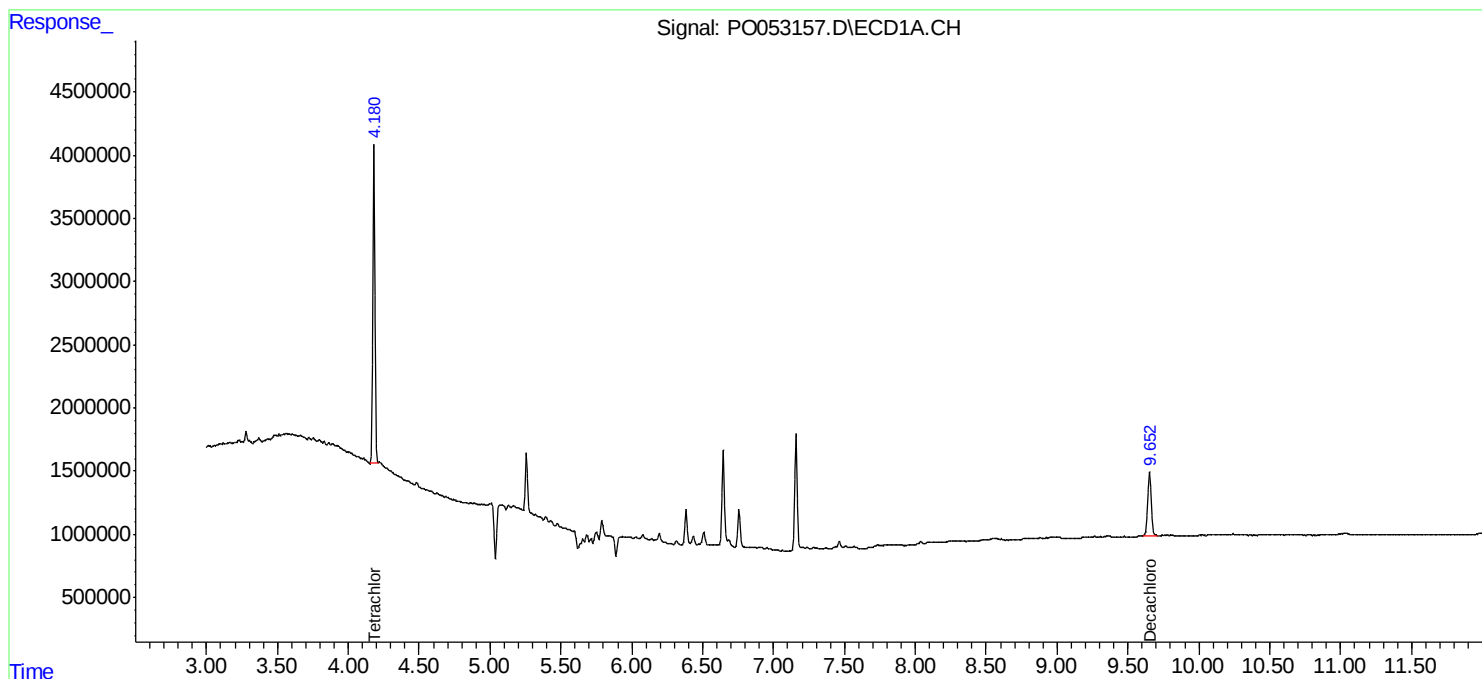


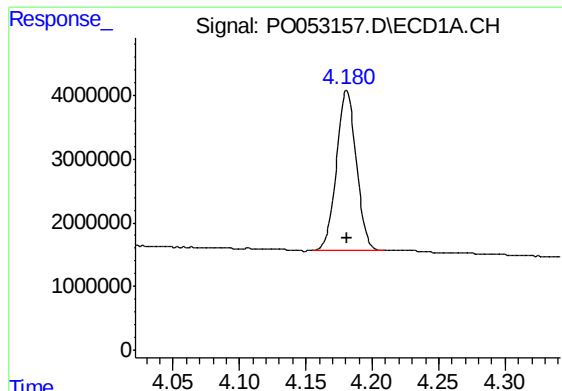

#1 Tetrachloro-m-xylene


R.T.: 4.181 min
Delta R.T.: 0.000 min
Response: 26281047
Conc: 20.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-010219-C

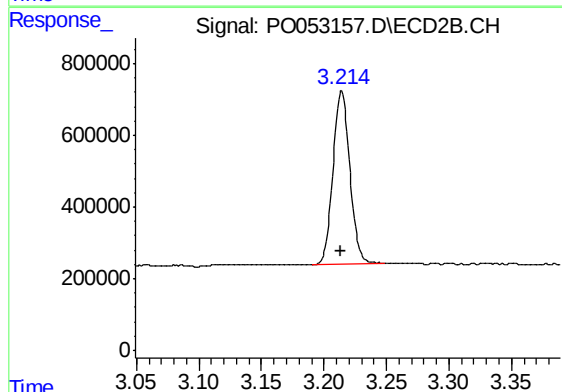


#1 Tetrachloro-m-xylene

R.T.: 3.214 min
Delta R.T.: 0.000 min
Response: 4538458
Conc: 20.23 ng/ml

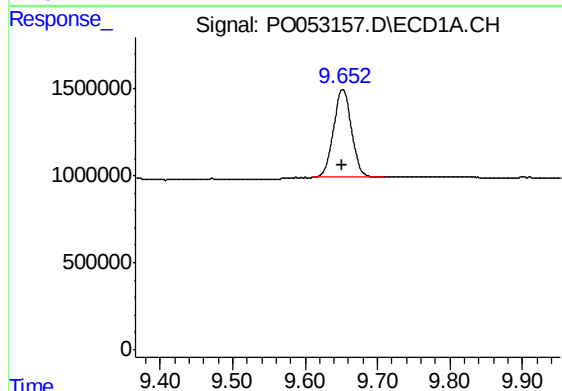

#2 Decachlorobiphenyl

R.T.: 9.652 min
Delta R.T.: 0.002 min
Response: 8677858
Conc: 10.95 ng/ml

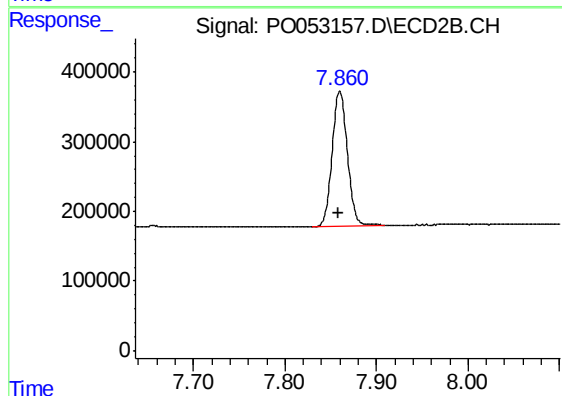

#2 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: 0.001 min
Response: 2218197
Conc: 8.63 ng/ml