

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
 Data File : P0053158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2019 18:07
 Operator : SM/SJ
 Sample : K1002-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-010219-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:19:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.214	26227026	4170383	20.045	18.585
2) SA Decachlor...	9.651	7.859	8013156	2127309	10.114	8.276

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
Data File : P0053158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 18:07
Operator : SM/SJ
Sample : K1002-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-05-010219-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:19:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

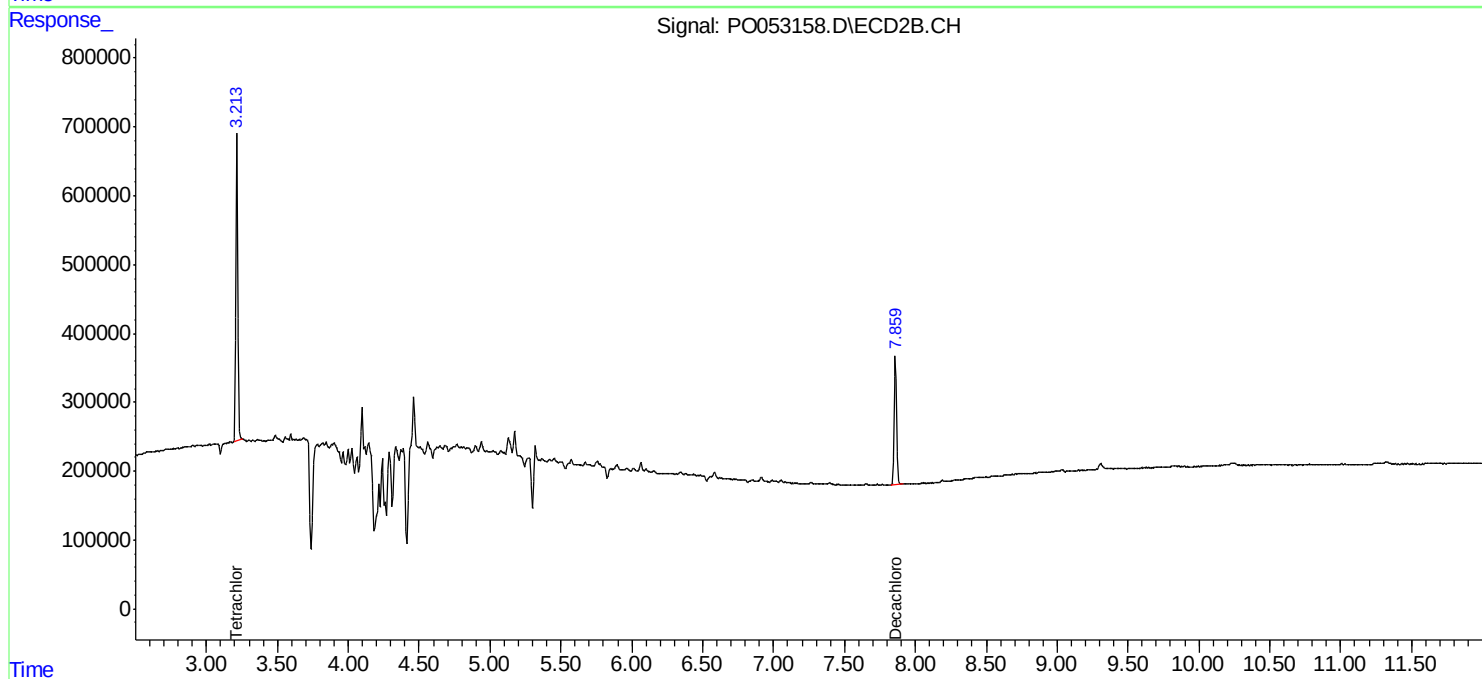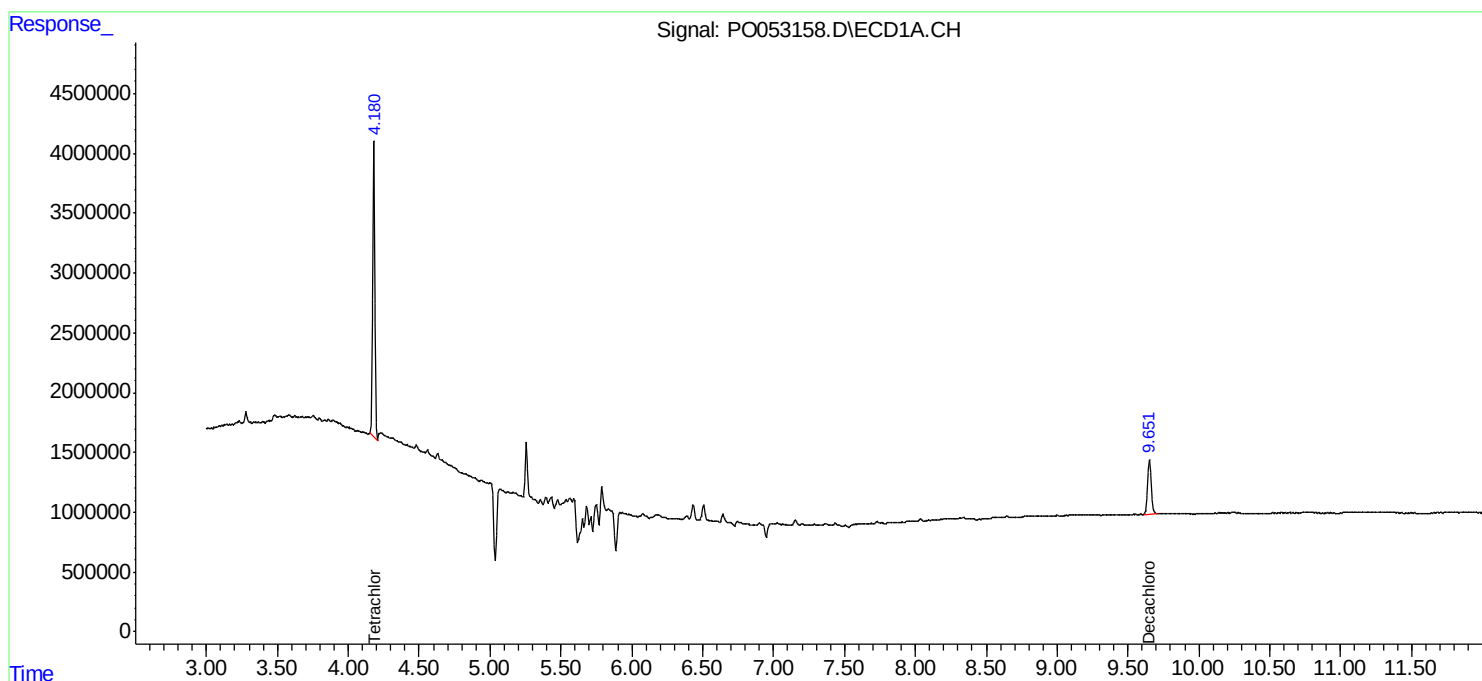


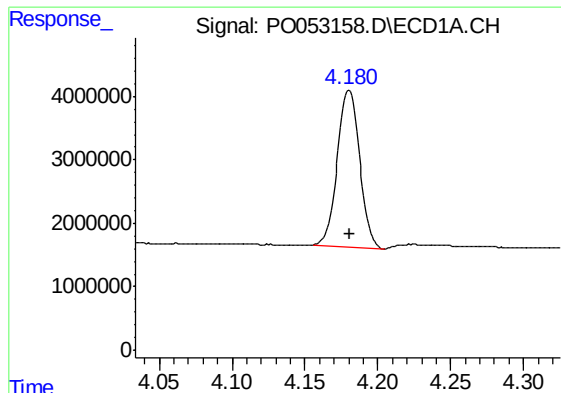

#1 Tetrachloro-m-xylene


R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 26227026
Conc: 20.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-010219-D

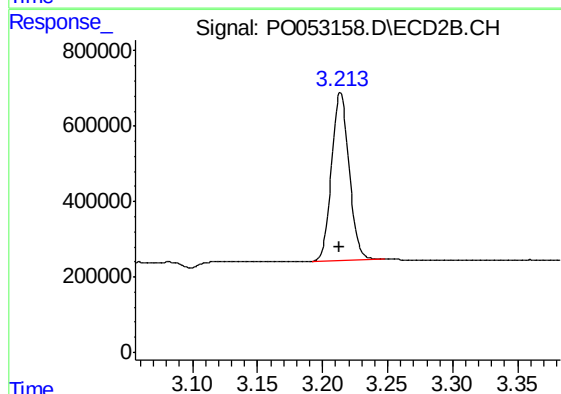


#1 Tetrachloro-m-xylene

R.T.: 3.214 min
Delta R.T.: 0.000 min
Response: 4170383
Conc: 18.59 ng/ml

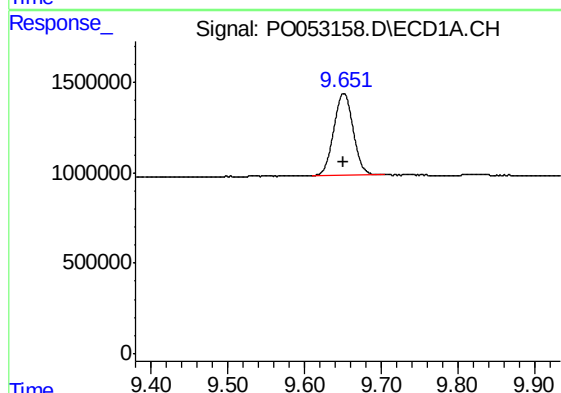

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: 0.000 min
Response: 8013156
Conc: 10.11 ng/ml

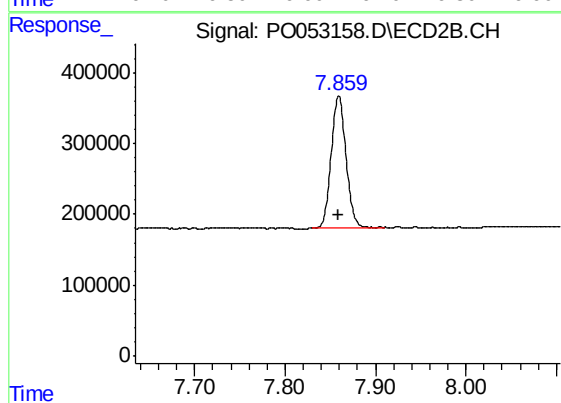

#2 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: 0.000 min
Response: 2127309
Conc: 8.28 ng/ml