

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
 Data File : P0053168.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2019 21:13
 Operator : SM/SJ
 Sample : K1019-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT-D-11-12-A

Manual Integrations
 APPROVED

Sohil
 1/4/2019 9:24:26 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:24:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.179	3.213	31156450	4902616	23.812	21.848
2)	SA Decachlor...	9.651	7.859	13135053	4138531	16.578	16.099

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010319\
Data File : P0053168.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2019 21:13
Operator : SM/SJ
Sample : K1019-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TEST-PIT-D-11-12-A


Manual Integrations
APPROVED

Sohil
1/4/2019 9:24:26 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:24:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

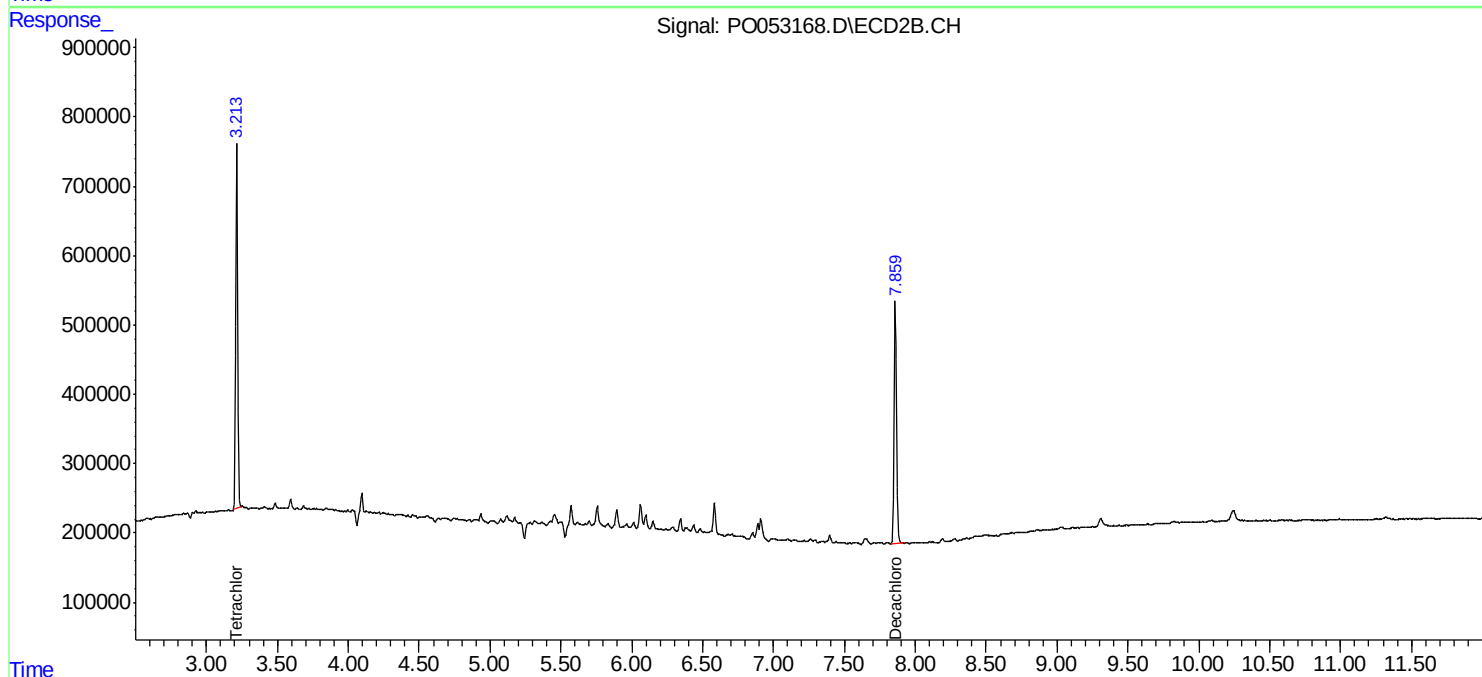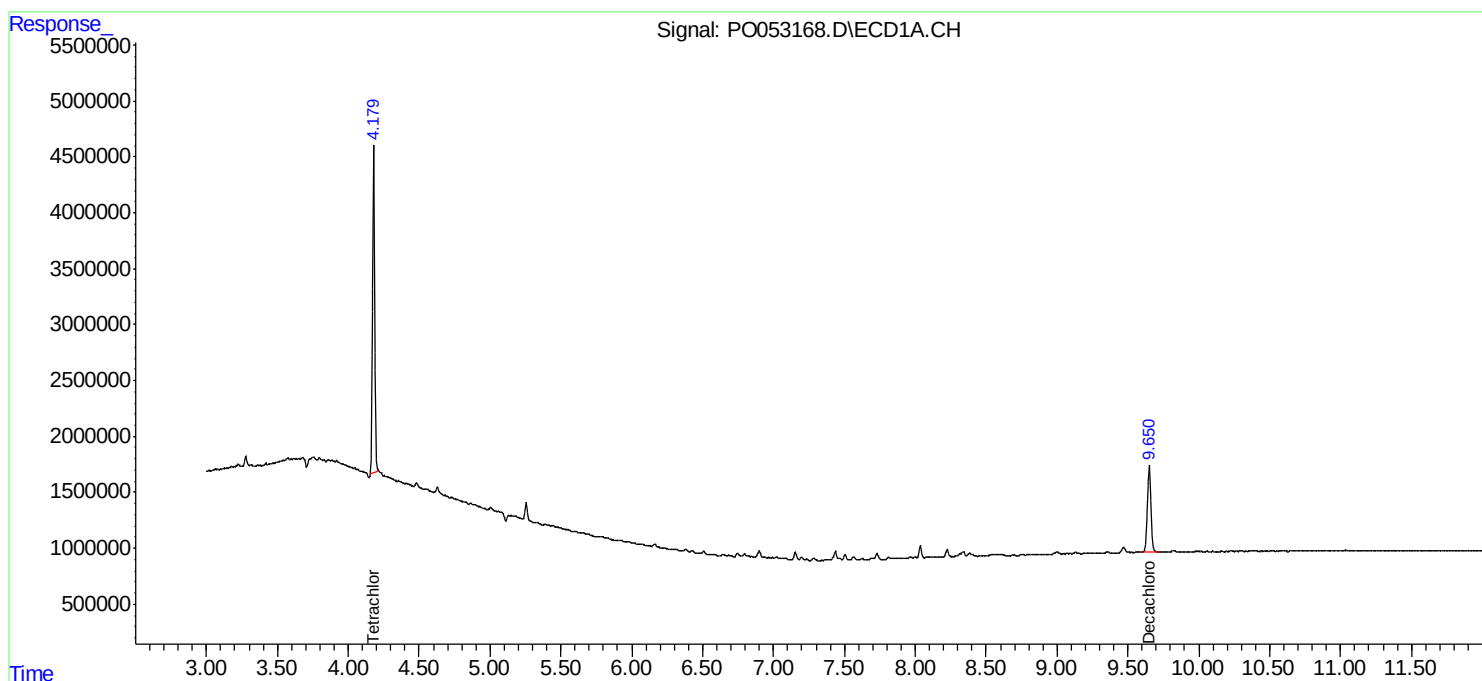

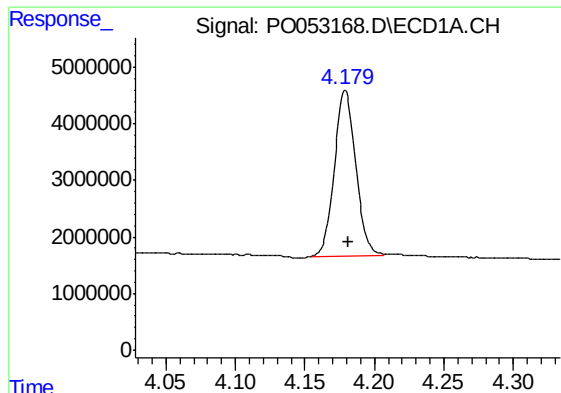


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: -0.002 min
Response: 31156450
Conc: 23.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-D-11-12-A


Manual Integrations
APPROVED

Sohil
1/4/2019 9:24:26 AM

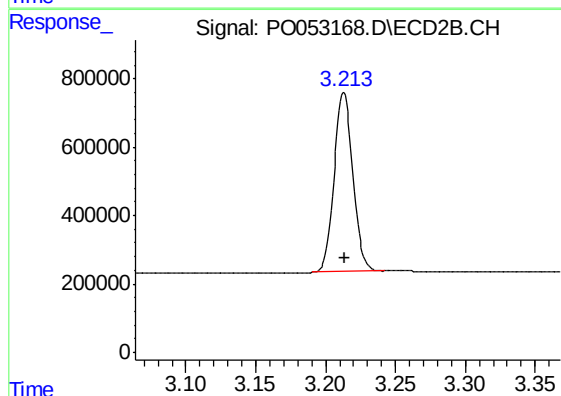


#1 Tetrachloro-m-xylene

R.T.: 3.213 min
Delta R.T.: 0.000 min
Response: 4902616
Conc: 21.85 ng/ml

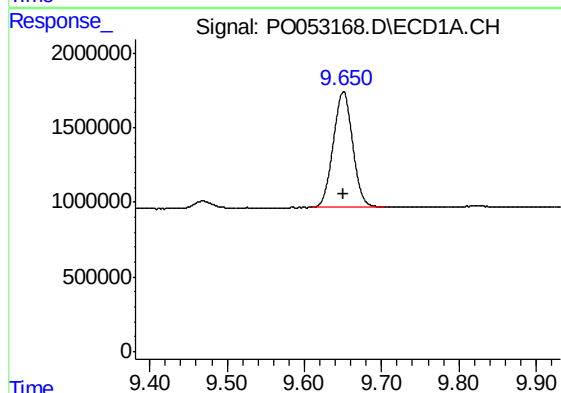

#2 Decachlorobiphenyl

R.T.: 9.651 min
Delta R.T.: 0.000 min
Response: 13135053
Conc: 16.58 ng/ml

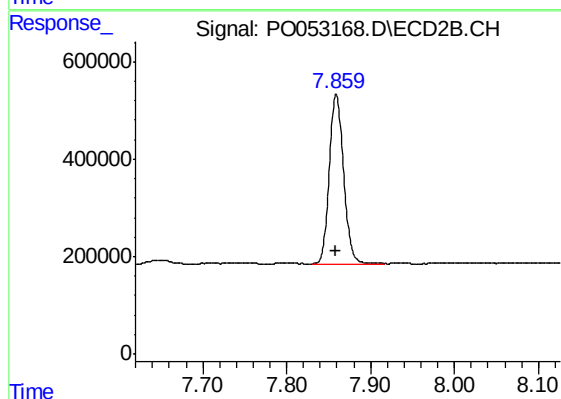

#2 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: 0.000 min
Response: 4138531
Conc: 16.10 ng/ml