

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010320\
 Data File : P0065267.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2020 12:05
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 12:22:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.172	3.442	444537	519130	21.076	20.549
2)	SA Decachlor...	9.684	8.354	655972	767297	21.495	19.938
Target Compounds							
3)	L1 AR-1016-1	0.000	4.500	0	63	N.D.	0.049 #
4)	L1 AR-1016-2	0.000	4.500	0	63	N.D.	0.035 #
5)	L1 AR-1016-3	0.000	4.694	0	729	N.D.	0.724 #
6)	L1 AR-1016-4	0.000	4.744	0	860	N.D.	0.975 #
7)	L1 AR-1016-5	0.000	5.008	0	728	N.D.	0.661 #
8)	L2 AR-1221-1	0.000	3.694	0	1239	N.D.	4.331 #
9)	L2 AR-1221-2	0.000	3.734	0	6750	N.D.	30.145 #
10)	L2 AR-1221-3	0.000	3.826	0	2108	N.D.	2.959 #
11)	L3 AR-1232-1	0.000	3.826	0	2108	N.D.	1.890 #
12)	L3 AR-1232-2	0.000	4.500	0	63	N.D.	0.047 #
13)	L3 AR-1232-3	0.000	4.694	0	729	N.D.	1.019 #
14)	L3 AR-1232-4	0.000	4.744	0	860	N.D.	1.272 #
15)	L3 AR-1232-5	0.000	5.008	0	728	N.D.	0.988 #
16)	L4 AR-1242-1	0.000	4.500	0	63	N.D.	0.066 #
17)	L4 AR-1242-2	0.000	4.500	0	63	N.D.	0.047 #
18)	L4 AR-1242-3	0.000	4.694	0	729	N.D.	0.995 #
19)	L4 AR-1242-4	0.000	4.744	0	860	N.D.	1.111 #
20)	L4 AR-1242-5	0.000	5.295	0	1000	N.D.	0.935 #
21)	L5 AR-1248-1	0.000	4.500	0	63	N.D.	0.083 #
22)	L5 AR-1248-2	0.000	4.744	0	860	N.D.	0.793 #
23)	L5 AR-1248-3	0.000	4.744	0	860	N.D.	0.771 #
24)	L5 AR-1248-4	0.000	5.008	0	728	N.D.	0.538 #
25)	L5 AR-1248-5	0.000	5.319	0	1352	N.D.	0.940 #
26)	L6 AR-1254-1	0.000	5.295	0	1000	N.D.	0.428 #
27)	L6 AR-1254-2	0.000	5.442	0	2265	N.D.	1.062 #
28)	L6 AR-1254-3	0.000	5.839	0	5471	N.D.	1.519 #
29)	L6 AR-1254-4	0.000	6.072	0	1921	N.D.	0.826 #
30)	L6 AR-1254-5	0.000	6.481	0	9532	N.D.	2.826 #
31)	L7 AR-1260-1	0.000	5.979	0	716	N.D.	0.302 #
32)	L7 AR-1260-2	0.000	6.160	0	2265	N.D.	0.742 #
33)	L7 AR-1260-3	0.000	6.311	0	554	N.D.	0.206 #
34)	L7 AR-1260-4	0.000	6.785	0	395	N.D.	0.170 #
35)	L7 AR-1260-5	0.000	7.029	0	516	N.D.	0.095 #
36)	L8 AR-1262-1	0.000	6.593	0	1772	N.D.	1.192 #
37)	L8 AR-1262-2	0.000	7.029	0	516	N.D.	0.077 #
38)	L8 AR-1262-3	0.000	7.310	0	1570	N.D.	0.608 #
39)	L8 AR-1262-4	0.000	7.370	0	2602	N.D.	0.539 #
40)	L8 AR-1262-5	0.000	7.865	0	1355	N.D.	0.683 #
41)	L9 AR-1268-1	0.000	7.310	0	1570	N.D.	0.222 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010320\
 Data File : P0065267.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2020 12:05
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 12:22:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0123119.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 31 07:42:34 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.370	0	2602	N.D.	0.404 #
43) L9	AR-1268-3	0.000	7.575	0	1968	N.D.	0.376 #
44) L9	AR-1268-4	0.000	7.865	0	1355	N.D.	0.640 #
45) L9	AR-1268-5	0.000	8.137	0	2128	N.D.	0.143 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010320\
Data File : PO065267.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2020 12:05
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 12:22:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO123119.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 31 07:42:34 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

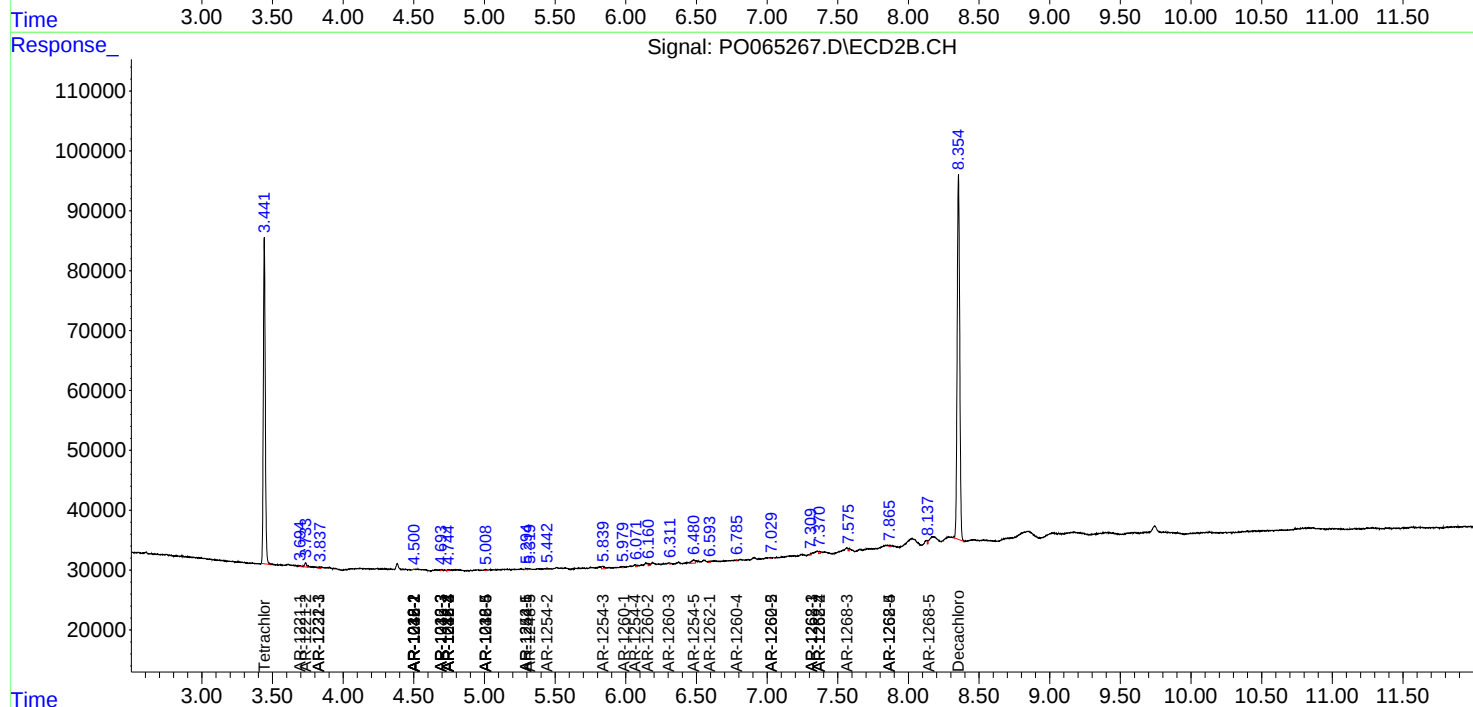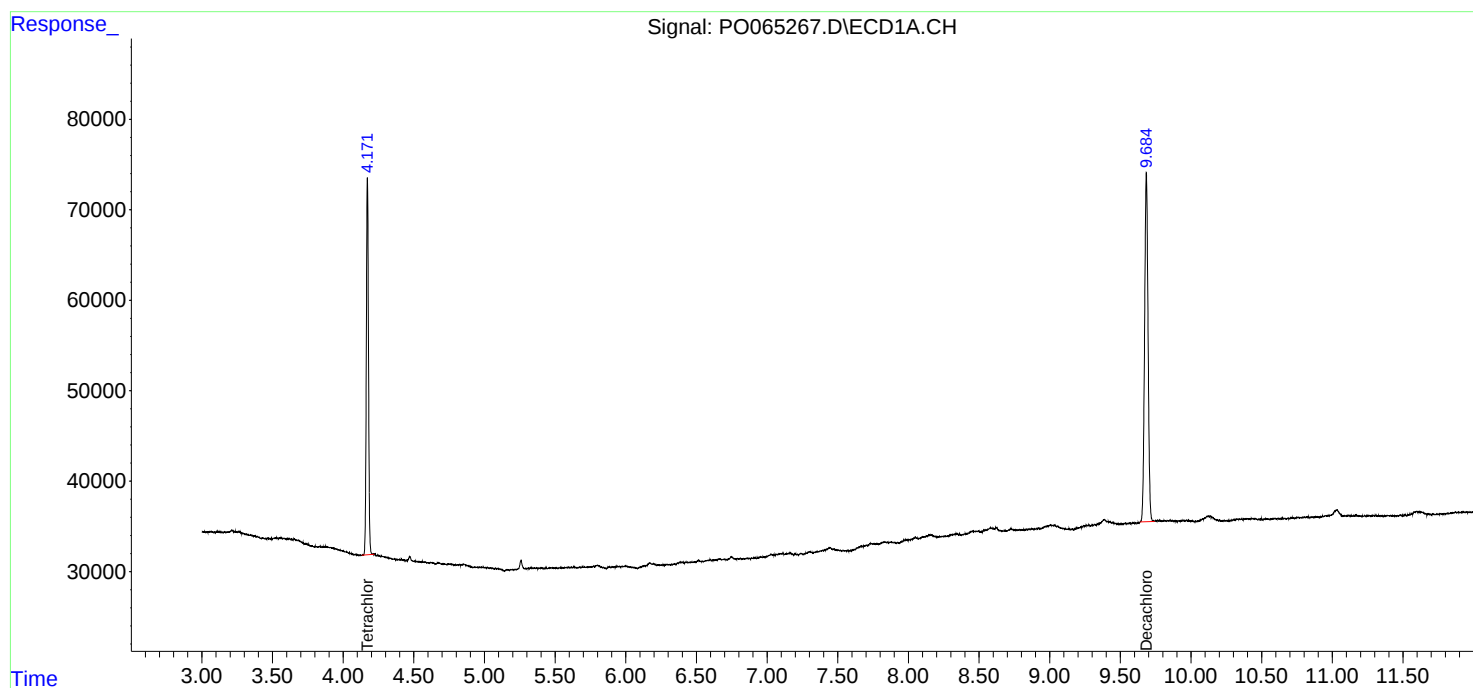


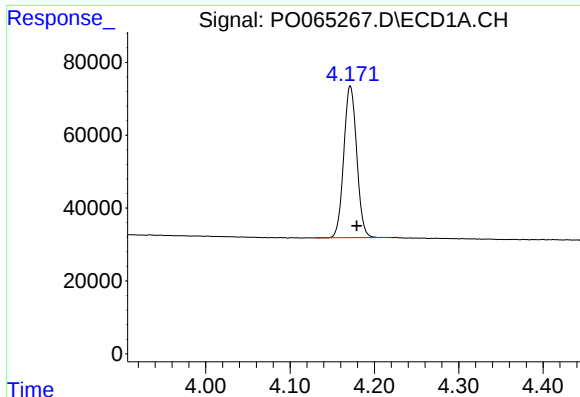

#1 Tetrachloro-m-xylene


R.T.: 4.172 min
Delta R.T.: -0.007 min
Response: 444537
Conc: 21.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

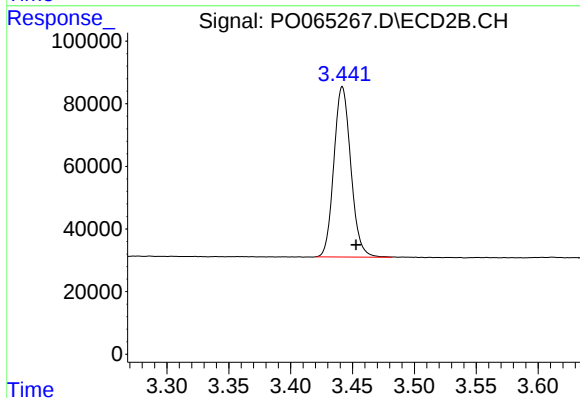


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: -0.011 min
Response: 519130
Conc: 20.55 ng/ml

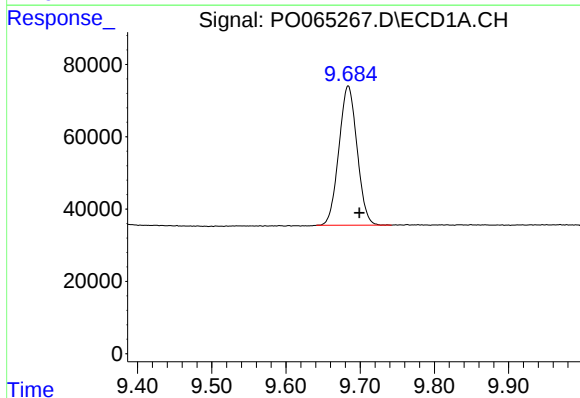


#2 Decachlorobiphenyl

R.T.: 9.684 min
Delta R.T.: -0.015 min
Response: 655972
Conc: 21.50 ng/ml

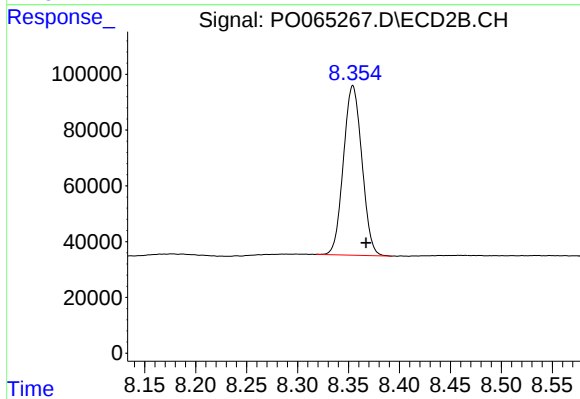

#2 Decachlorobiphenyl


R.T.: 8.354 min
Delta R.T.: -0.013 min
Response: 767297
Conc: 19.94 ng/ml

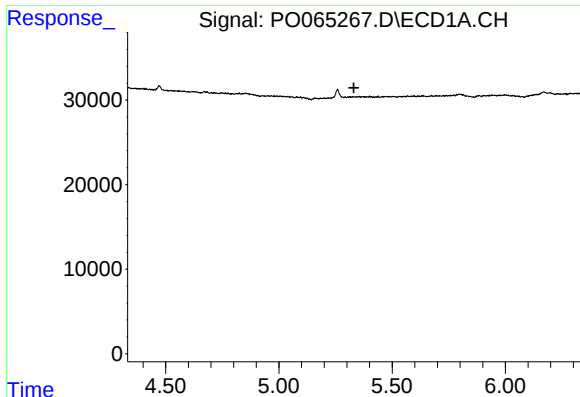

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

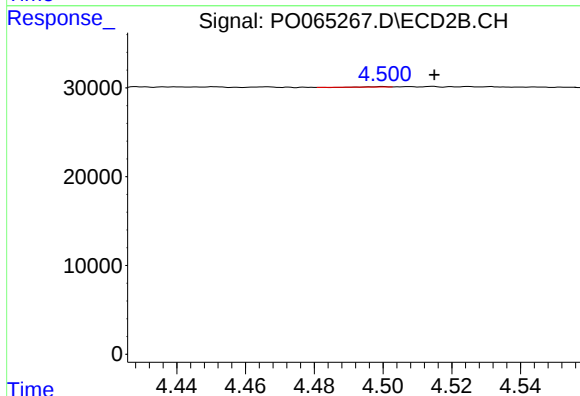


#3 AR-1016-1

R.T.: 4.500 min
Delta R.T.: -0.015 min
Response: 63
Conc: 0.05 ng/ml

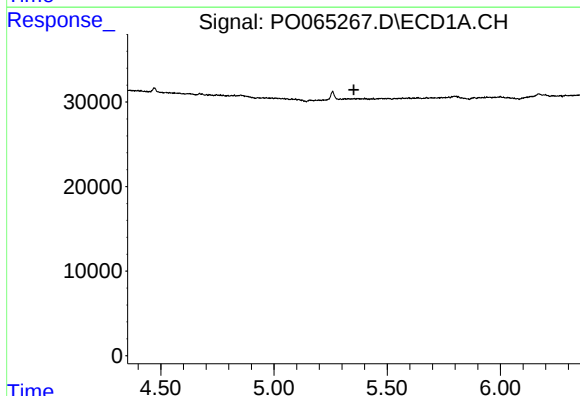


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.353 min
Response: 0
Conc: N.D.

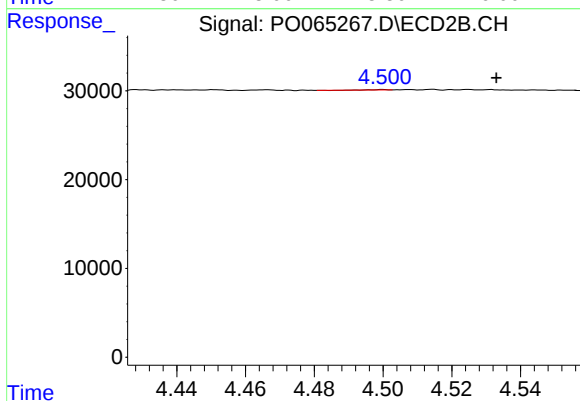

#4 AR-1016-2


R.T.: 4.500 min
Delta R.T.: -0.033 min
Response: 63
Conc: 0.03 ng/ml

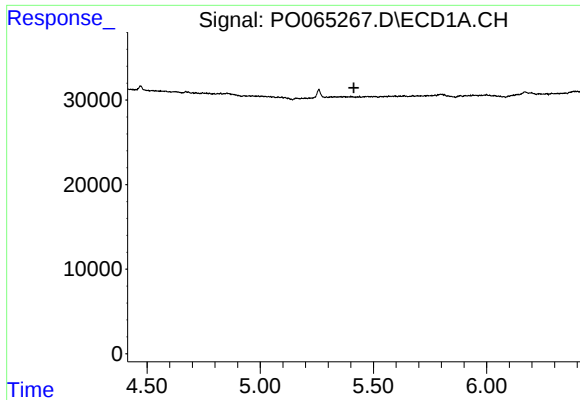

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

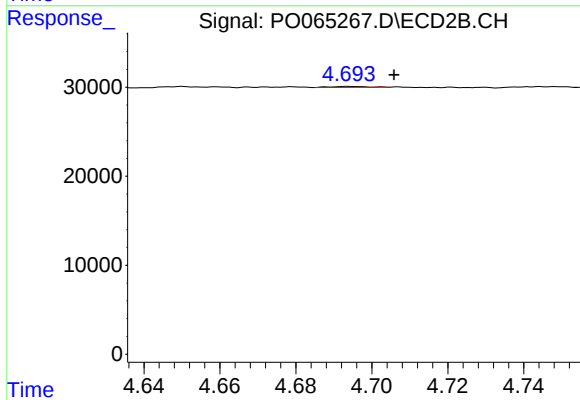


#5 AR-1016-3

R.T.: 4.694 min
Delta R.T.: -0.012 min
Response: 729
Conc: 0.72 ng/ml

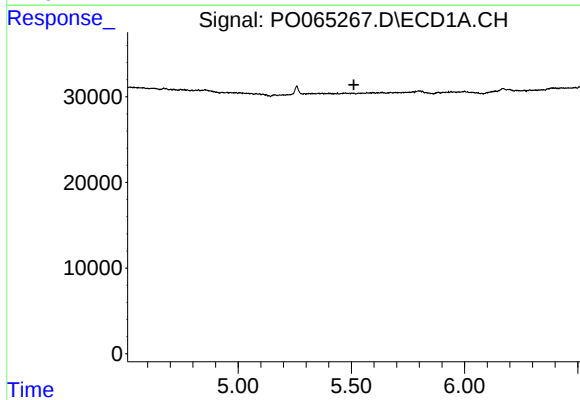


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

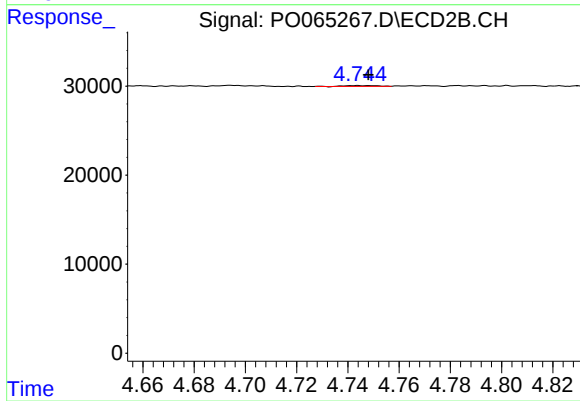

#6 AR-1016-4


R.T.: 4.744 min
Delta R.T.: -0.004 min
Response: 860
Conc: 0.98 ng/ml

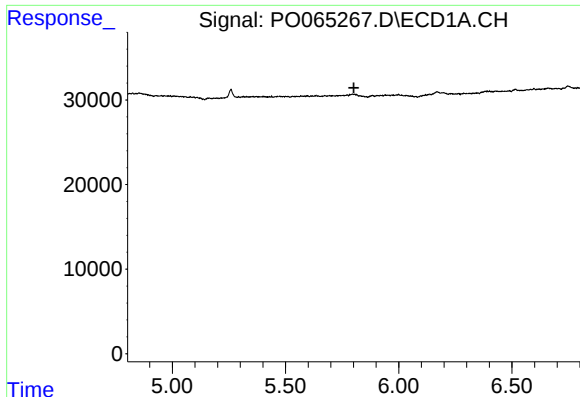

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

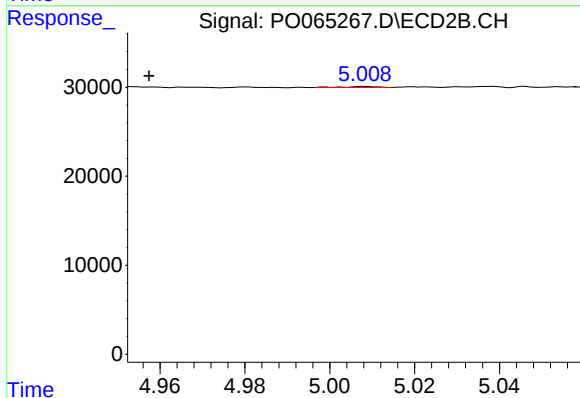


#7 AR-1016-5

R.T.: 5.008 min
Delta R.T.: 0.051 min
Response: 728
Conc: 0.66 ng/ml

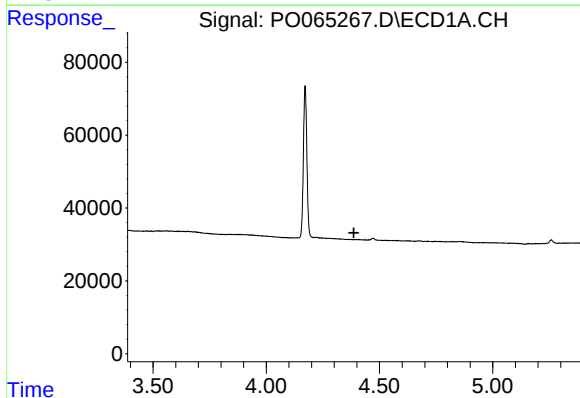


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.387 min
Response: 0
Conc: N.D.

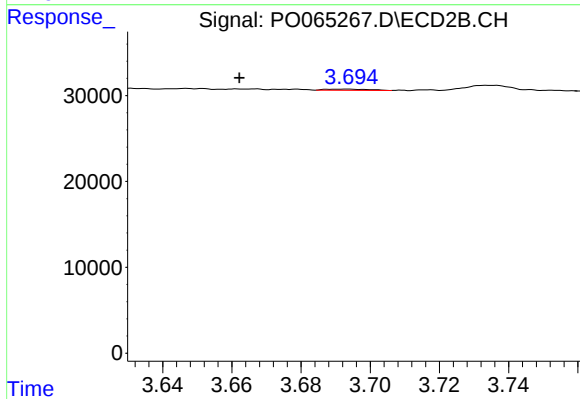

#8 AR-1221-1


R.T.: 3.694 min
Delta R.T.: 0.032 min
Response: 1239
Conc: 4.33 ng/ml

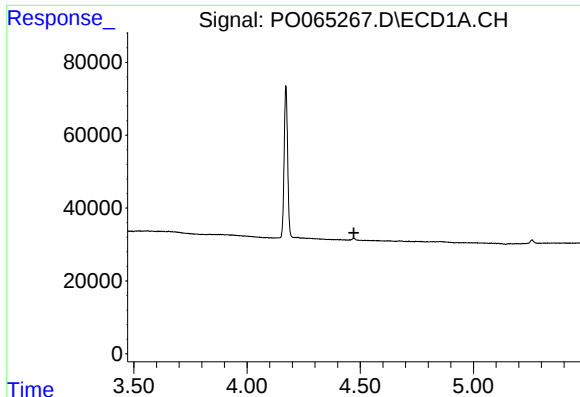

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

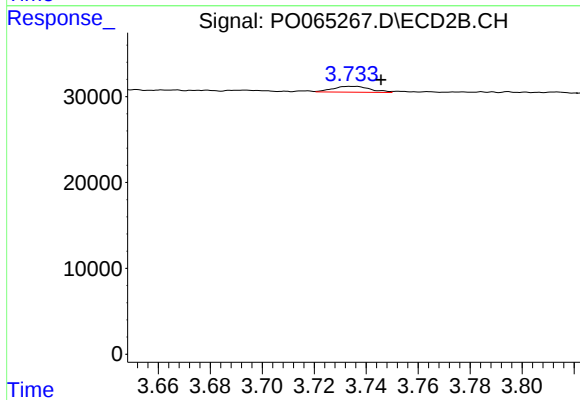


#9 AR-1221-2

R.T.: 3.734 min
Delta R.T.: -0.012 min
Response: 6750
Conc: 30.14 ng/ml

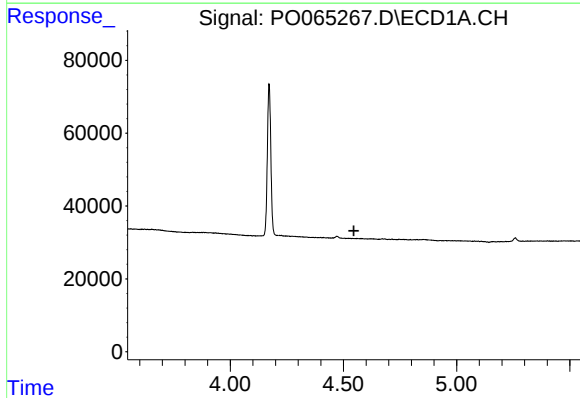


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.546 min
Response: 0
Conc: N.D.

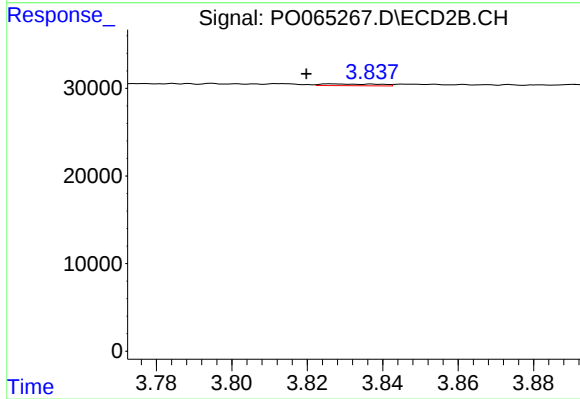

#10 AR-1221-3


R.T.: 3.826 min
Delta R.T.: 0.006 min
Response: 2108
Conc: 2.96 ng/ml

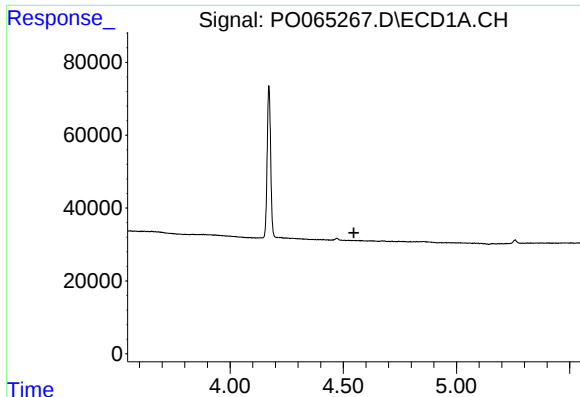

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.547 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

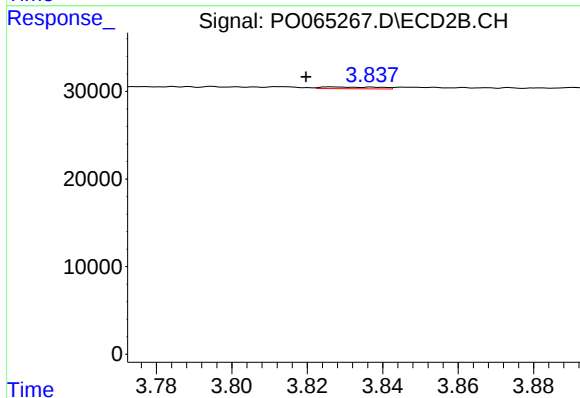


#11 AR-1232-1

R.T.: 3.826 min
Delta R.T.: 0.006 min
Response: 2108
Conc: 1.89 ng/ml

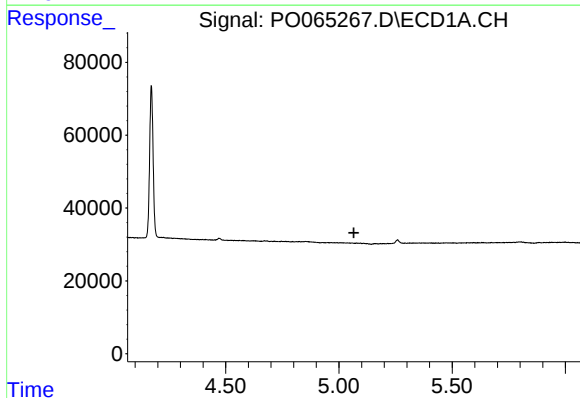


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.066 min
Response: 0
Conc: N.D.

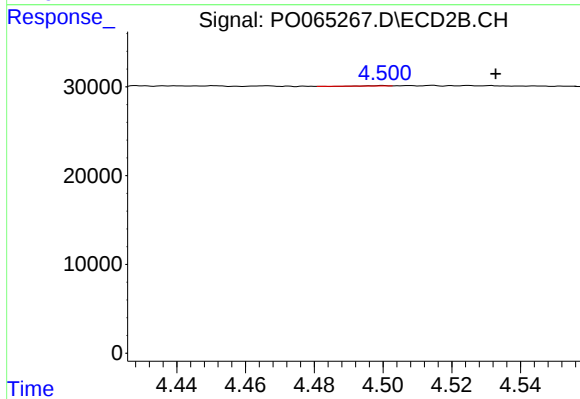

#12 AR-1232-2


R.T.: 4.500 min
Delta R.T.: -0.033 min
Response: 63
Conc: 0.05 ng/ml

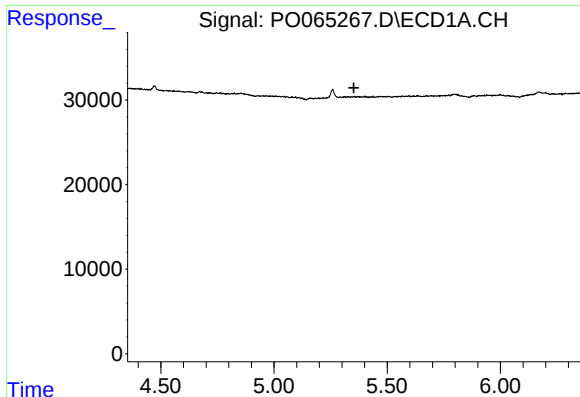

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.353 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

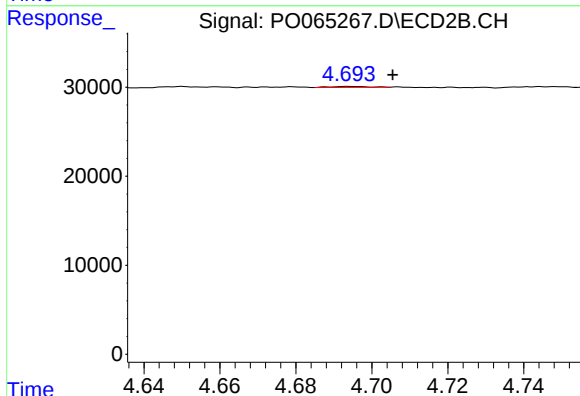


#13 AR-1232-3

R.T.: 4.694 min
Delta R.T.: -0.012 min
Response: 729
Conc: 1.02 ng/ml

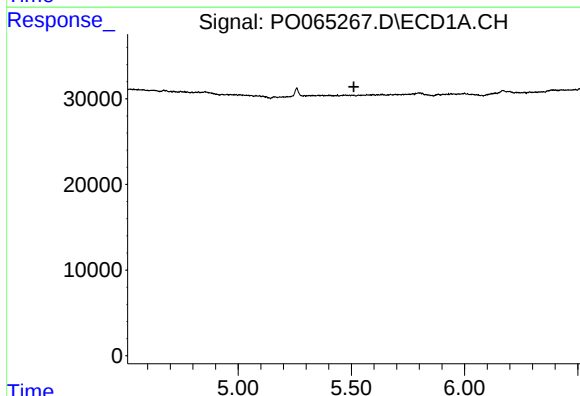


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

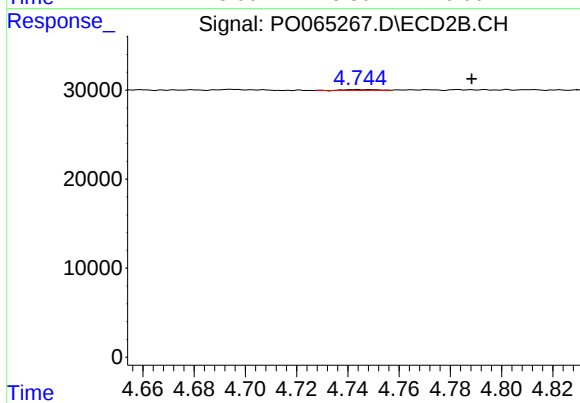

#14 AR-1232-4


R.T.: 4.744 min
Delta R.T.: -0.044 min
Response: 860
Conc: 1.27 ng/ml

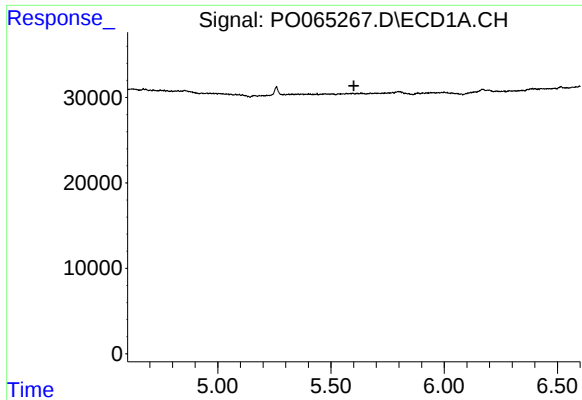

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

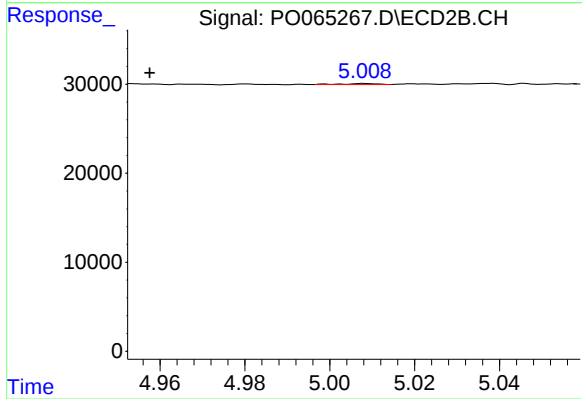


#15 AR-1232-5

R.T.: 5.008 min
Delta R.T.: 0.051 min
Response: 728
Conc: 0.99 ng/ml

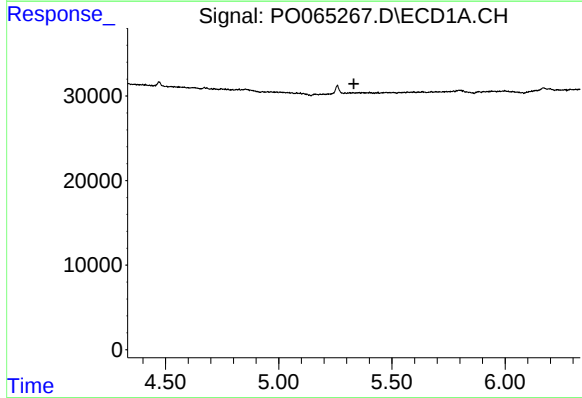


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.332 min
Response: 0
Conc: N.D.

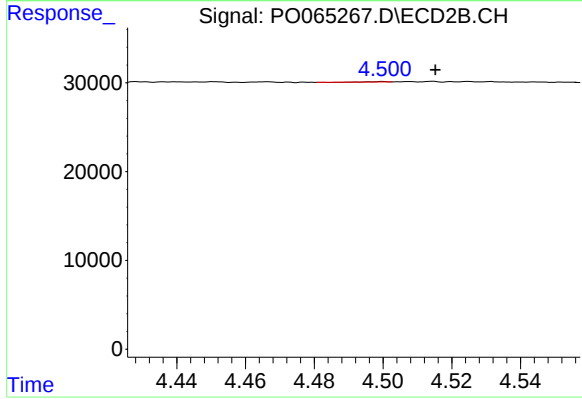

#16 AR-1242-1


R.T.: 4.500 min
Delta R.T.: -0.015 min
Response: 63
Conc: 0.07 ng/ml

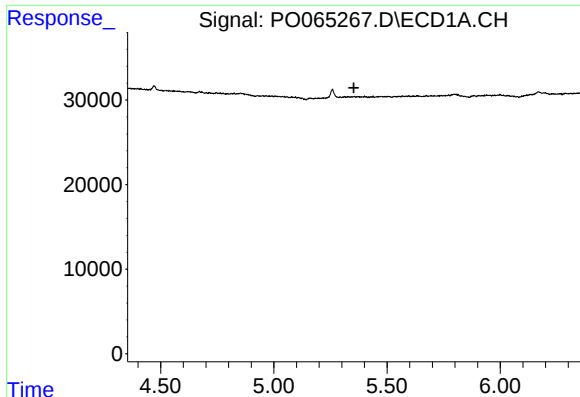

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.353 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

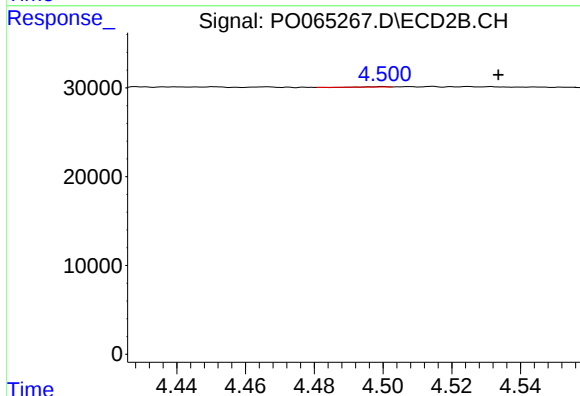


#17 AR-1242-2

R.T.: 4.500 min
Delta R.T.: -0.033 min
Response: 63
Conc: 0.05 ng/ml

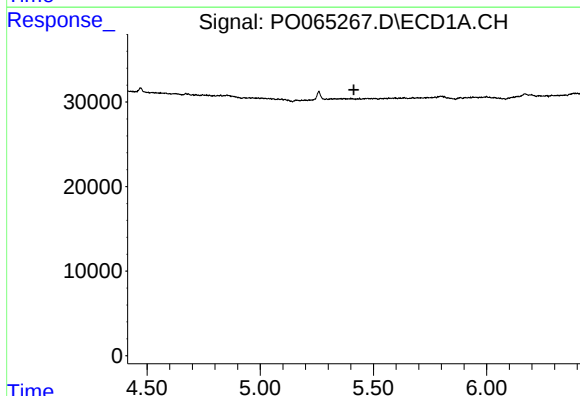


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

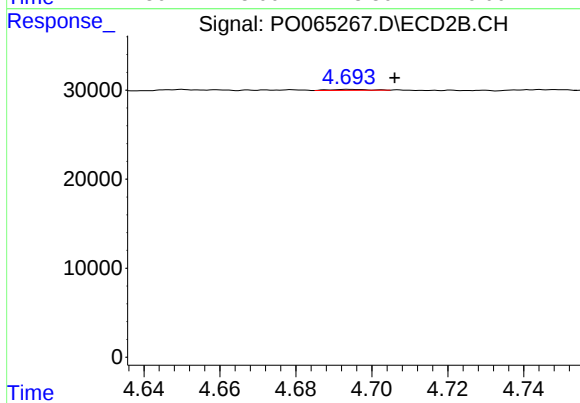

#18 AR-1242-3


R.T.: 4.694 min
Delta R.T.: -0.012 min
Response: 729
Conc: 0.99 ng/ml

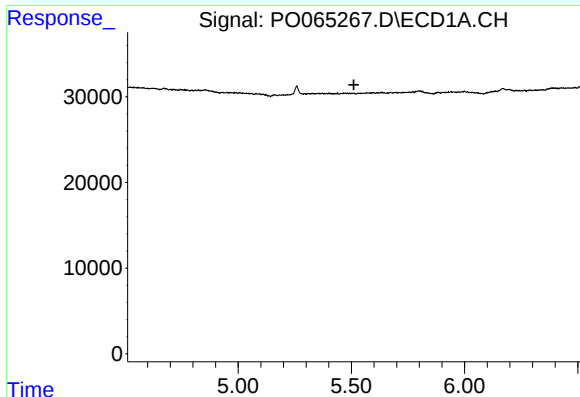

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

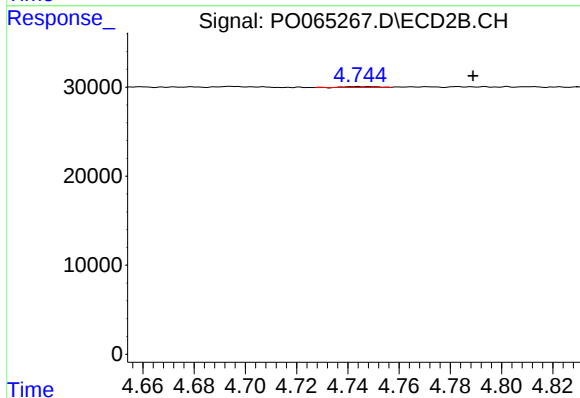


#19 AR-1242-4

R.T.: 4.744 min
Delta R.T.: -0.045 min
Response: 860
Conc: 1.11 ng/ml

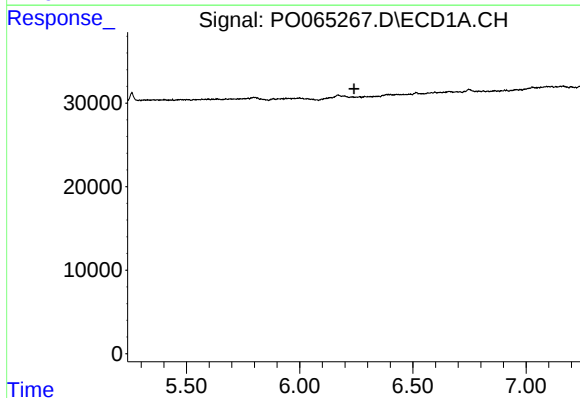


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.240 min
Response: 0
Conc: N.D.

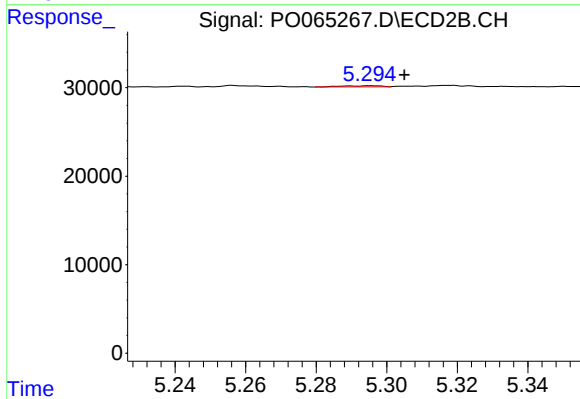

#20 AR-1242-5


R.T.: 5.295 min
Delta R.T.: -0.010 min
Response: 1000
Conc: 0.94 ng/ml

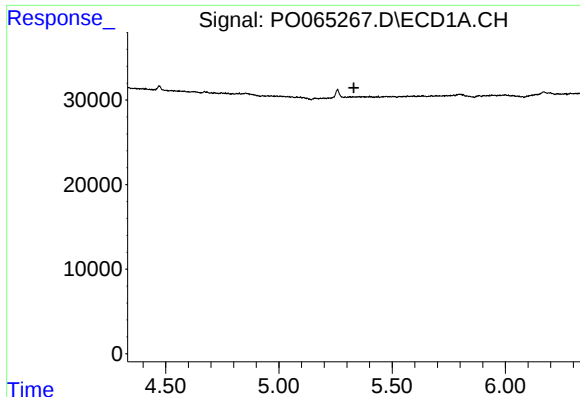

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

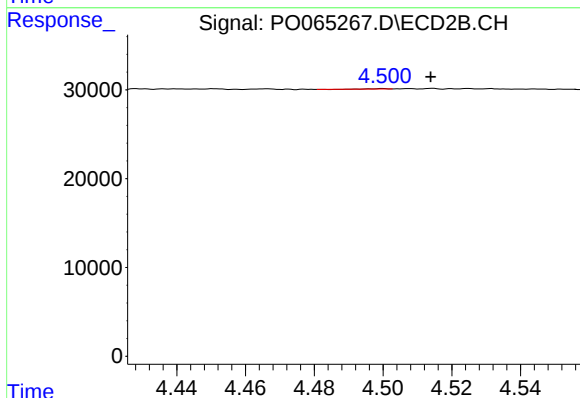


#21 AR-1248-1

R.T.: 4.500 min
Delta R.T.: -0.014 min
Response: 63
Conc: 0.08 ng/ml

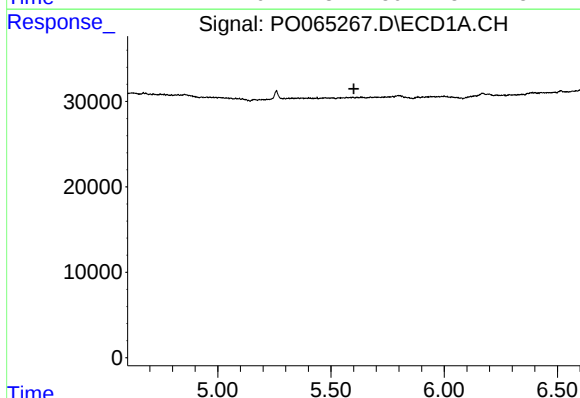


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.601 min
Response: 0
Conc: N.D.

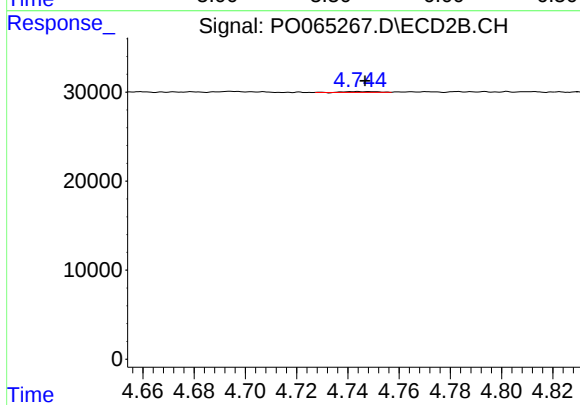

#22 AR-1248-2


R.T.: 4.744 min
Delta R.T.: -0.003 min
Response: 860
Conc: 0.79 ng/ml

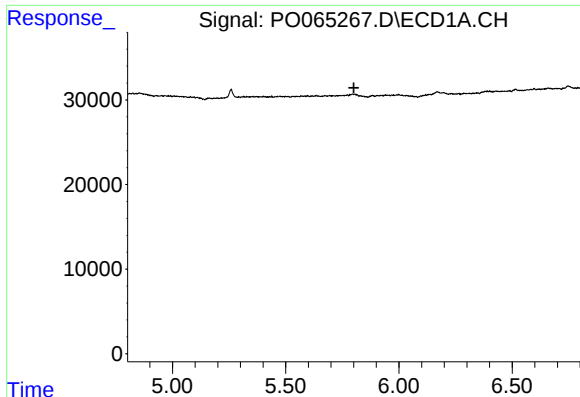

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

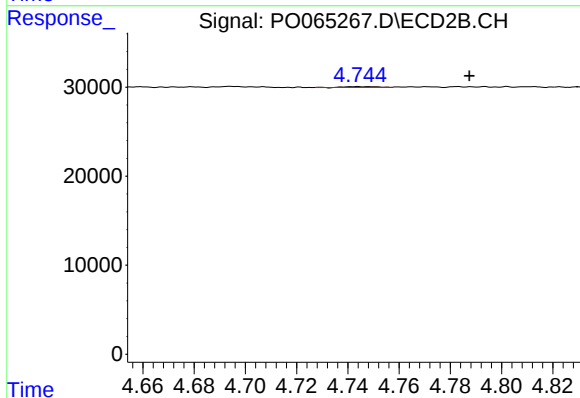


#23 AR-1248-3

R.T.: 4.744 min
Delta R.T.: -0.043 min
Response: 860
Conc: 0.77 ng/ml

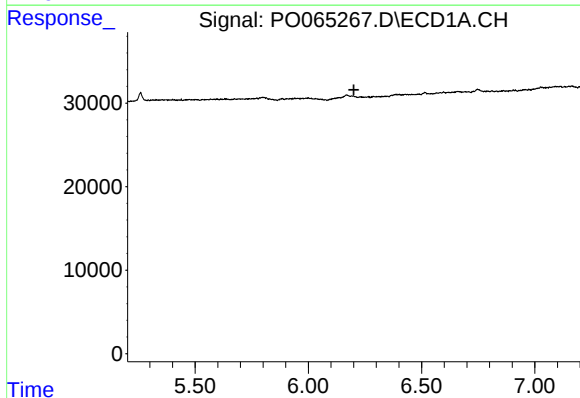


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.201 min
Response: 0
Conc: N.D.

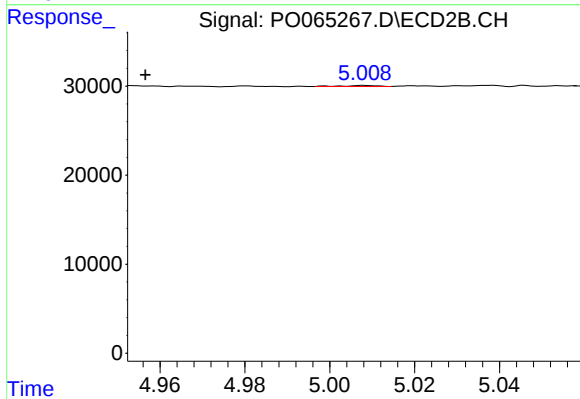

#24 AR-1248-4


R.T.: 5.008 min
Delta R.T.: 0.052 min
Response: 728
Conc: 0.54 ng/ml

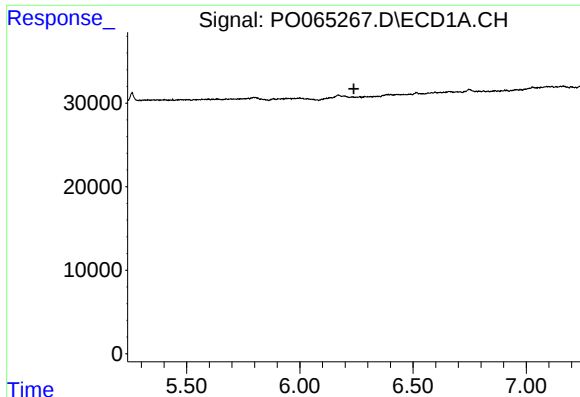

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

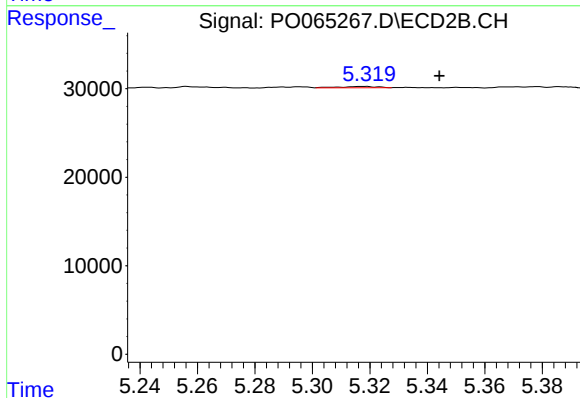


#25 AR-1248-5

R.T.: 5.319 min
Delta R.T.: -0.025 min
Response: 1352
Conc: 0.94 ng/ml

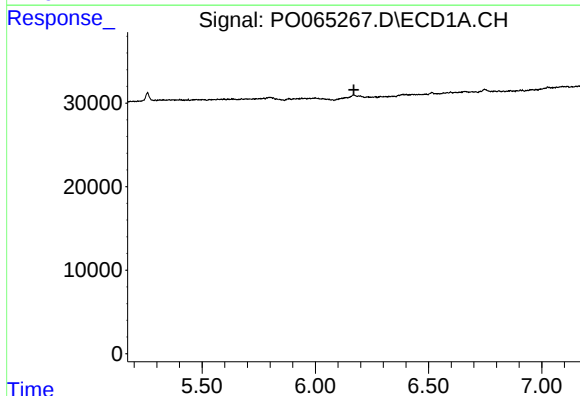


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

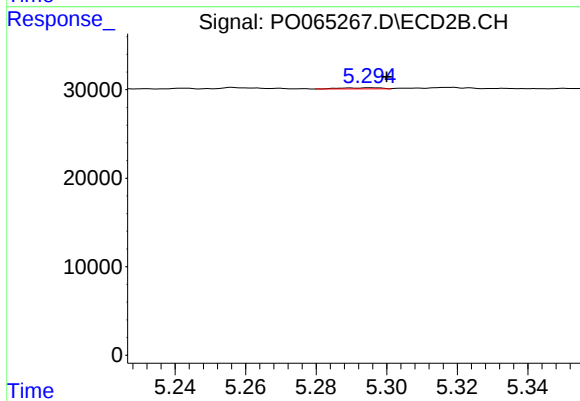

#26 AR-1254-1


R.T.: 5.295 min
Delta R.T.: -0.005 min
Response: 1000
Conc: 0.43 ng/ml

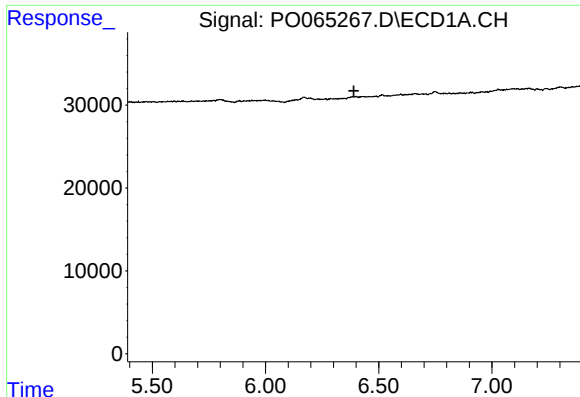

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

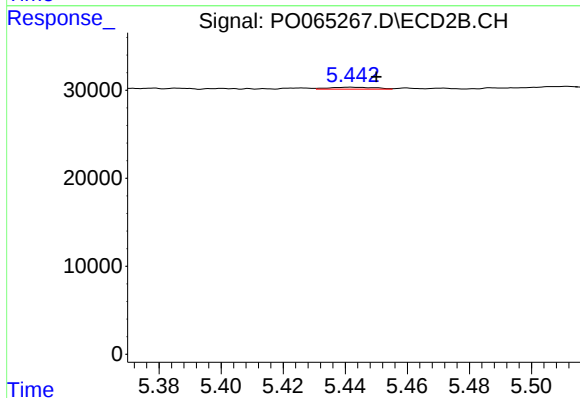


#27 AR-1254-2

R.T.: 5.442 min
Delta R.T.: -0.008 min
Response: 2265
Conc: 1.06 ng/ml

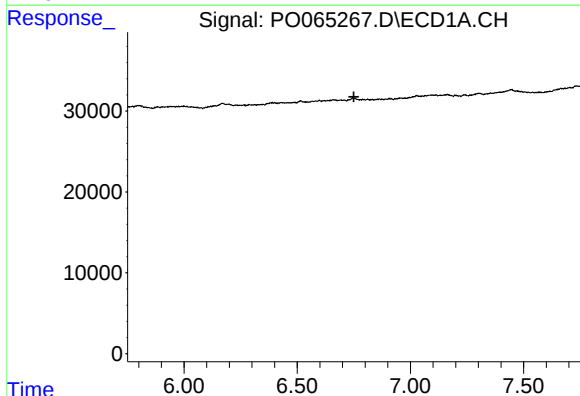


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.750 min
Response: 0
Conc: N.D.

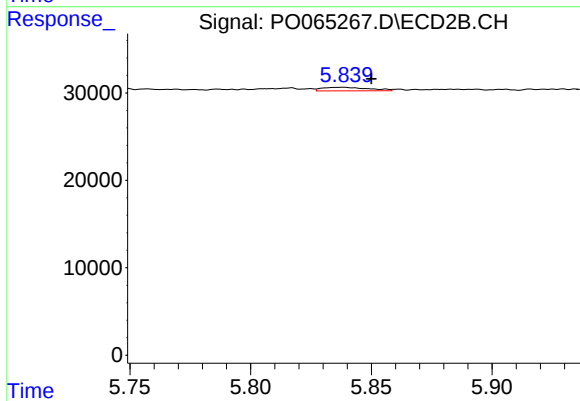

#28 AR-1254-3


R.T.: 5.839 min
Delta R.T.: -0.011 min
Response: 5471
Conc: 1.52 ng/ml

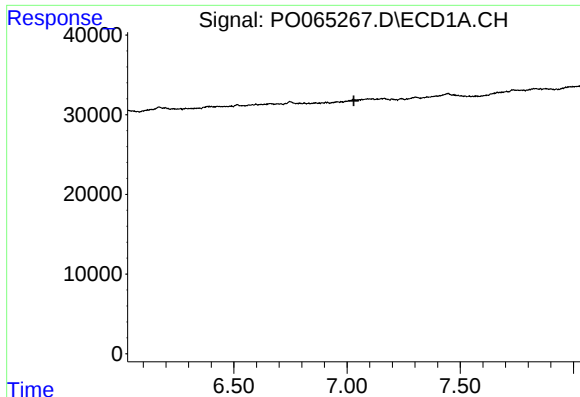

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

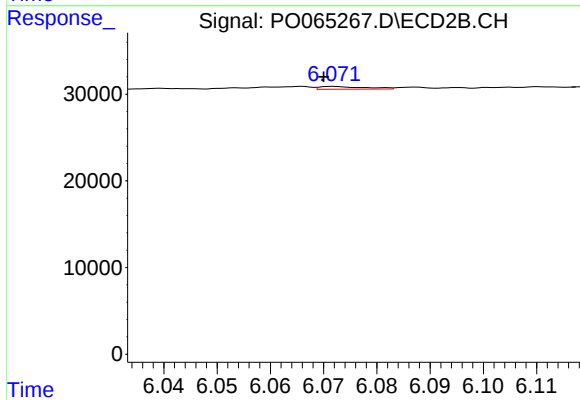


#29 AR-1254-4

R.T.: 6.072 min
Delta R.T.: 0.002 min
Response: 1921
Conc: 0.83 ng/ml

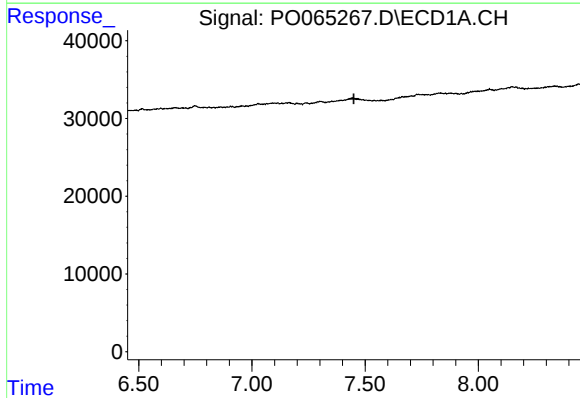


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.450 min
Response: 0
Conc: N.D.

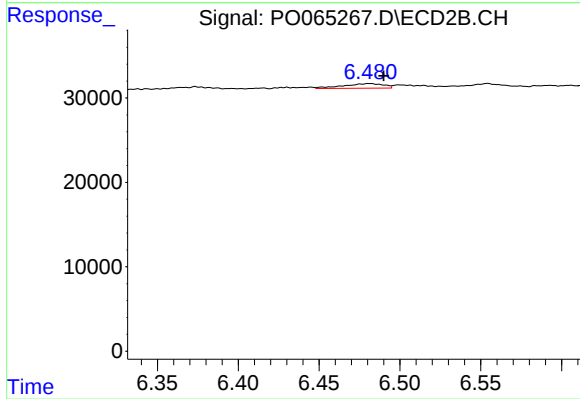

#30 AR-1254-5


R.T.: 6.481 min
Delta R.T.: -0.009 min
Response: 9532
Conc: 2.83 ng/ml

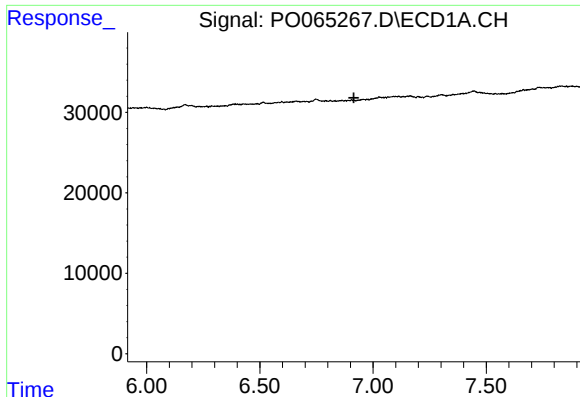

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

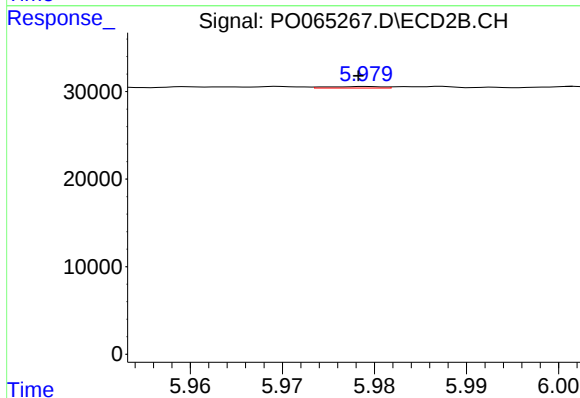


#31 AR-1260-1

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 716
Conc: 0.30 ng/ml

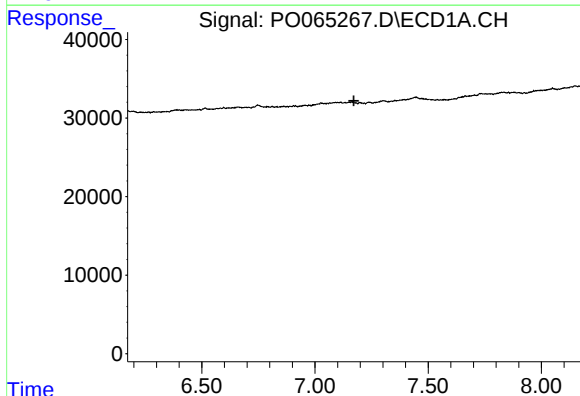


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.172 min
Response: 0
Conc: N.D.

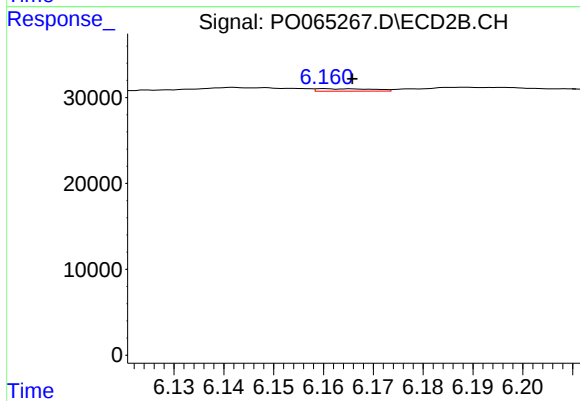

#32 AR-1260-2


R.T.: 6.160 min
Delta R.T.: -0.005 min
Response: 2265
Conc: 0.74 ng/ml

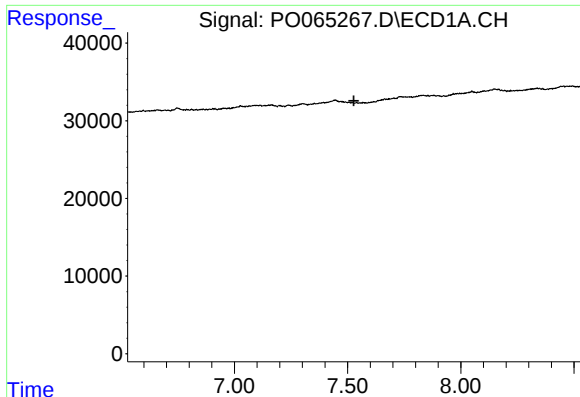

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

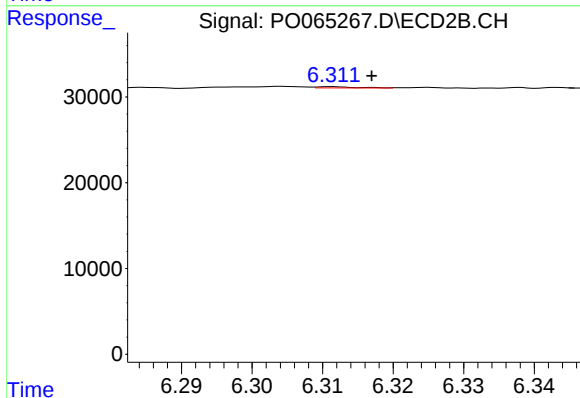


#33 AR-1260-3

R.T.: 6.311 min
Delta R.T.: -0.005 min
Response: 554
Conc: 0.21 ng/ml

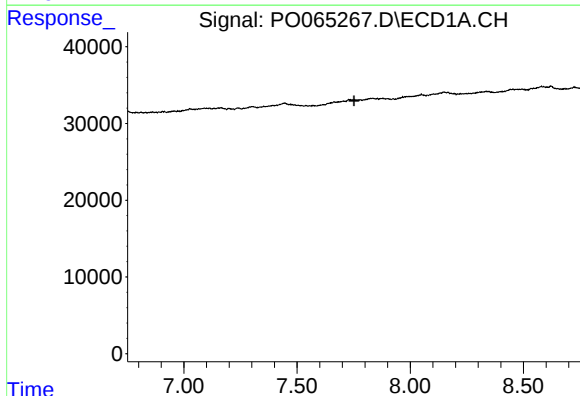


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.752 min
Response: 0
Conc: N.D.

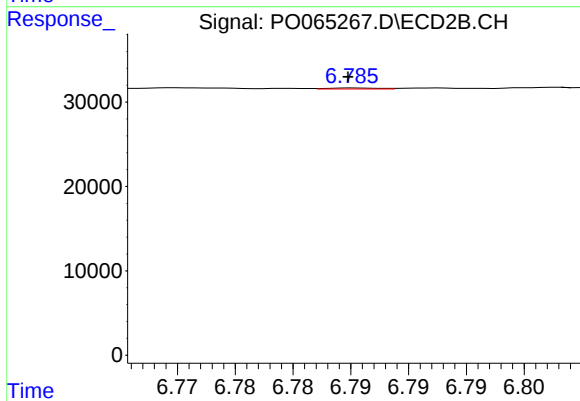

#34 AR-1260-4


R.T.: 6.785 min
Delta R.T.: 0.000 min
Response: 395
Conc: 0.17 ng/ml

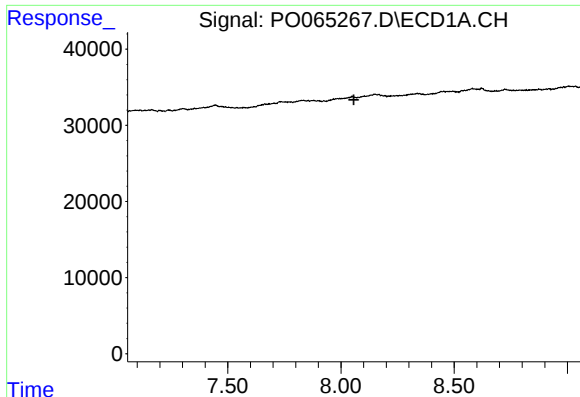

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

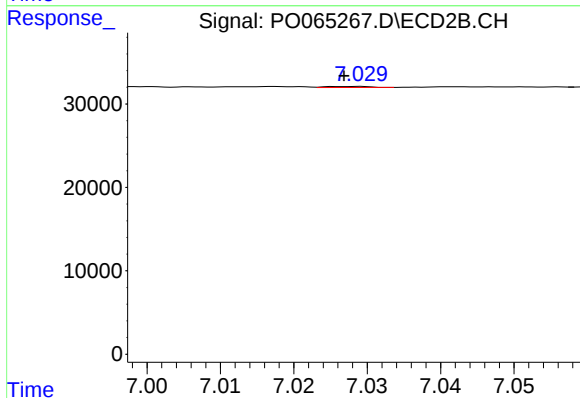


#35 AR-1260-5

R.T.: 7.029 min
Delta R.T.: 0.002 min
Response: 516
Conc: 0.10 ng/ml

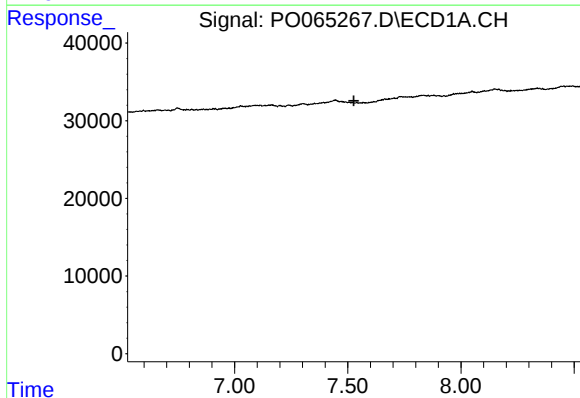


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.527 min
Response: 0
Conc: N.D.

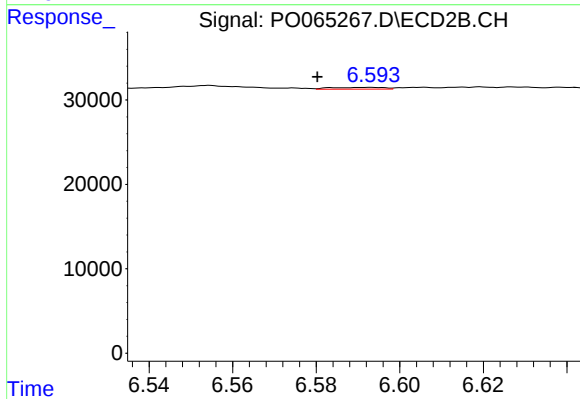

#36 AR-1262-1


R.T.: 6.593 min
Delta R.T.: 0.013 min
Response: 1772
Conc: 1.19 ng/ml

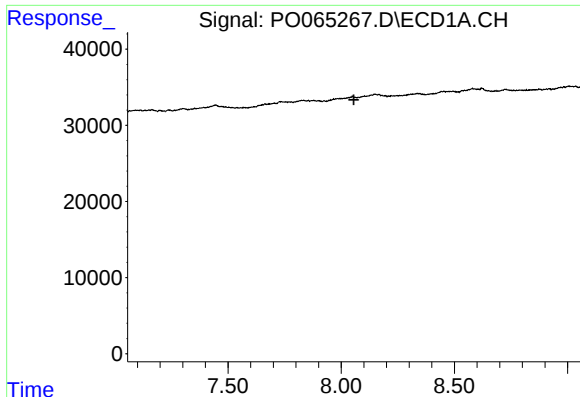

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.056 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

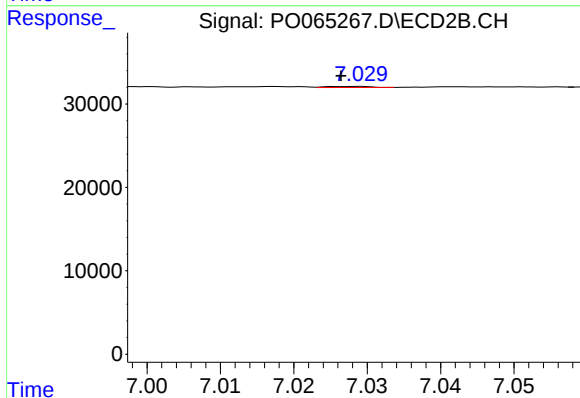


#37 AR-1262-2

R.T.: 7.029 min
Delta R.T.: 0.003 min
Response: 516
Conc: 0.08 ng/ml

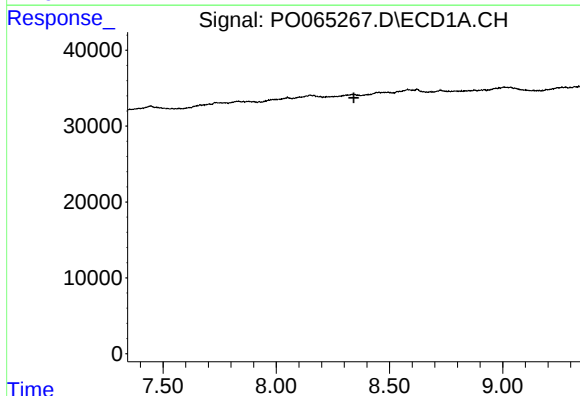


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

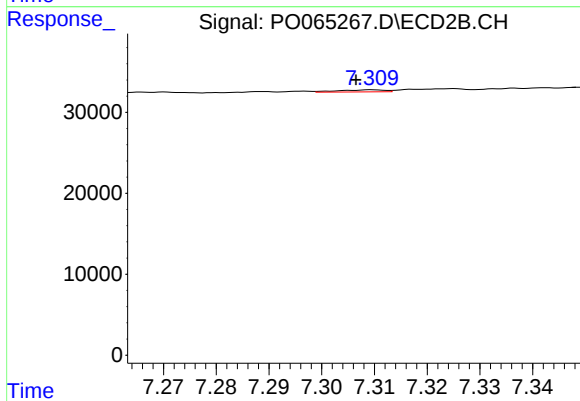

#38 AR-1262-3


R.T.: 7.310 min
Delta R.T.: 0.003 min
Response: 1570
Conc: 0.61 ng/ml

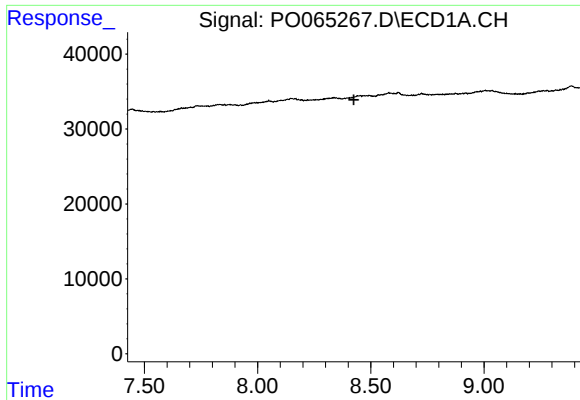

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.425 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

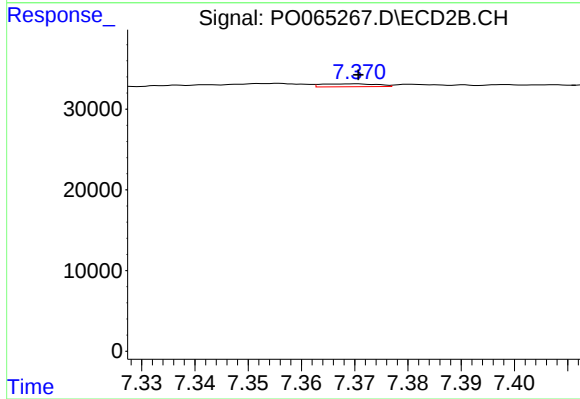


#39 AR-1262-4

R.T.: 7.370 min
Delta R.T.: 0.000 min
Response: 2602
Conc: 0.54 ng/ml

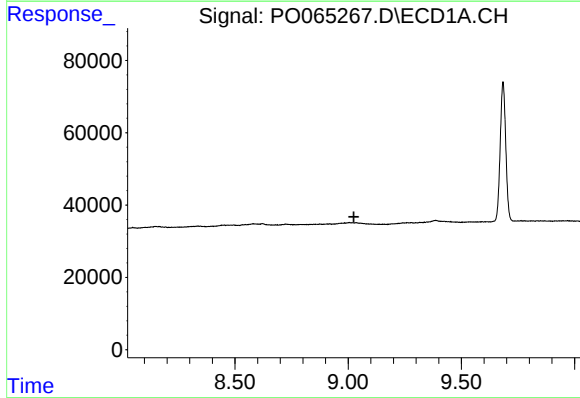


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.025 min
Response: 0
Conc: N.D.

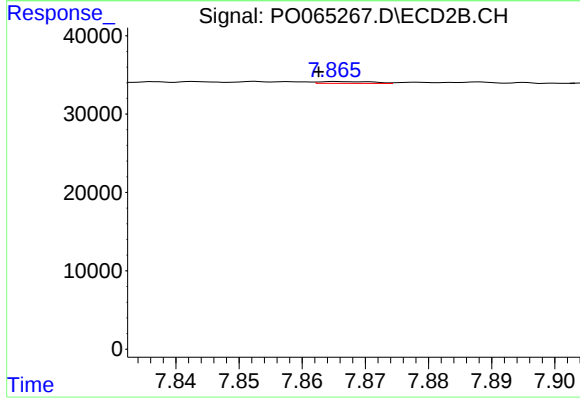

#40 AR-1262-5


R.T.: 7.865 min
Delta R.T.: 0.003 min
Response: 1355
Conc: 0.68 ng/ml

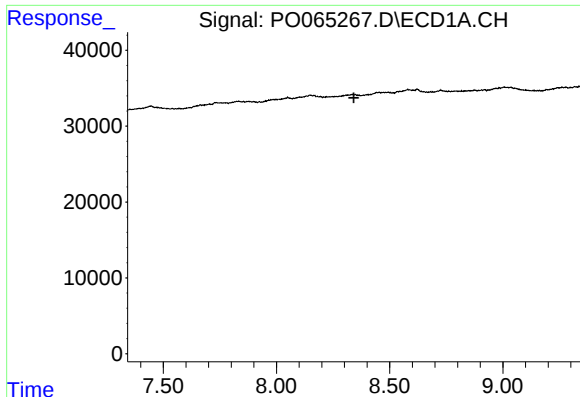

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

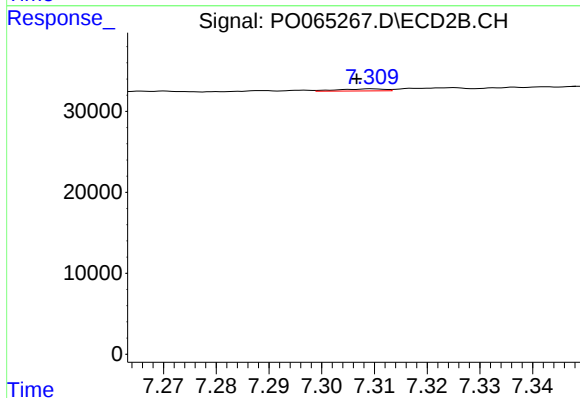


#41 AR-1268-1

R.T.: 7.310 min
Delta R.T.: 0.003 min
Response: 1570
Conc: 0.22 ng/ml

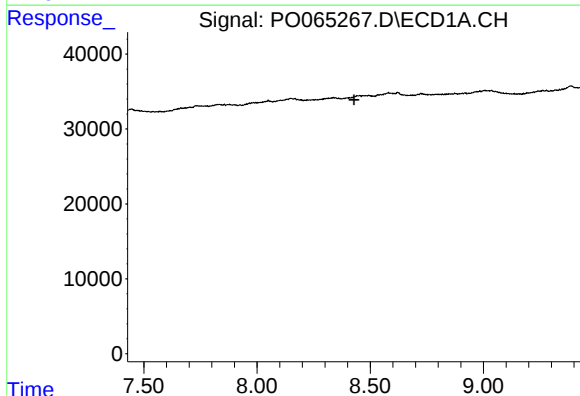


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.428 min
Response: 0
Conc: N.D.

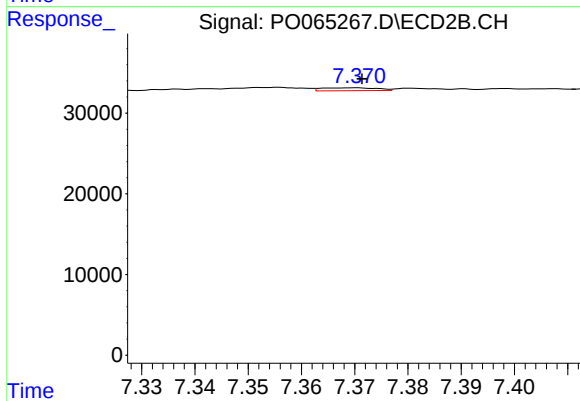

#42 AR-1268-2


R.T.: 7.370 min
Delta R.T.: -0.001 min
Response: 2602
Conc: 0.40 ng/ml

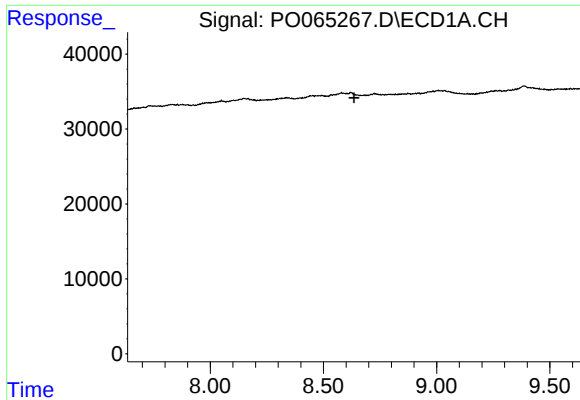

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

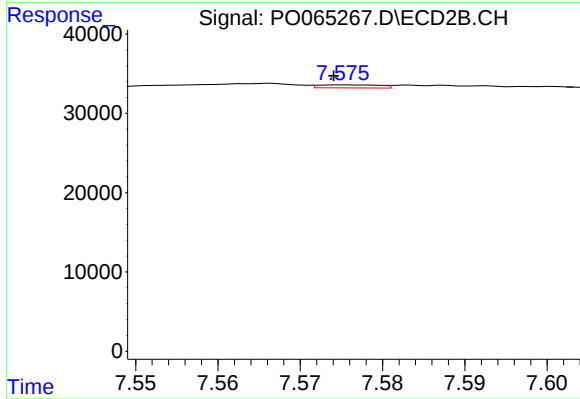


#43 AR-1268-3

R.T.: 7.575 min
Delta R.T.: 0.001 min
Response: 1968
Conc: 0.38 ng/ml

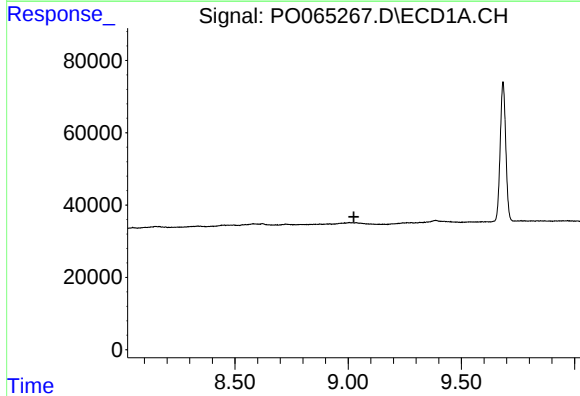


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.025 min
Response: 0
Conc: N.D.

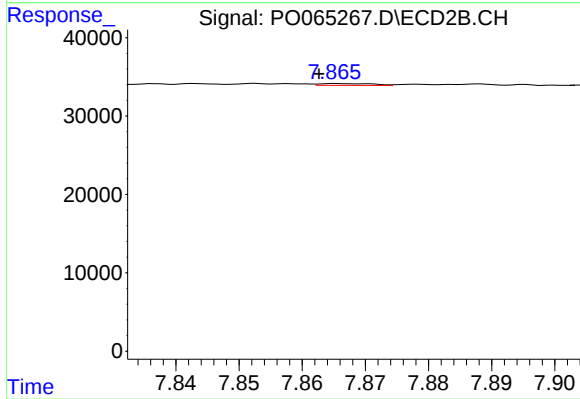

#44 AR-1268-4


R.T.: 7.865 min
Delta R.T.: 0.003 min
Response: 1355
Conc: 0.64 ng/ml

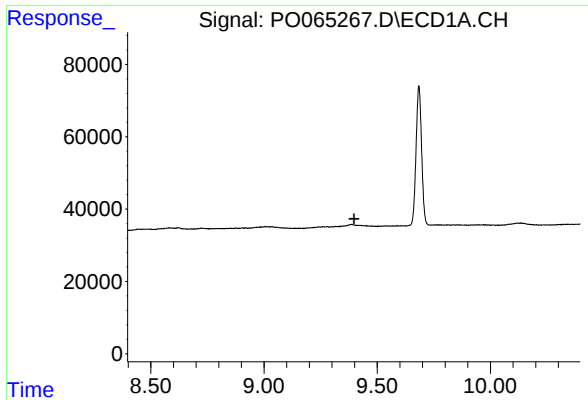

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

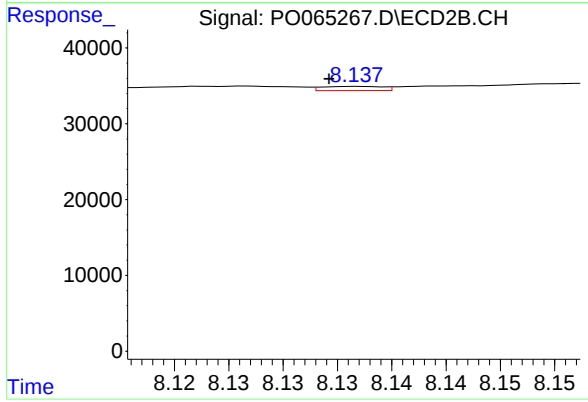

#45 AR-1268-5

R.T.: 8.137 min
Delta R.T.: 0.003 min
Response: 2128
Conc: 0.14 ng/ml