

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053224.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 2:00
 Operator : SM/SJ
 Sample : K1023-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PURGE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 03:14:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

20)	L4	AR-1242-5	0.000	4.997	0	436842	N.D.	57.338 #
25)	L5	AR-1248-5	0.000	4.997	0	436842	N.D.	43.543 #
26)	L6	AR-1254-1	0.000	4.997	0	436842	N.D.	26.646 #
27)	L6	AR-1254-2	0.000	5.028	0	24726	N.D.	1.762 #
38)	L8	AR-1262-3	0.000	6.865	0	811300	N.D.	62.655 #
39)	L8	AR-1262-4	0.000	6.865	0	811300	N.D.	33.417 #
41)	L9	AR-1268-1	0.000	6.865	0	811300	N.D.	18.674 #
42)	L9	AR-1268-2	0.000	6.865	0	811300	N.D.	19.727 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053224.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 2:00
Operator : SM/SJ
Sample : K1023-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 03:14:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

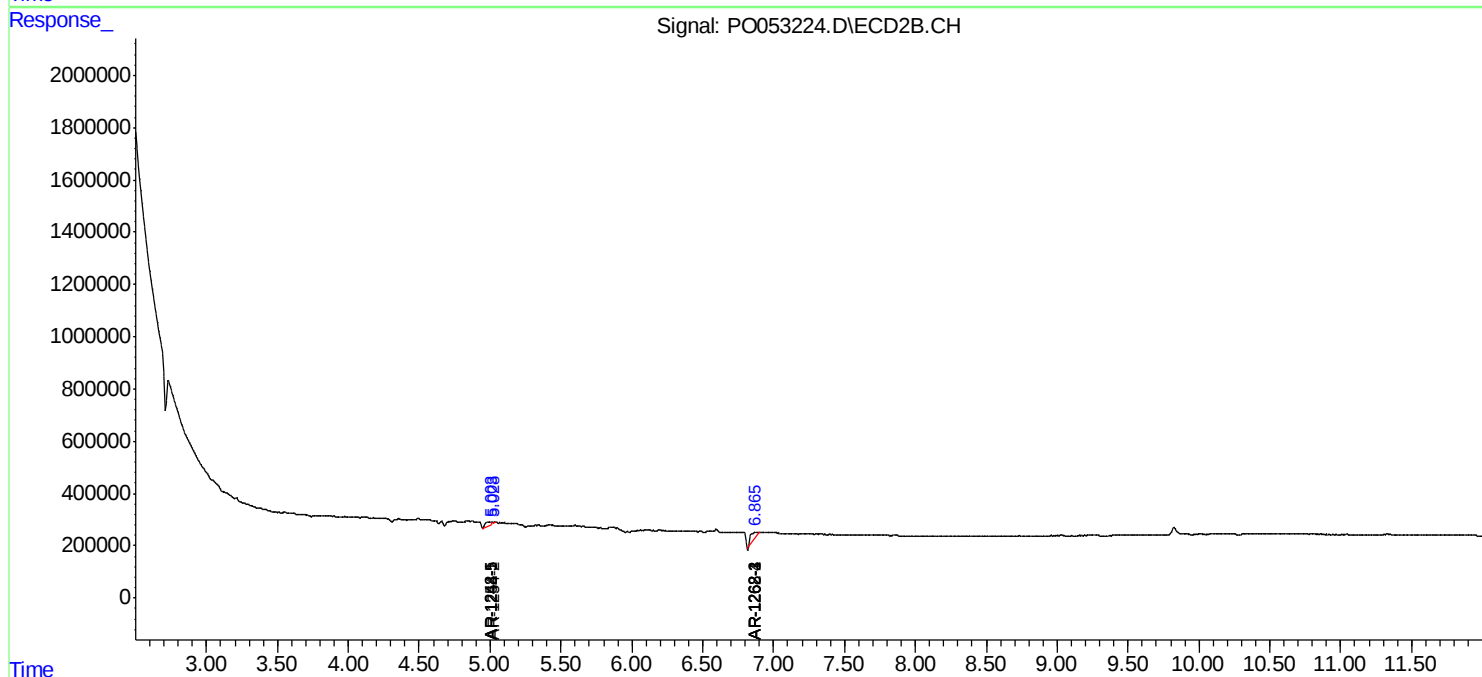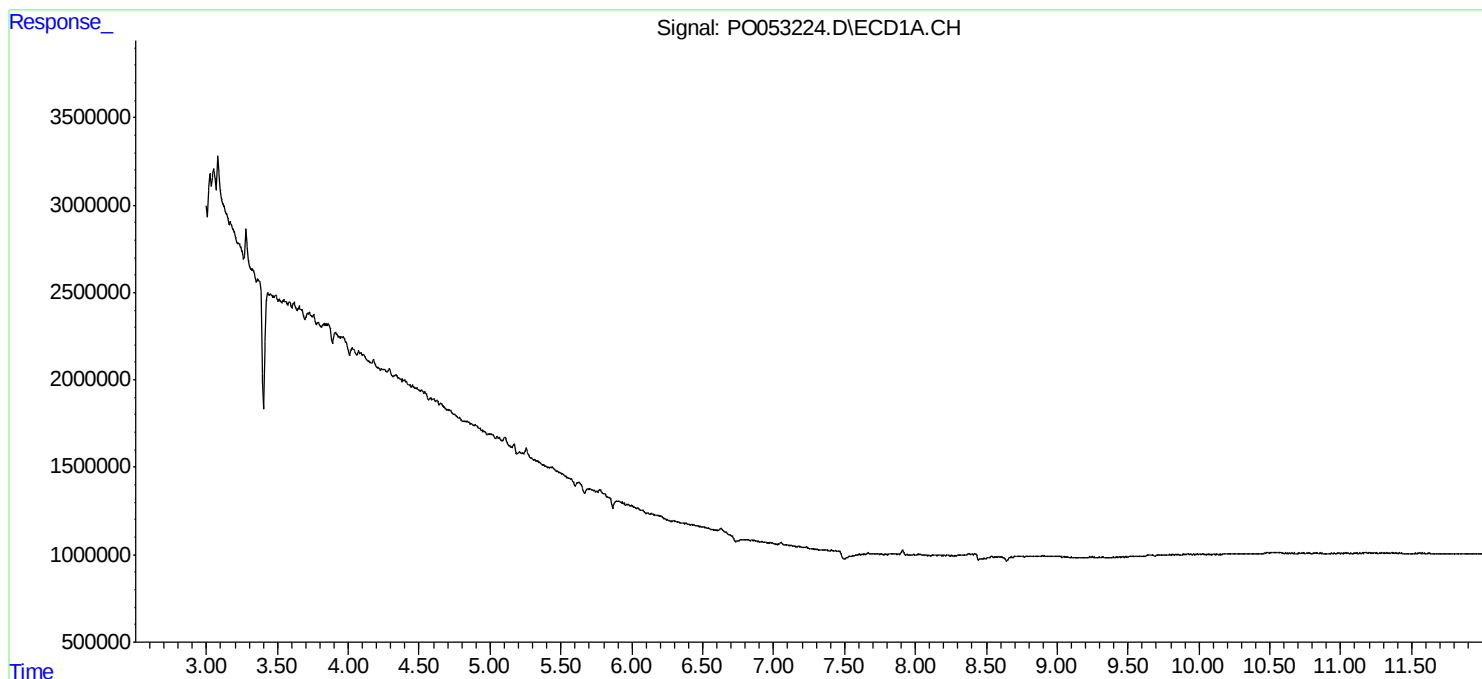


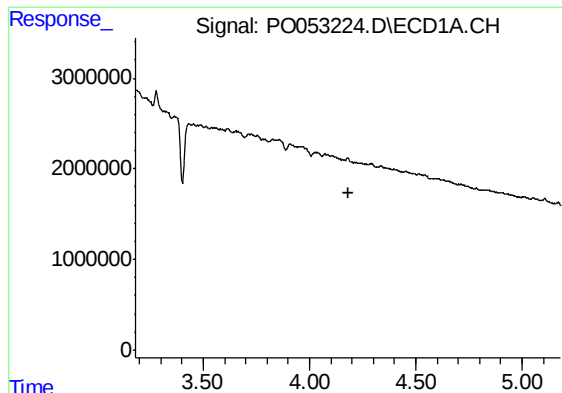

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

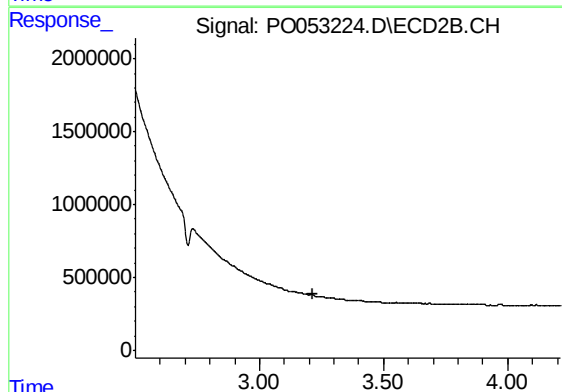


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.214 min
Response: 0
Conc: N.D.

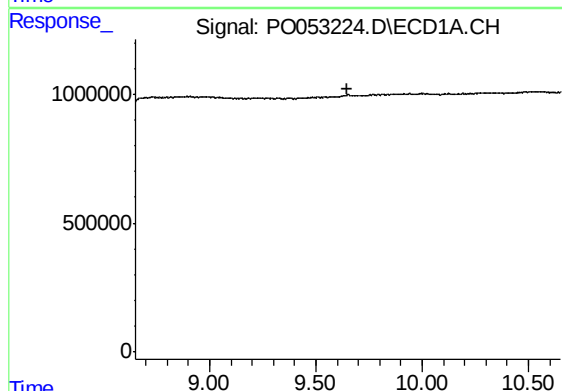


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.651 min
Response: 0
Conc: N.D.

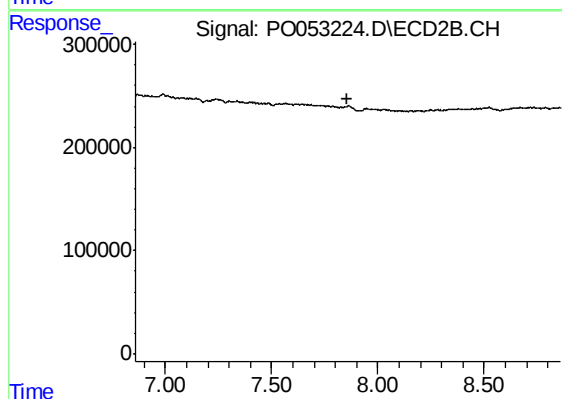

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 7.859 min
Response: 0
Conc: N.D.

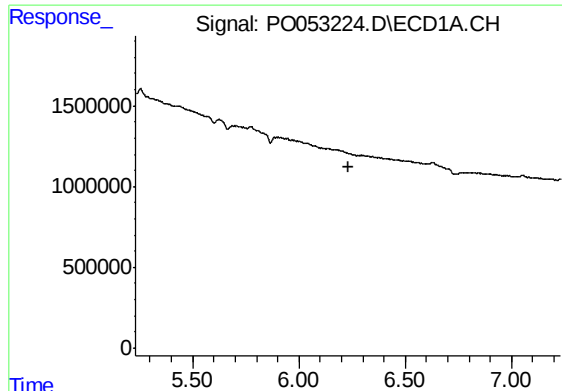

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

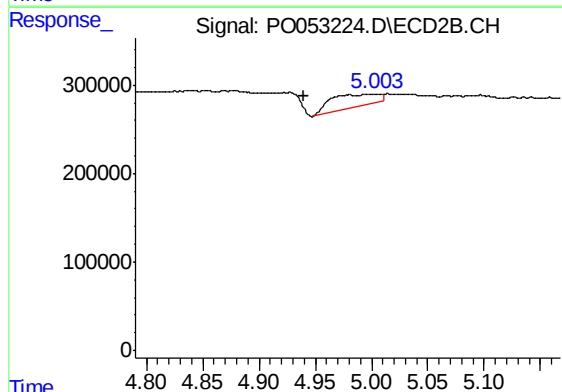


#20 AR-1242-5

R.T.: 4.997 min
Delta R.T.: 0.057 min
Response: 436842
Conc: 57.34 ng/ml

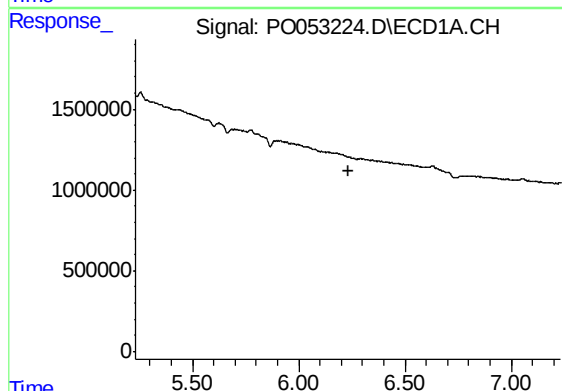


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

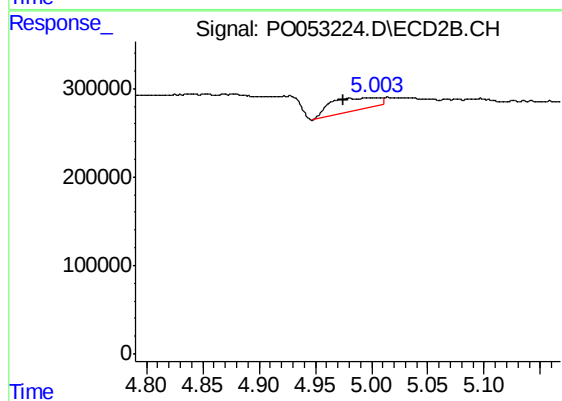

#25 AR-1248-5


R.T.: 4.997 min
Delta R.T.: 0.021 min
Response: 436842
Conc: 43.54 ng/ml

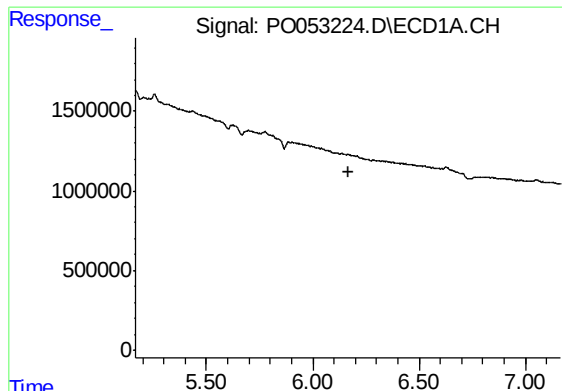

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

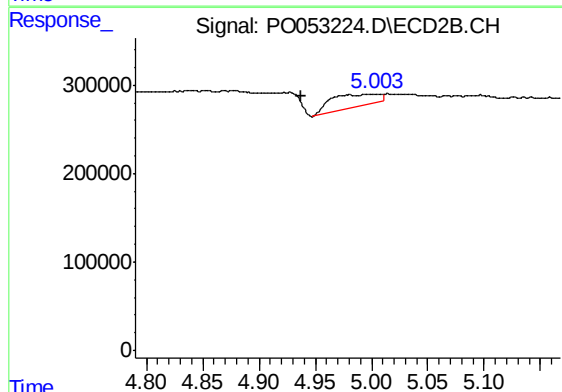


#26 AR-1254-1

R.T.: 4.997 min
Delta R.T.: 0.059 min
Response: 436842
Conc: 26.65 ng/ml

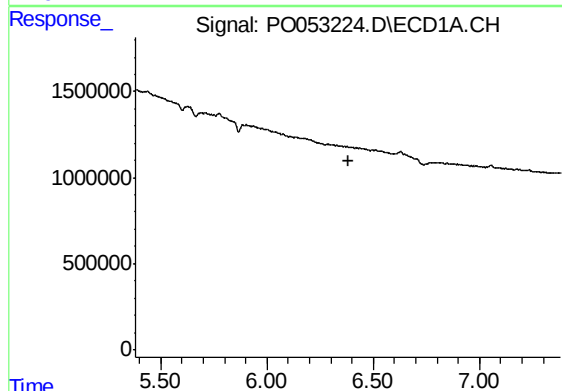


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.381 min
Response: 0
Conc: N.D.

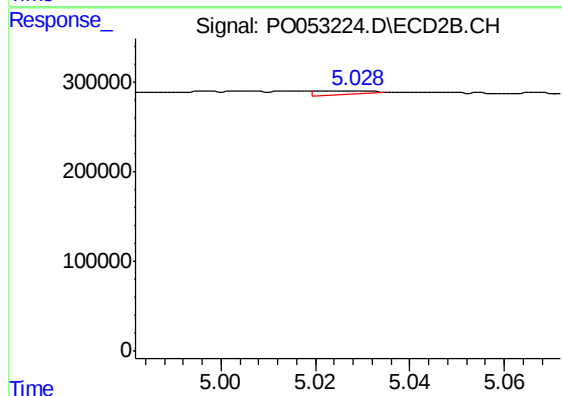

#27 AR-1254-2


R.T.: 5.028 min
Delta R.T.: -0.049 min
Response: 24726
Conc: 1.76 ng/ml

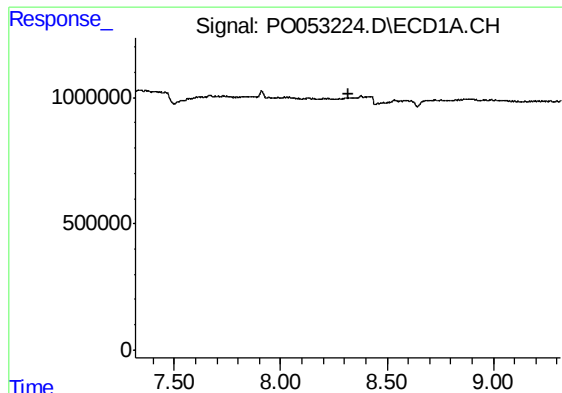

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

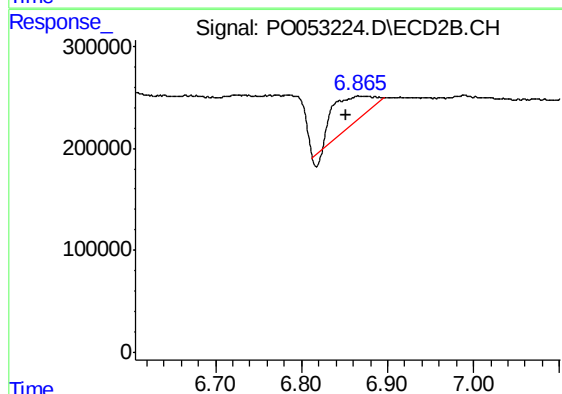


#38 AR-1262-3

R.T.: 6.865 min
Delta R.T.: 0.014 min
Response: 811300
Conc: 62.65 ng/ml

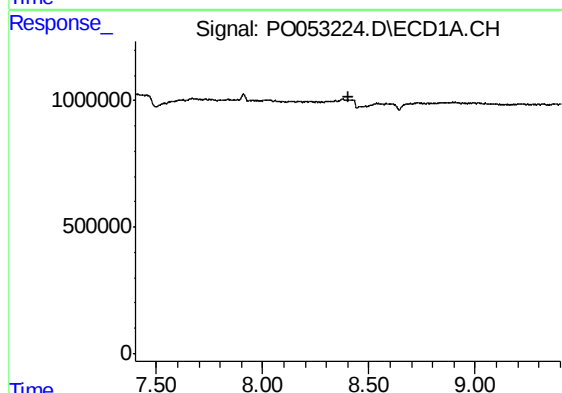


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.402 min
Response: 0
Conc: N.D.

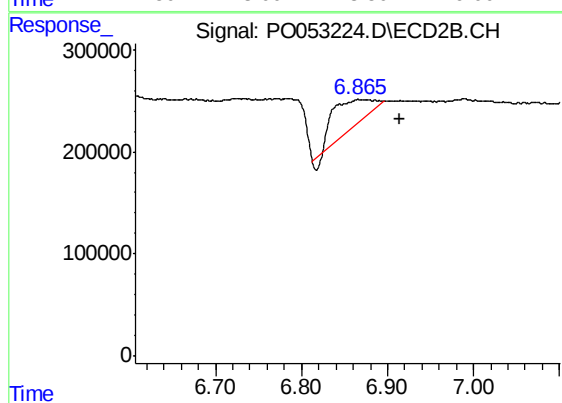

#39 AR-1262-4


R.T.: 6.865 min
Delta R.T.: -0.048 min
Response: 811300
Conc: 33.42 ng/ml

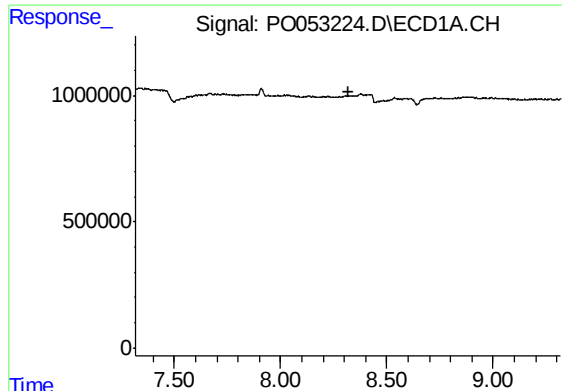

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
PURGE-WATER

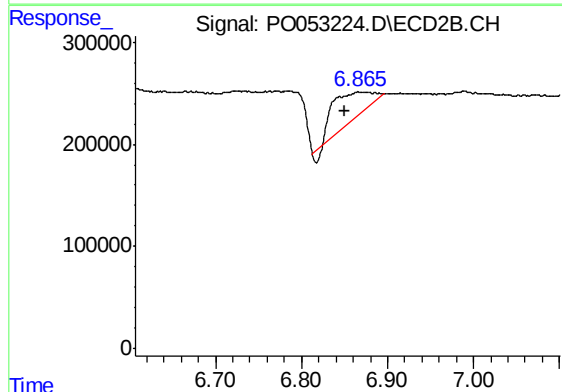


#41 AR-1268-1

R.T.: 6.865 min
Delta R.T.: 0.015 min
Response: 811300
Conc: 18.67 ng/ml

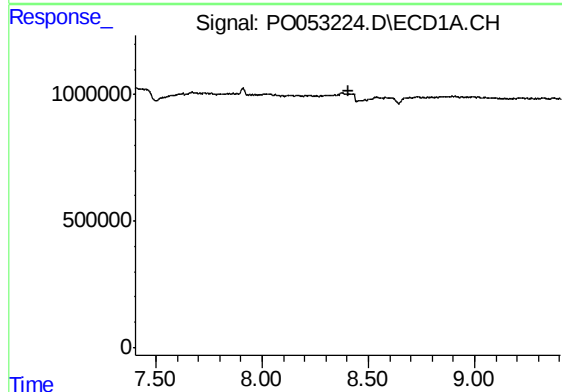

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.404 min
Response: 0
Conc: N.D.

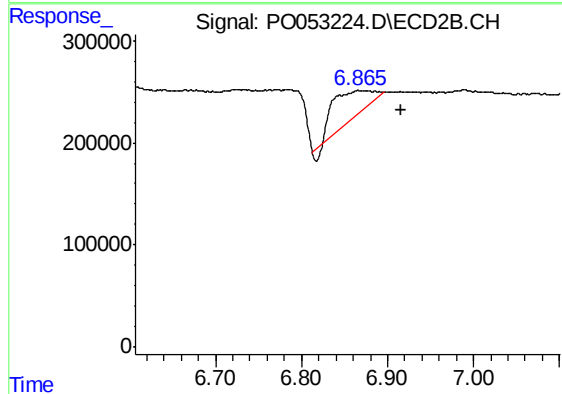

#42 AR-1268-2

R.T.: 6.865 min
Delta R.T.: -0.050 min
Response: 811300
Conc: 19.73 ng/ml