

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 5:22
 Operator : SM/SJ
 Sample : K1034-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:02:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.178	3.212	36545940	5166205	27.931	23.023
2)	SA Decachlor...	9.650	7.861	17111336	5726999	21.596	22.279
Target Compounds							
9)	L2 AR-1221-2	4.479	0.000	219644	0	25.430	N.D. #
10)	L2 AR-1221-3	0.000	3.607	0	372014	N.D.	65.358 #
11)	L3 AR-1232-1	0.000	3.607	0	372014	N.D.	79.098 #
29)	L6 AR-1254-4	0.000	5.704	0	974817	N.D.	64.309 #
30)	L6 AR-1254-5	0.000	6.065	0	234976	N.D.	11.738 #
31)	L7 AR-1260-1	6.897	5.572	2583932	159047	57.626	10.361 #
32)	L7 AR-1260-2	7.155	5.704	518891	974817	9.343	50.937 #
34)	L7 AR-1260-4	7.762	6.372	693735	614221	17.844	53.097 #
35)	L7 AR-1260-5	0.000	6.544	0	365144	N.D.	12.675 #
36)	L8 AR-1262-1	0.000	6.065	0	234976	N.D.	12.008 #
37)	L8 AR-1262-2	0.000	6.544	0	365144	N.D.	10.996 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
Data File : P0053234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 5:22
Operator : SM/SJ
Sample : K1034-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:02:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

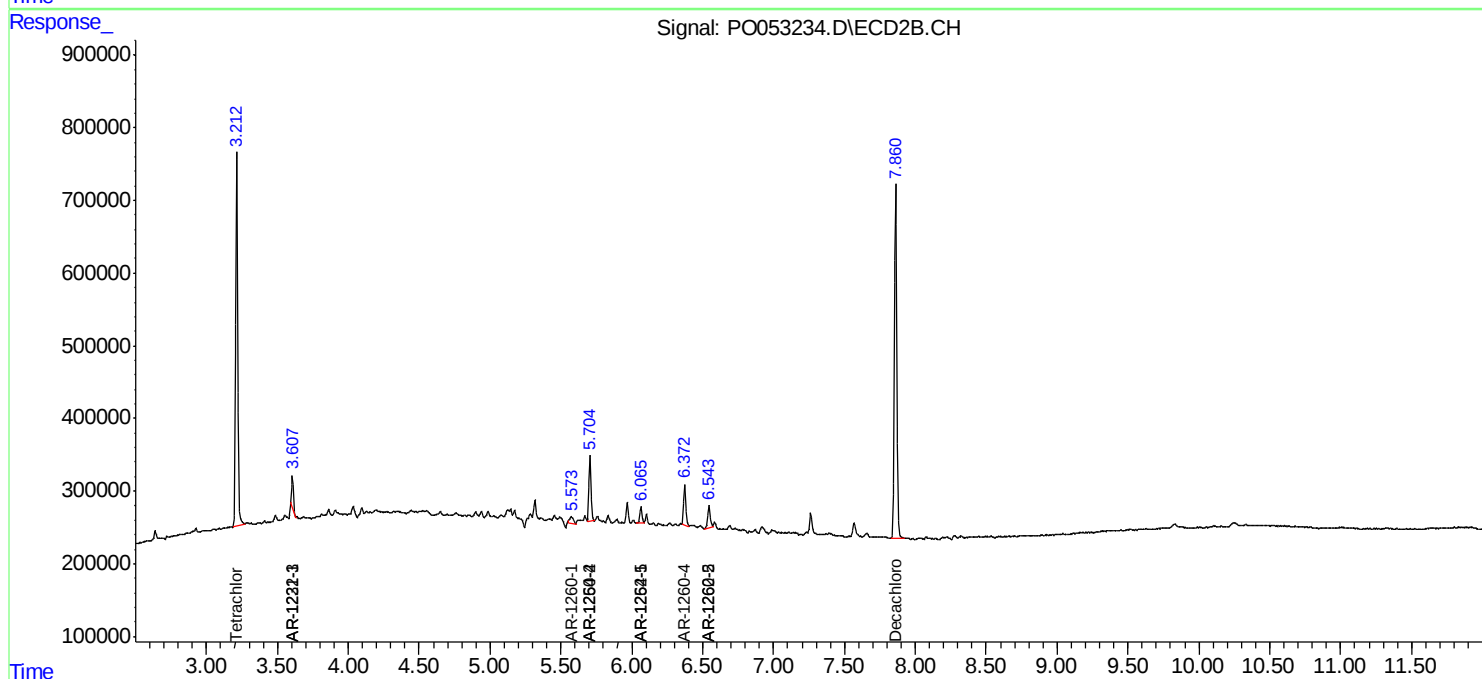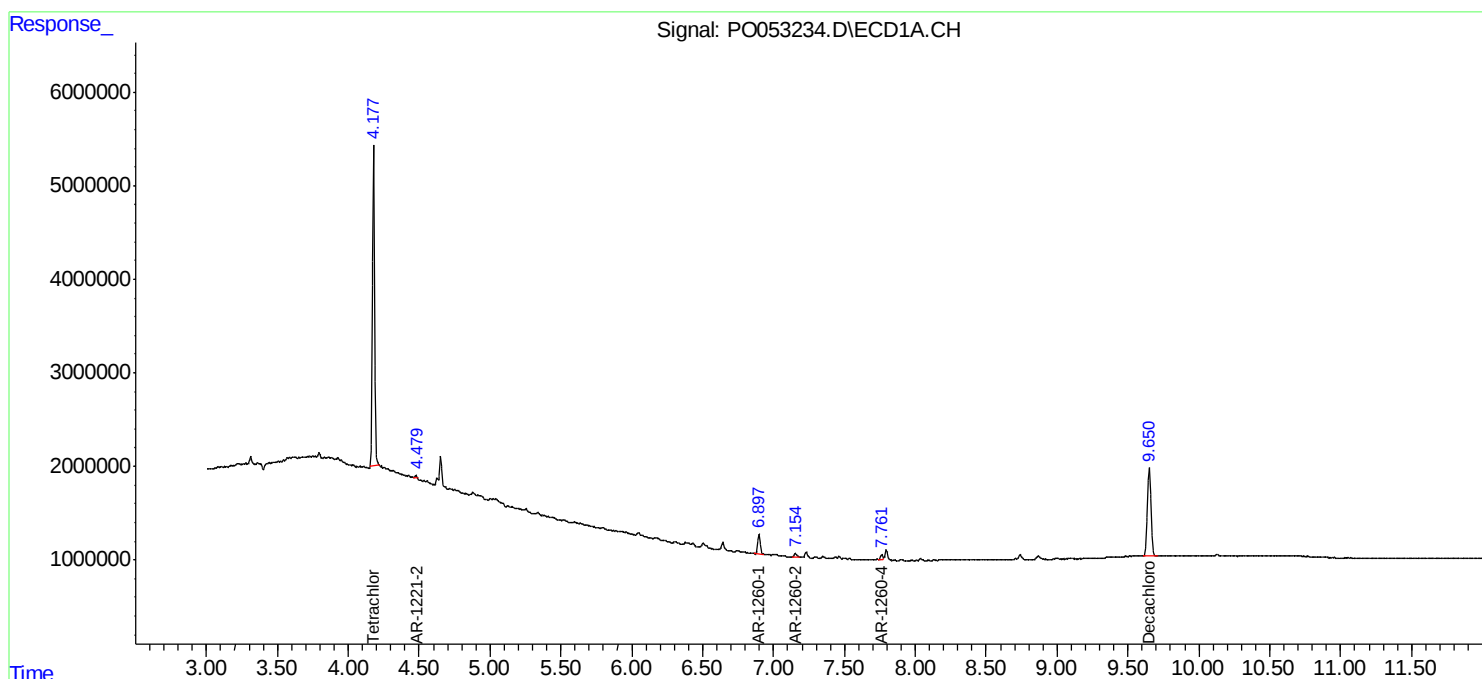


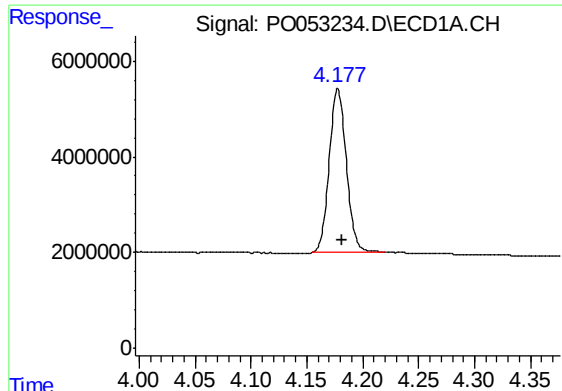

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: -0.003 min
Response: 36545940
Conc: 27.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

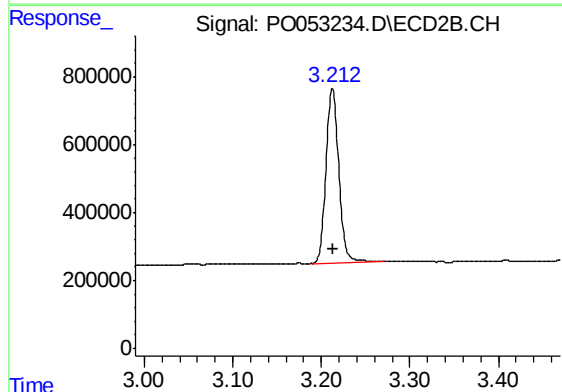


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.001 min
Response: 5166205
Conc: 23.02 ng/ml

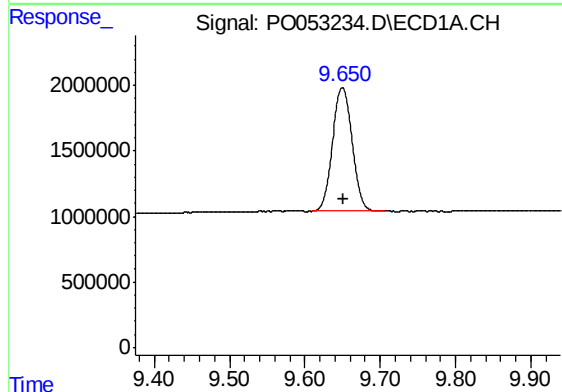


#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 17111336
Conc: 21.60 ng/ml

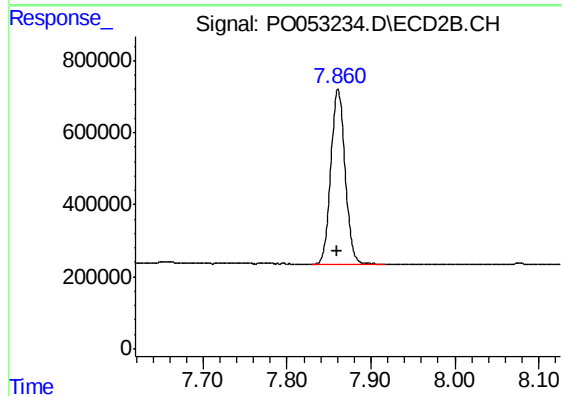

#2 Decachlorobiphenyl


R.T.: 7.861 min
Delta R.T.: 0.002 min
Response: 5726999
Conc: 22.28 ng/ml

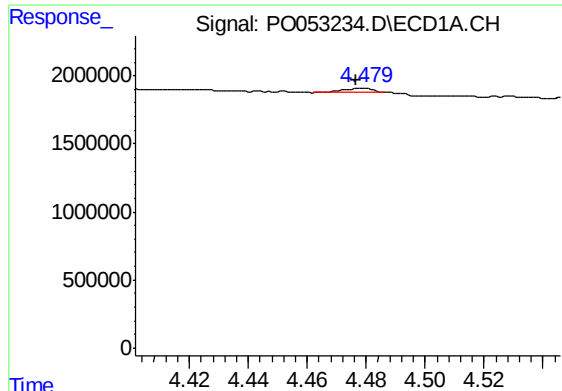

#9 AR-1221-2


R.T.: 4.479 min
Delta R.T.: 0.003 min
Response: 219644
Conc: 25.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

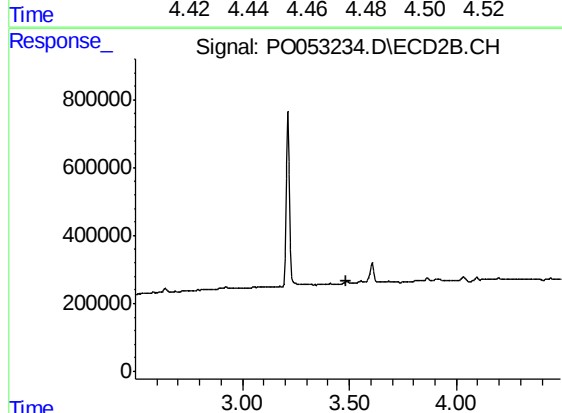


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

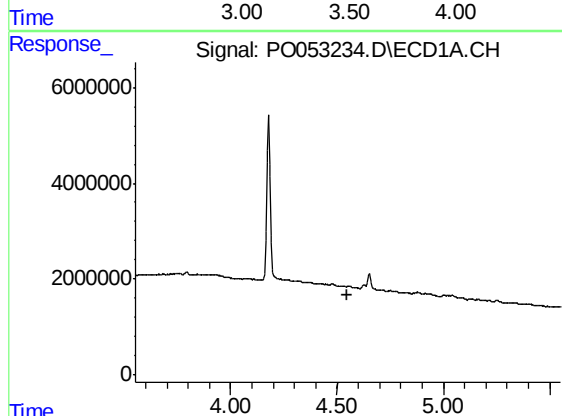


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

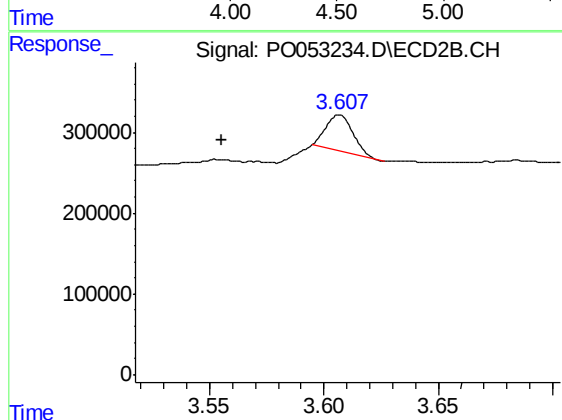

#10 AR-1221-3


R.T.: 3.607 min
Delta R.T.: 0.051 min
Response: 372014
Conc: 65.36 ng/ml

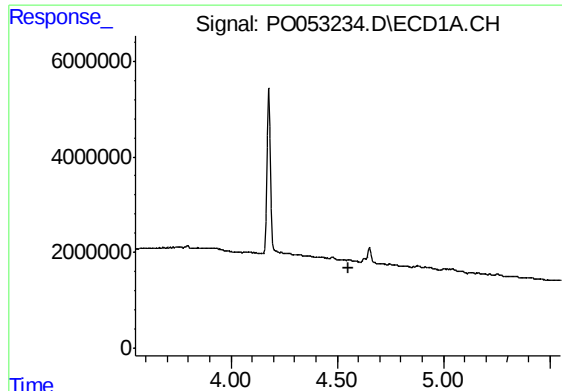

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

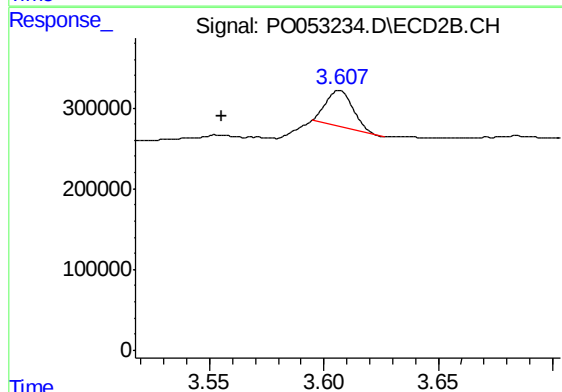


#11 AR-1232-1

R.T.: 3.607 min
Delta R.T.: 0.051 min
Response: 372014
Conc: 79.10 ng/ml

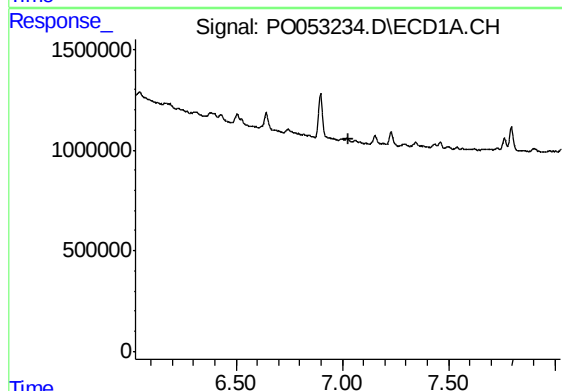


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

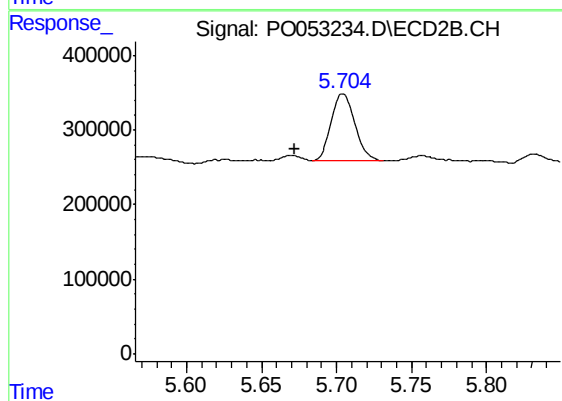

#29 AR-1254-4


R.T.: 5.704 min
Delta R.T.: 0.033 min
Response: 974817
Conc: 64.31 ng/ml

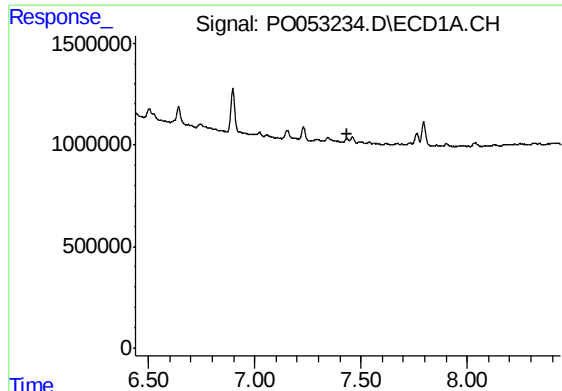

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

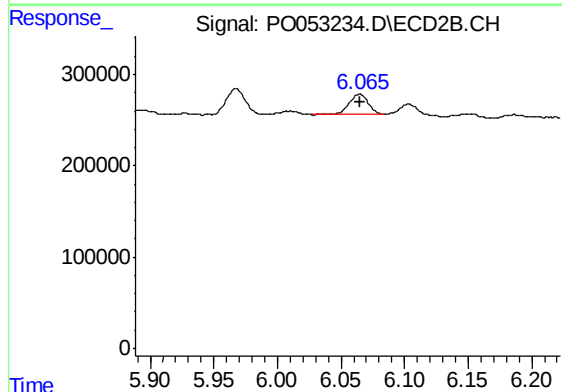


#30 AR-1254-5

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 234976
Conc: 11.74 ng/ml

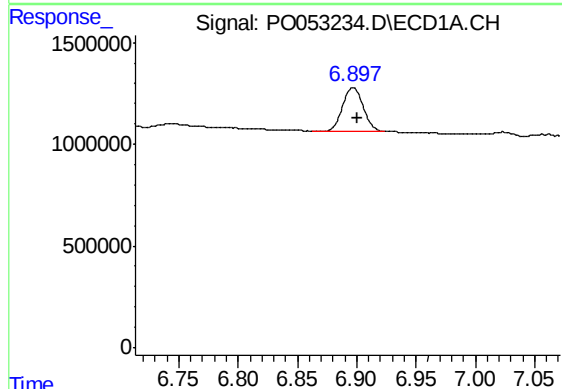


#31 AR-1260-1

R.T.: 6.897 min
Delta R.T.: -0.004 min
Response: 2583932
Conc: 57.63 ng/ml

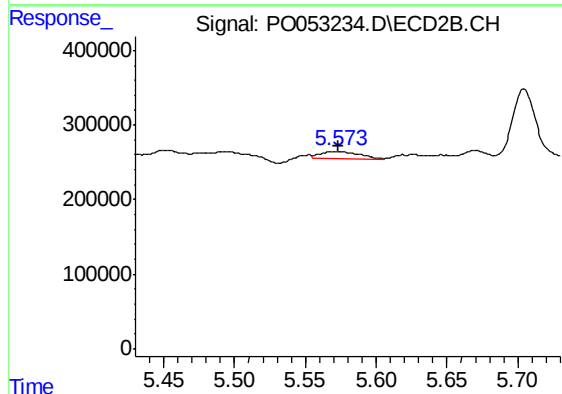

#31 AR-1260-1


R.T.: 5.572 min
Delta R.T.: -0.001 min
Response: 159047
Conc: 10.36 ng/ml

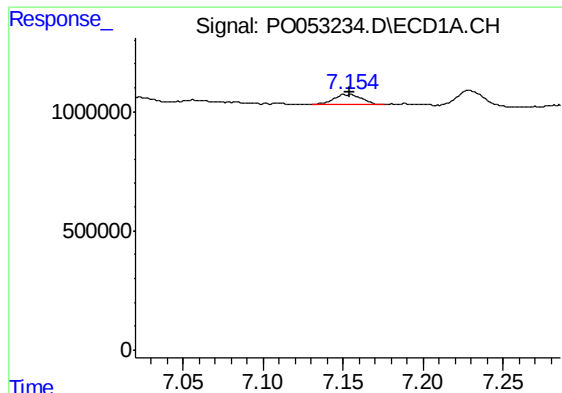

#32 AR-1260-2


R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 518891
Conc: 9.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

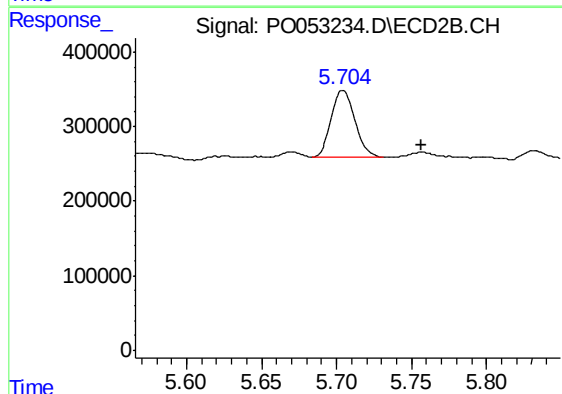


#32 AR-1260-2

R.T.: 5.704 min
Delta R.T.: -0.052 min
Response: 974817
Conc: 50.94 ng/ml

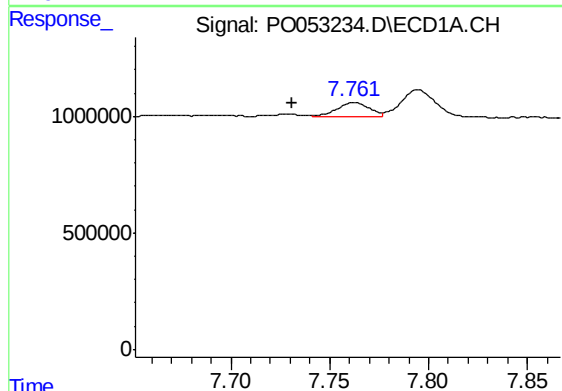


#34 AR-1260-4

R.T.: 7.762 min
Delta R.T.: 0.031 min
Response: 693735
Conc: 17.84 ng/ml

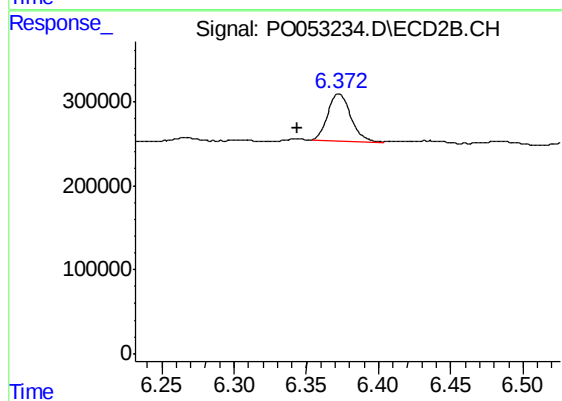

#34 AR-1260-4


R.T.: 6.372 min
Delta R.T.: 0.029 min
Response: 614221
Conc: 53.10 ng/ml

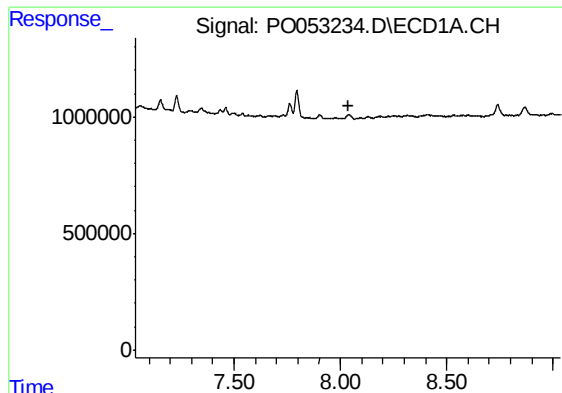

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

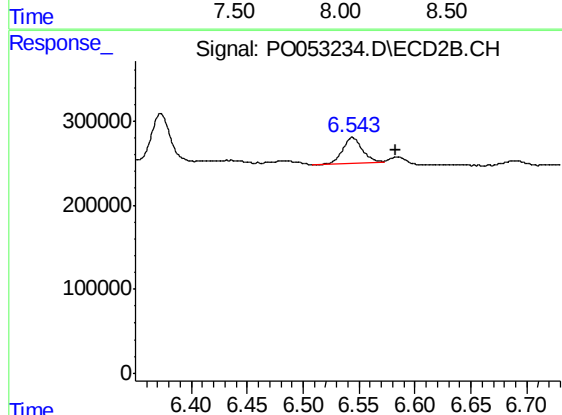


#35 AR-1260-5

R.T.: 6.544 min
Delta R.T.: -0.039 min
Response: 365144
Conc: 12.68 ng/ml

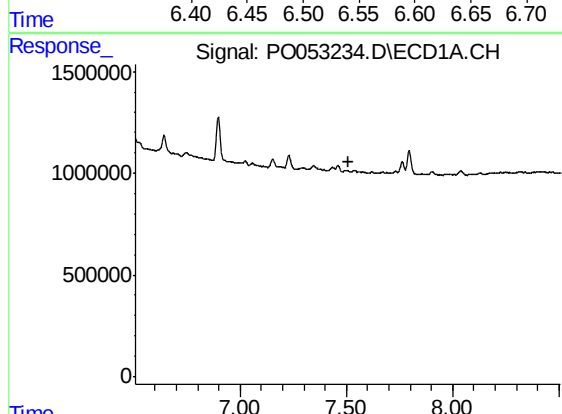


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

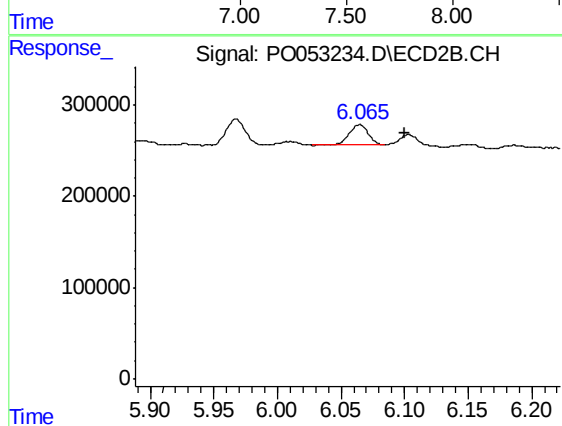

#36 AR-1262-1


R.T.: 6.065 min
Delta R.T.: -0.036 min
Response: 234976
Conc: 12.01 ng/ml

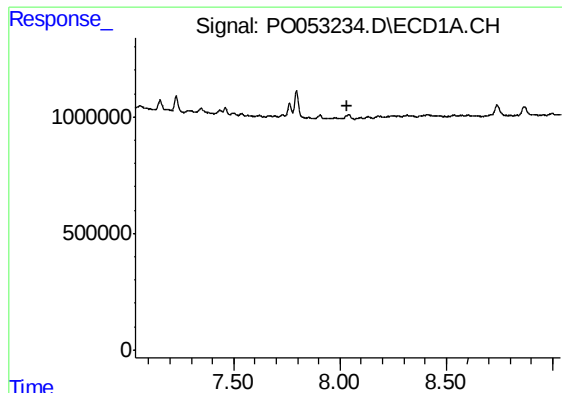

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

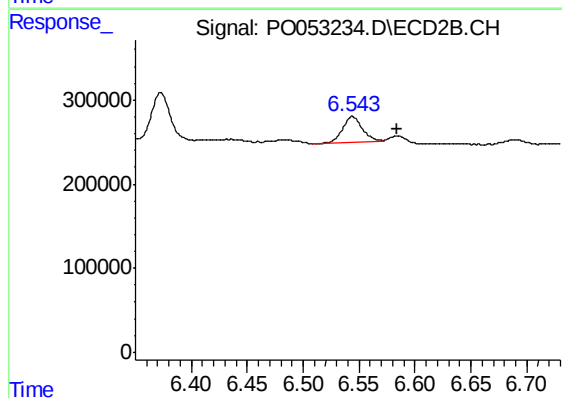

#37 AR-1262-2

R.T.: 6.544 min
Delta R.T.: -0.041 min
Response: 365144
Conc: 11.00 ng/ml