

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053235.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 5:39
 Operator : SM/SJ
 Sample : K1034-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:03:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.178	3.212	37346023	5183845	28.543	23.102
2)	SA Decachlor...	9.650	7.860	18179220	6040747	22.944	23.499
Target Compounds							
9)	L2 AR-1221-2	4.476	0.000	530543	0	61.426	N.D. #
10)	L2 AR-1221-3	0.000	3.570	0	177407	N.D.	31.168 #
11)	L3 AR-1232-1	0.000	3.570	0	177407	N.D.	37.721 #
12)	L3 AR-1232-2	5.039	0.000	1374904	0	121.336	N.D. #
27)	L6 AR-1254-2	6.428	5.124	510695	296871	8.612	21.158 #
29)	L6 AR-1254-4	0.000	5.704	0	246670	N.D.	16.273 #
31)	L7 AR-1260-1	6.897	0.000	684248	0	15.260	N.D. #
32)	L7 AR-1260-2	0.000	5.704	0	246670	N.D.	12.889 #
35)	L7 AR-1260-5	0.000	6.542	0	132058	N.D.	4.584 #
37)	L8 AR-1262-2	0.000	6.542	0	132058	N.D.	3.977 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053235.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 5:39
Operator : SM/SJ
Sample : K1034-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:03:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

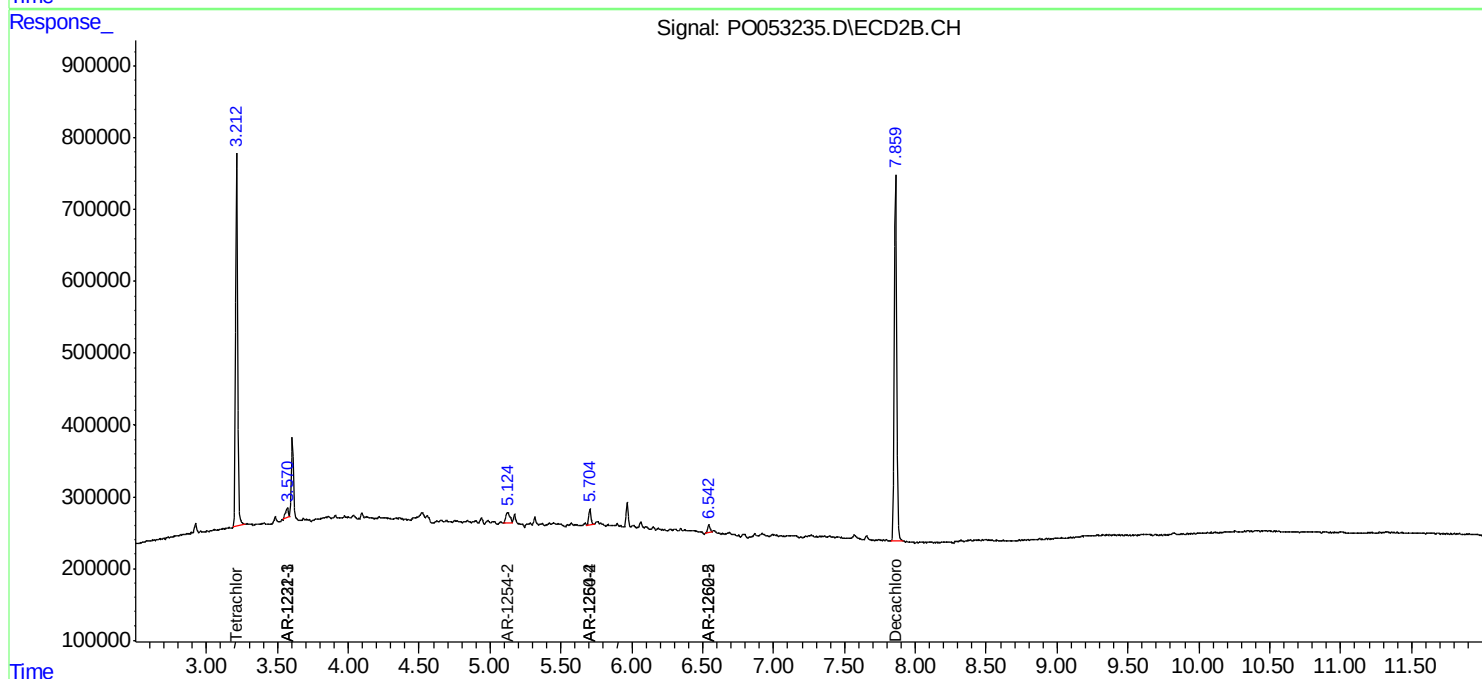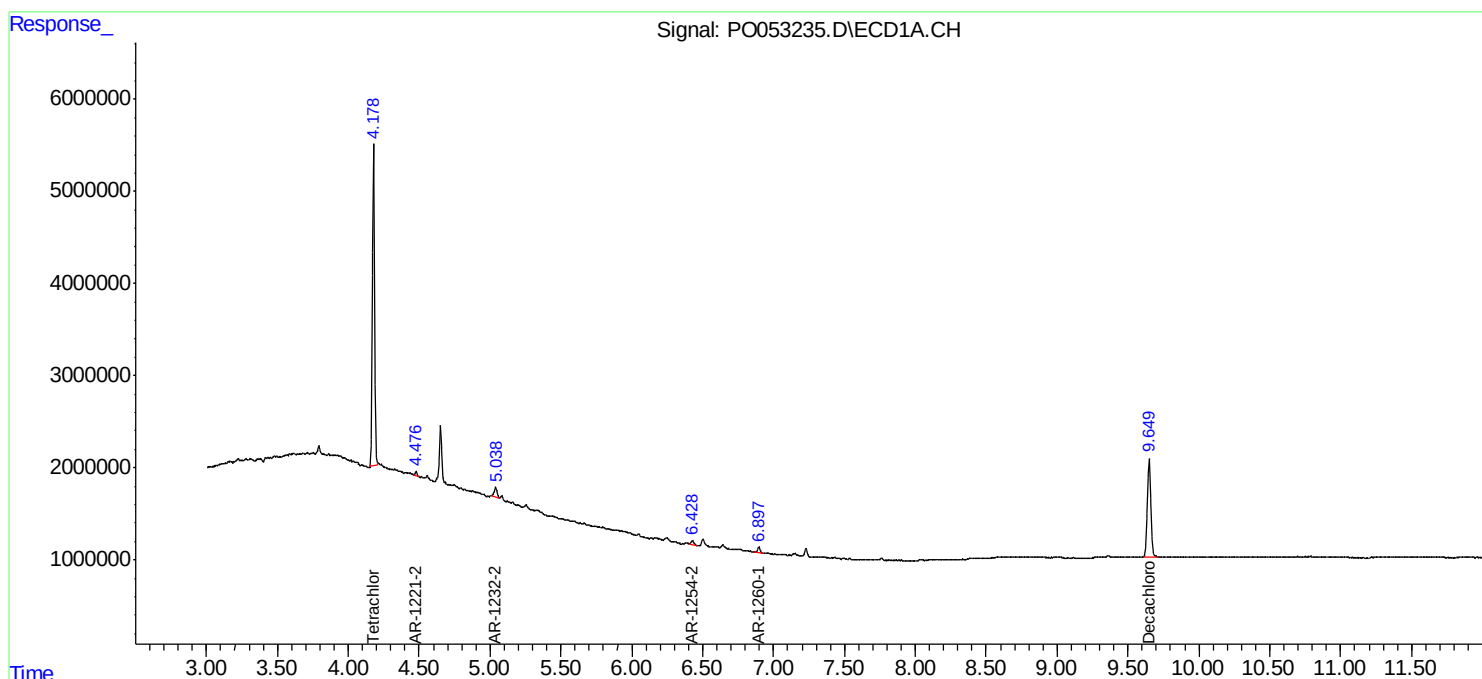


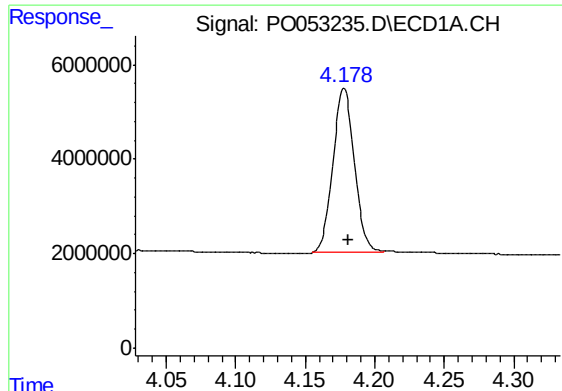

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: -0.003 min
Response: 37346023
Conc: 28.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

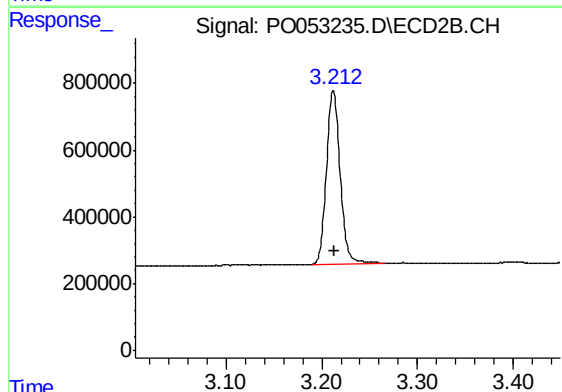


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.001 min
Response: 5183845
Conc: 23.10 ng/ml

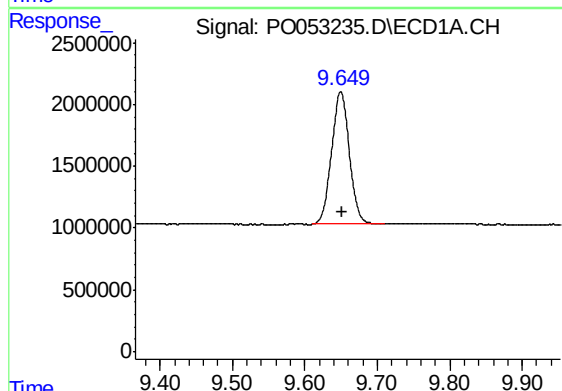


#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 18179220
Conc: 22.94 ng/ml

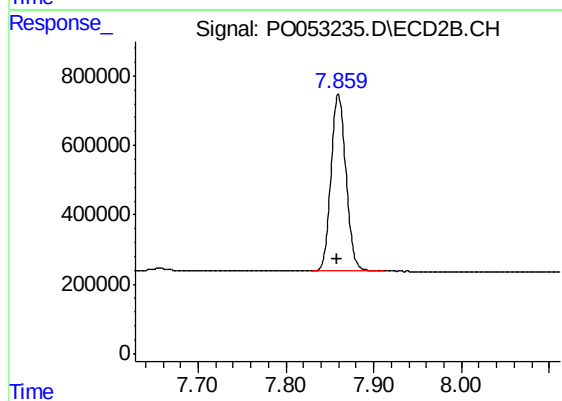

#2 Decachlorobiphenyl


R.T.: 7.860 min
Delta R.T.: 0.000 min
Response: 6040747
Conc: 23.50 ng/ml

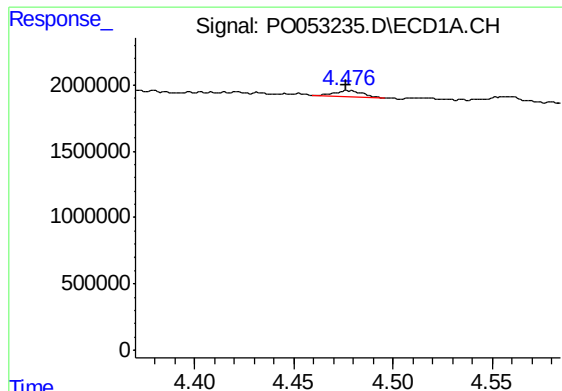

#9 AR-1221-2


R.T.: 4.476 min
Delta R.T.: 0.000 min
Response: 530543
Conc: 61.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

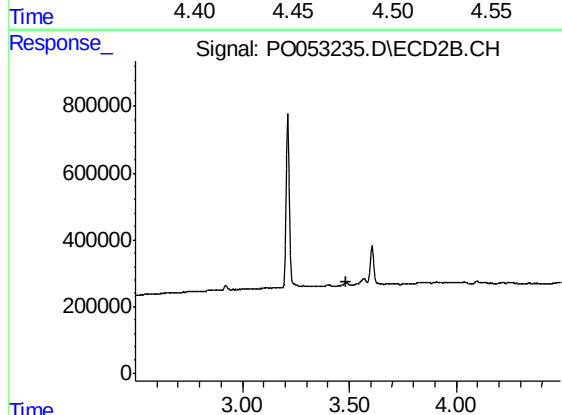


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

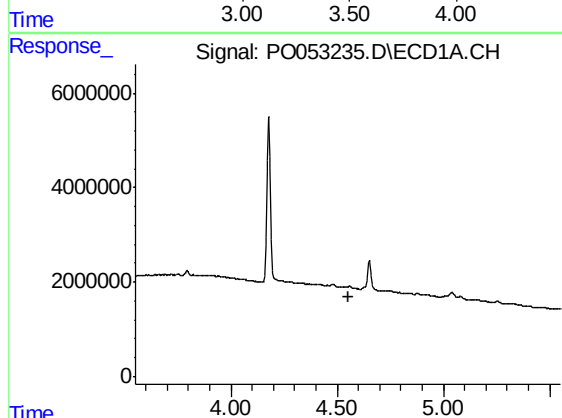


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

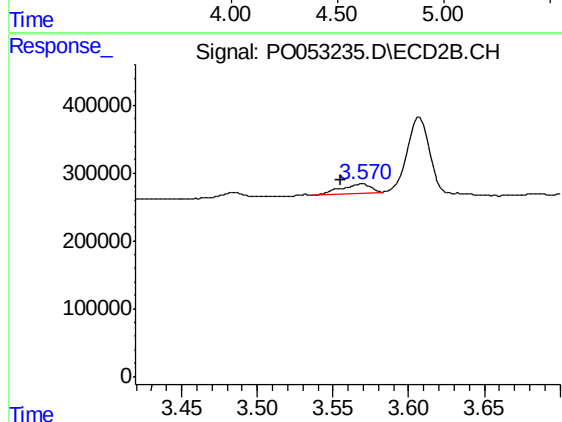

#10 AR-1221-3


R.T.: 3.570 min
Delta R.T.: 0.015 min
Response: 177407
Conc: 31.17 ng/ml

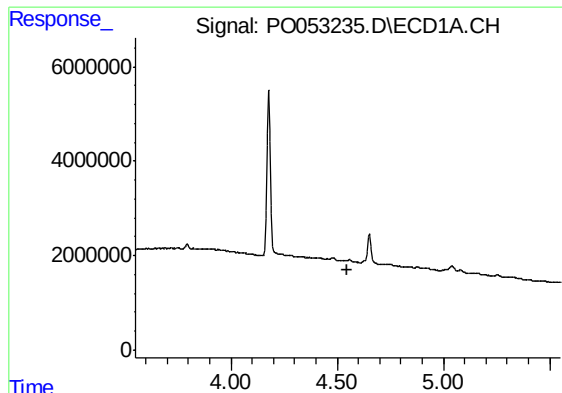

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

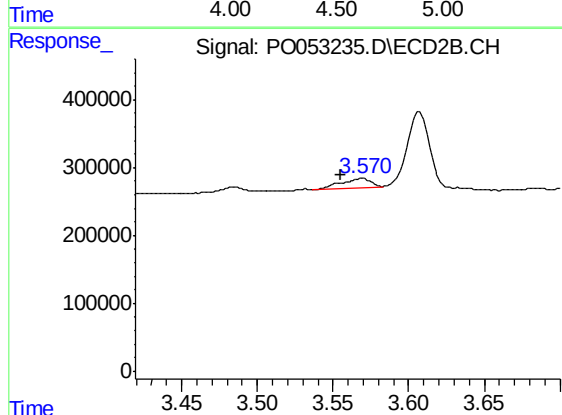


#11 AR-1232-1

R.T.: 3.570 min
Delta R.T.: 0.015 min
Response: 177407
Conc: 37.72 ng/ml

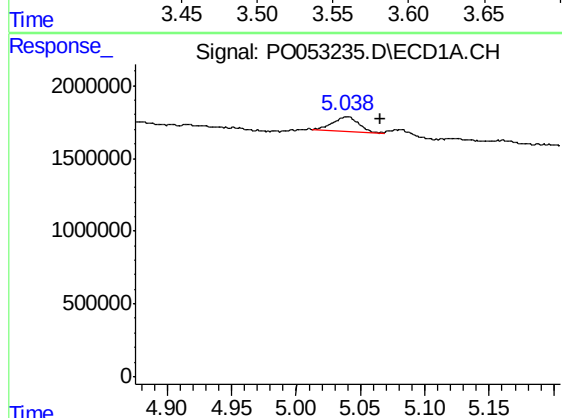


#12 AR-1232-2

R.T.: 5.039 min
Delta R.T.: -0.027 min
Response: 1374904
Conc: 121.34 ng/ml

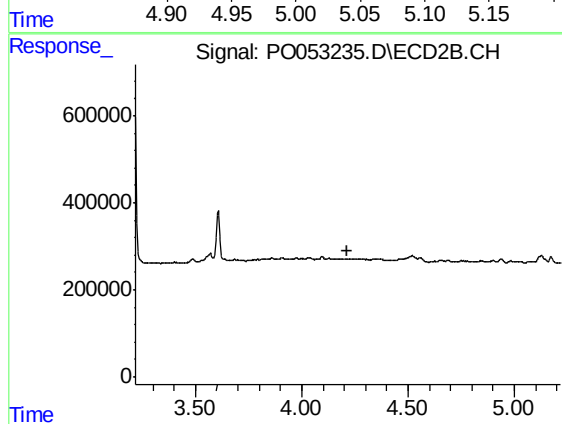

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

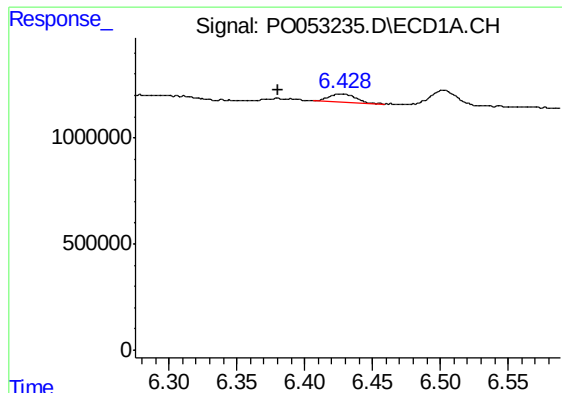

#27 AR-1254-2


R.T.: 6.428 min
Delta R.T.: 0.047 min
Response: 510695
Conc: 8.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

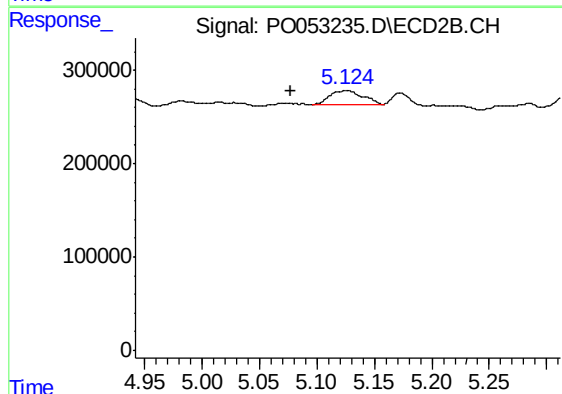


#27 AR-1254-2

R.T.: 5.124 min
Delta R.T.: 0.046 min
Response: 296871
Conc: 21.16 ng/ml

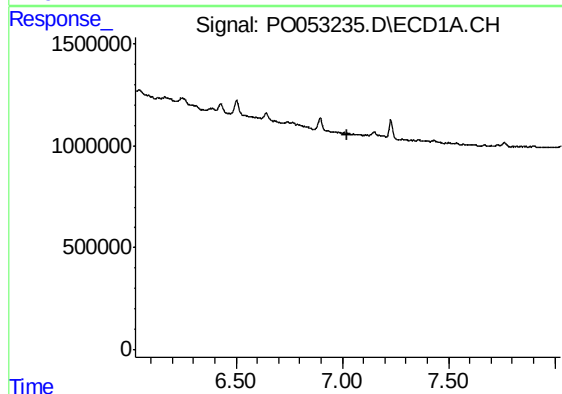


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

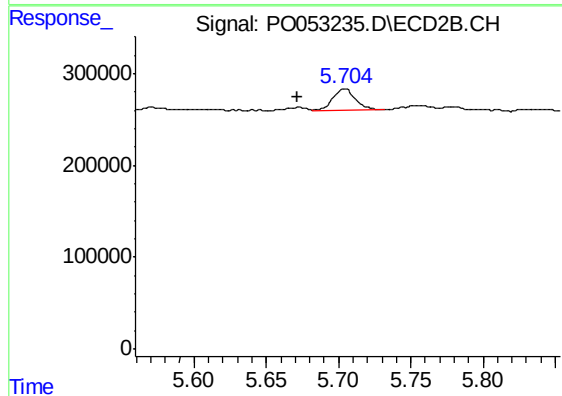

#29 AR-1254-4


R.T.: 5.704 min
Delta R.T.: 0.032 min
Response: 246670
Conc: 16.27 ng/ml

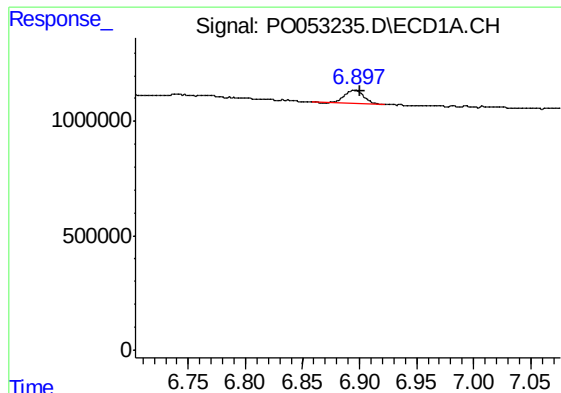

#31 AR-1260-1


R.T.: 6.897 min
Delta R.T.: -0.004 min
Response: 684248
Conc: 15.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

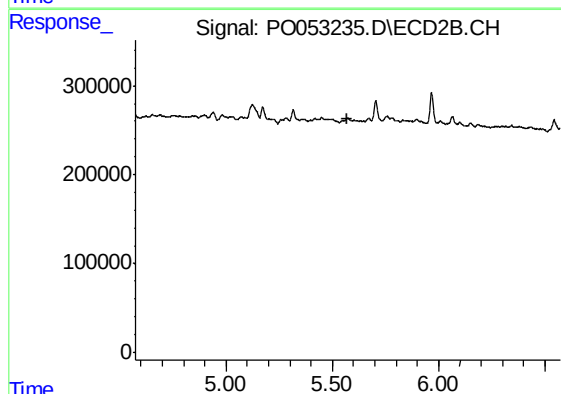


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.573 min
Response: 0
Conc: N.D.

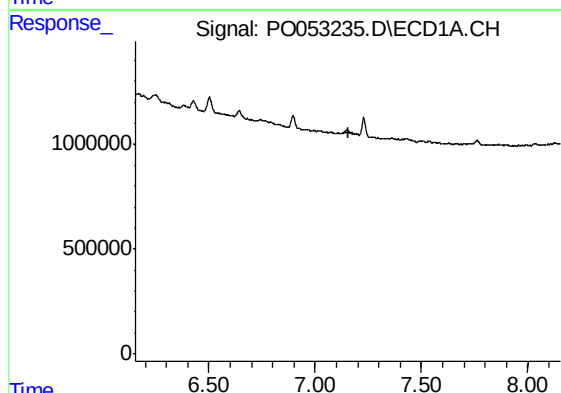


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

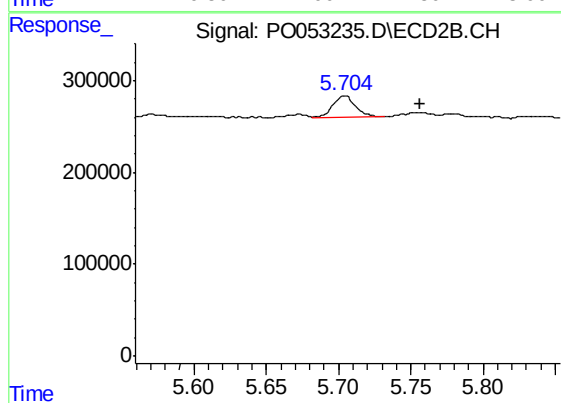

#32 AR-1260-2


R.T.: 5.704 min
Delta R.T.: -0.053 min
Response: 246670
Conc: 12.89 ng/ml

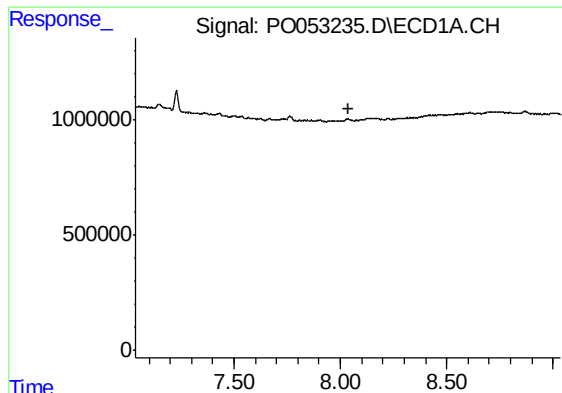

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

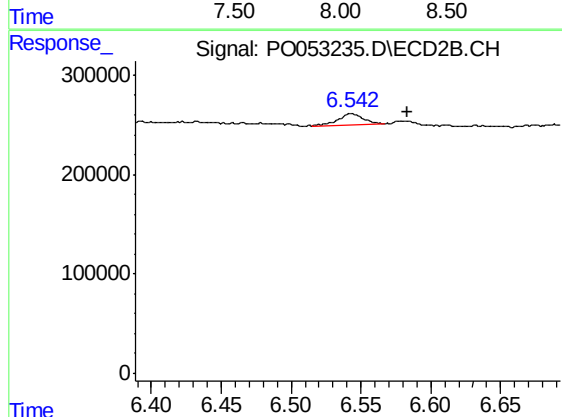


#35 AR-1260-5

R.T.: 6.542 min
Delta R.T.: -0.041 min
Response: 132058
Conc: 4.58 ng/ml

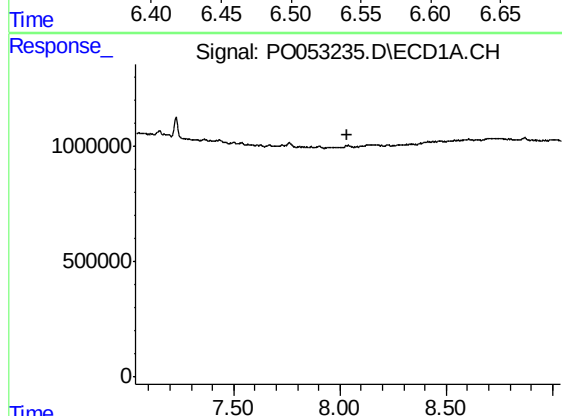

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.037 min
Response: 0
Conc: N.D.

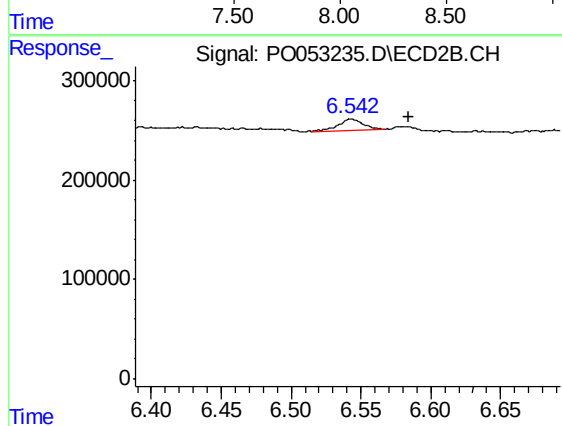

#37 AR-1262-2

R.T.: 6.542 min
Delta R.T.: -0.042 min
Response: 132058
Conc: 3.98 ng/ml