

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053236.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 5:55
 Operator : SM/SJ
 Sample : K1034-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:03:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.178	3.212	40114651	5631744	30.659	25.098
2)	SA Decachlor...	9.649	7.860	18177994	6126647	22.943	23.834
Target Compounds							
8)	L2 AR-1221-1	0.000	3.408	0	359297	N.D.	154.369 #
9)	L2 AR-1221-2	4.479	0.000	378159	0	43.783	N.D. #
10)	L2 AR-1221-3	0.000	3.607	0	465396	N.D.	81.764 #
11)	L3 AR-1232-1	0.000	3.607	0	465396	N.D.	98.953 #
12)	L3 AR-1232-2	5.101	0.000	287150	0	25.341	N.D. #
27)	L6 AR-1254-2	6.380	0.000	14062	0	0.237	N.D. #
28)	L6 AR-1254-3	6.742	5.451	285702	151048	4.633	6.695 #
29)	L6 AR-1254-4	0.000	5.704	0	207782	N.D.	13.707 #
30)	L6 AR-1254-5	7.434	6.064	404340	263822	8.908	13.178 #
31)	L7 AR-1260-1	6.897	5.570	651464	505040	14.529	32.902 #
32)	L7 AR-1260-2	7.152	5.756	672948	140672	12.116	7.351 #
34)	L7 AR-1260-4	7.763	6.372	967655	2240764	24.889	193.705 #
35)	L7 AR-1260-5	8.035	6.585	643702	222775	8.340	7.733
36)	L8 AR-1262-1	0.000	6.064	0	263822	N.D.	13.482 #
37)	L8 AR-1262-2	8.035	6.585	643702	222775	6.898	6.709
38)	L8 AR-1262-3	0.000	6.914	0	395150	N.D.	30.516 #
39)	L8 AR-1262-4	0.000	6.914	0	395150	N.D.	16.276 #
41)	L9 AR-1268-1	0.000	6.914	0	395150	N.D.	9.095 #
42)	L9 AR-1268-2	0.000	6.914	0	395150	N.D.	9.608 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053236.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 5:55
Operator : SM/SJ
Sample : K1034-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:03:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

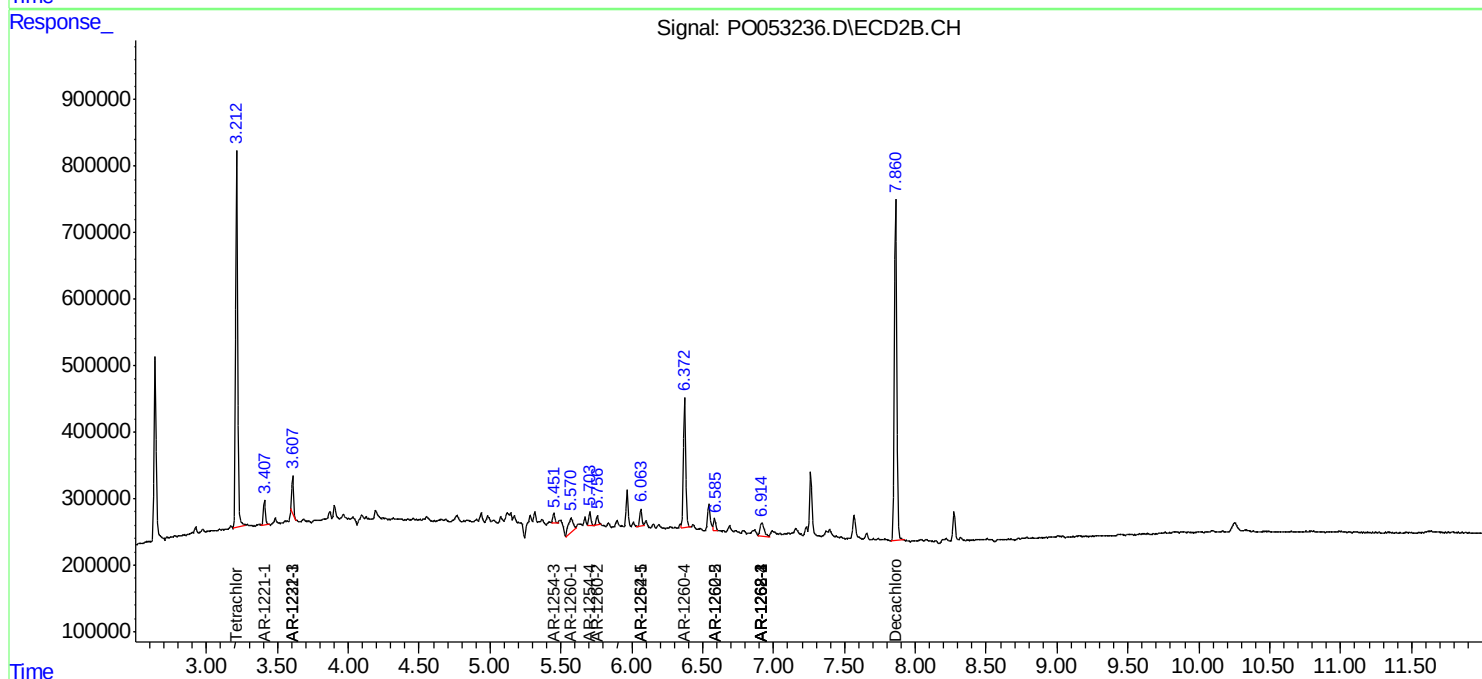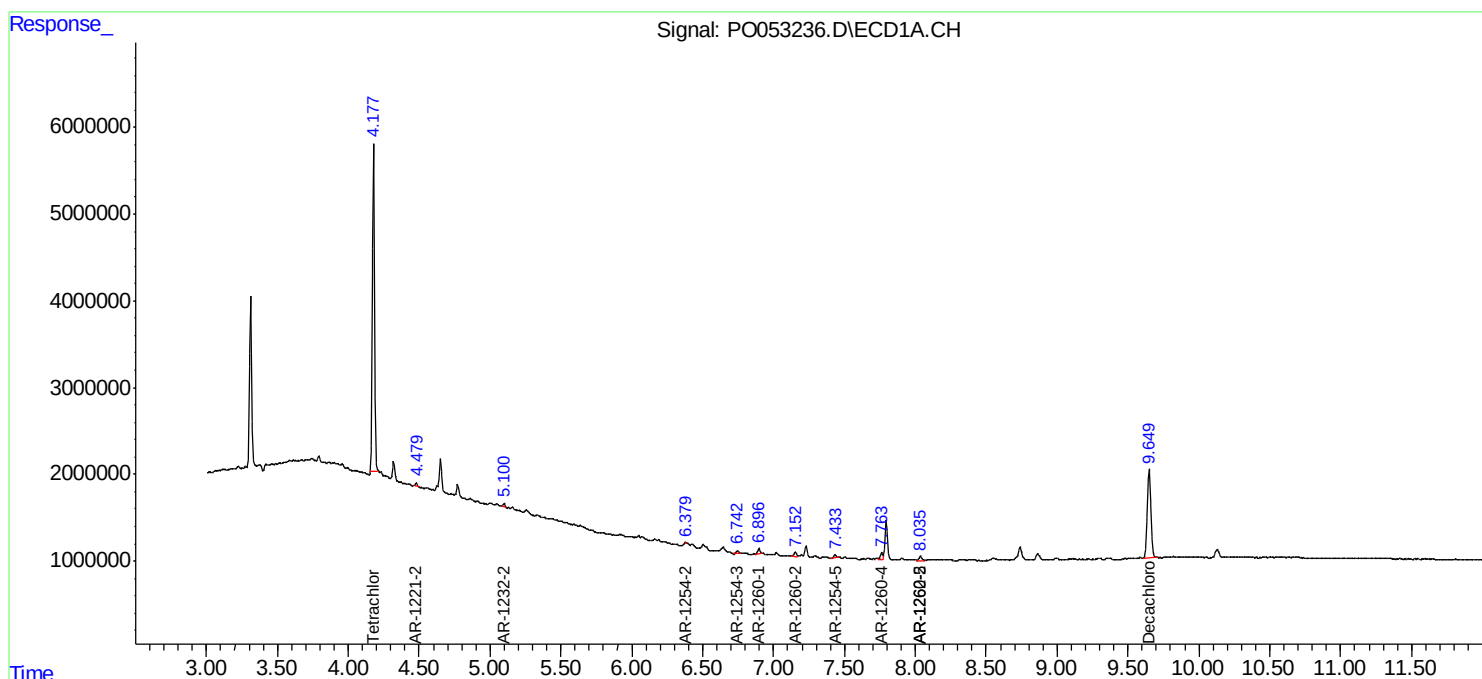


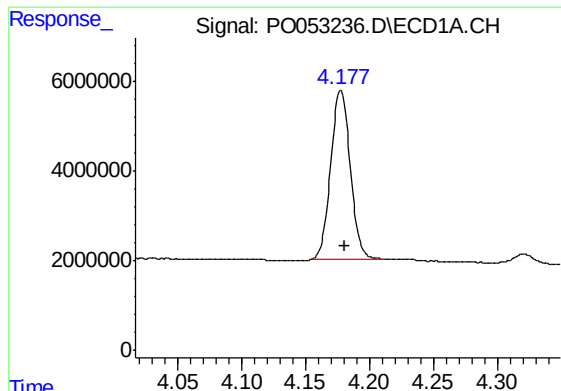

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: -0.003 min
Response: 40114651
Conc: 30.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

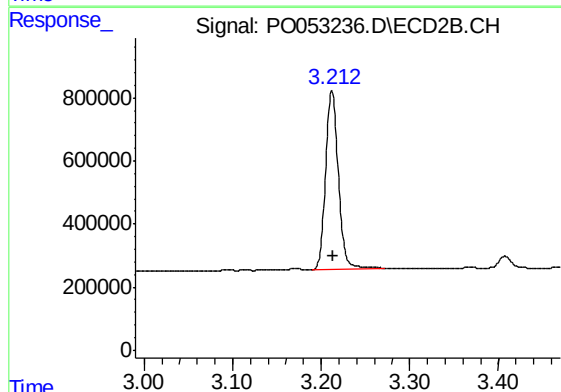


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 5631744
Conc: 25.10 ng/ml

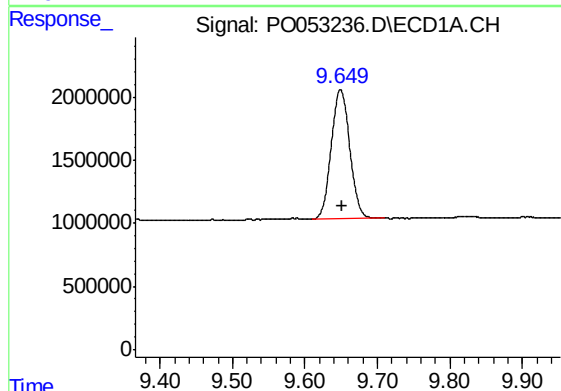


#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.002 min
Response: 18177994
Conc: 22.94 ng/ml

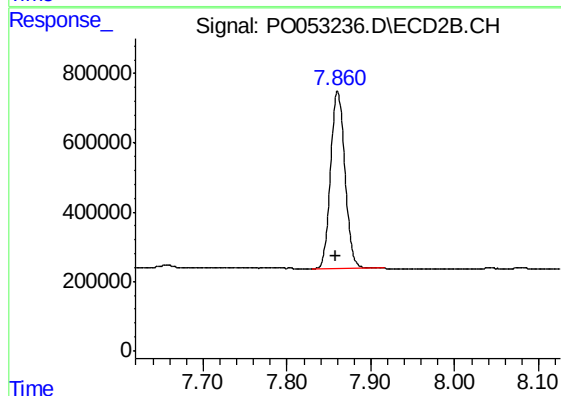

#2 Decachlorobiphenyl


R.T.: 7.860 min
Delta R.T.: 0.002 min
Response: 6126647
Conc: 23.83 ng/ml

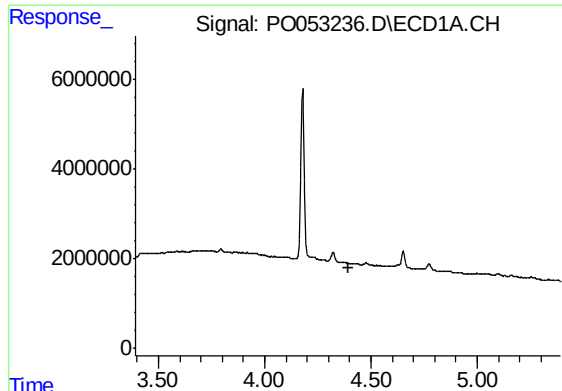

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

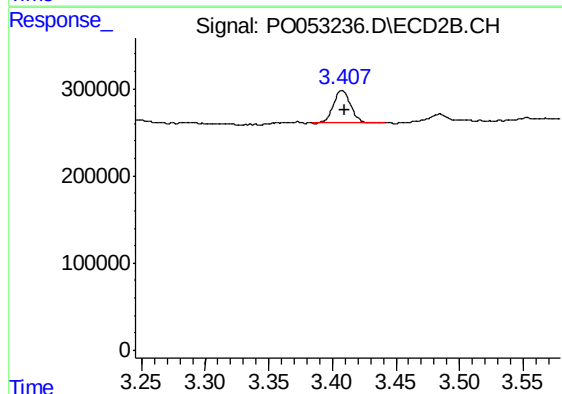


#8 AR-1221-1

R.T.: 3.408 min
Delta R.T.: -0.002 min
Response: 359297
Conc: 154.37 ng/ml

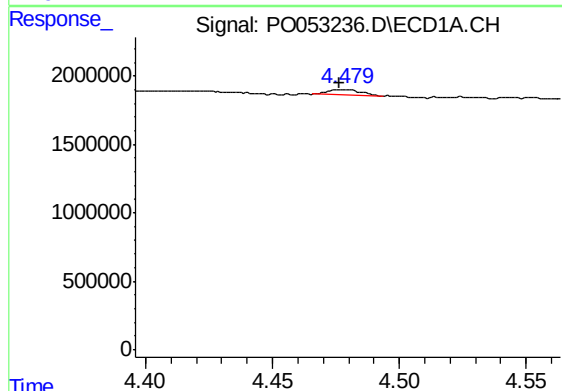


#9 AR-1221-2

R.T.: 4.479 min
Delta R.T.: 0.003 min
Response: 378159
Conc: 43.78 ng/ml

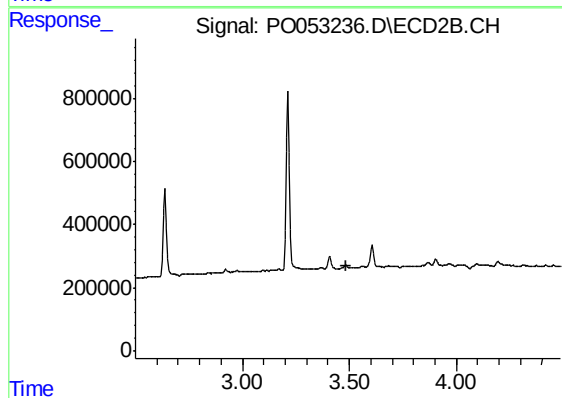

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

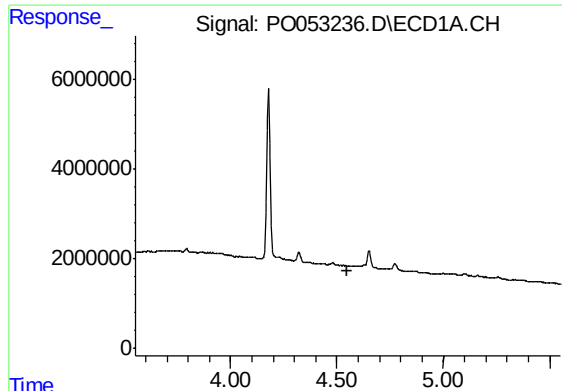

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

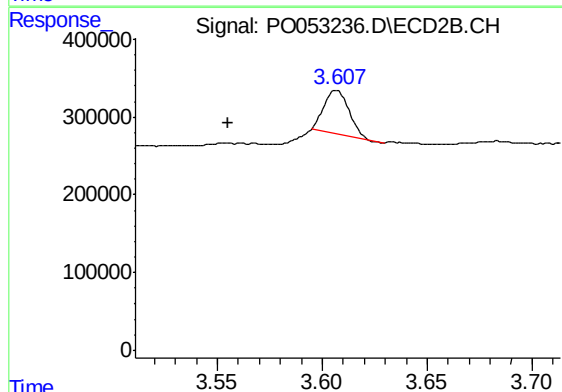


#10 AR-1221-3

R.T.: 3.607 min
Delta R.T.: 0.051 min
Response: 465396
Conc: 81.76 ng/ml

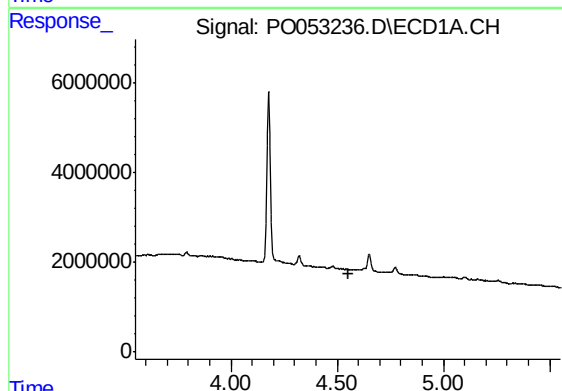


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

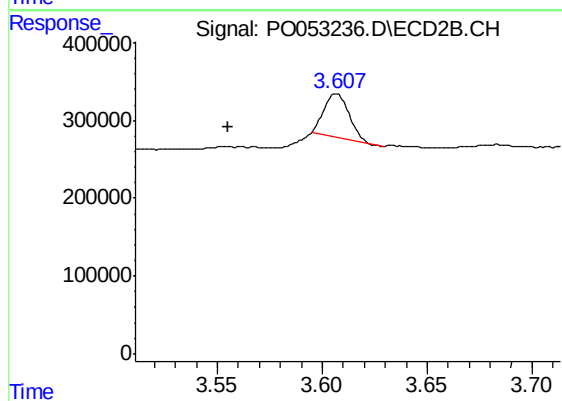

#11 AR-1232-1


R.T.: 3.607 min
Delta R.T.: 0.051 min
Response: 465396
Conc: 98.95 ng/ml

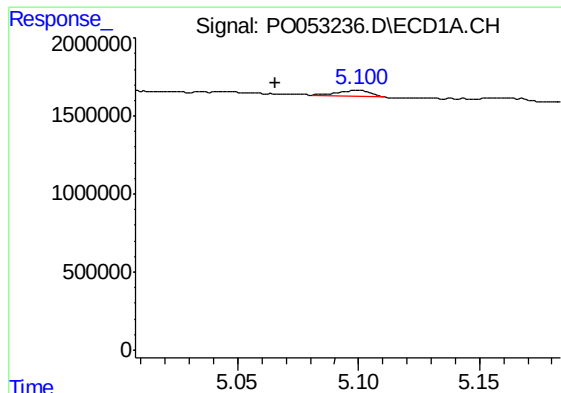

#12 AR-1232-2


R.T.: 5.101 min
Delta R.T.: 0.035 min
Response: 287150
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

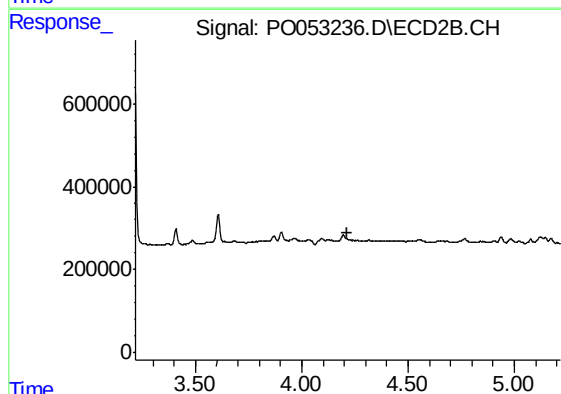


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

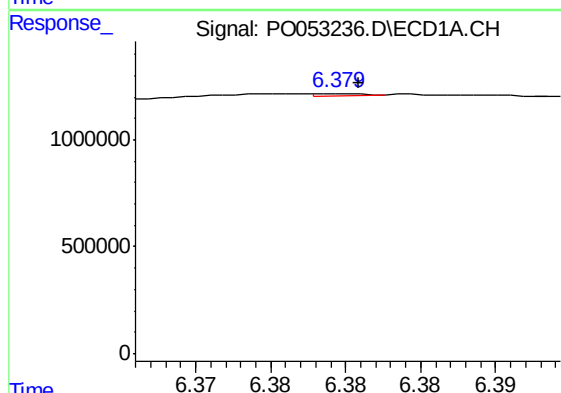


#27 AR-1254-2

R.T.: 6.380 min
Delta R.T.: -0.001 min
Response: 14062
Conc: 0.24 ng/ml

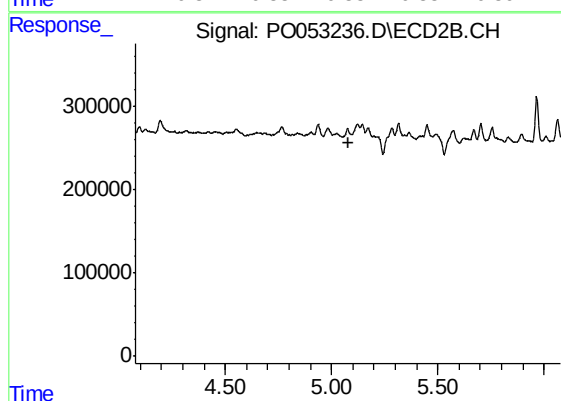

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.078 min
Response: 0
Conc: N.D.

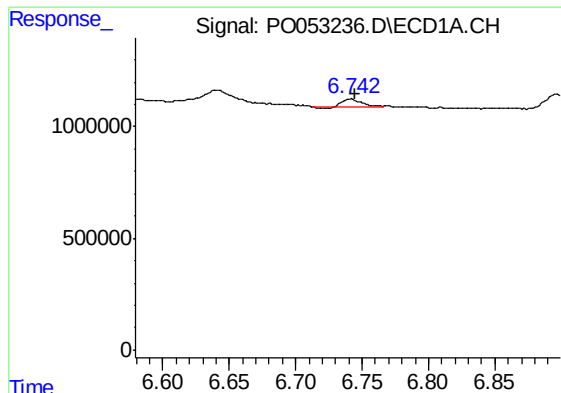

#28 AR-1254-3


R.T.: 6.742 min
Delta R.T.: -0.002 min
Response: 285702
Conc: 4.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

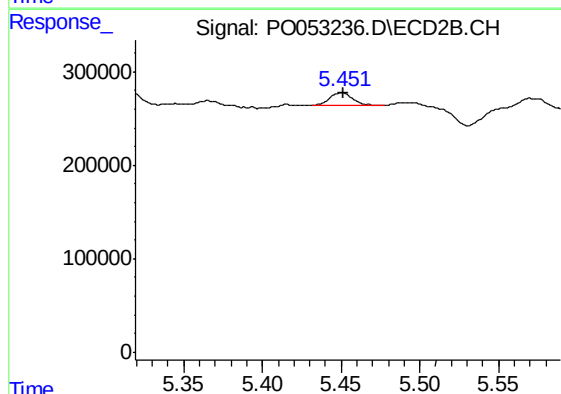


#28 AR-1254-3

R.T.: 5.451 min
Delta R.T.: -0.001 min
Response: 151048
Conc: 6.70 ng/ml

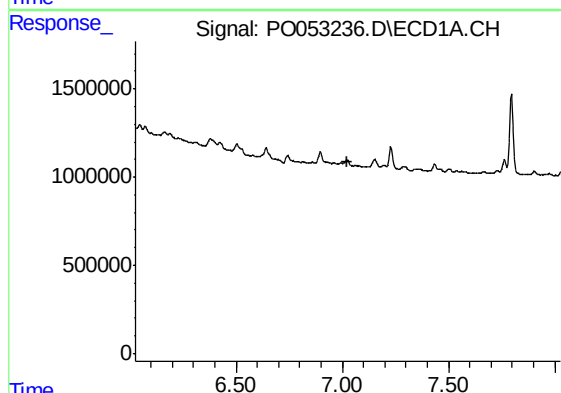


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

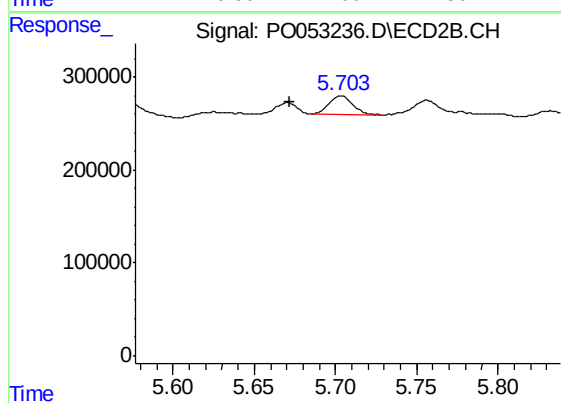

#29 AR-1254-4


R.T.: 5.704 min
Delta R.T.: 0.032 min
Response: 207782
Conc: 13.71 ng/ml

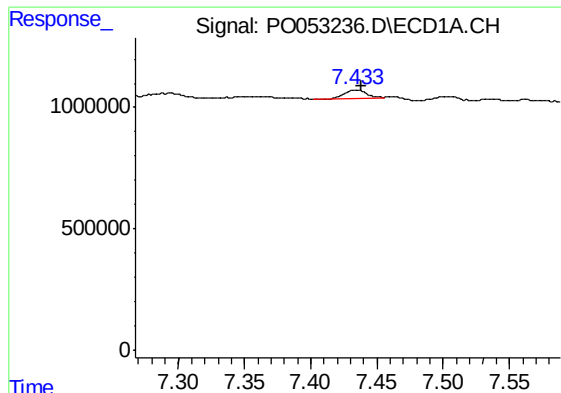

#30 AR-1254-5


R.T.: 7.434 min
Delta R.T.: -0.005 min
Response: 404340
Conc: 8.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

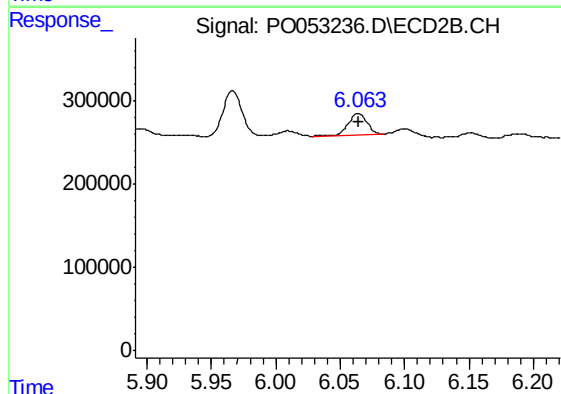


#30 AR-1254-5

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 263822
Conc: 13.18 ng/ml

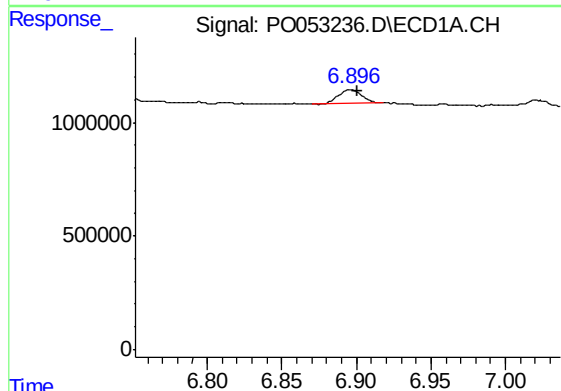


#31 AR-1260-1

R.T.: 6.897 min
Delta R.T.: -0.004 min
Response: 651464
Conc: 14.53 ng/ml

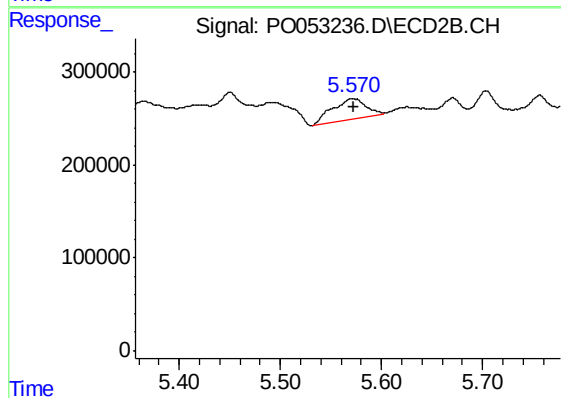

#31 AR-1260-1


R.T.: 5.570 min
Delta R.T.: -0.003 min
Response: 505040
Conc: 32.90 ng/ml

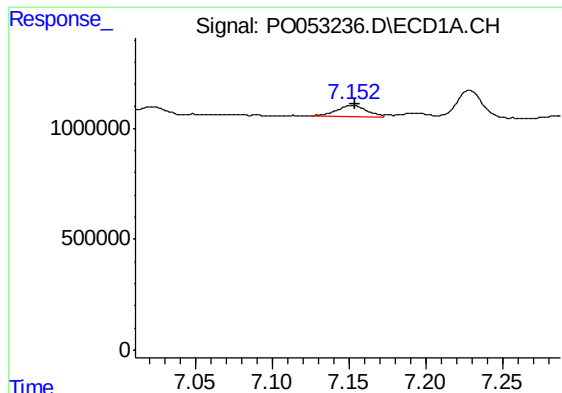

#32 AR-1260-2


R.T.: 7.152 min
Delta R.T.: -0.002 min
Response: 672948
Conc: 12.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

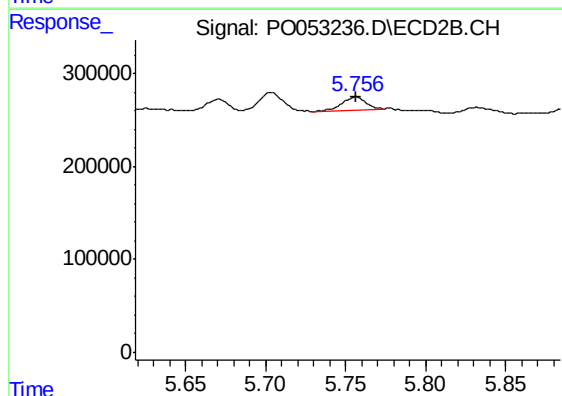


#32 AR-1260-2

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 140672
Conc: 7.35 ng/ml

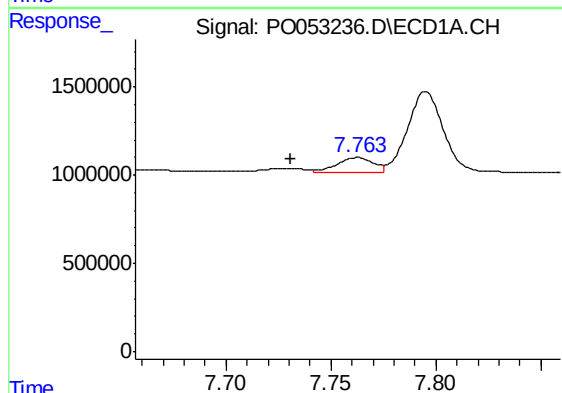


#34 AR-1260-4

R.T.: 7.763 min
Delta R.T.: 0.032 min
Response: 967655
Conc: 24.89 ng/ml

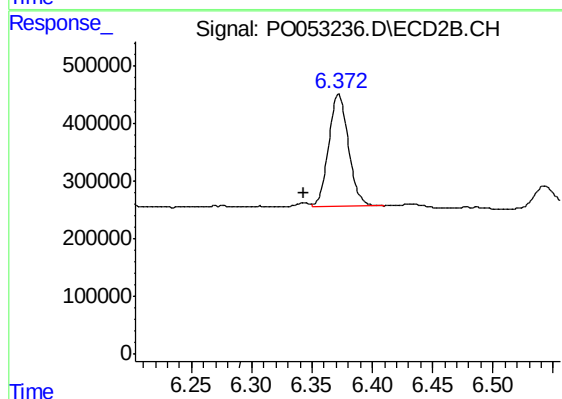

#34 AR-1260-4


R.T.: 6.372 min
Delta R.T.: 0.029 min
Response: 2240764
Conc: 193.70 ng/ml

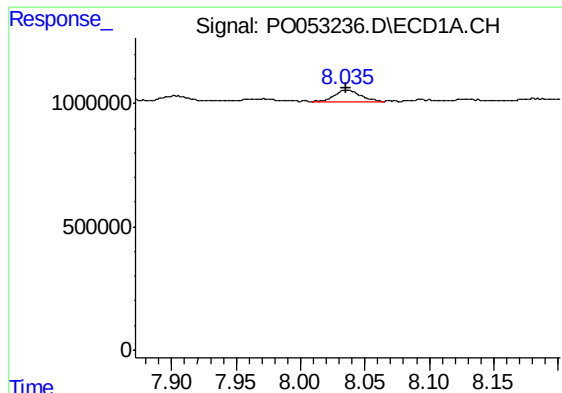

#35 AR-1260-5


R.T.: 8.035 min
Delta R.T.: 0.000 min
Response: 643702
Conc: 8.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

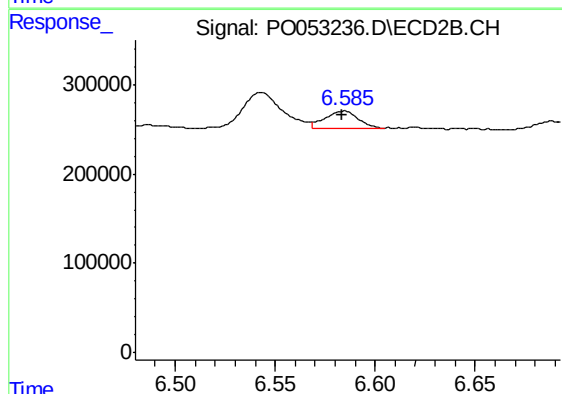


#35 AR-1260-5

R.T.: 6.585 min
Delta R.T.: 0.002 min
Response: 222775
Conc: 7.73 ng/ml

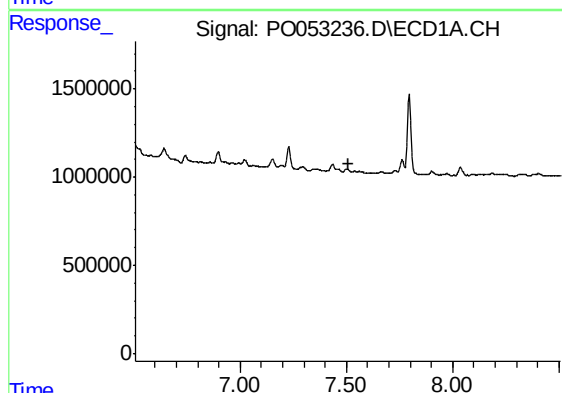


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

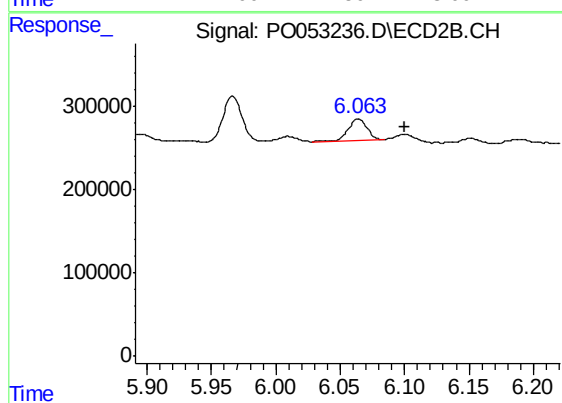

#36 AR-1262-1


R.T.: 6.064 min
Delta R.T.: -0.037 min
Response: 263822
Conc: 13.48 ng/ml

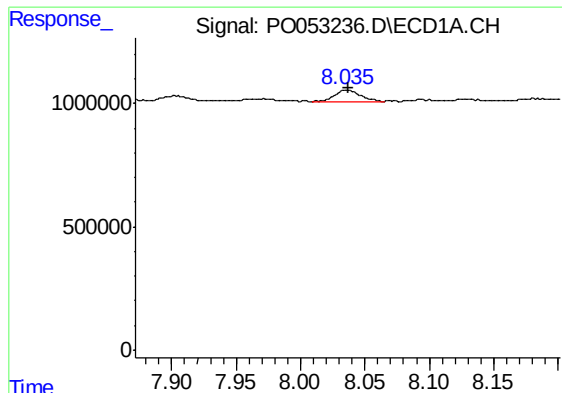

#37 AR-1262-2


R.T.: 8.035 min
Delta R.T.: -0.002 min
Response: 643702
Conc: 6.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

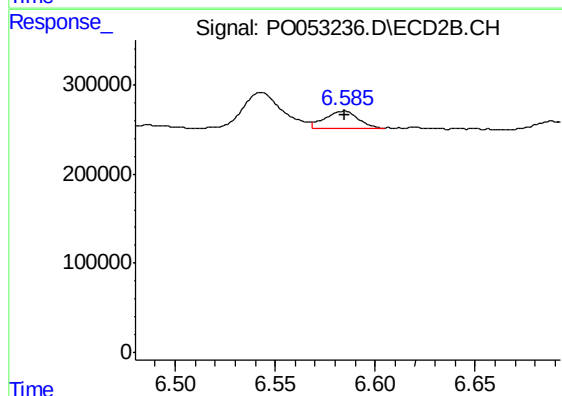


#37 AR-1262-2

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 222775
Conc: 6.71 ng/ml

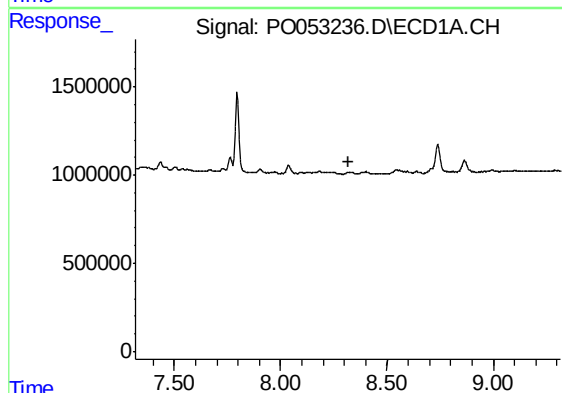


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.317 min
Response: 0
Conc: N.D.

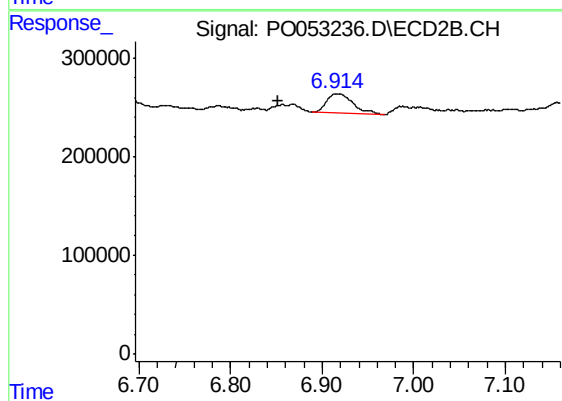

#38 AR-1262-3


R.T.: 6.914 min
Delta R.T.: 0.063 min
Response: 395150
Conc: 30.52 ng/ml

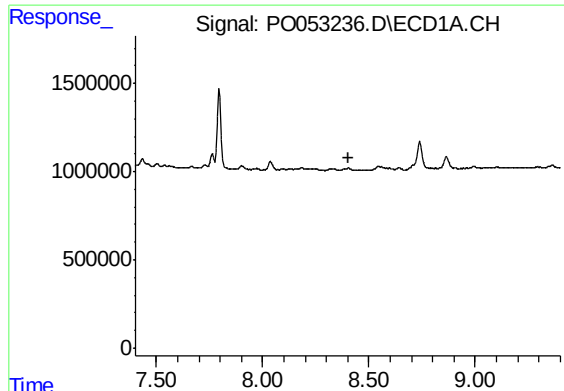

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

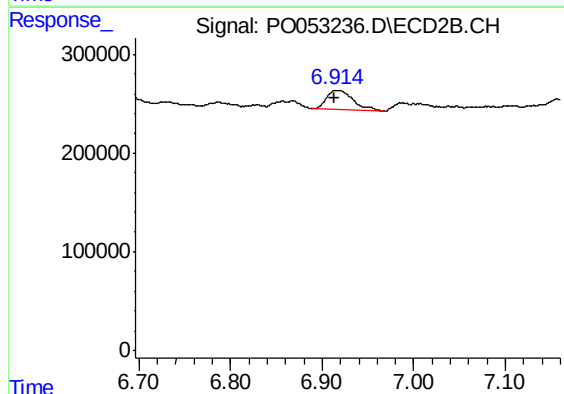


#39 AR-1262-4

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 395150
Conc: 16.28 ng/ml

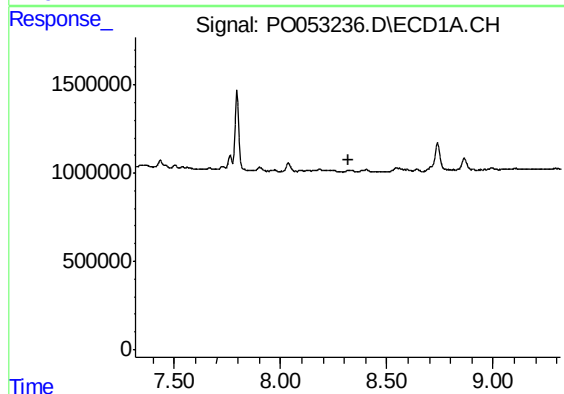


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.318 min
Response: 0
Conc: N.D.

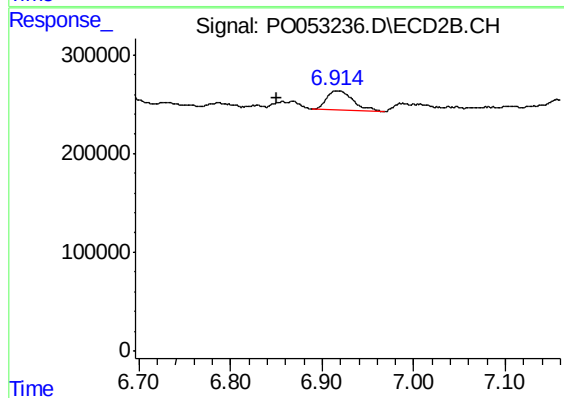

#41 AR-1268-1


R.T.: 6.914 min
Delta R.T.: 0.064 min
Response: 395150
Conc: 9.10 ng/ml

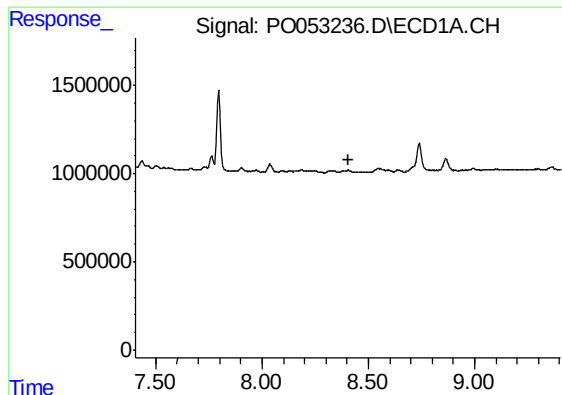

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

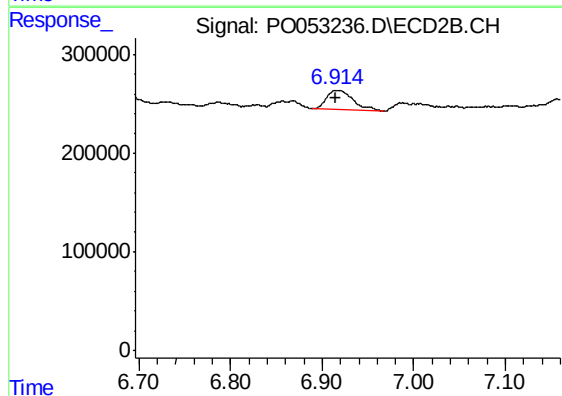

#42 AR-1268-2

R.T.: 6.914 min
Delta R.T.: -0.001 min
Response: 395150
Conc: 9.61 ng/ml