

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053237.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 6:12
 Operator : SM/SJ
 Sample : K1034-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:04:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.177	3.212	40402101	5638044	30.878	25.126
2)	SA Decachlor...	9.648	7.859	18989136	6337449	23.966	24.654
Target Compounds							
9)	L2 AR-1221-2	4.478	0.000	466502	0	54.011	N.D. #
10)	L2 AR-1221-3	4.556	3.569	350075	436483	12.523	76.684 #
11)	L3 AR-1232-1	4.556	3.569	350075	436483	15.396	92.806 #
12)	L3 AR-1232-2	5.080	0.000	2058803	0	181.691	N.D. #
14)	L3 AR-1232-4	0.000	4.519	0	70399	N.D.	26.609 #
19)	L4 AR-1242-4	0.000	4.519	0	70399	N.D.	12.816 #
20)	L4 AR-1242-5	6.247	4.983	1743382	146632	79.676	19.246 #
23)	L5 AR-1248-3	0.000	4.519	0	70399	N.D.	8.965 #
24)	L5 AR-1248-4	6.247	0.000	1743382	0	46.667	N.D. #
25)	L5 AR-1248-5	6.247	4.983	1743382	146632	48.932	14.616 #
26)	L6 AR-1254-1	0.000	4.983	0	146632	N.D.	8.944 #
27)	L6 AR-1254-2	6.427	5.121	411840	2763	6.945	0.197 #
29)	L6 AR-1254-4	0.000	5.703	0	231167	N.D.	15.250 #
30)	L6 AR-1254-5	7.432	0.000	1109847	0	24.452	N.D. #
31)	L7 AR-1260-1	6.895	0.000	778519	0	17.362	N.D. #
32)	L7 AR-1260-2	0.000	5.703	0	231167	N.D.	12.079 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053237.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 6:12
Operator : SM/SJ
Sample : K1034-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:04:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

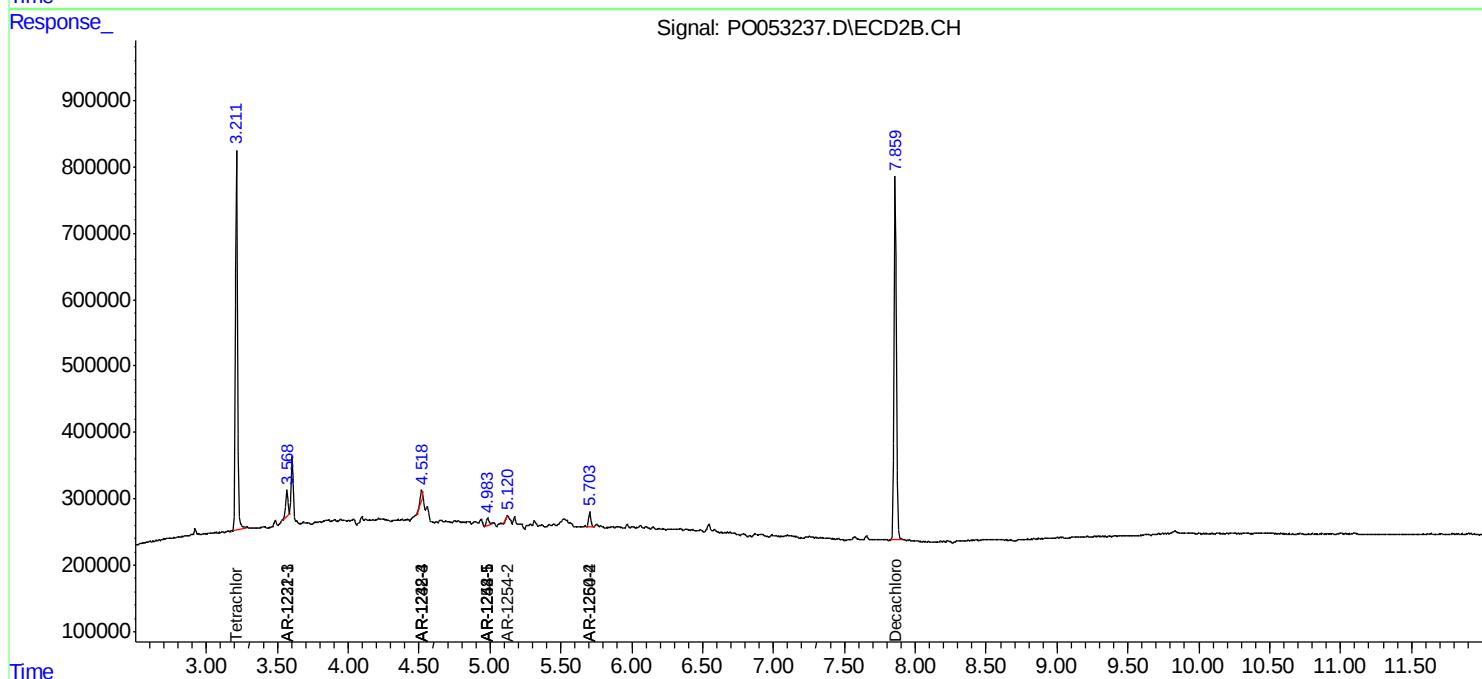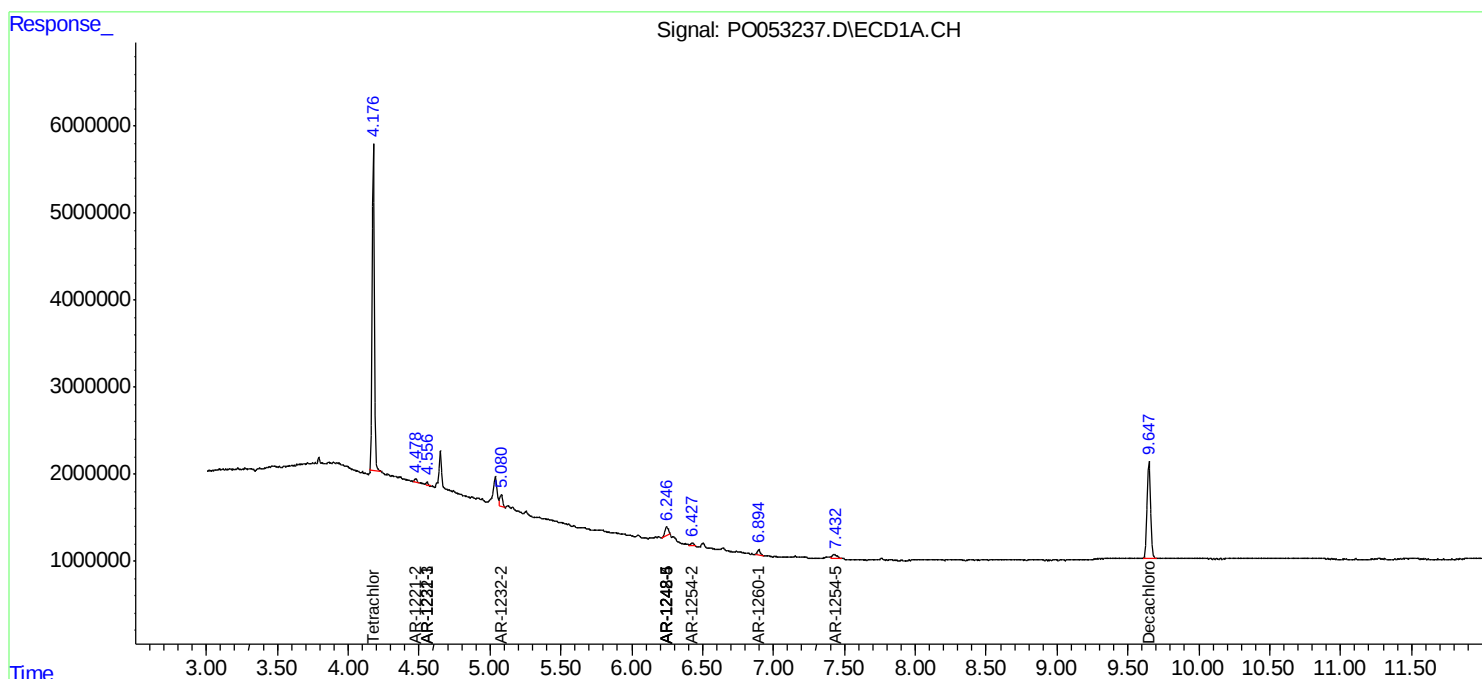


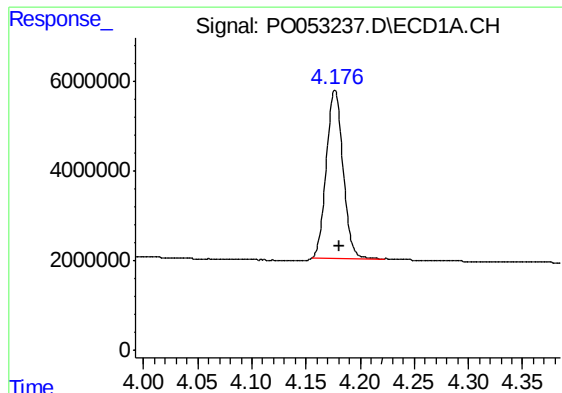

#1 Tetrachloro-m-xylene


R.T.: 4.177 min
Delta R.T.: -0.004 min
Response: 40402101
Conc: 30.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

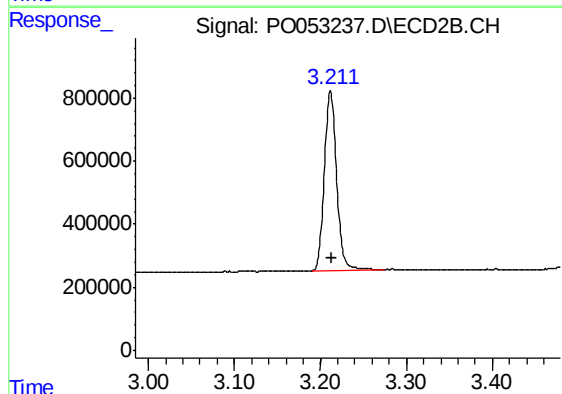


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 5638044
Conc: 25.13 ng/ml

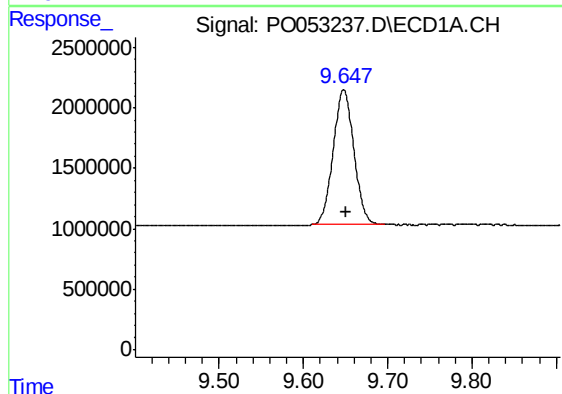


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.003 min
Response: 18989136
Conc: 23.97 ng/ml

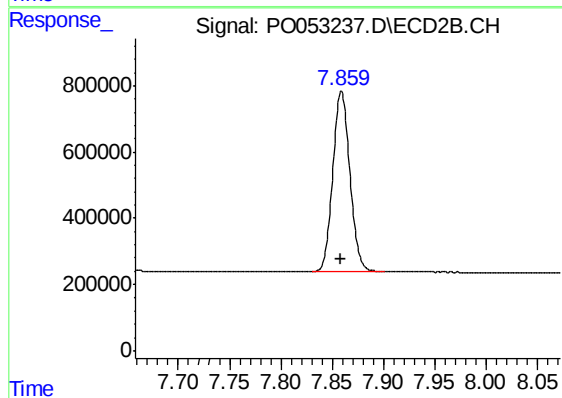

#2 Decachlorobiphenyl


R.T.: 7.859 min
Delta R.T.: 0.000 min
Response: 6337449
Conc: 24.65 ng/ml

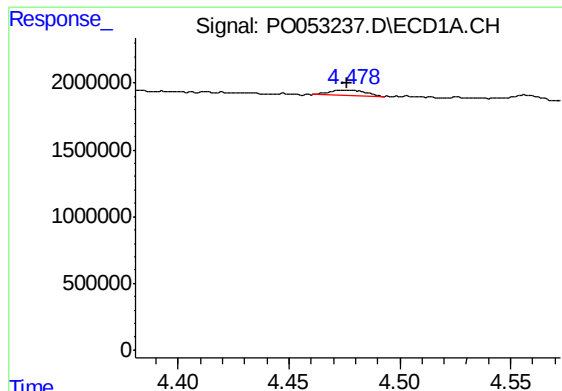

#9 AR-1221-2


R.T.: 4.478 min
Delta R.T.: 0.001 min
Response: 466502
Conc: 54.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

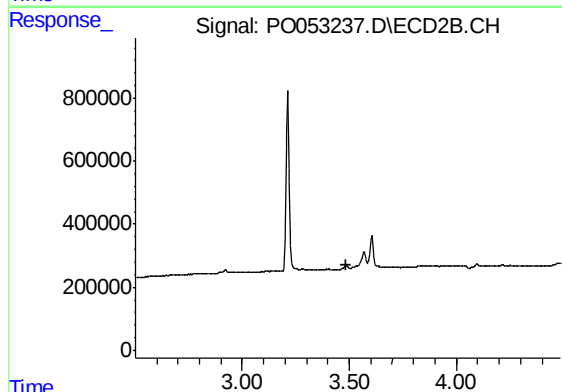


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

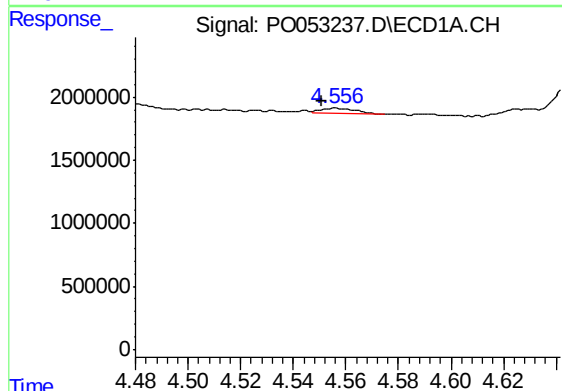


#10 AR-1221-3

R.T.: 4.556 min
Delta R.T.: 0.005 min
Response: 350075
Conc: 12.52 ng/ml

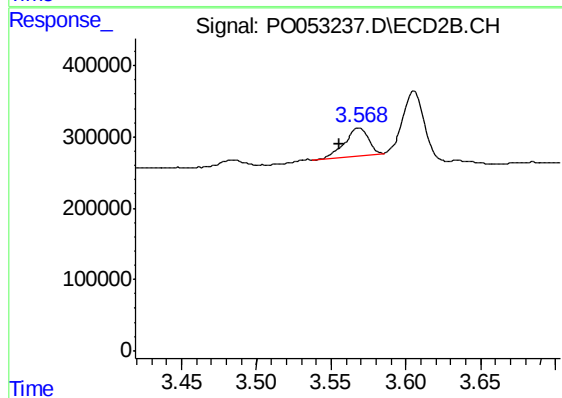

#10 AR-1221-3


R.T.: 3.569 min
Delta R.T.: 0.013 min
Response: 436483
Conc: 76.68 ng/ml

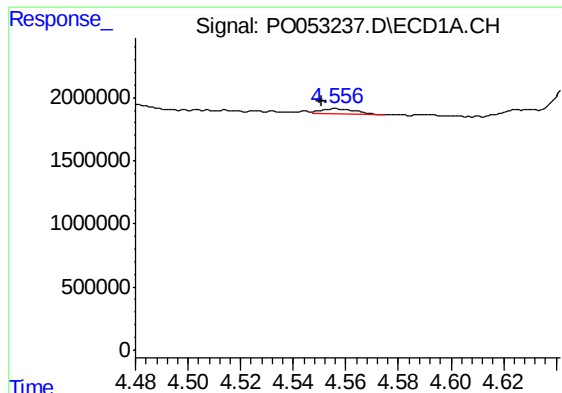

#11 AR-1232-1


R.T.: 4.556 min
Delta R.T.: 0.005 min
Response: 350075
Conc: 15.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

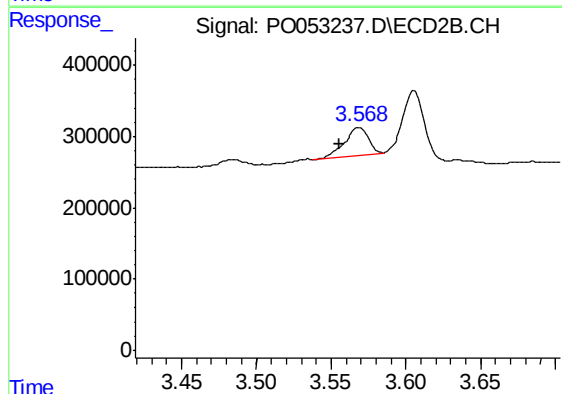


#11 AR-1232-1

R.T.: 3.569 min
Delta R.T.: 0.013 min
Response: 436483
Conc: 92.81 ng/ml

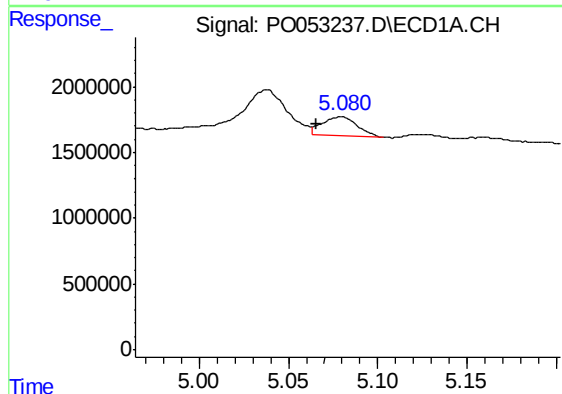


#12 AR-1232-2

R.T.: 5.080 min
Delta R.T.: 0.014 min
Response: 2058803
Conc: 181.69 ng/ml

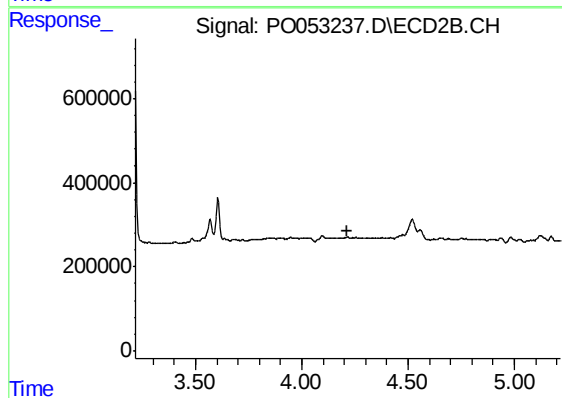

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

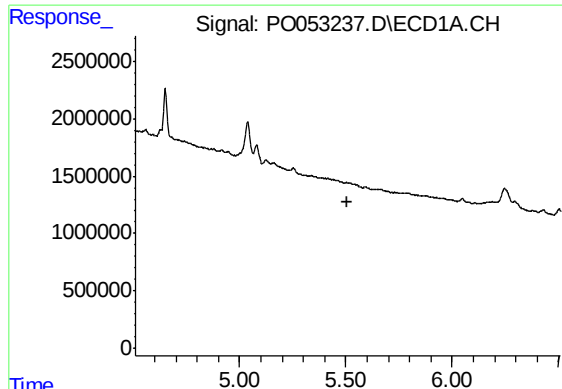

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

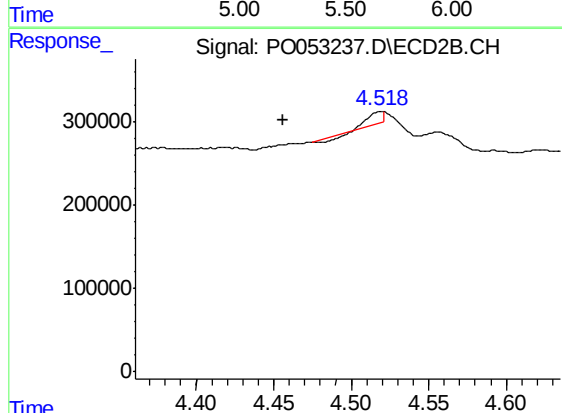


#14 AR-1232-4

R.T.: 4.519 min
Delta R.T.: 0.063 min
Response: 70399
Conc: 26.61 ng/ml

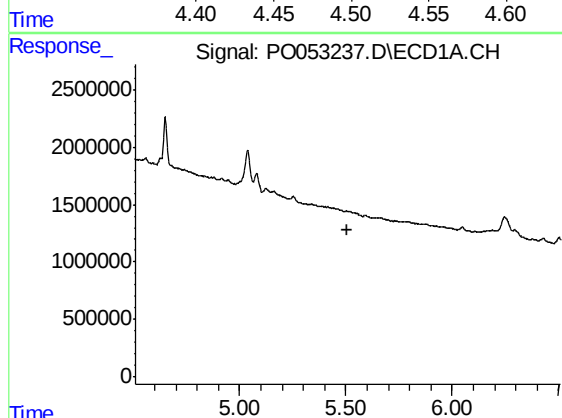


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.509 min
Response: 0
Conc: N.D.

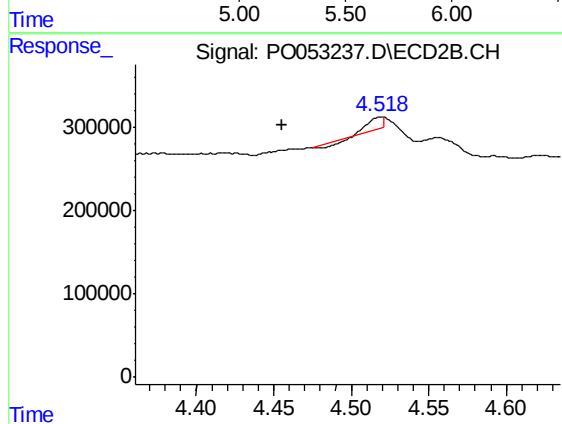

#19 AR-1242-4


R.T.: 4.519 min
Delta R.T.: 0.064 min
Response: 70399
Conc: 12.82 ng/ml

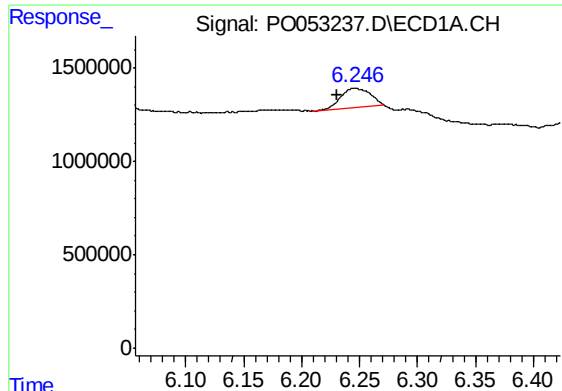

#20 AR-1242-5


R.T.: 6.247 min
Delta R.T.: 0.016 min
Response: 1743382
Conc: 79.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

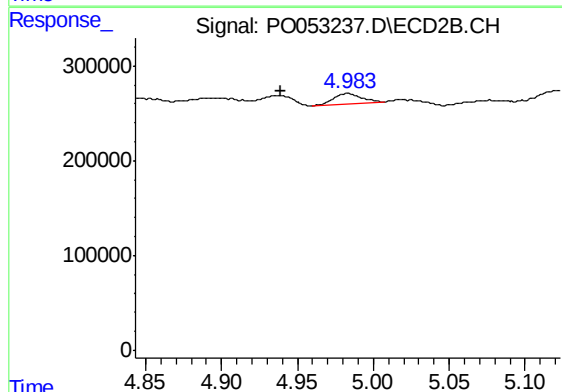


#20 AR-1242-5

R.T.: 4.983 min
Delta R.T.: 0.044 min
Response: 146632
Conc: 19.25 ng/ml

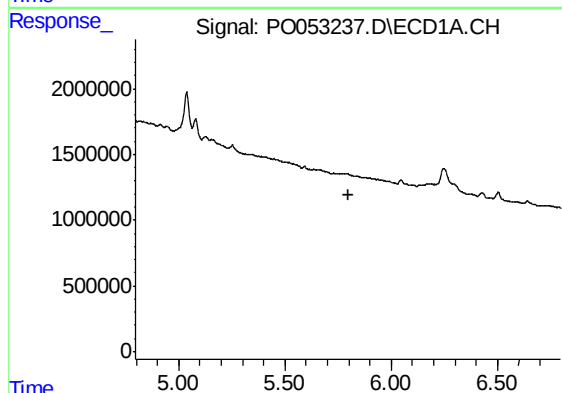


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.796 min
Response: 0
Conc: N.D.

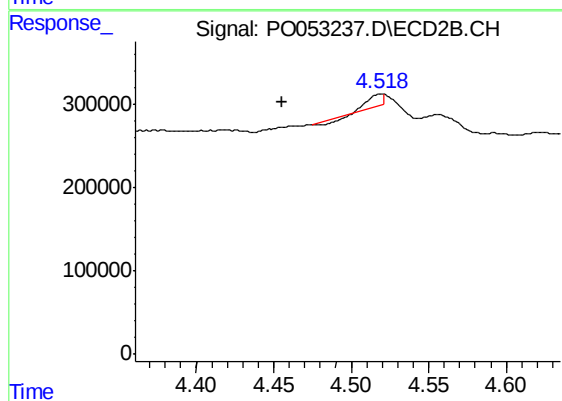

#23 AR-1248-3


R.T.: 4.519 min
Delta R.T.: 0.064 min
Response: 70399
Conc: 8.96 ng/ml

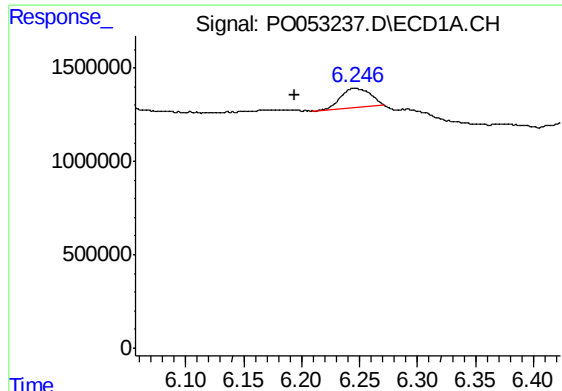

#24 AR-1248-4


R.T.: 6.247 min
Delta R.T.: 0.052 min
Response: 1743382
Conc: 46.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

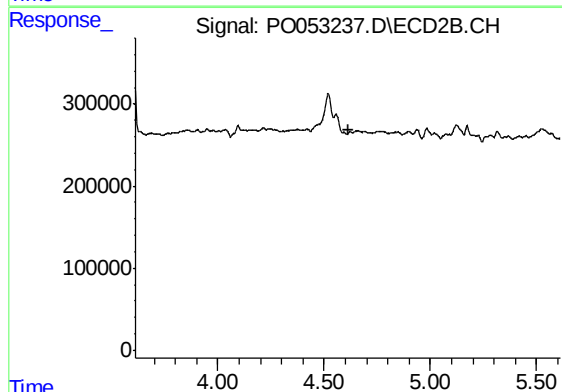


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

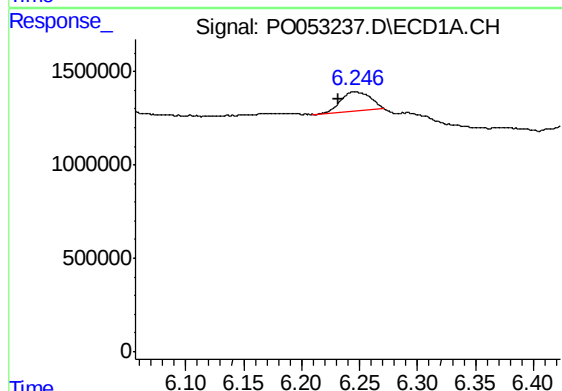


#25 AR-1248-5

R.T.: 6.247 min
Delta R.T.: 0.015 min
Response: 1743382
Conc: 48.93 ng/ml

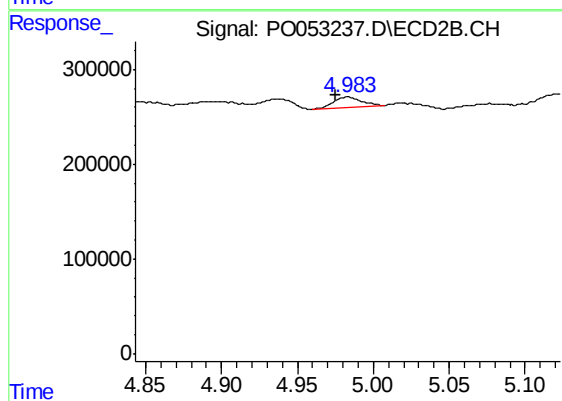

#25 AR-1248-5


R.T.: 4.983 min
Delta R.T.: 0.008 min
Response: 146632
Conc: 14.62 ng/ml

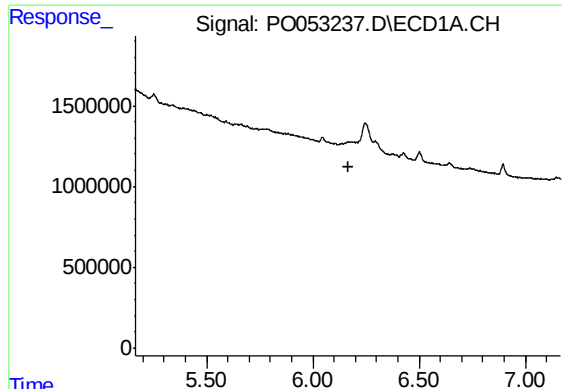

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

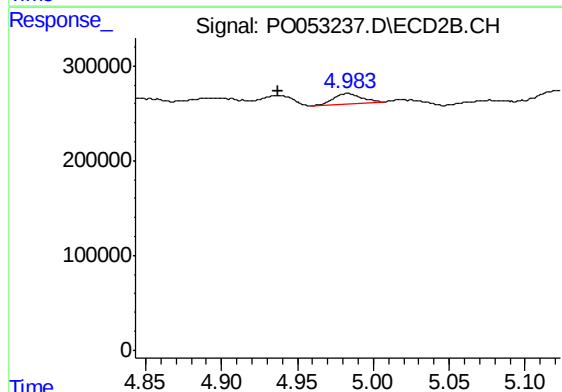


#26 AR-1254-1

R.T.: 4.983 min
Delta R.T.: 0.046 min
Response: 146632
Conc: 8.94 ng/ml

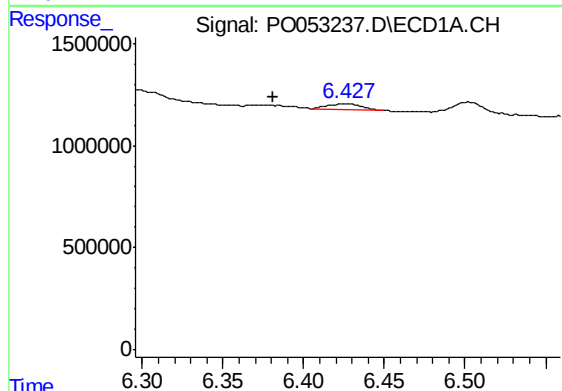


#27 AR-1254-2

R.T.: 6.427 min
Delta R.T.: 0.046 min
Response: 411840
Conc: 6.94 ng/ml

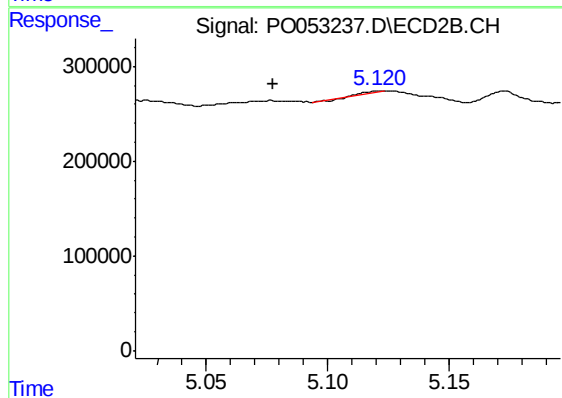

#27 AR-1254-2


R.T.: 5.121 min
Delta R.T.: 0.043 min
Response: 2763
Conc: 0.20 ng/ml

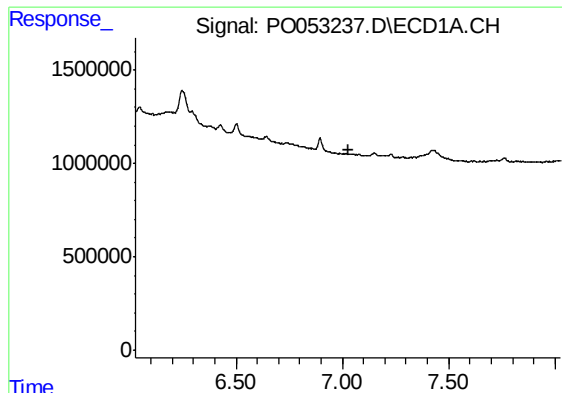

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

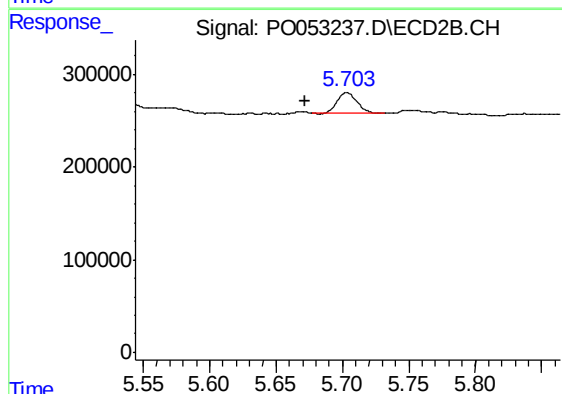


#29 AR-1254-4

R.T.: 5.703 min
Delta R.T.: 0.032 min
Response: 231167
Conc: 15.25 ng/ml

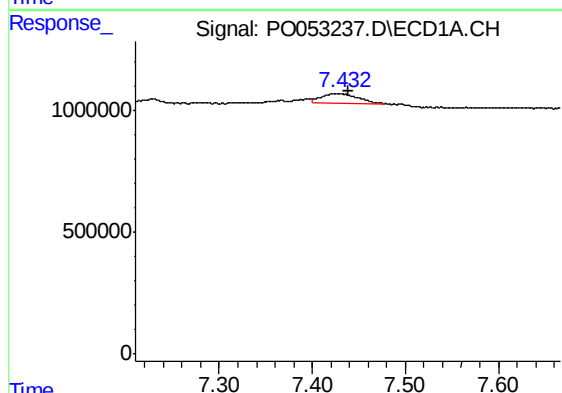


#30 AR-1254-5

R.T.: 7.432 min
Delta R.T.: -0.007 min
Response: 1109847
Conc: 24.45 ng/ml

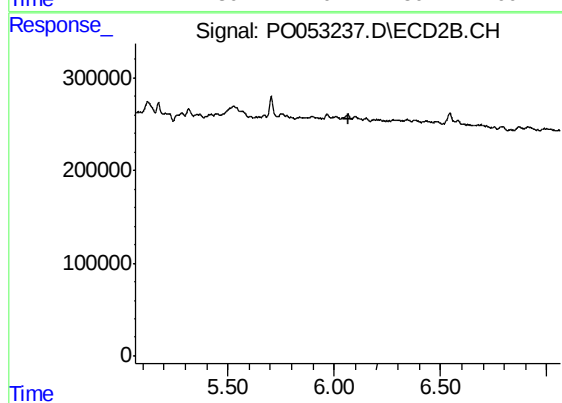

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.065 min
Response: 0
Conc: N.D.

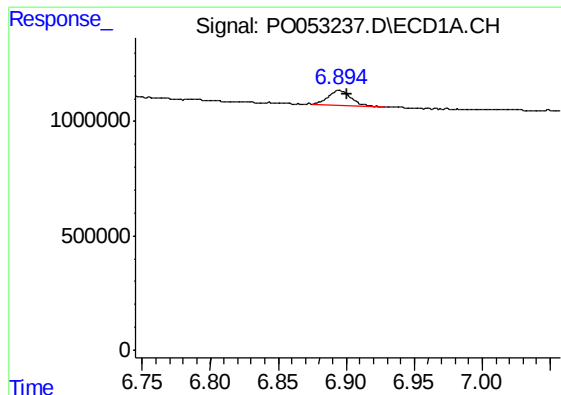

#31 AR-1260-1


R.T.: 6.895 min
Delta R.T.: -0.006 min
Response: 778519
Conc: 17.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

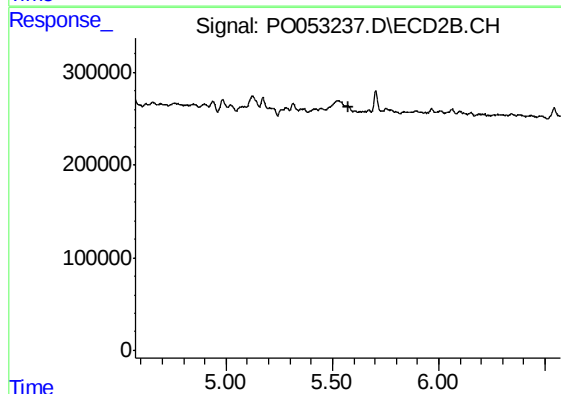


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 5.573 min
Response: 0
Conc: N.D.

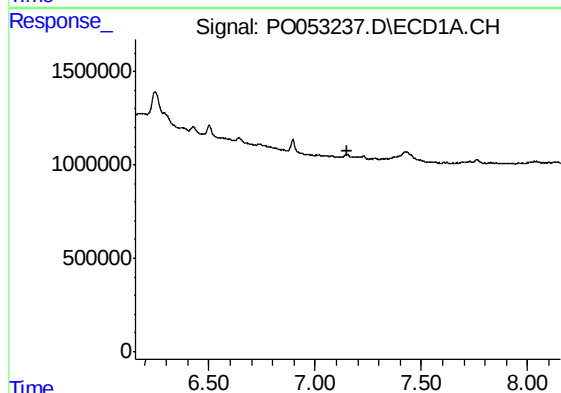

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

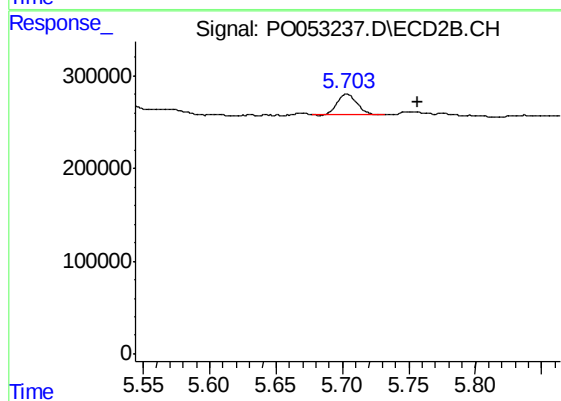

#32 AR-1260-2

R.T.: 5.703 min
Delta R.T.: -0.053 min
Response: 231167
Conc: 12.08 ng/ml