

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053238.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 6:29
 Operator : SM/SJ
 Sample : K1034-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:04:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.178	3.212	46909469	6424041	35.852	28.629
2)	SA Decachlor...	9.650	7.860	20706113	6800458	26.133	26.455
Target Compounds							
3)	L1 AR-1016-1	0.000	4.152	0	51376	N.D.	5.699 #
4)	L1 AR-1016-2	0.000	4.152	0	51376	N.D.	3.730 #
9)	L2 AR-1221-2	4.478	0.000	478010	0	55.343	N.D. #
10)	L2 AR-1221-3	0.000	3.606	0	382845	N.D.	67.261 #
11)	L3 AR-1232-1	0.000	3.606	0	382845	N.D.	81.401 #
12)	L3 AR-1232-2	5.130	4.152	1343138	51376	118.533	8.653 #
16)	L4 AR-1242-1	0.000	4.152	0	51376	N.D.	7.364 #
17)	L4 AR-1242-2	0.000	4.152	0	51376	N.D.	4.722 #
20)	L4 AR-1242-5	6.244	0.000	530822	0	24.260	N.D. #
21)	L5 AR-1248-1	0.000	4.152	0	51376	N.D.	9.195 #
24)	L5 AR-1248-4	6.244	0.000	530822	0	14.209	N.D. #
25)	L5 AR-1248-5	6.244	0.000	530822	0	14.899	N.D. #
28)	L6 AR-1254-3	6.747	5.425	94076	277327	1.525	12.293 #
29)	L6 AR-1254-4	0.000	5.662	0	232718	N.D.	15.352 #
31)	L7 AR-1260-1	0.000	5.571	0	1065231	N.D.	69.397 #
32)	L7 AR-1260-2	0.000	5.699	0	65456	N.D.	3.420 #
34)	L7 AR-1260-4	7.761	0.000	940686	0	24.195	N.D. #
35)	L7 AR-1260-5	0.000	6.542	0	460301	N.D.	15.978 #
37)	L8 AR-1262-2	0.000	6.542	0	460301	N.D.	13.862 #
39)	L8 AR-1262-4	0.000	6.922	0	710818	N.D.	29.278 #
42)	L9 AR-1268-2	0.000	6.922	0	710818	N.D.	17.284 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053238.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 6:29
Operator : SM/SJ
Sample : K1034-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:04:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

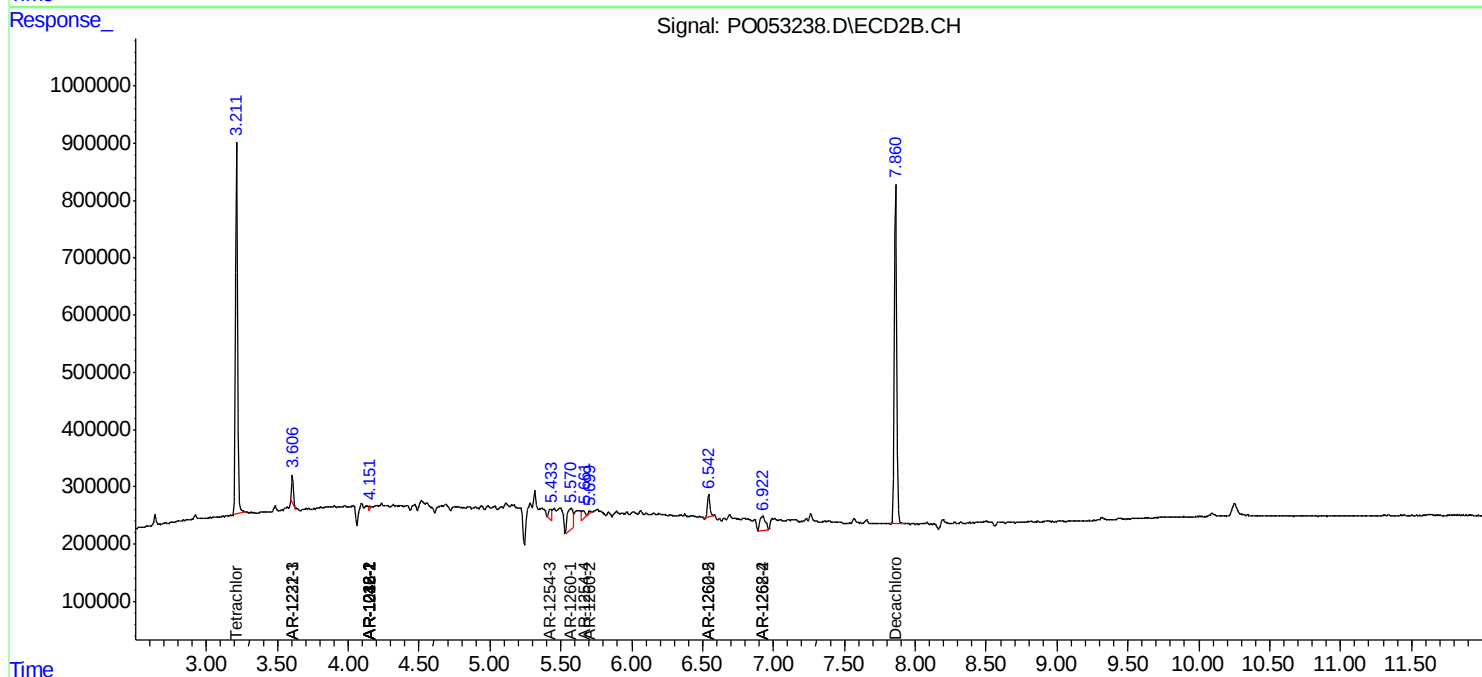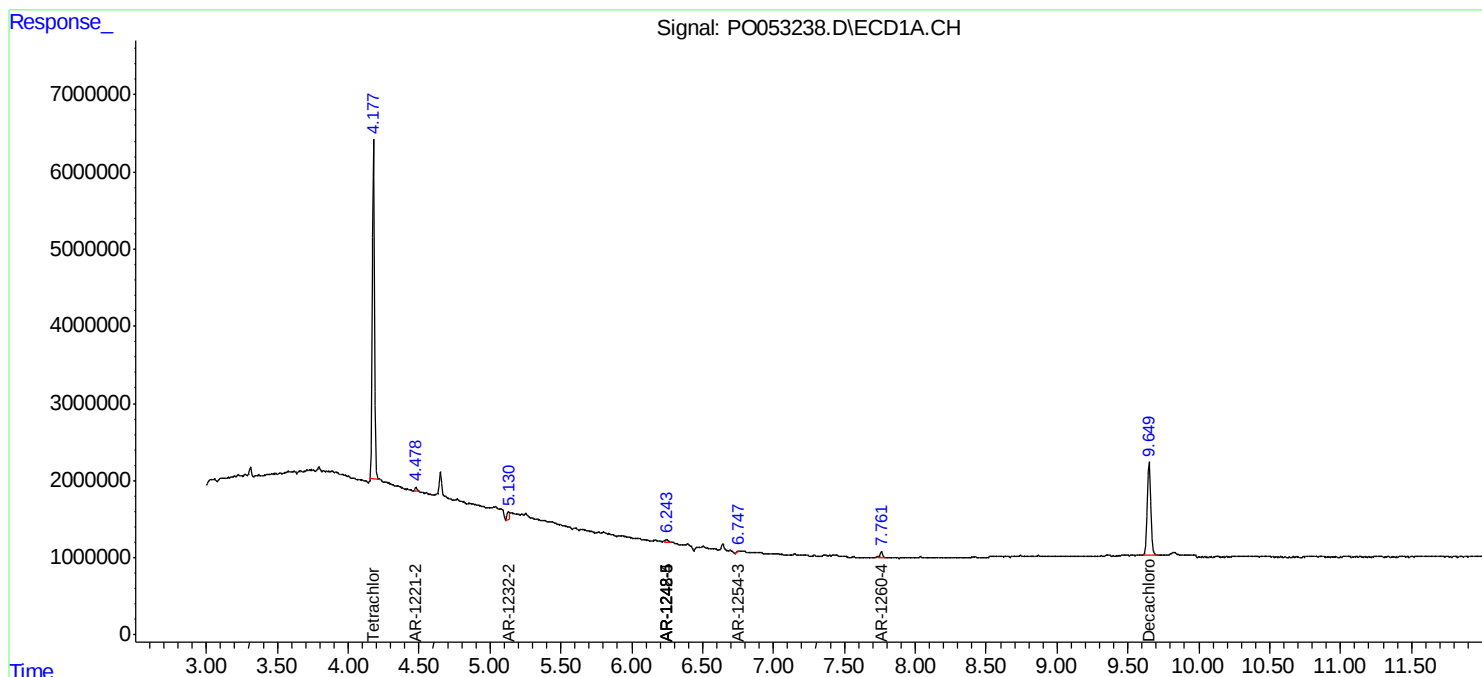


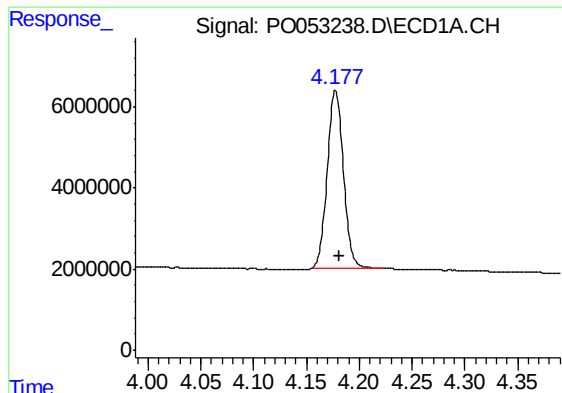

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: -0.003 min
Response: 46909469
Conc: 35.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

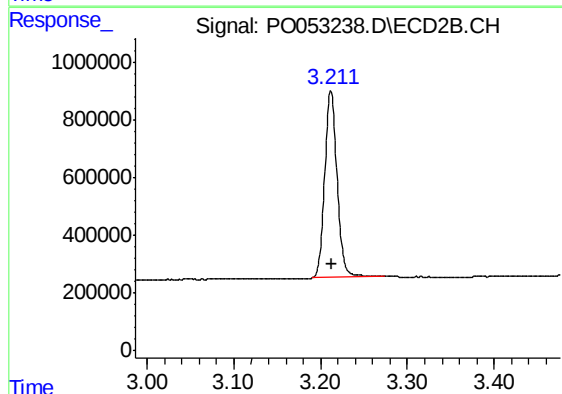


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 6424041
Conc: 28.63 ng/ml

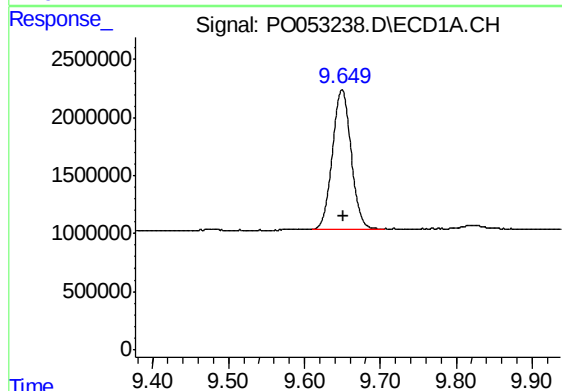


#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.001 min
Response: 20706113
Conc: 26.13 ng/ml

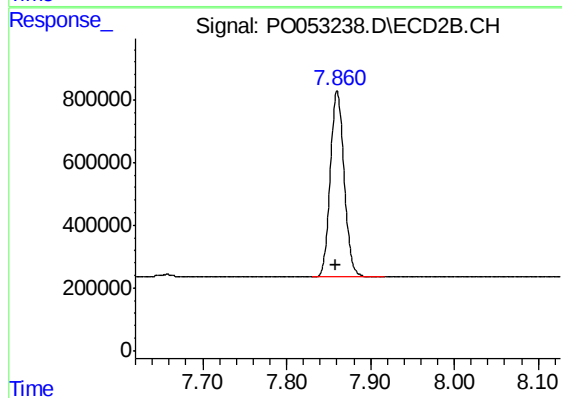

#2 Decachlorobiphenyl


R.T.: 7.860 min
Delta R.T.: 0.001 min
Response: 6800458
Conc: 26.45 ng/ml

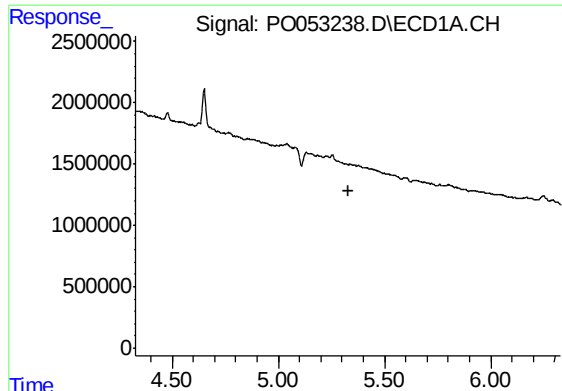

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

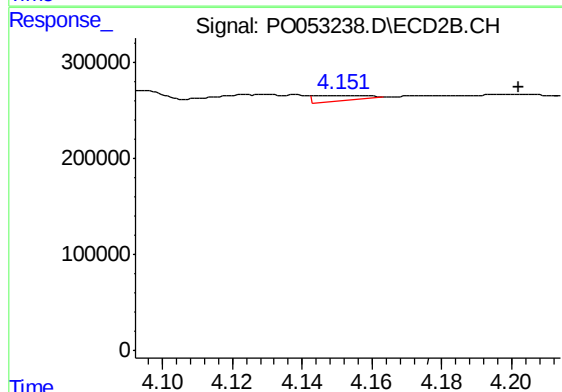


#3 AR-1016-1

R.T.: 4.152 min
Delta R.T.: -0.051 min
Response: 51376
Conc: 5.70 ng/ml

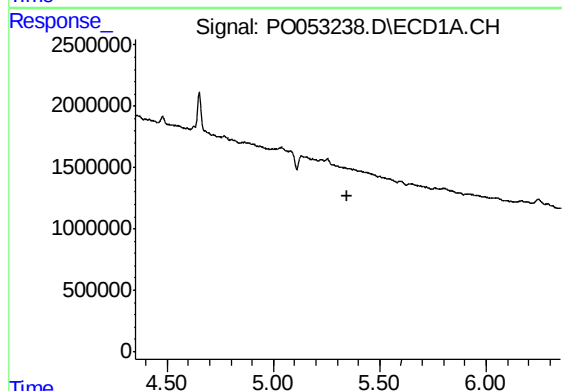


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

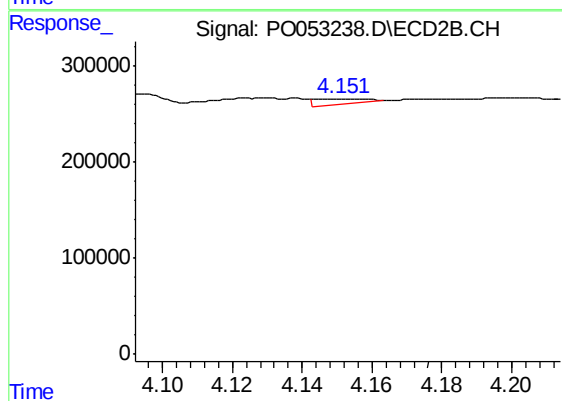

#4 AR-1016-2


R.T.: 4.152 min
Delta R.T.: -0.065 min
Response: 51376
Conc: 3.73 ng/ml

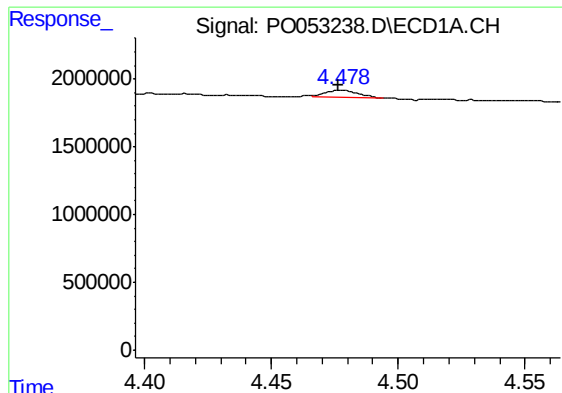

#9 AR-1221-2


R.T.: 4.478 min
Delta R.T.: 0.002 min
Response: 478010
Conc: 55.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

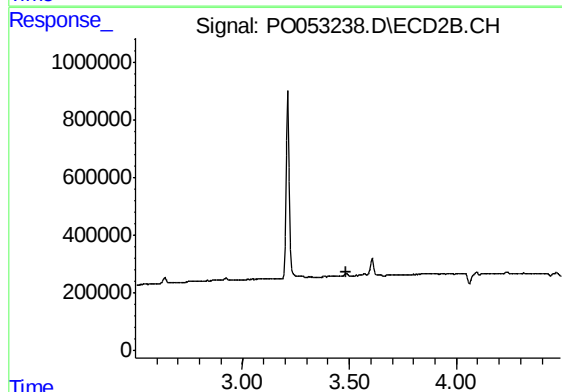


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

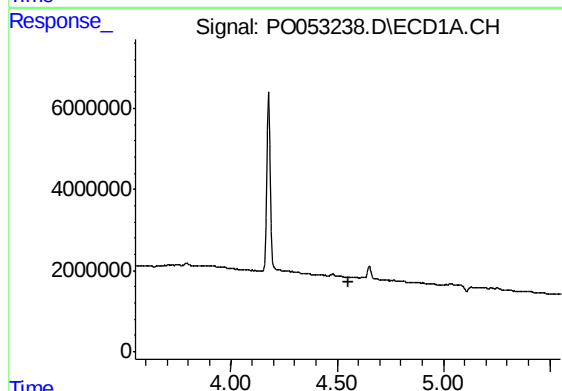


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.551 min
Response: 0
Conc: N.D.

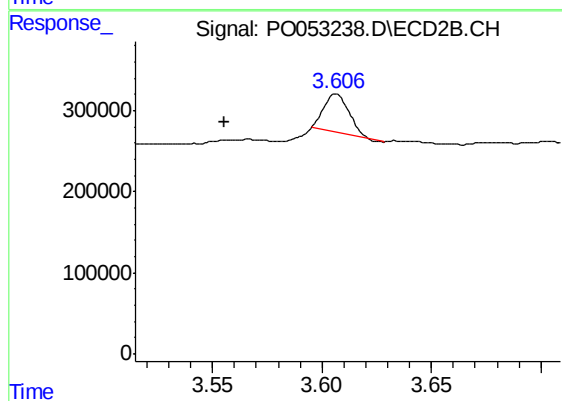

#10 AR-1221-3


R.T.: 3.606 min
Delta R.T.: 0.051 min
Response: 382845
Conc: 67.26 ng/ml

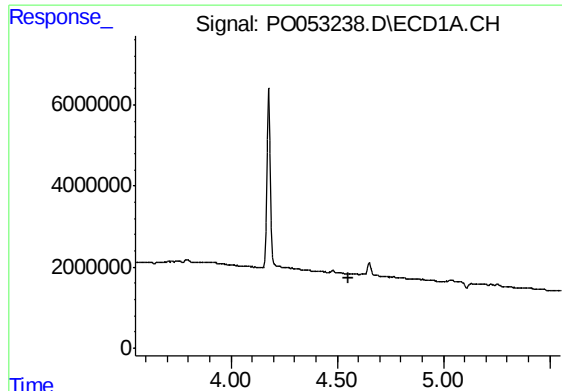

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

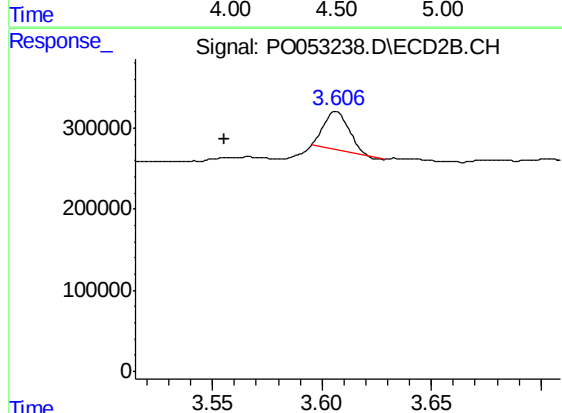


#11 AR-1232-1

R.T.: 3.606 min
Delta R.T.: 0.051 min
Response: 382845
Conc: 81.40 ng/ml

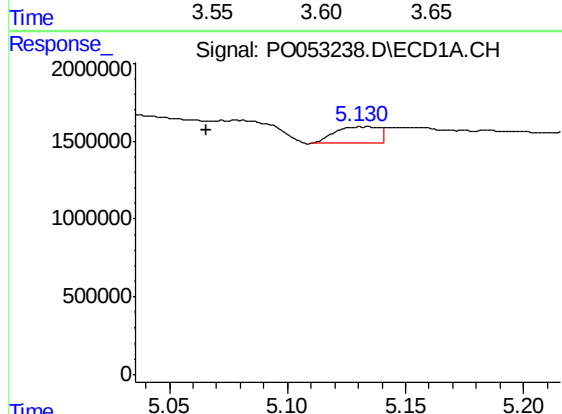


#12 AR-1232-2

R.T.: 5.130 min
Delta R.T.: 0.065 min
Response: 1343138
Conc: 118.53 ng/ml

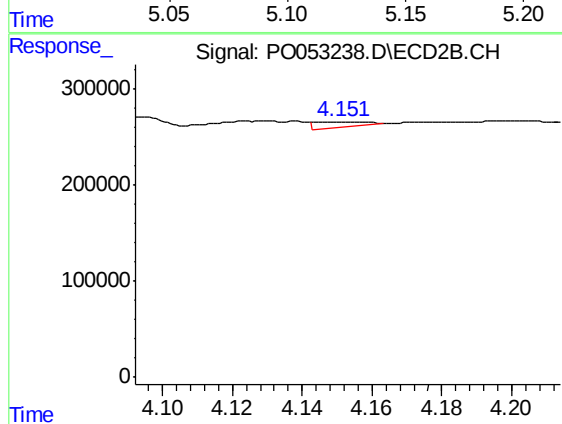

#12 AR-1232-2


R.T.: 4.152 min
Delta R.T.: -0.065 min
Response: 51376
Conc: 8.65 ng/ml

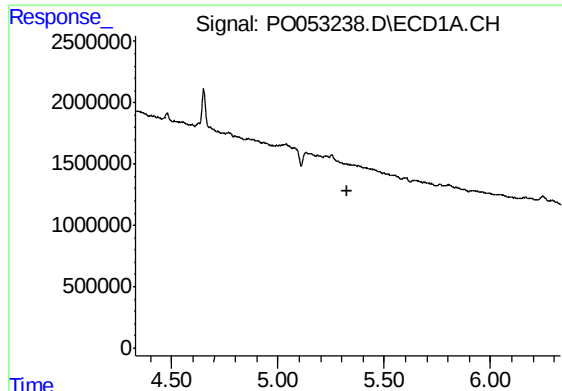

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 5.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

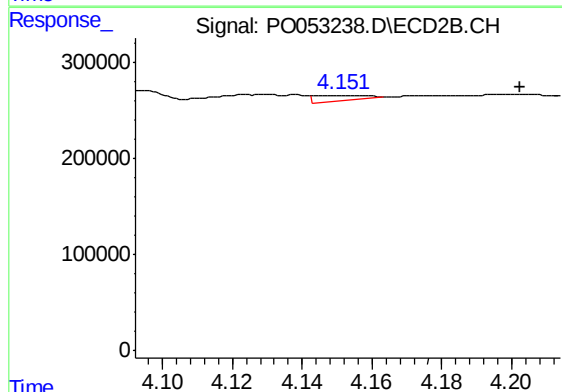


#16 AR-1242-1

R.T.: 4.152 min
Delta R.T.: -0.051 min
Response: 51376
Conc: 7.36 ng/ml

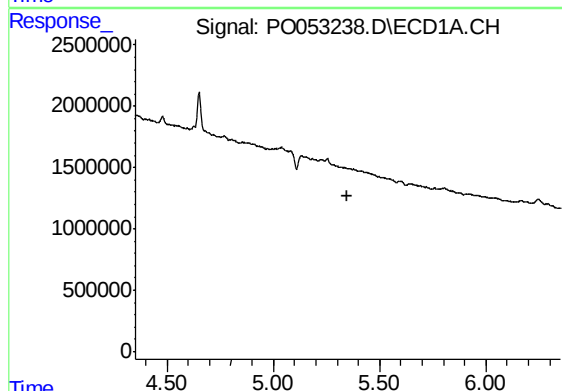


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.351 min
Response: 0
Conc: N.D.

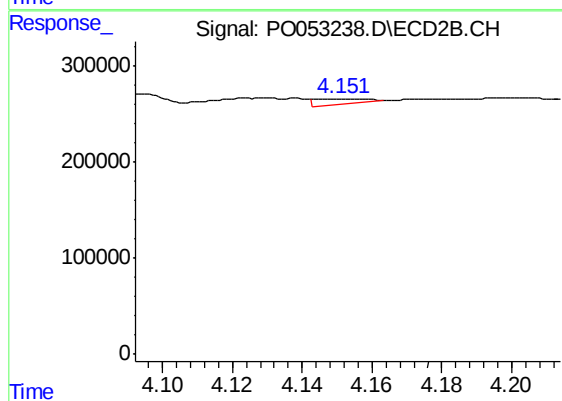

#17 AR-1242-2


R.T.: 4.152 min
Delta R.T.: -0.065 min
Response: 51376
Conc: 4.72 ng/ml

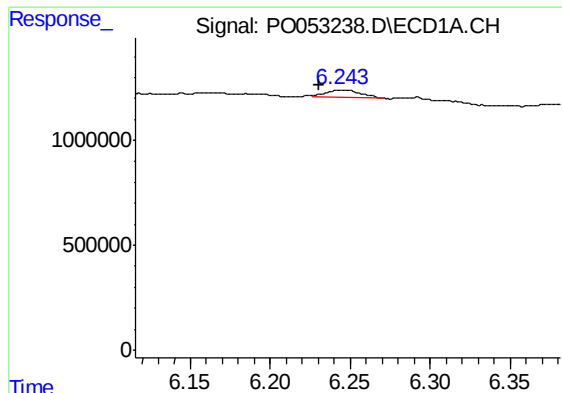

#20 AR-1242-5


R.T.: 6.244 min
Delta R.T.: 0.013 min
Response: 530822
Conc: 24.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

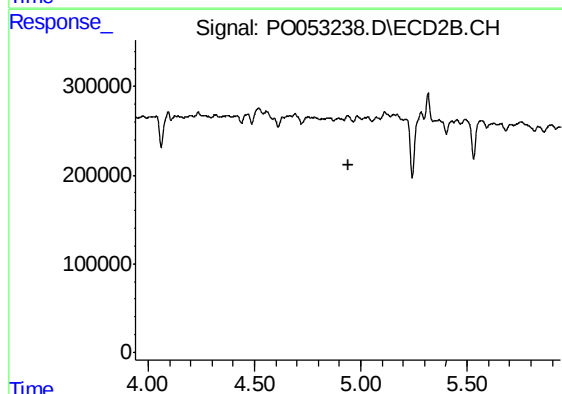


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 4.939 min
Response: 0
Conc: N.D.

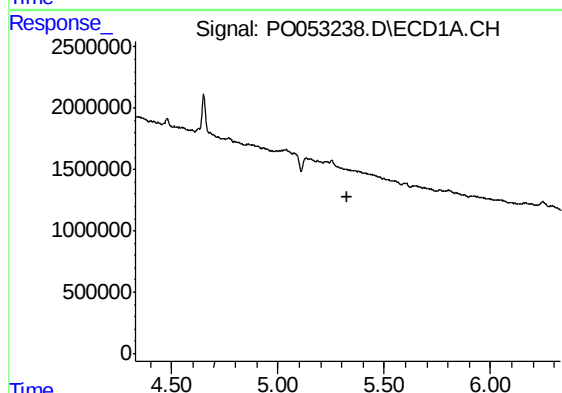


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 5.329 min
Response: 0
Conc: N.D.

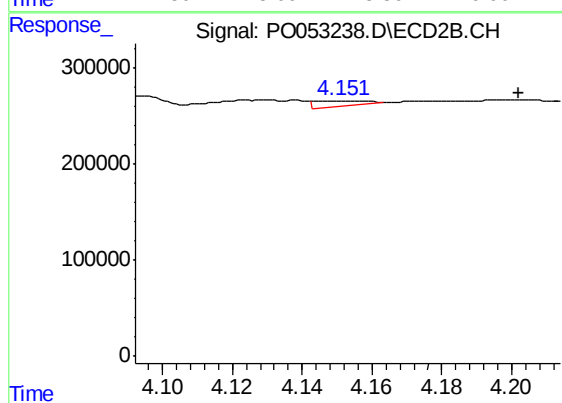

#21 AR-1248-1


R.T.: 4.152 min
Delta R.T.: -0.050 min
Response: 51376
Conc: 9.19 ng/ml

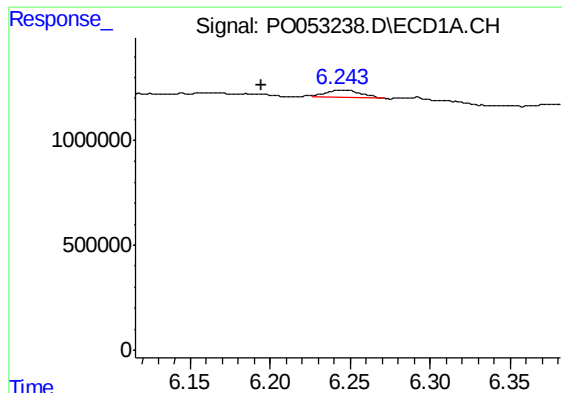

#24 AR-1248-4


R.T.: 6.244 min
Delta R.T.: 0.049 min
Response: 530822
Conc: 14.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

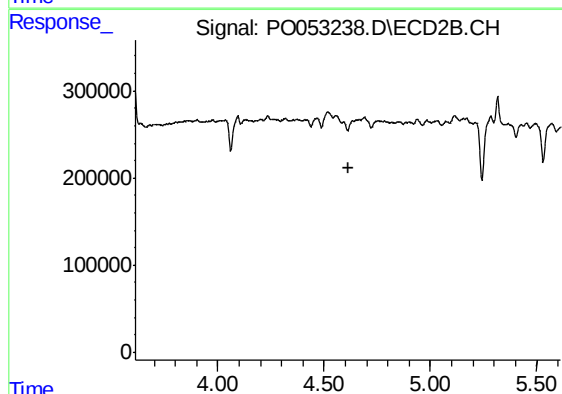


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

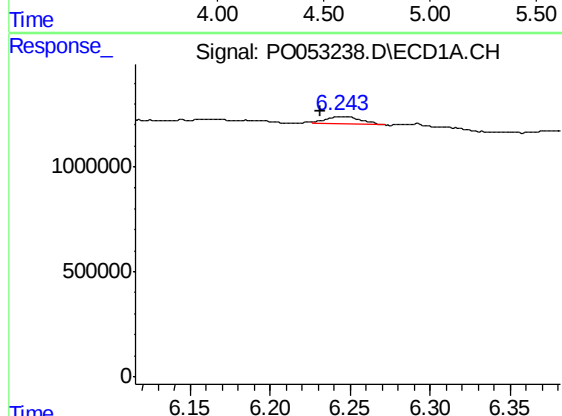


#25 AR-1248-5

R.T.: 6.244 min
Delta R.T.: 0.012 min
Response: 530822
Conc: 14.90 ng/ml

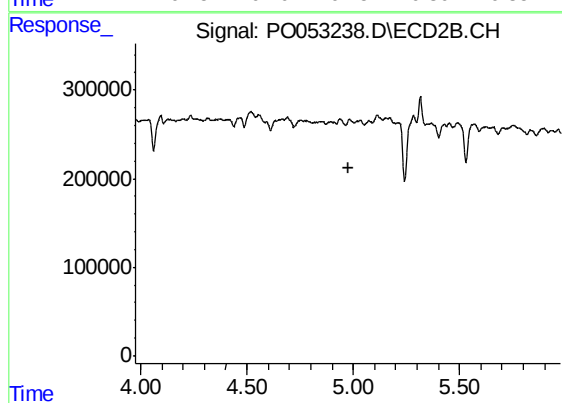

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

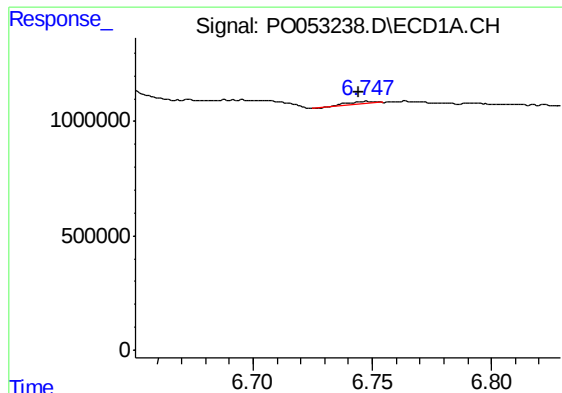

#28 AR-1254-3


R.T.: 6.747 min
Delta R.T.: 0.003 min
Response: 94076
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

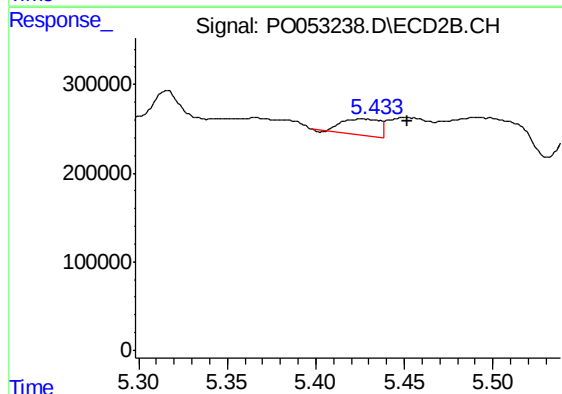


#28 AR-1254-3

R.T.: 5.425 min
Delta R.T.: -0.027 min
Response: 277327
Conc: 12.29 ng/ml

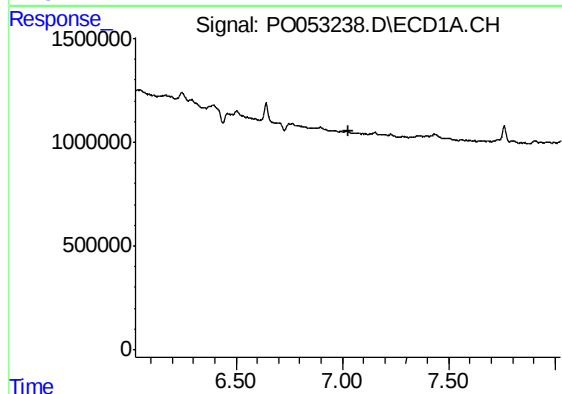


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

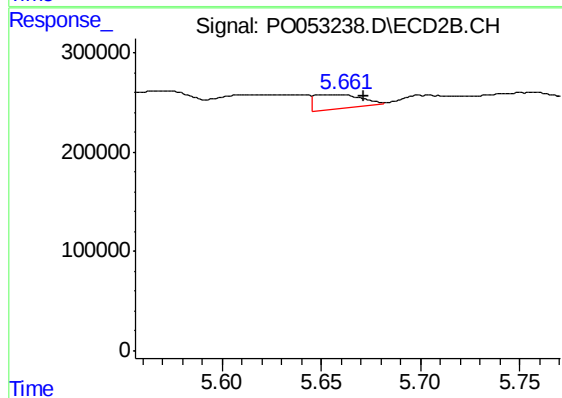

#29 AR-1254-4


R.T.: 5.662 min
Delta R.T.: -0.010 min
Response: 232718
Conc: 15.35 ng/ml

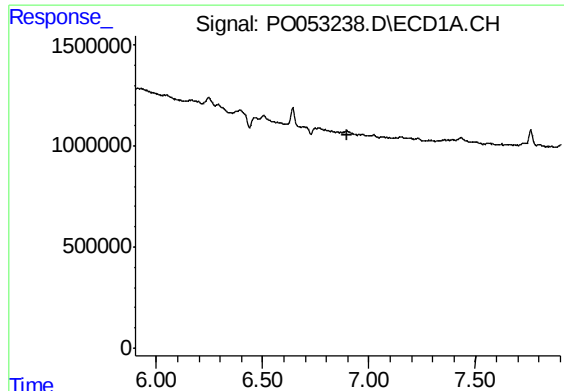

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

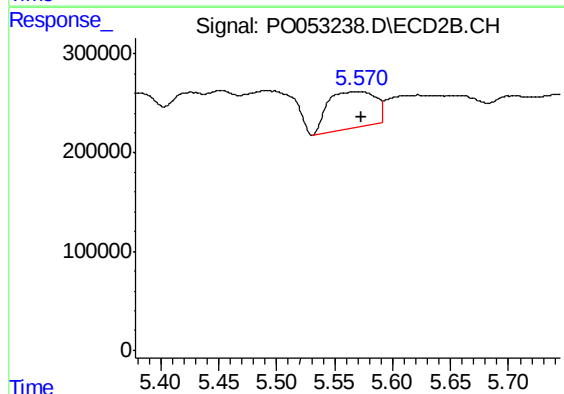


#31 AR-1260-1

R.T.: 5.571 min
Delta R.T.: -0.002 min
Response: 1065231
Conc: 69.40 ng/ml

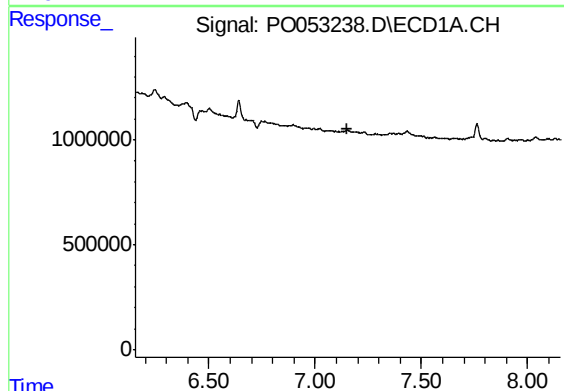


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

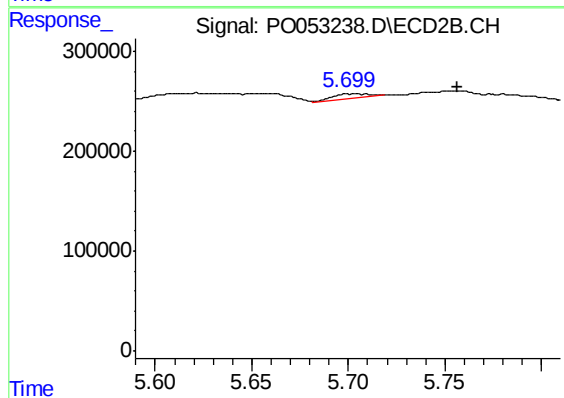

#32 AR-1260-2


R.T.: 5.699 min
Delta R.T.: -0.058 min
Response: 65456
Conc: 3.42 ng/ml

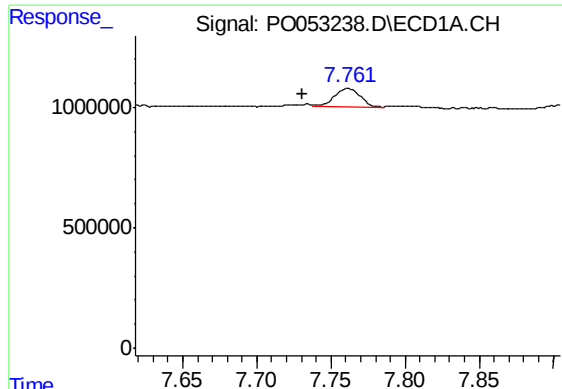

#34 AR-1260-4


R.T.: 7.761 min
Delta R.T.: 0.030 min
Response: 940686
Conc: 24.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

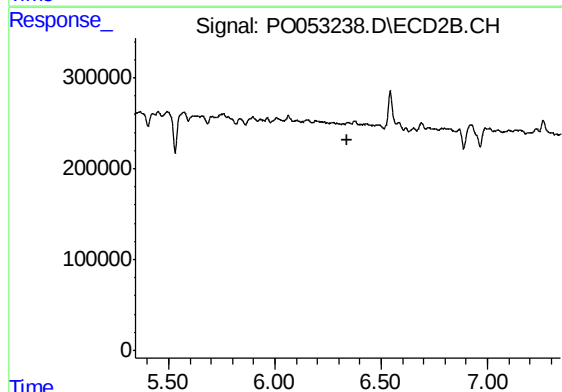


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 6.343 min
Response: 0
Conc: N.D.

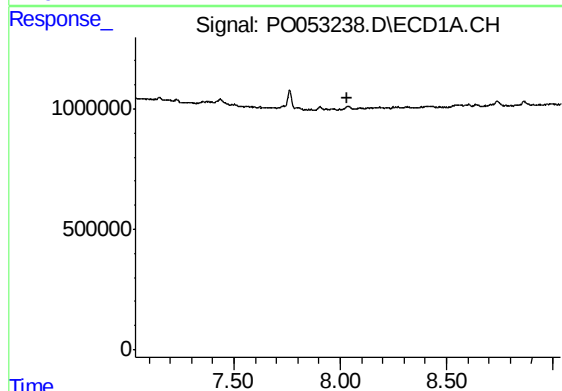


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.036 min
Response: 0
Conc: N.D.

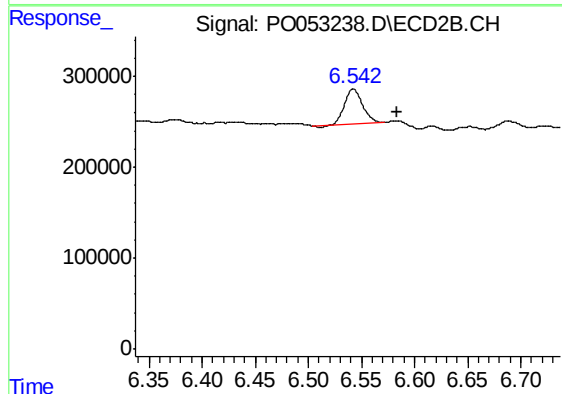

#35 AR-1260-5


R.T.: 6.542 min
Delta R.T.: -0.041 min
Response: 460301
Conc: 15.98 ng/ml

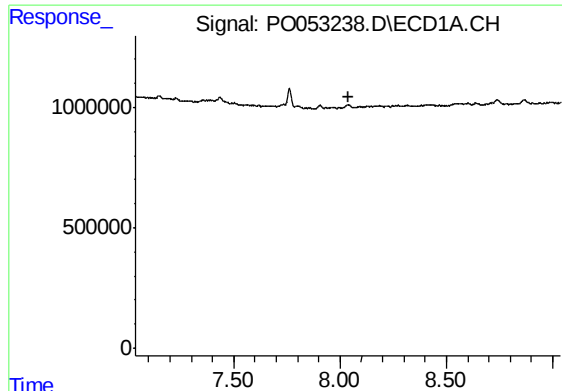

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

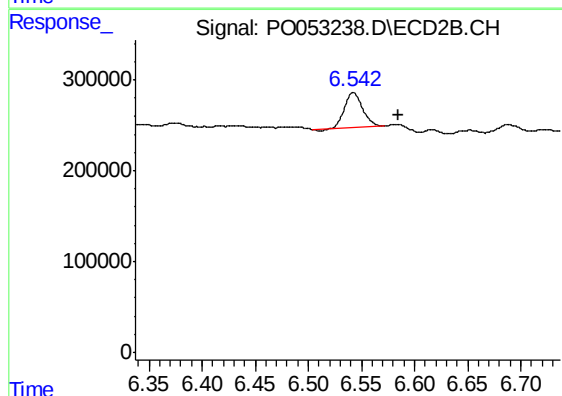


#37 AR-1262-2

R.T.: 6.542 min
Delta R.T.: -0.042 min
Response: 460301
Conc: 13.86 ng/ml

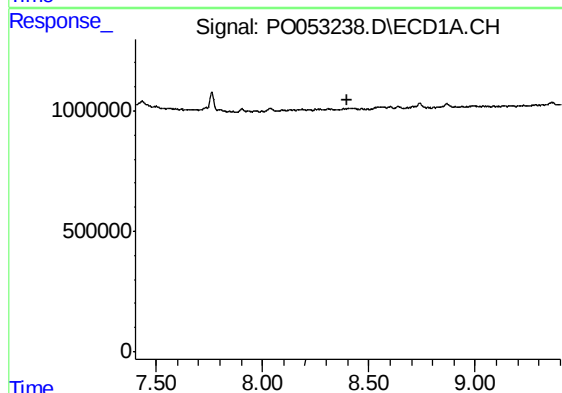


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.402 min
Response: 0
Conc: N.D.

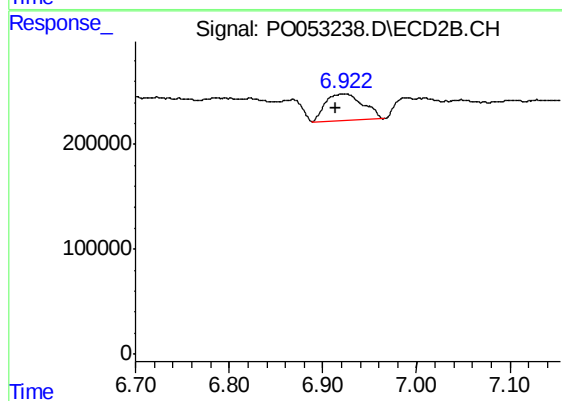

#39 AR-1262-4


R.T.: 6.922 min
Delta R.T.: 0.008 min
Response: 710818
Conc: 29.28 ng/ml

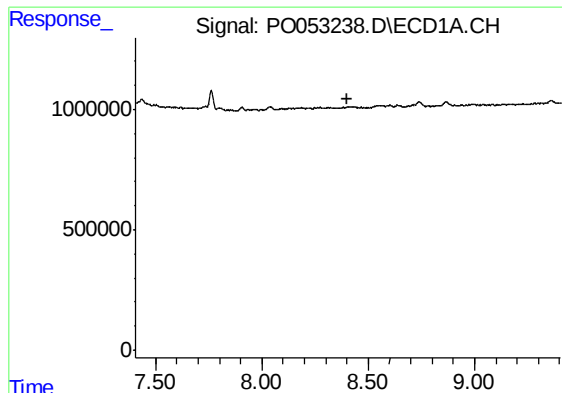

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

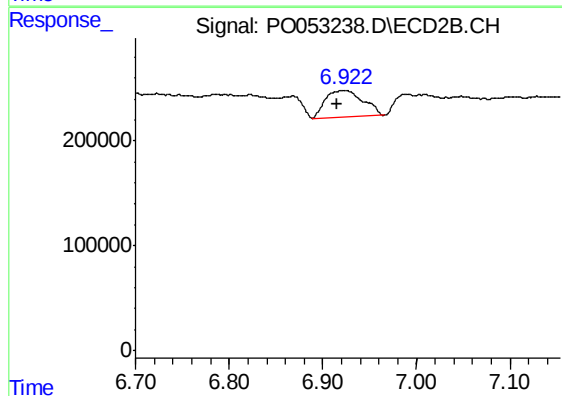

#42 AR-1268-2

R.T.: 6.922 min
Delta R.T.: 0.007 min
Response: 710818
Conc: 17.28 ng/ml