

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053239.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 6:46
 Operator : SM/SJ
 Sample : K1034-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:05:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.177	3.212	37451179	5235785	28.623	23.333
2)	SA Decachlor...	9.649	7.860	15673220	5480771	19.781	21.321
Target Compounds							
9)	L2 AR-1221-2	4.477	0.000	473558	0	54.828	N.D. #
12)	L3 AR-1232-2	5.131	0.000	128629	0	11.352	N.D. #
20)	L4 AR-1242-5	6.243	0.000	64642	0	2.954	N.D. #
24)	L5 AR-1248-4	6.243	0.000	64642	0	1.730	N.D. #
25)	L5 AR-1248-5	6.243	0.000	64642	0	1.814	N.D. #
30)	L6 AR-1254-5	0.000	6.066	0	200977	N.D.	10.039 #
31)	L7 AR-1260-1	0.000	5.570	0	140616	N.D.	9.161 #
33)	L7 AR-1260-3	7.537	0.000	287929	0	8.223	N.D. #
34)	L7 AR-1260-4	7.764	0.000	584111	0	15.024	N.D. #
35)	L7 AR-1260-5	0.000	6.543	0	313419	N.D.	10.880 #
36)	L8 AR-1262-1	7.537	6.066	287929	200977	5.167	10.271 #
37)	L8 AR-1262-2	0.000	6.543	0	313419	N.D.	9.438 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010419\
Data File : PO053239.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 6:46
Operator : SM/SJ
Sample : K1034-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:05:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

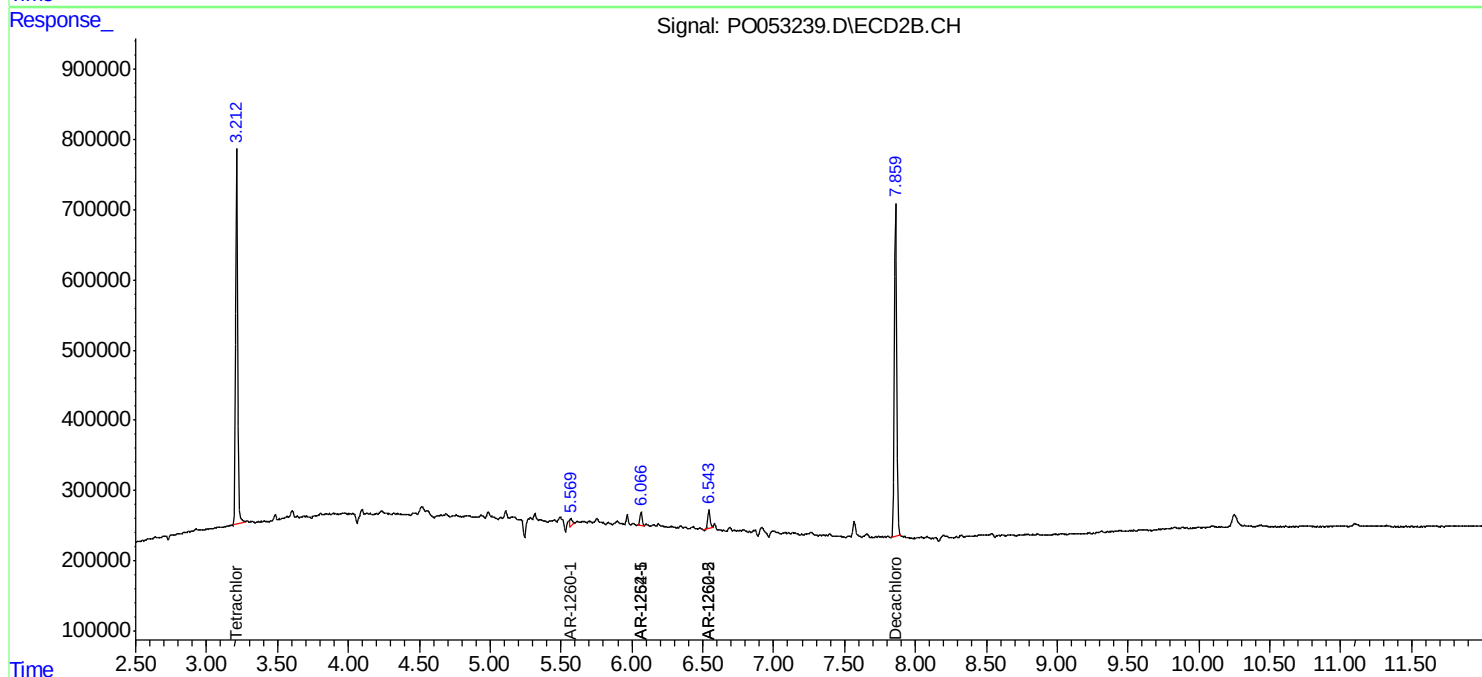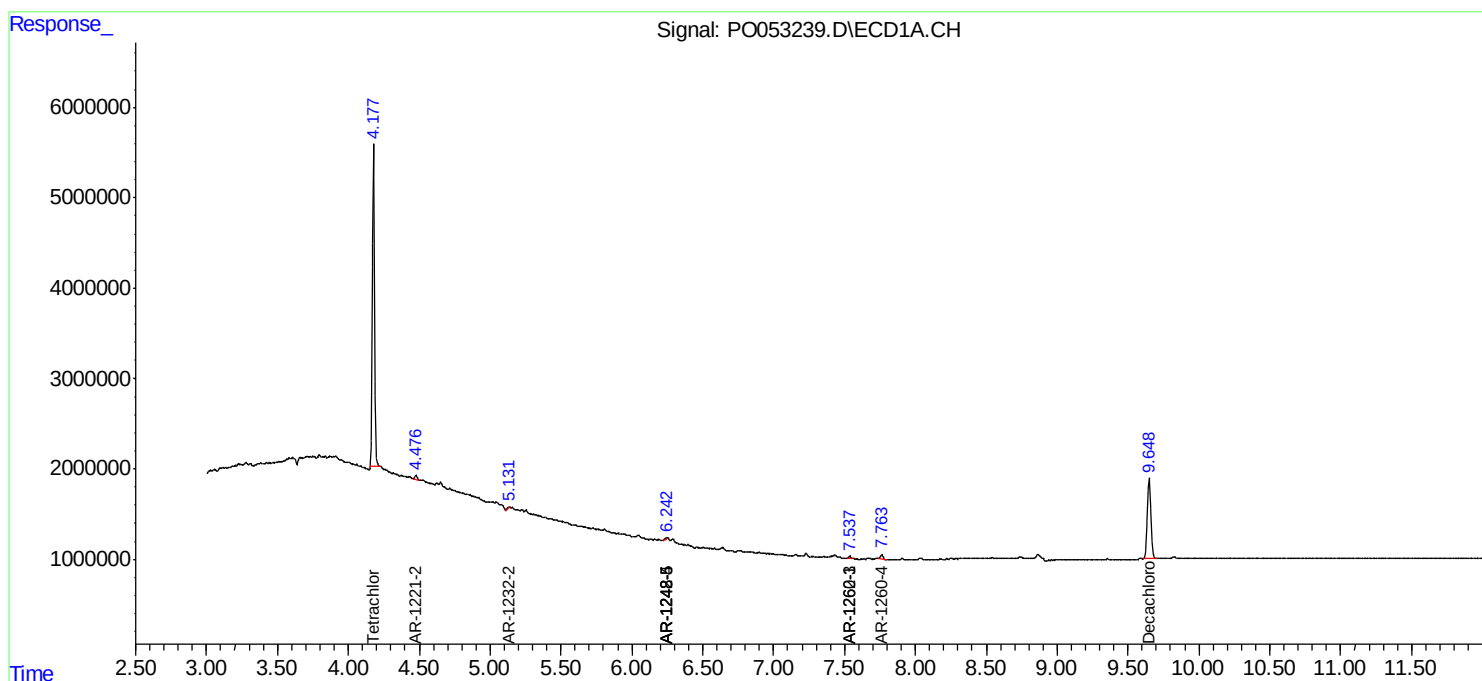


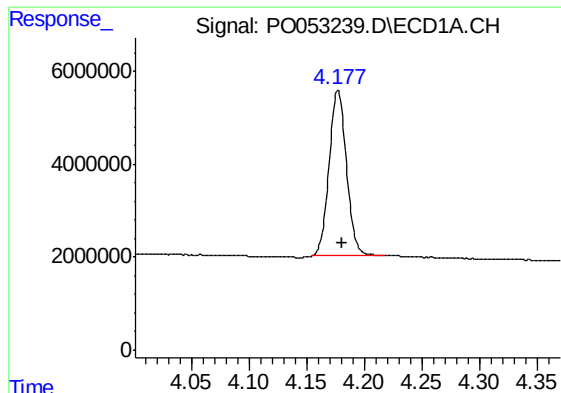

#1 Tetrachloro-m-xylene


R.T.: 4.177 min
Delta R.T.: -0.004 min
Response: 37451179
Conc: 28.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

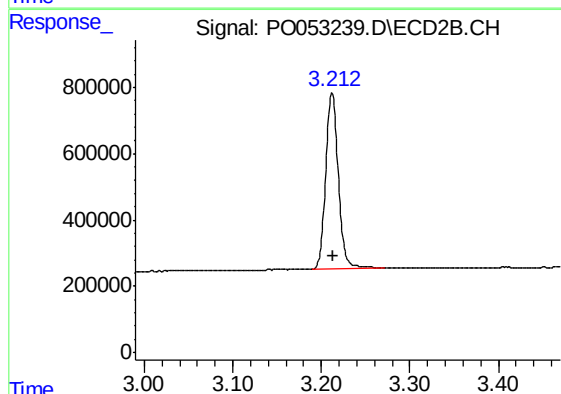


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 5235785
Conc: 23.33 ng/ml

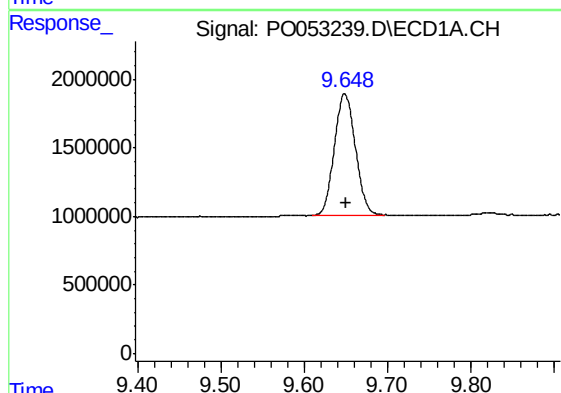


#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.002 min
Response: 15673220
Conc: 19.78 ng/ml

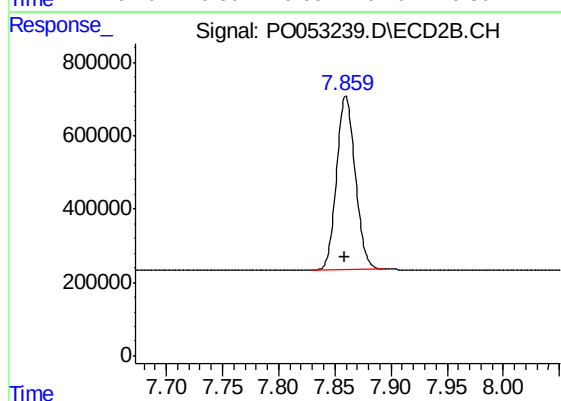

#2 Decachlorobiphenyl


R.T.: 7.860 min
Delta R.T.: 0.000 min
Response: 5480771
Conc: 21.32 ng/ml

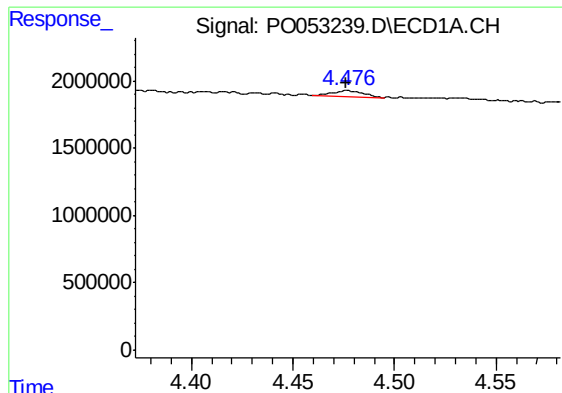

#9 AR-1221-2


R.T.: 4.477 min
Delta R.T.: 0.000 min
Response: 473558
Conc: 54.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

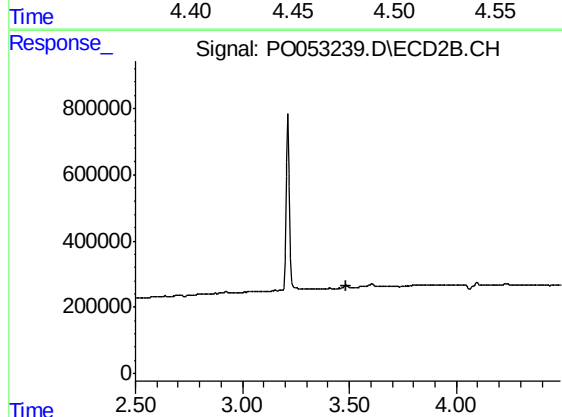


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

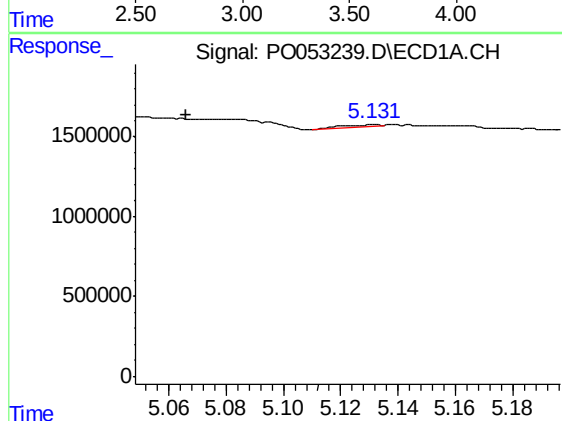


#12 AR-1232-2

R.T.: 5.131 min
Delta R.T.: 0.066 min
Response: 128629
Conc: 11.35 ng/ml

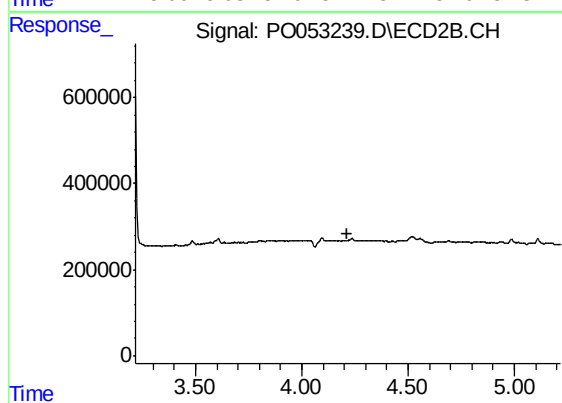

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

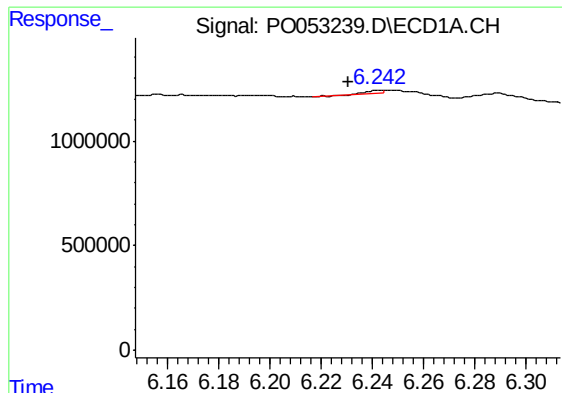

#20 AR-1242-5


R.T.: 6.243 min
Delta R.T.: 0.012 min
Response: 64642
Conc: 2.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

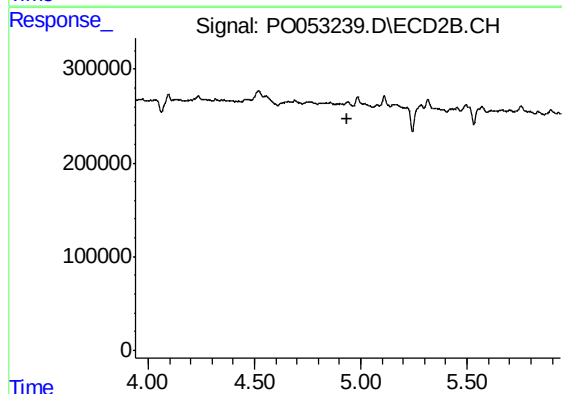


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 4.939 min
Response: 0
Conc: N.D.

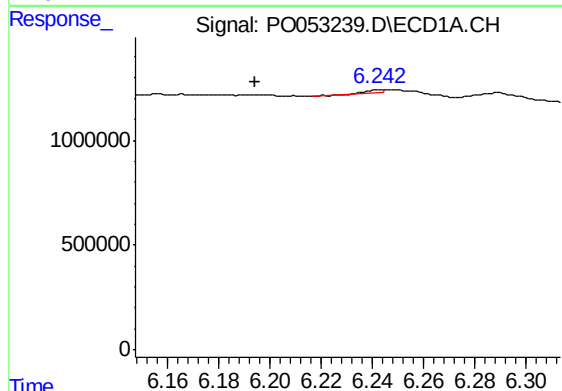


#24 AR-1248-4

R.T.: 6.243 min
Delta R.T.: 0.048 min
Response: 64642
Conc: 1.73 ng/ml

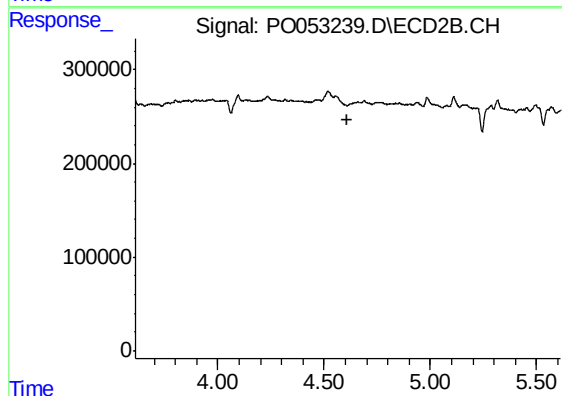

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.612 min
Response: 0
Conc: N.D.

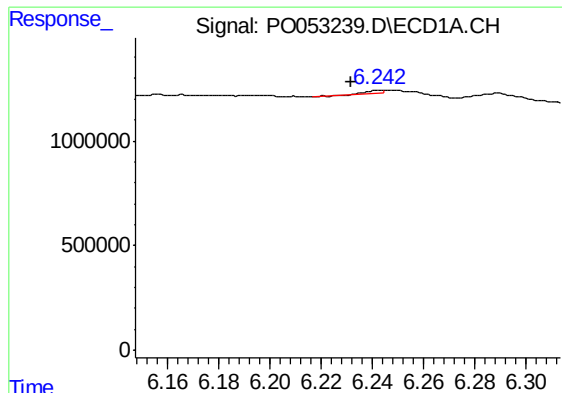

#25 AR-1248-5


R.T.: 6.243 min
Delta R.T.: 0.011 min
Response: 64642
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

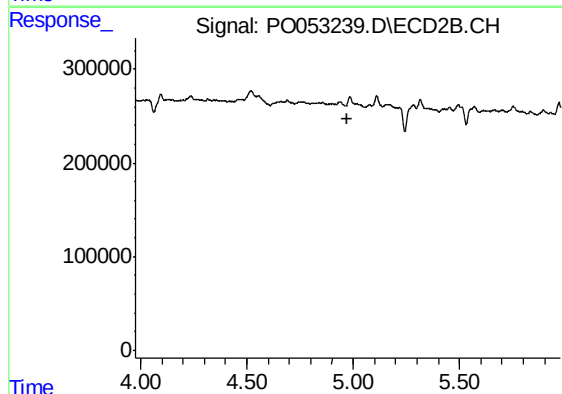


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

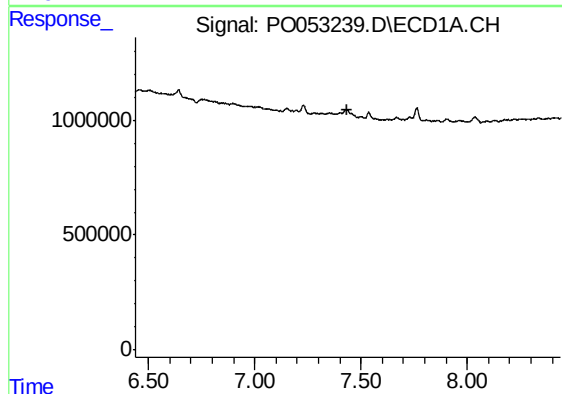


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

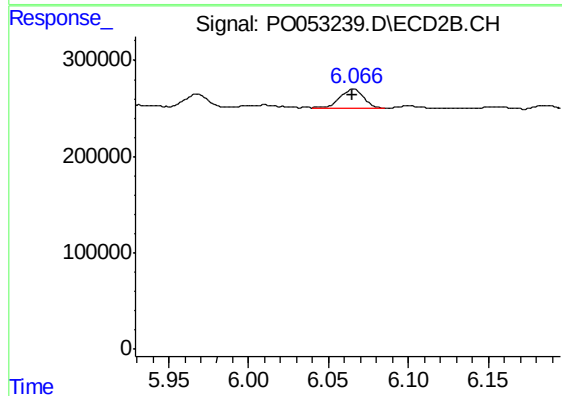

#30 AR-1254-5


R.T.: 6.066 min
Delta R.T.: 0.001 min
Response: 200977
Conc: 10.04 ng/ml

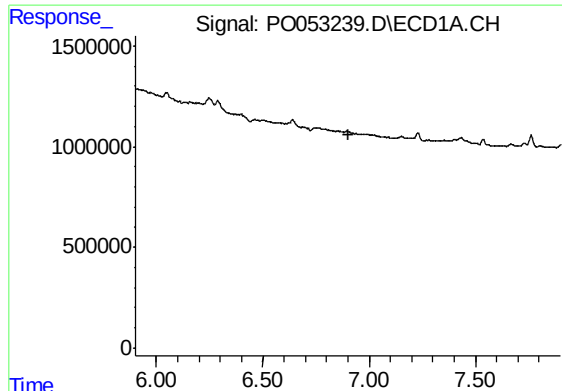

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

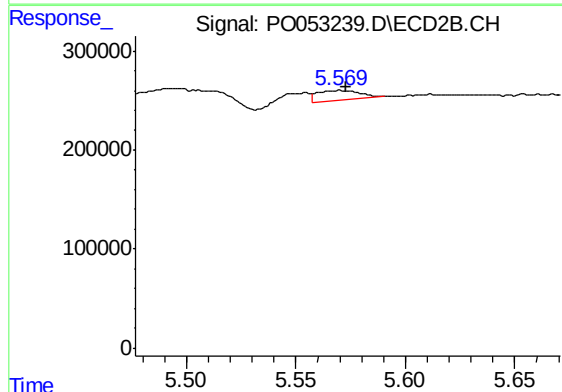


#31 AR-1260-1

R.T.: 5.570 min
Delta R.T.: -0.003 min
Response: 140616
Conc: 9.16 ng/ml

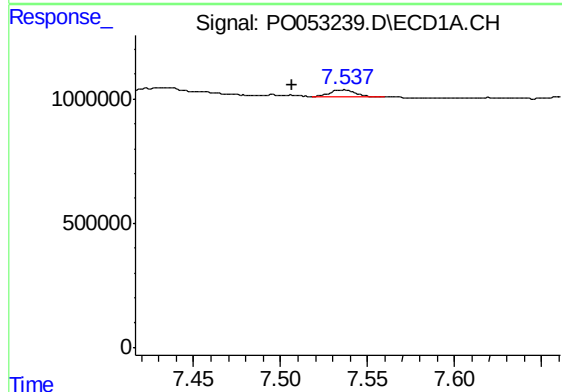


#33 AR-1260-3

R.T.: 7.537 min
Delta R.T.: 0.030 min
Response: 287929
Conc: 8.22 ng/ml

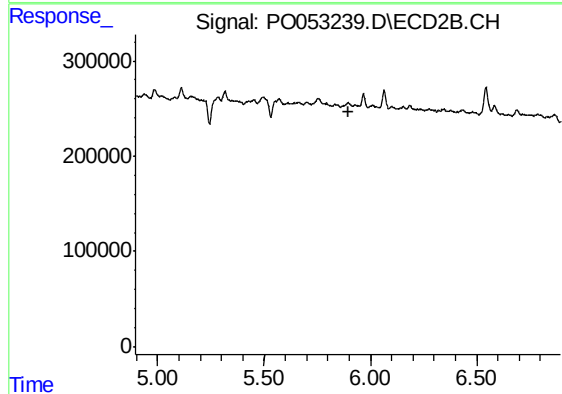

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 5.895 min
Response: 0
Conc: N.D.

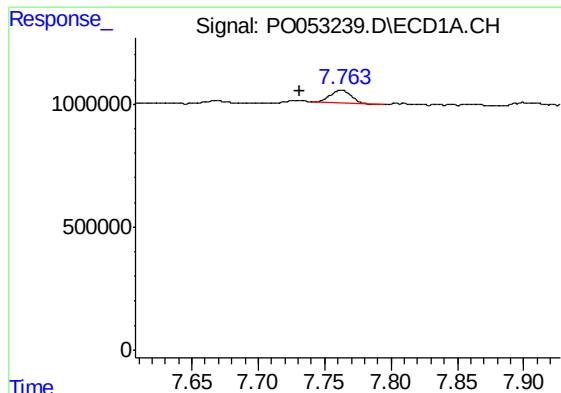

#34 AR-1260-4


R.T.: 7.764 min
Delta R.T.: 0.033 min
Response: 584111
Conc: 15.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

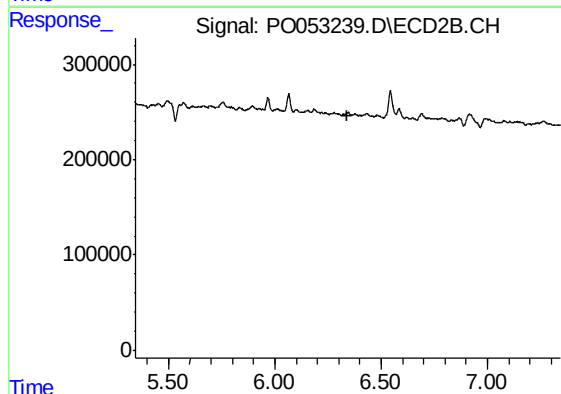


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 6.343 min
Response: 0
Conc: N.D.

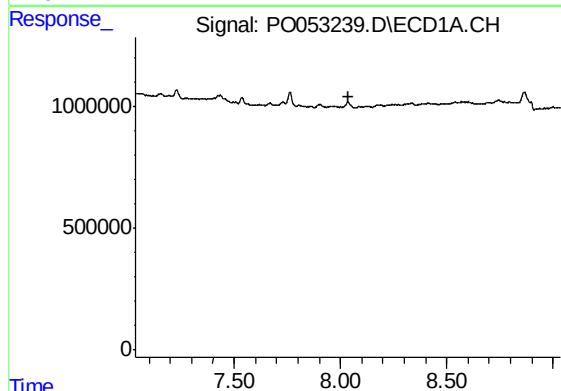


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.036 min
Response: 0
Conc: N.D.

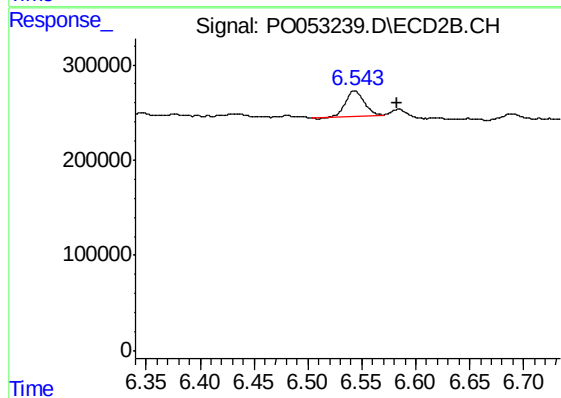

#35 AR-1260-5


R.T.: 6.543 min
Delta R.T.: -0.040 min
Response: 313419
Conc: 10.88 ng/ml

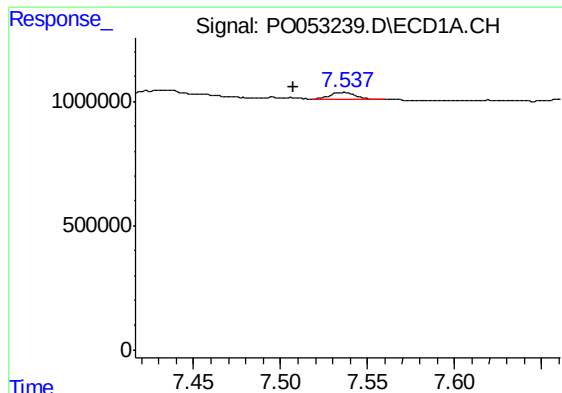

#36 AR-1262-1


R.T.: 7.537 min
Delta R.T.: 0.030 min
Response: 287929
Conc: 5.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-6

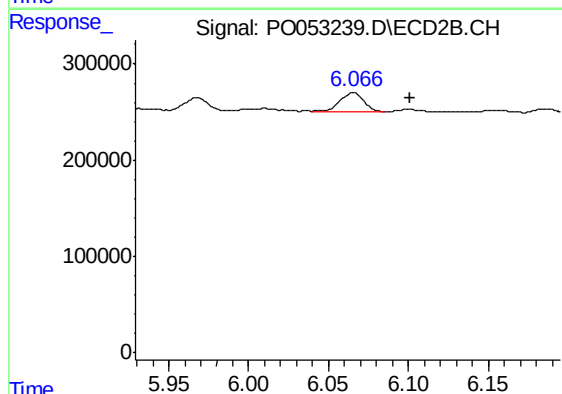


#36 AR-1262-1

R.T.: 6.066 min
Delta R.T.: -0.035 min
Response: 200977
Conc: 10.27 ng/ml

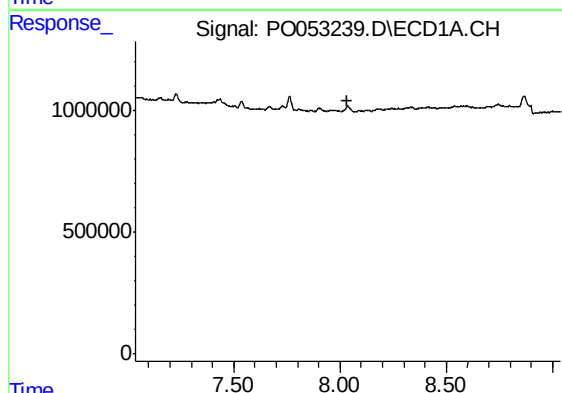

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.037 min
Response: 0
Conc: N.D.

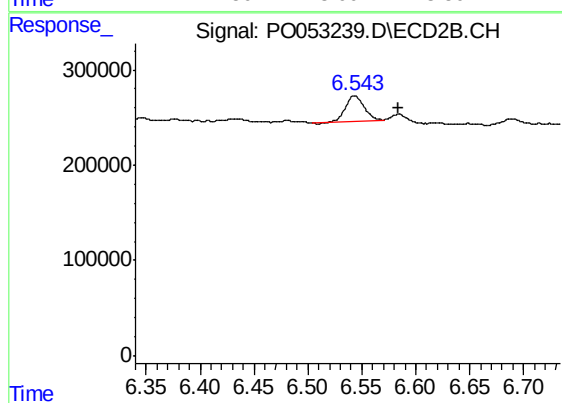

#37 AR-1262-2

R.T.: 6.543 min
Delta R.T.: -0.041 min
Response: 313419
Conc: 9.44 ng/ml