

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053231.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 4:31
 Operator : SM/SJ
 Sample : K1043-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HB-1319-WS

Manual Integrations
 APPROVED

Sohil
 1/7/2019 3:40:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:01:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.177	3.212	34901607	4891975	26.674m	21.801
2) SA Decachlor...	9.650	7.860	13103736	4493438	16.538	17.480

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
Data File : P0053231.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 4:31
Operator : SM/SJ
Sample : K1043-01
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HB-1319-WS


Manual Integrations
APPROVED

Sohil
1/7/2019 3:40:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:01:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

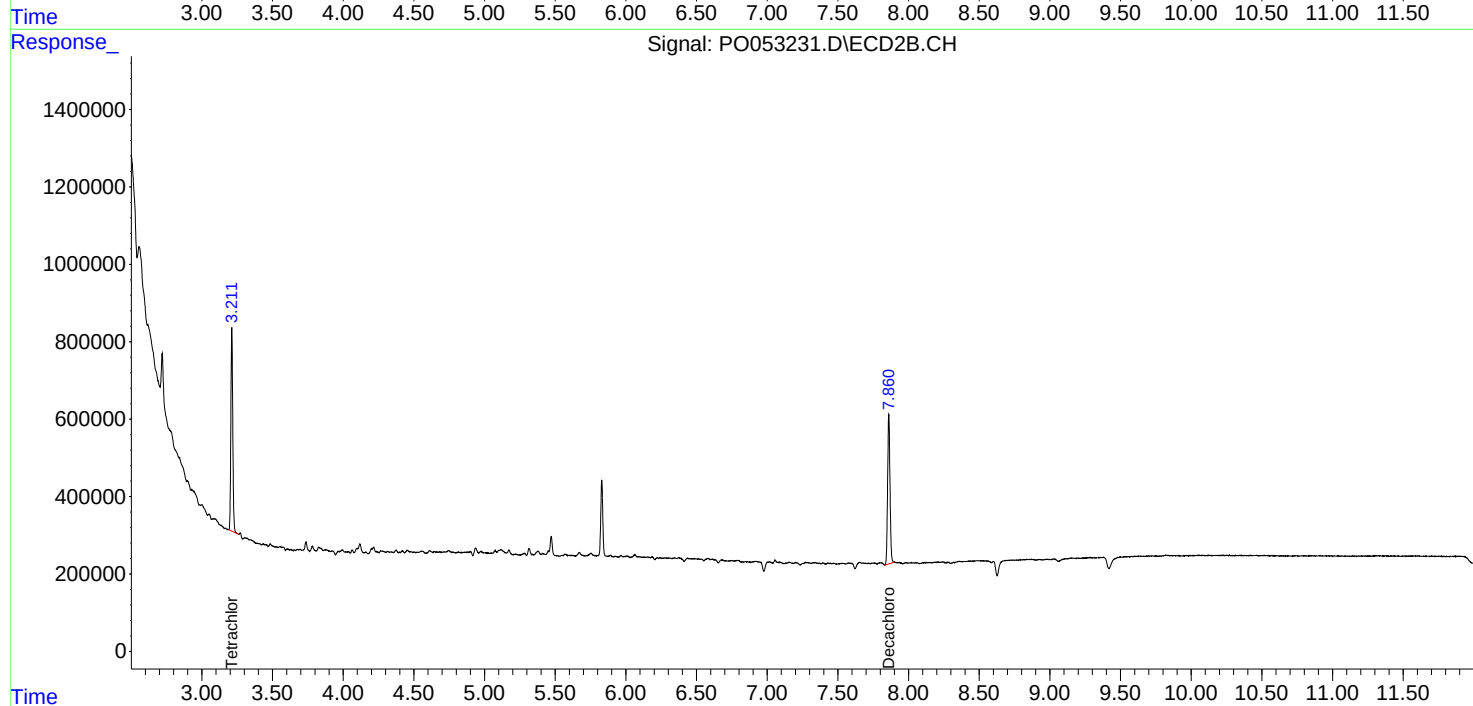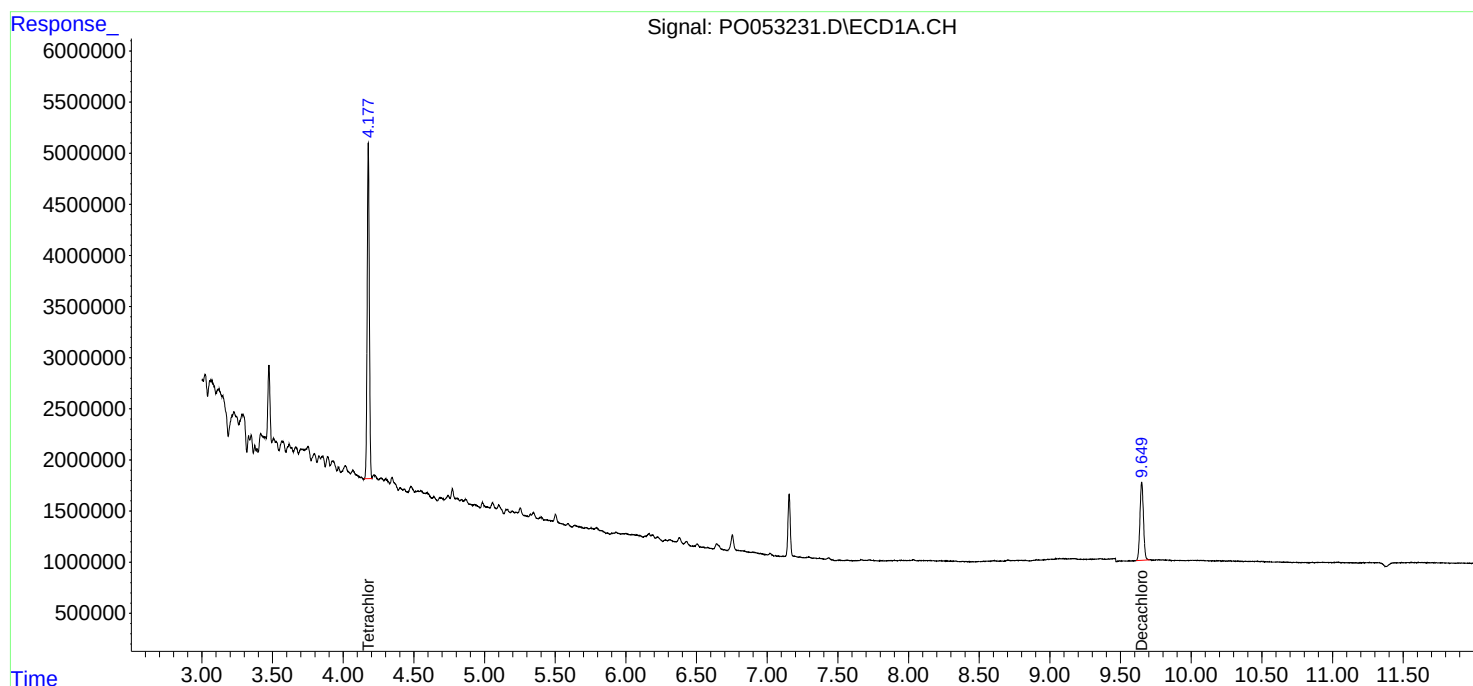

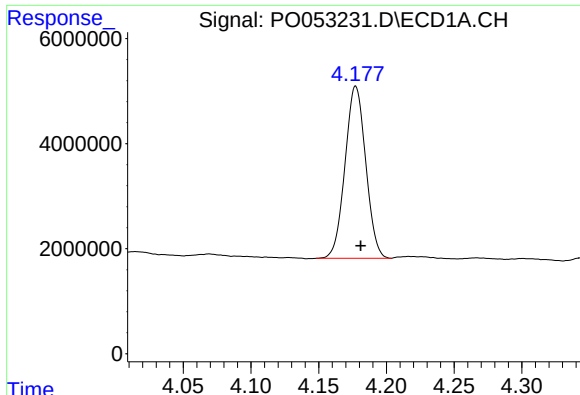


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: -0.004 min
Response: 34901607
Conc: 26.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HB-1319-WS


Manual Integrations
APPROVED

Sohil
1/7/2019 3:40:58 PM

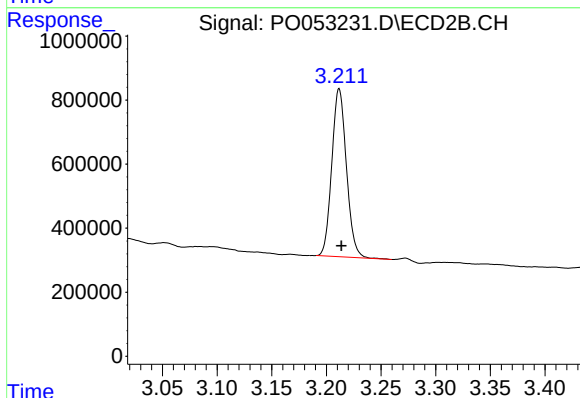


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 4891975
Conc: 21.80 ng/ml

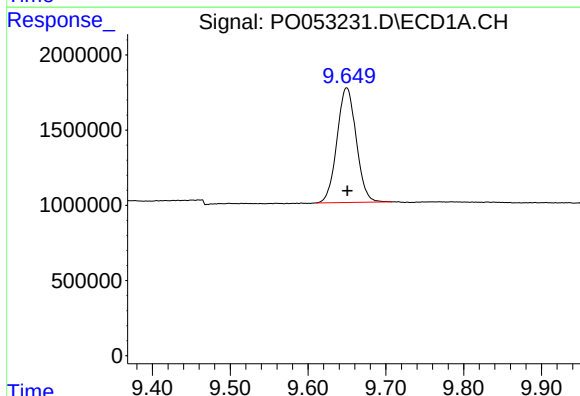

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 13103736
Conc: 16.54 ng/ml

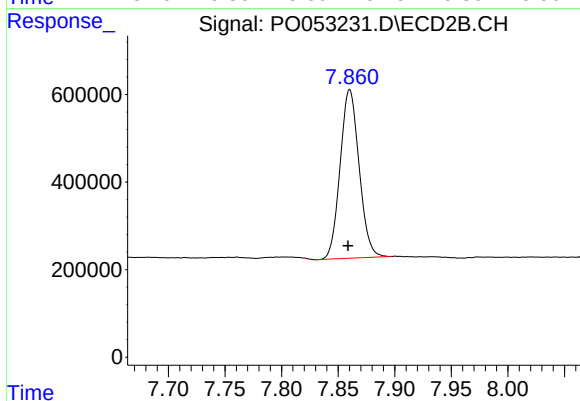

#2 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: 0.001 min
Response: 4493438
Conc: 17.48 ng/ml