

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
 Data File : P0053238.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2019 6:29
 Operator : SM/SJ
 Sample : K1034-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-5

Manual Integrations
 APPROVED

Sohil
 1/7/2019 3:41:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:04:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.177	3.212	47751823	6424041	36.496m	28.629
2) SA Decachlor...	9.650	7.860	20706113	6800458	26.133	26.455

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010419\
Data File : P0053238.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2019 6:29
Operator : SM/SJ
Sample : K1034-05
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5


Manual Integrations
APPROVED

Sohil
1/7/2019 3:41:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:04:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

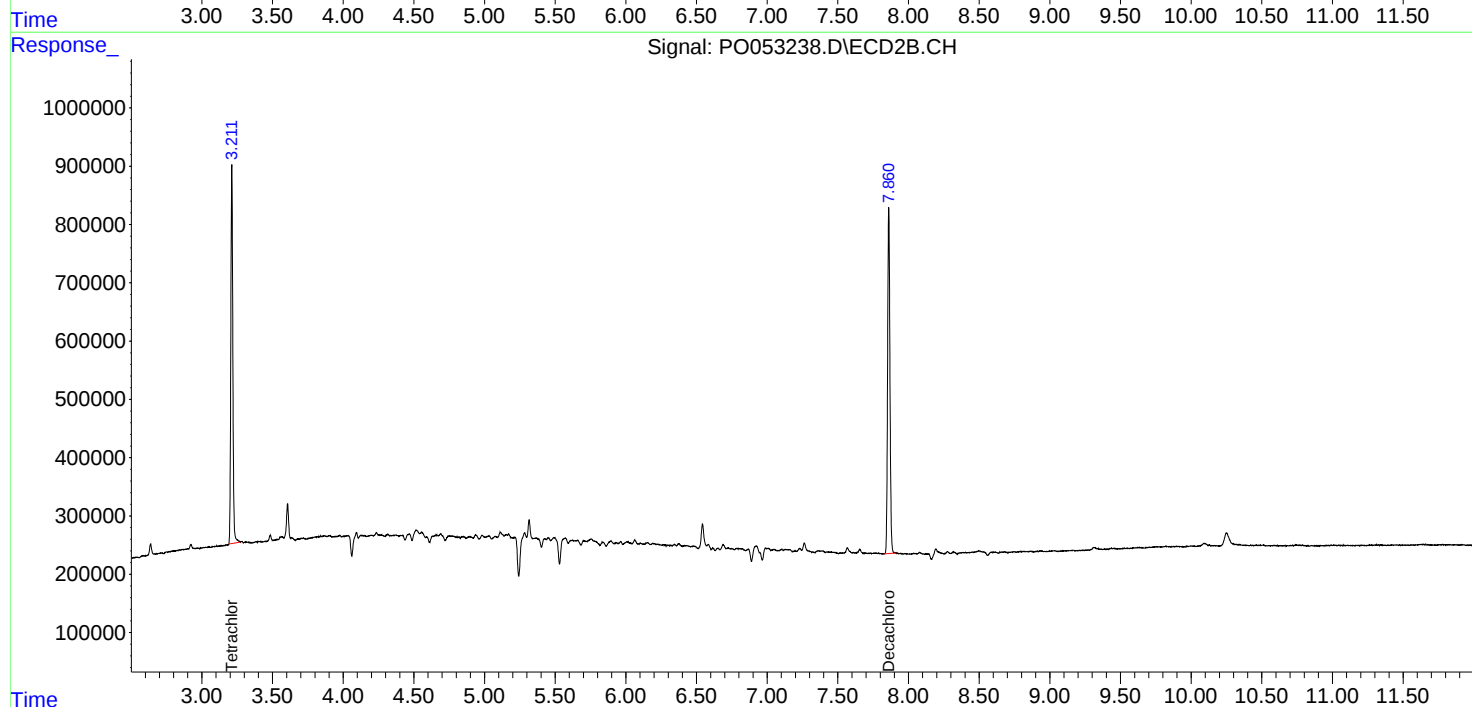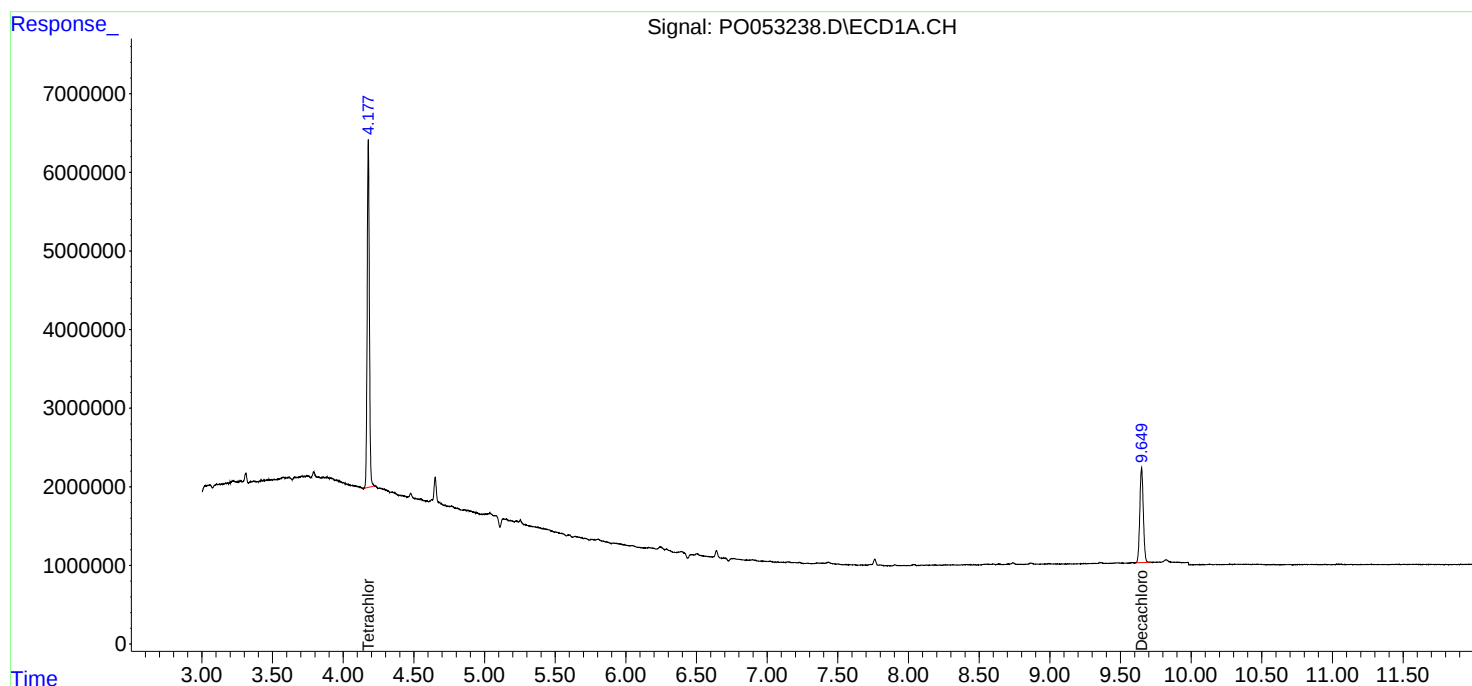

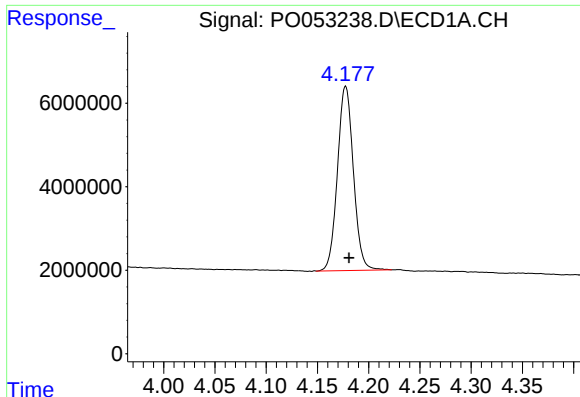


#1 Tetrachloro-m-xylene

R.T.: 4.177 min
Delta R.T.: -0.004 min
Response: 47751823
Conc: 36.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5


Manual Integrations
APPROVED

Sohil
1/7/2019 3:41:05 PM

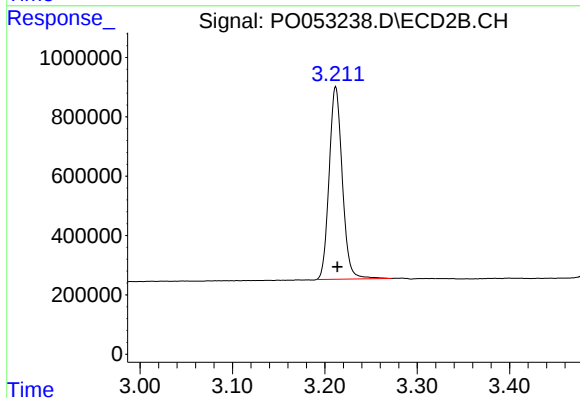


#1 Tetrachloro-m-xylene

R.T.: 3.212 min
Delta R.T.: -0.002 min
Response: 6424041
Conc: 28.63 ng/ml

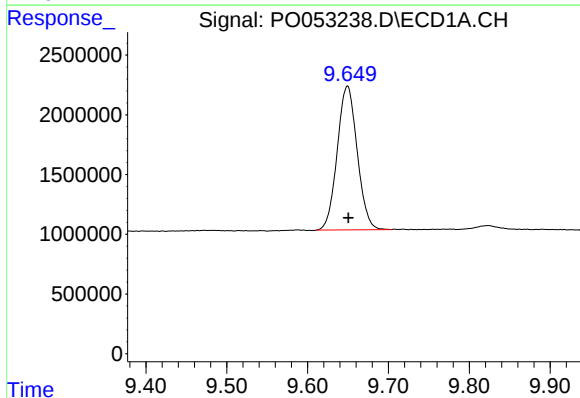

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.001 min
Response: 20706113
Conc: 26.13 ng/ml

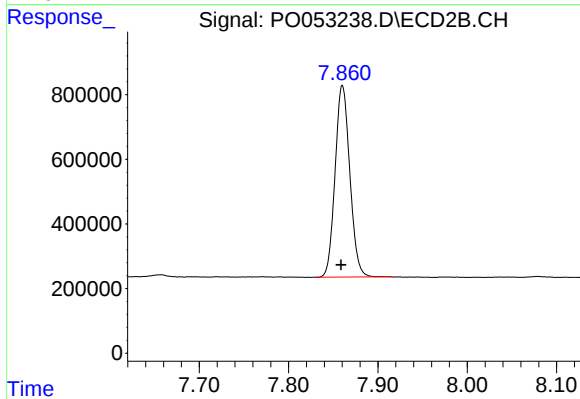

#2 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: 0.001 min
Response: 6800458
Conc: 26.45 ng/ml