

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
 Data File : P0065292.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jan 2020 23:45
 Operator : AJ/MA
 Sample : L1011-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-010220-0-2-COMP-B7

Manual Integrations
 APPROVED

mohammad
 1/6/2020 11:38:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 04:12:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.167	3.441	352244	434882	19.290	19.770
2)	SA Decachlor...	9.677	8.352	538106	691086	15.882	16.665

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
Data File : P0065292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jan 2020 23:45
Operator : AJ/MA
Sample : L1011-06
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MC-010220-0-2-COMP-B7


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 04:12:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

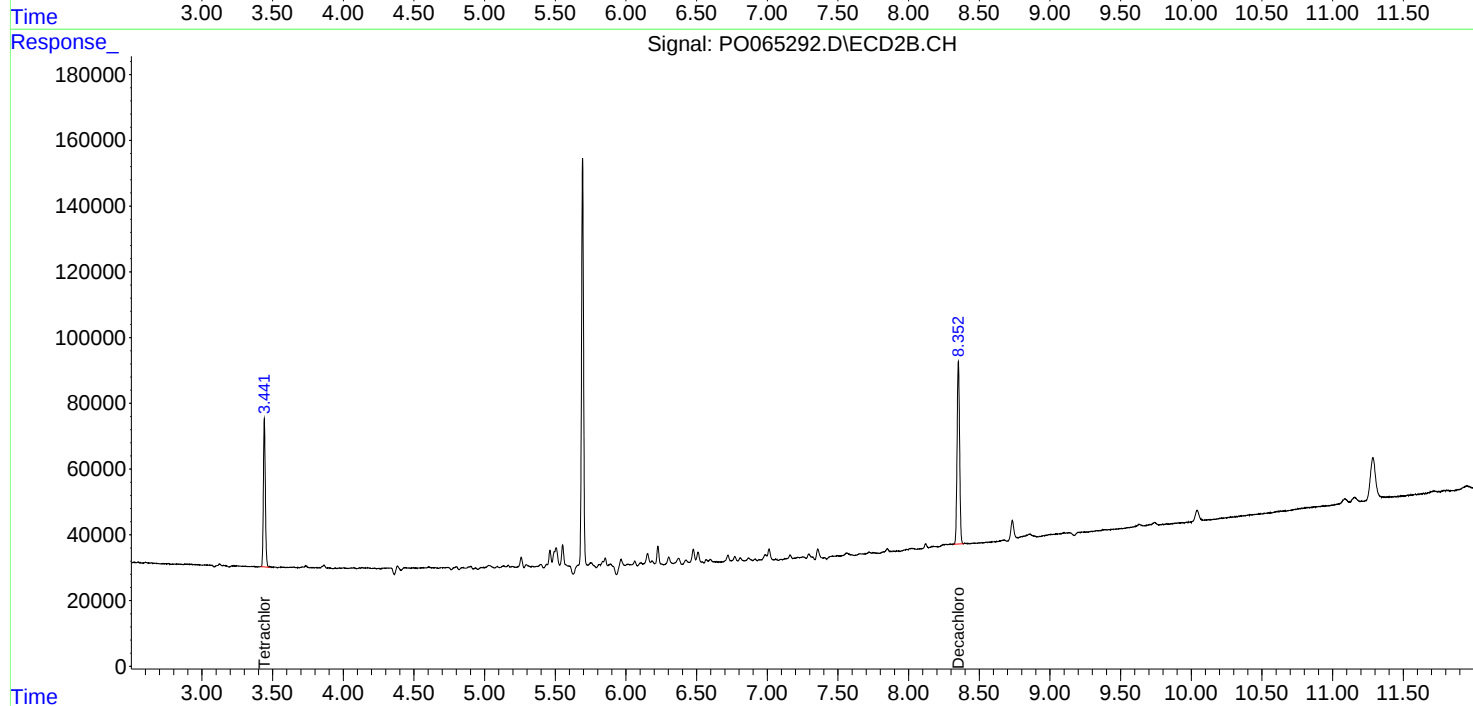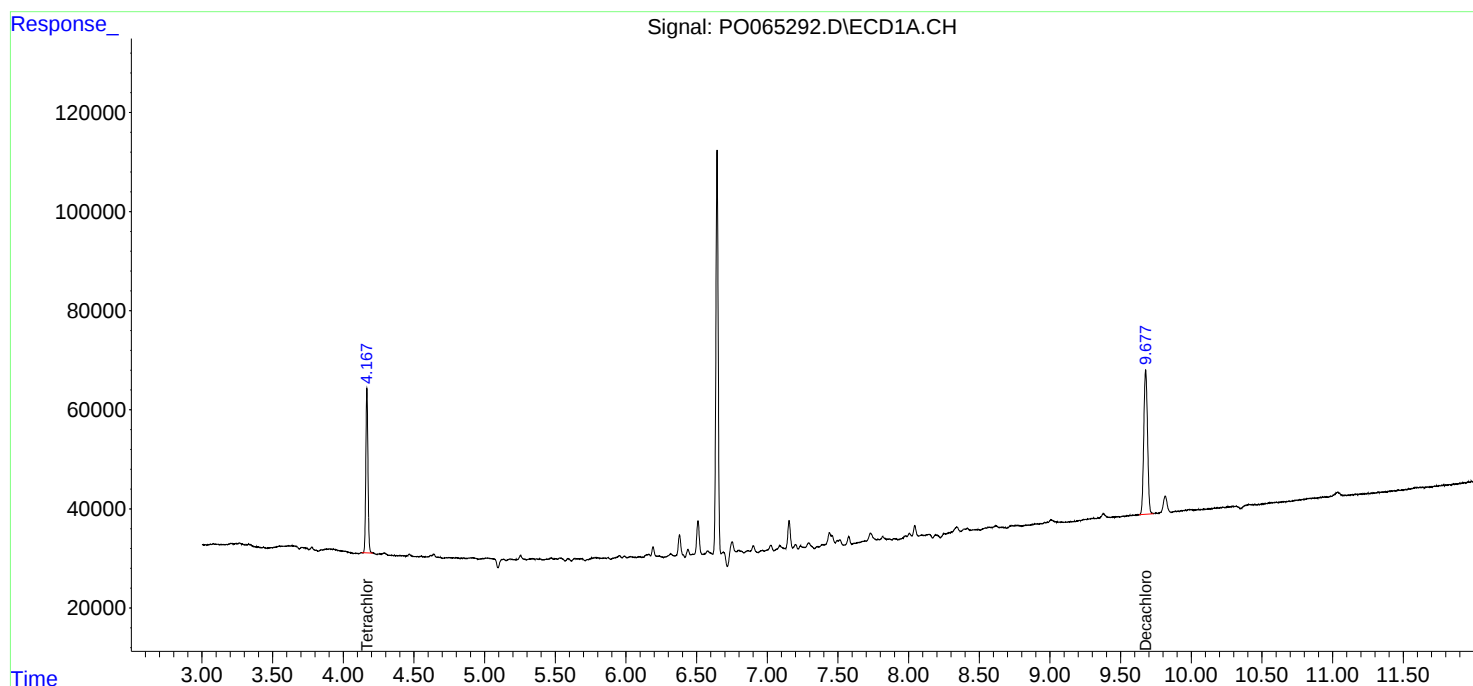

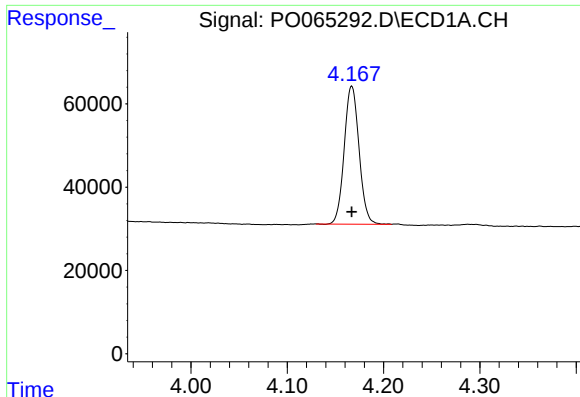


#1 Tetrachloro-m-xylene

R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 352244
Conc: 19.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MC-010220-0-2-COMP-B7


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:28 AM

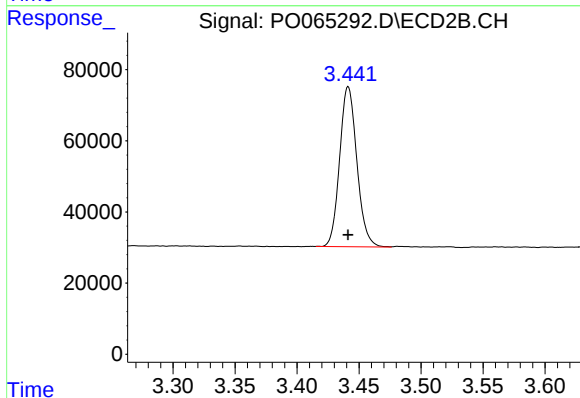


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 434882
Conc: 19.77 ng/ml

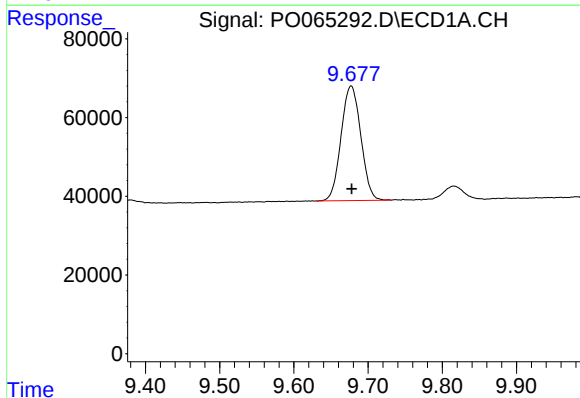

#2 Decachlorobiphenyl

R.T.: 9.677 min
Delta R.T.: 0.000 min
Response: 538106
Conc: 15.88 ng/ml

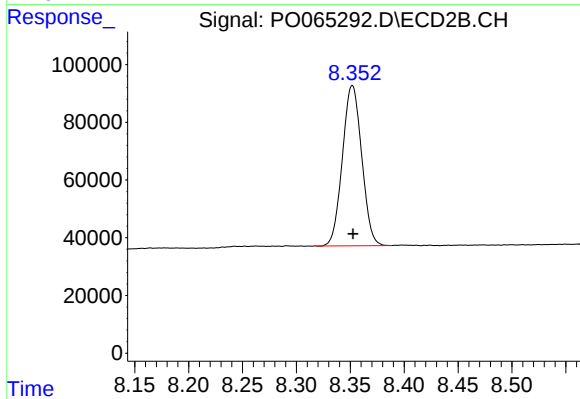

#2 Decachlorobiphenyl

R.T.: 8.352 min
Delta R.T.: 0.000 min
Response: 691086
Conc: 16.66 ng/ml