

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
 Data File : P0065294.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jan 2020 00:18
 Operator : AJ/MA
 Sample : L1011-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MC-010220-2-5-COMP-B7

Manual Integrations
 APPROVED

mohammad
 1/6/2020 11:38:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 04:13:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.166	3.441	498106	646376	27.278m	29.384
2) SA Decachlor...	9.677	8.351	600792	707344	17.732	17.057

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010420\
Data File : PO065294.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jan 2020 00:18
Operator : AJ/MA
Sample : L1011-08
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MC-010220-2-5-COMP-B7


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 04:13:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

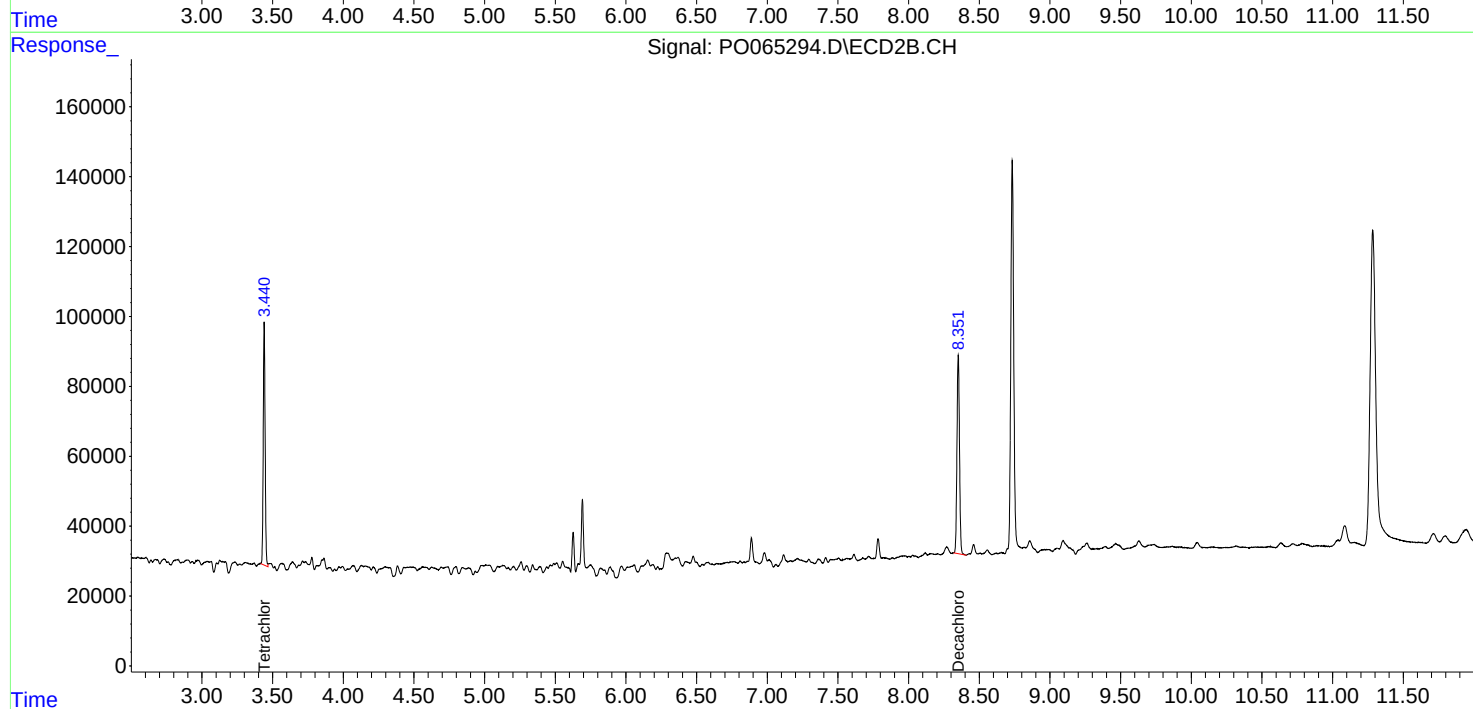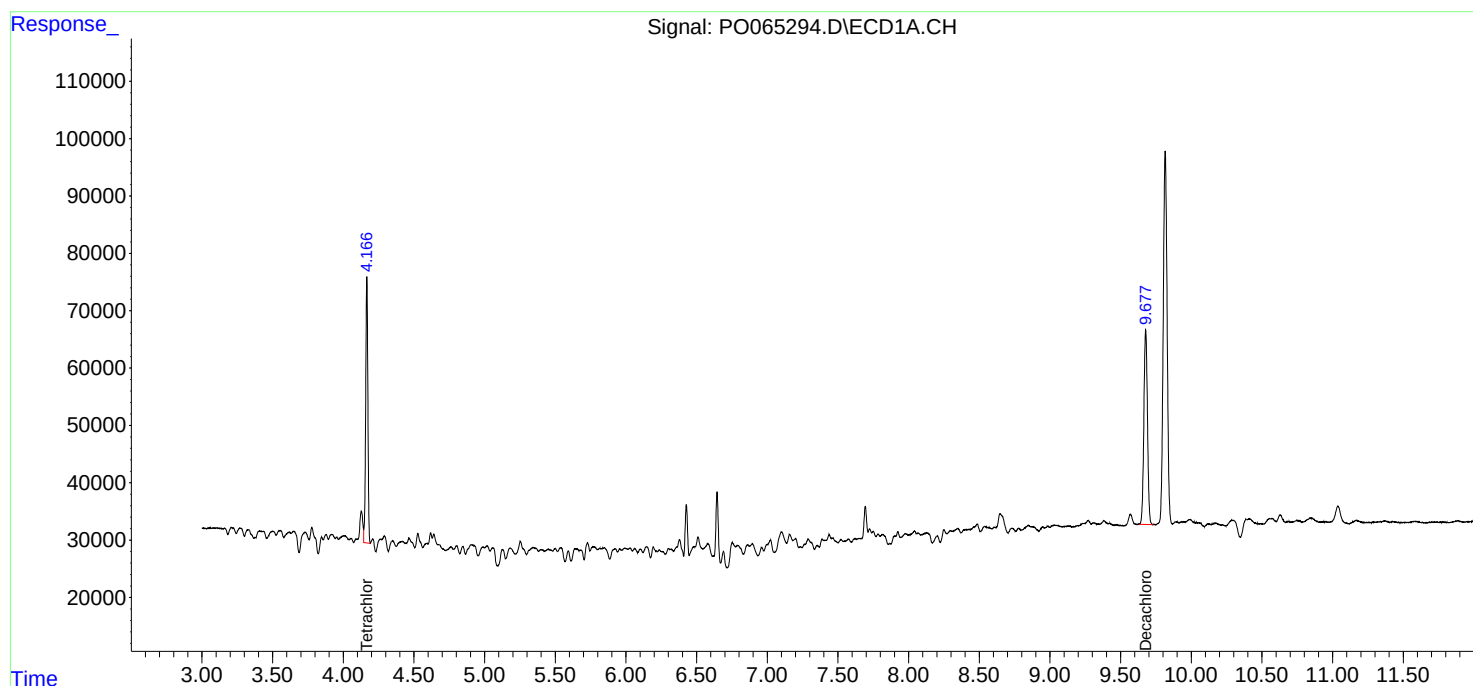

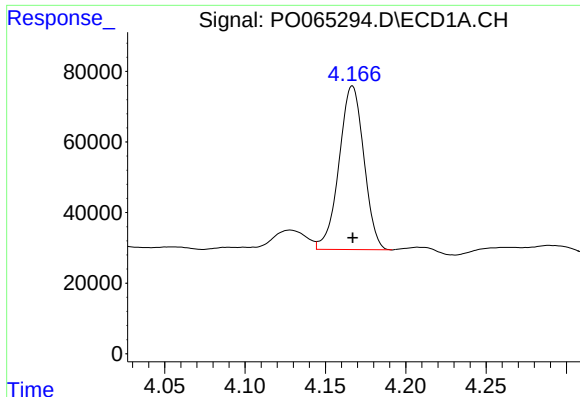


#1 Tetrachloro-m-xylene

R.T.: 4.166 min
Delta R.T.: 0.000 min
Response: 498106
Conc: 27.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MC-010220-2-5-COMP-B7


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:34 AM

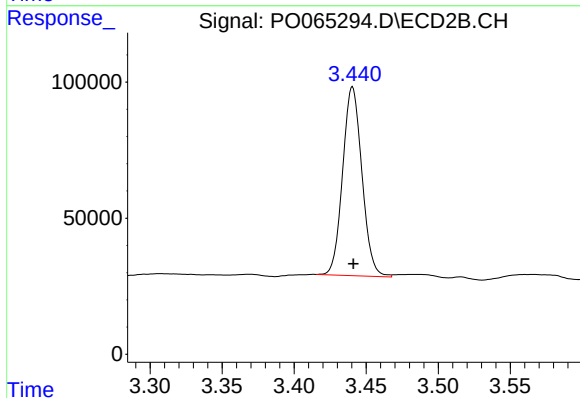


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 646376
Conc: 29.38 ng/ml

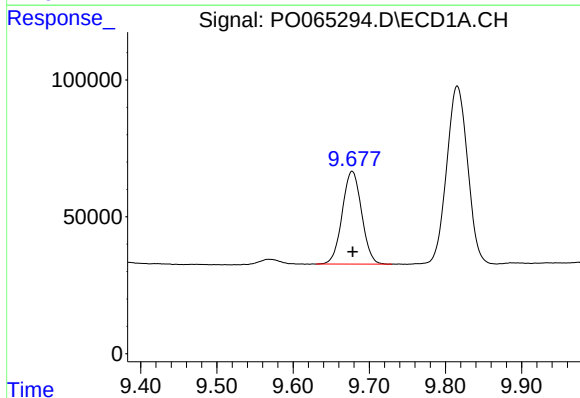

#2 Decachlorobiphenyl

R.T.: 9.677 min
Delta R.T.: 0.000 min
Response: 600792
Conc: 17.73 ng/ml

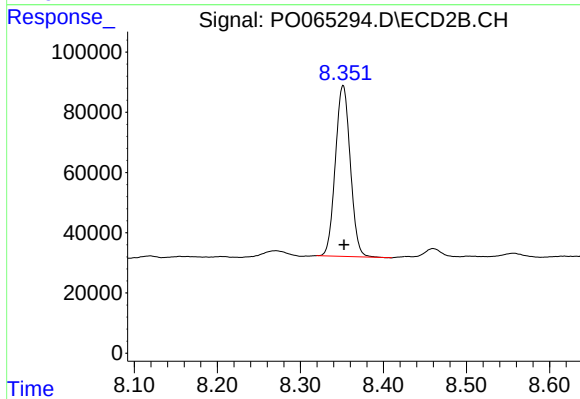

#2 Decachlorobiphenyl

R.T.: 8.351 min
Delta R.T.: -0.001 min
Response: 707344
Conc: 17.06 ng/ml