

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
 Data File : P0065303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jan 2020 3:23
 Operator : AJ/MA
 Sample : L1027-01 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-01

Manual Integrations
 APPROVED

mohammad
 1/6/2020 11:38:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 04:19:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.441	98670	118144	5.404	5.371
2) SA Decachlor...	9.687	8.356	120005	87787	3.542m	2.117m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
Data File : P0065303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jan 2020 3:23
Operator : AJ/MA
Sample : L1027-01 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-01


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 04:19:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

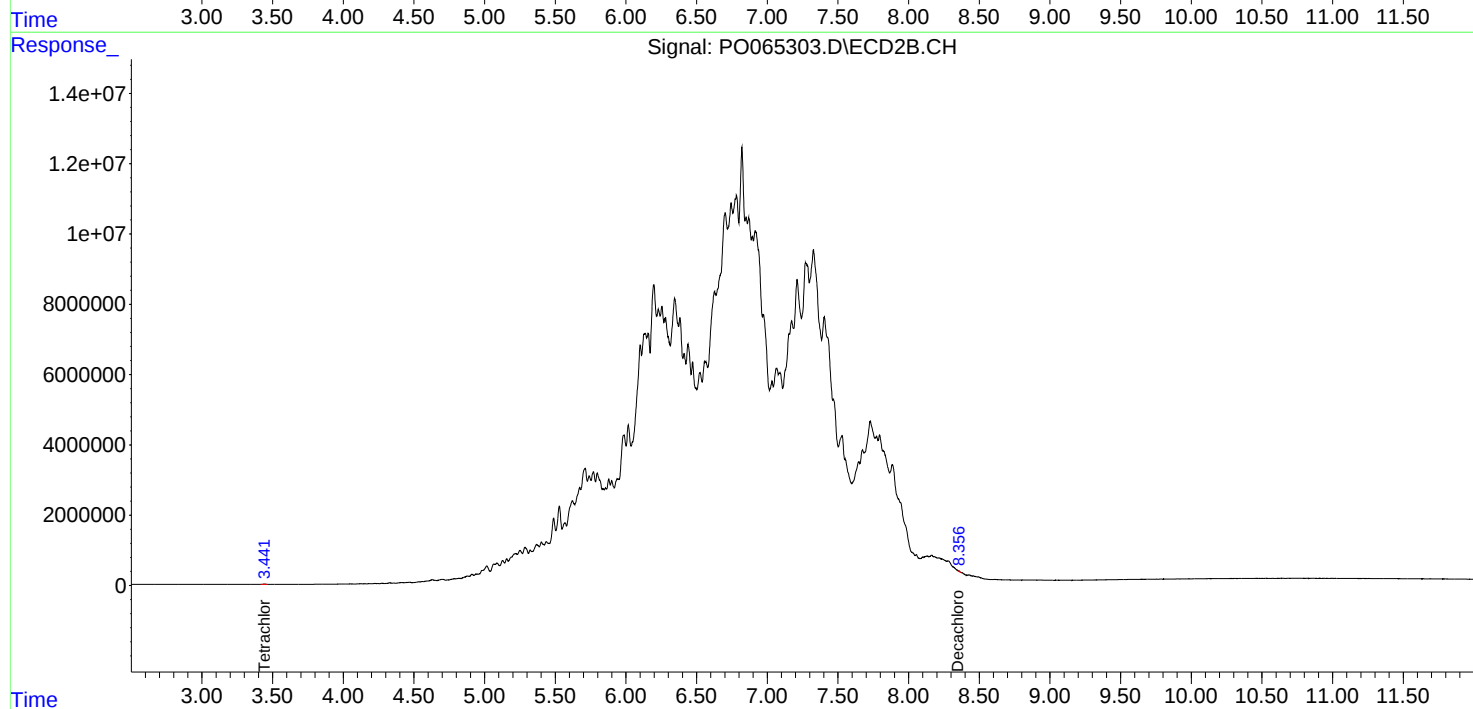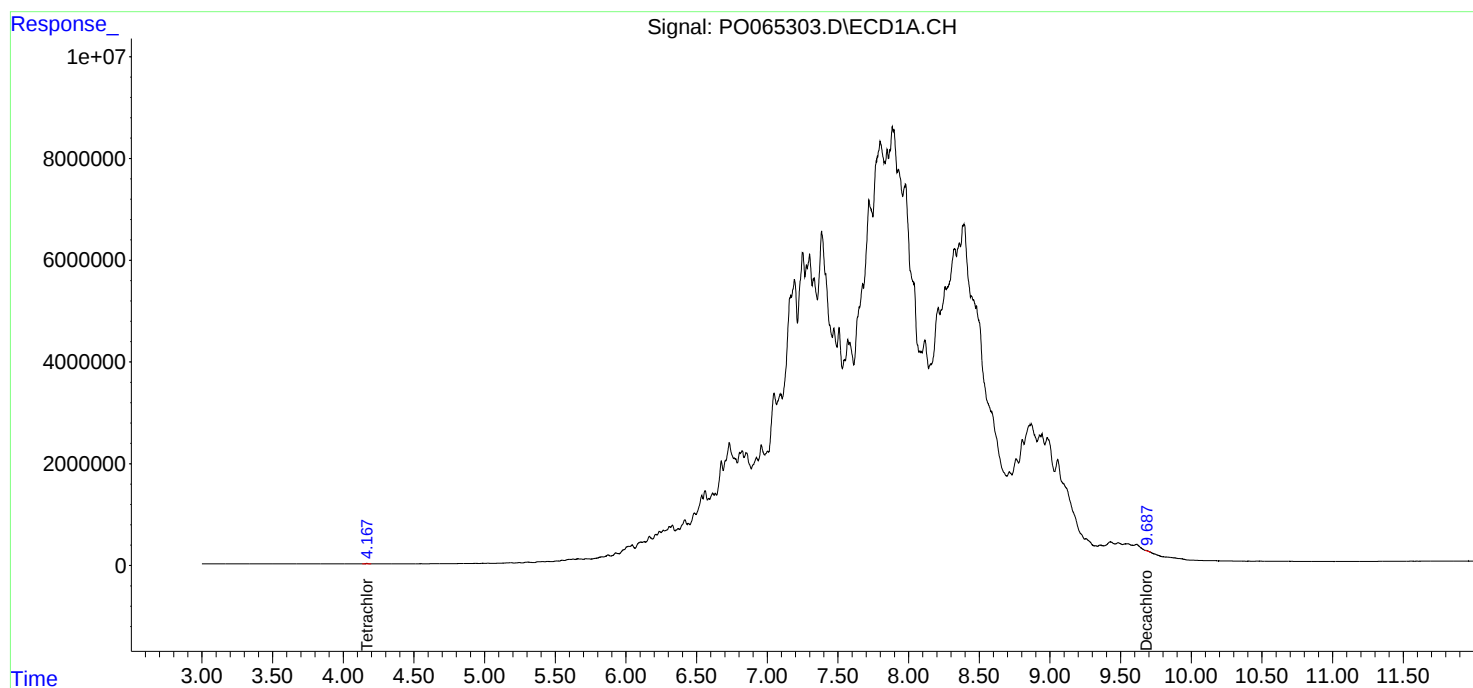

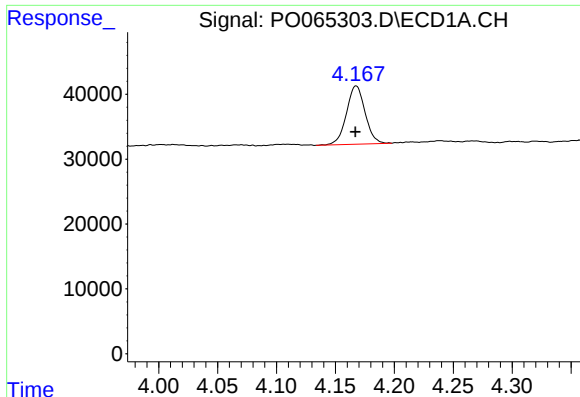


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.000 min
Response: 98670
Conc: 5.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-01


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:47 AM

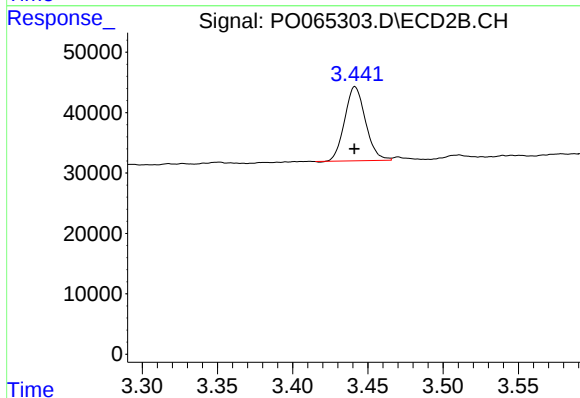


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 118144
Conc: 5.37 ng/ml

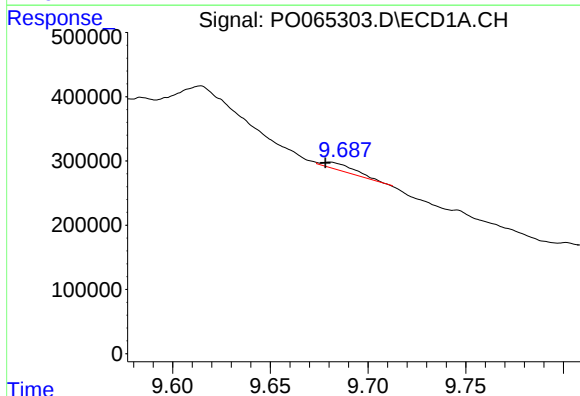

#2 Decachlorobiphenyl

R.T.: 9.687 min
Delta R.T.: 0.009 min
Response: 120005
Conc: 3.54 ng/ml m

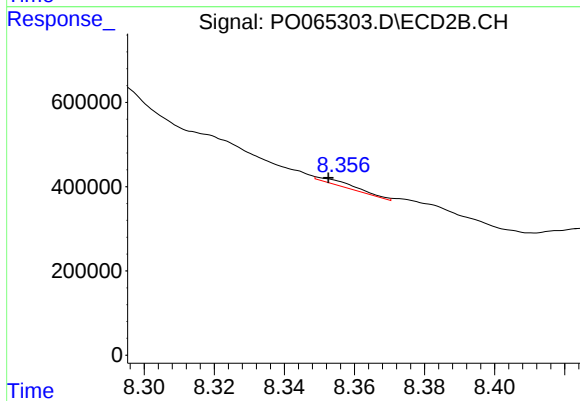

#2 Decachlorobiphenyl

R.T.: 8.356 min
Delta R.T.: 0.004 min
Response: 87787
Conc: 2.12 ng/ml m