

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
 Data File : P0065306.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jan 2020 4:13
 Operator : AJ/MA
 Sample : L1027-02 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-02

Manual Integrations
 APPROVED

mohammad
 1/6/2020 11:38:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 05:21:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.442	85931	112243	4.706	5.103
2) SA Decachlor...	9.675	8.354	135075	504221	3.987m	12.159m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010420\
Data File : P0065306.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jan 2020 4:13
Operator : AJ/MA
Sample : L1027-02 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 05:21:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

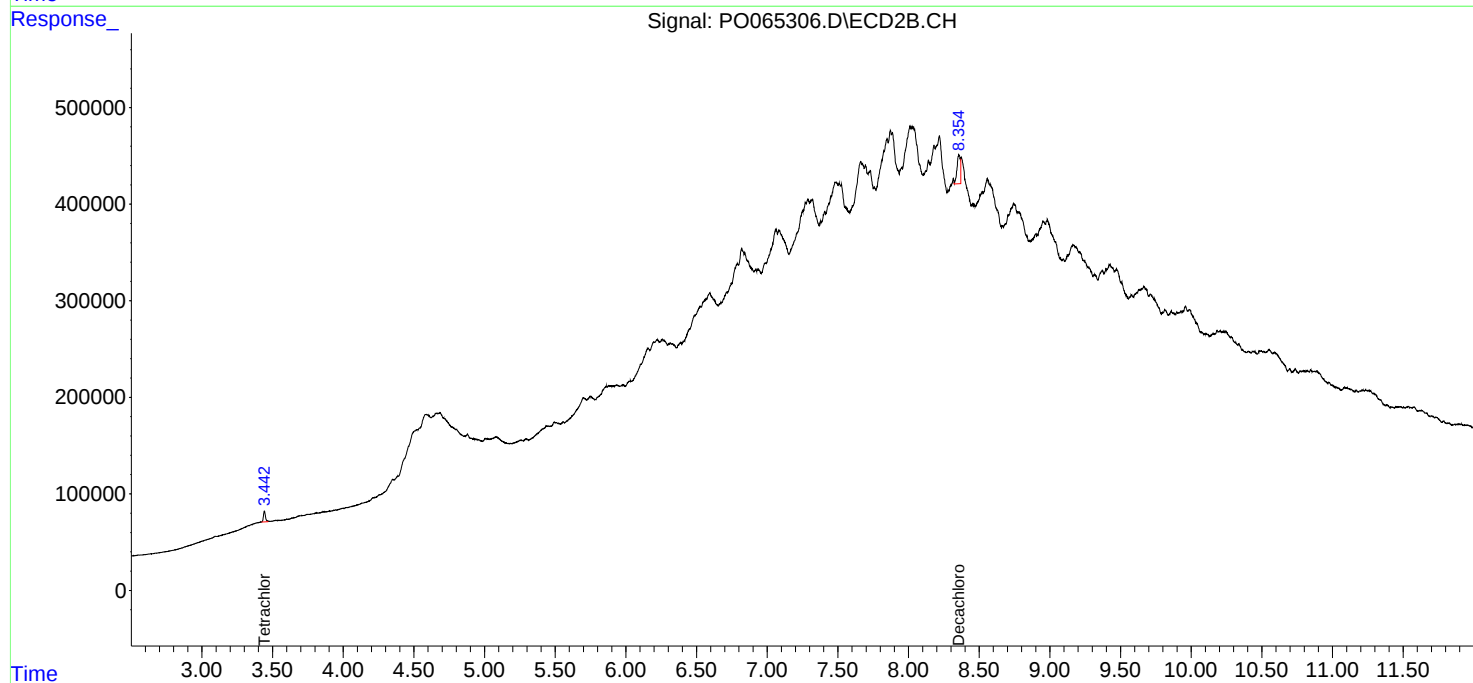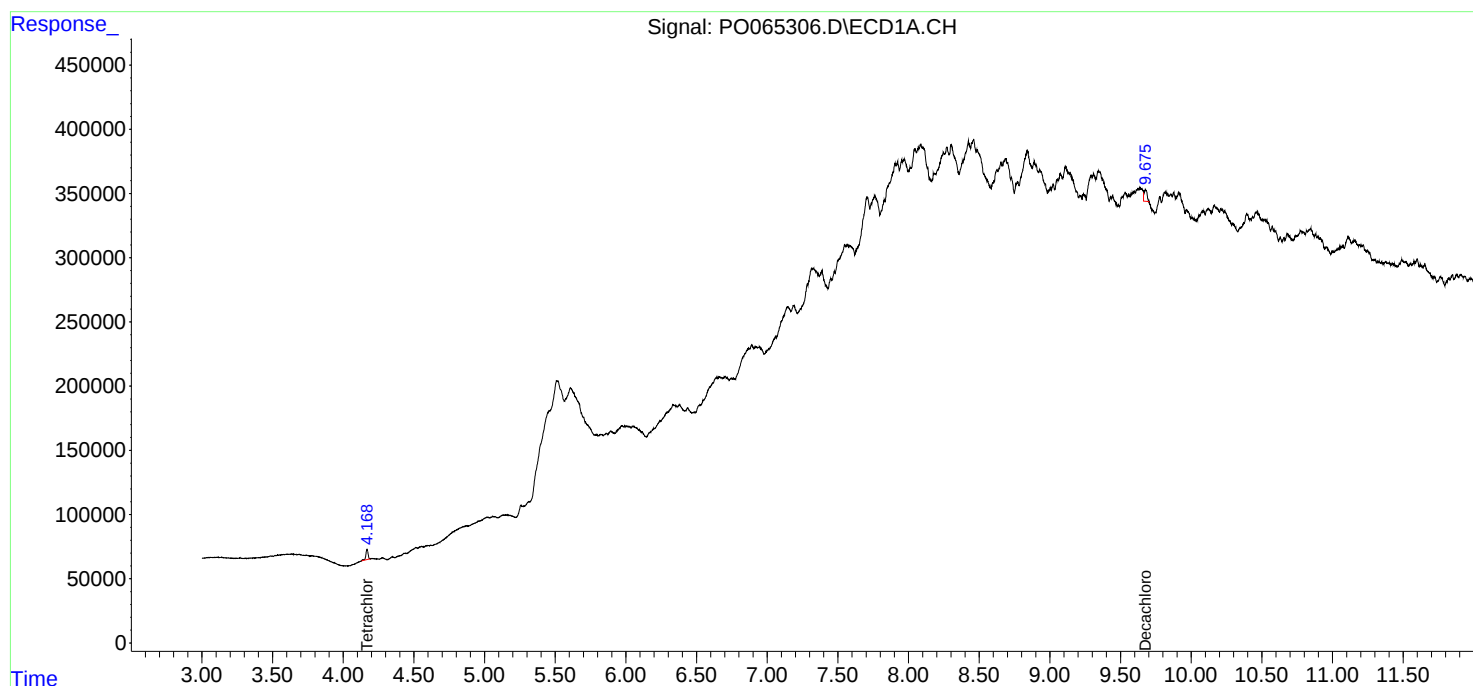

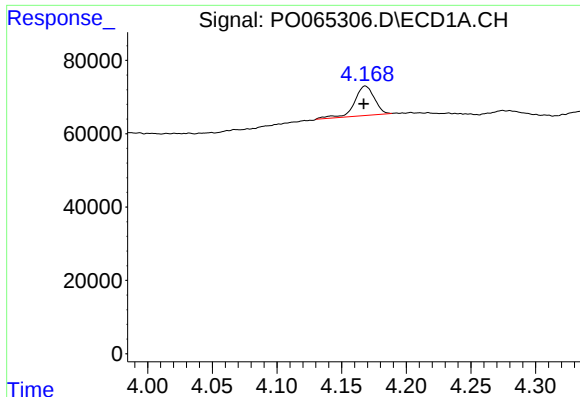


#1 Tetrachloro-m-xylene

R.T.: 4.168 min
Delta R.T.: 0.001 min
Response: 85931
Conc: 4.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

mohammad
1/6/2020 11:38:53 AM

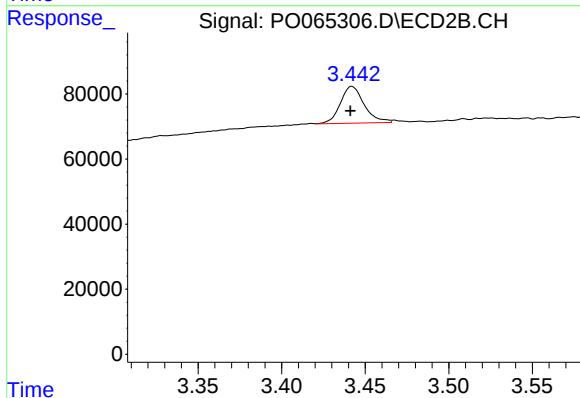


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 112243
Conc: 5.10 ng/ml

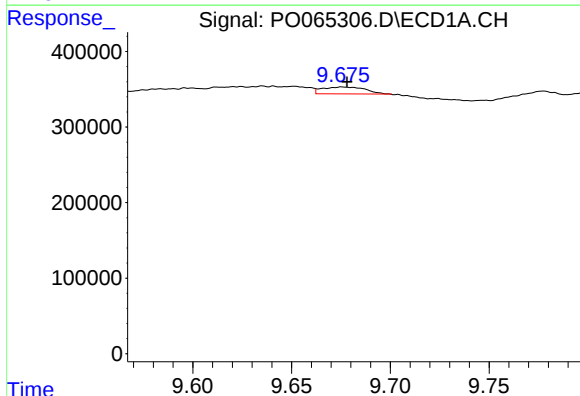

#2 Decachlorobiphenyl

R.T.: 9.675 min
Delta R.T.: -0.003 min
Response: 135075
Conc: 3.99 ng/ml m

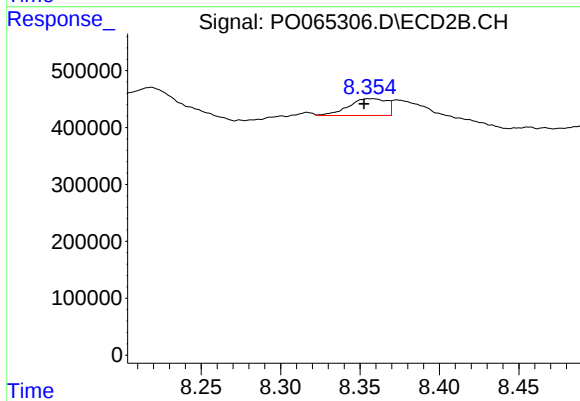

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: 0.002 min
Response: 504221
Conc: 12.16 ng/ml m