

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
Data File : P0084010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jan 2022 20:11
Operator : AJ\MA
Sample : M5337-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 08:01:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.064	2011788	548206	22.878	23.970
2) SA Decachlor...	11.163	9.524	941934	310057	23.782	21.254

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010422\
Data File : PO084010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jan 2022 20:11
Operator : AJ\MA
Sample : M5337-09
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 08:01:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

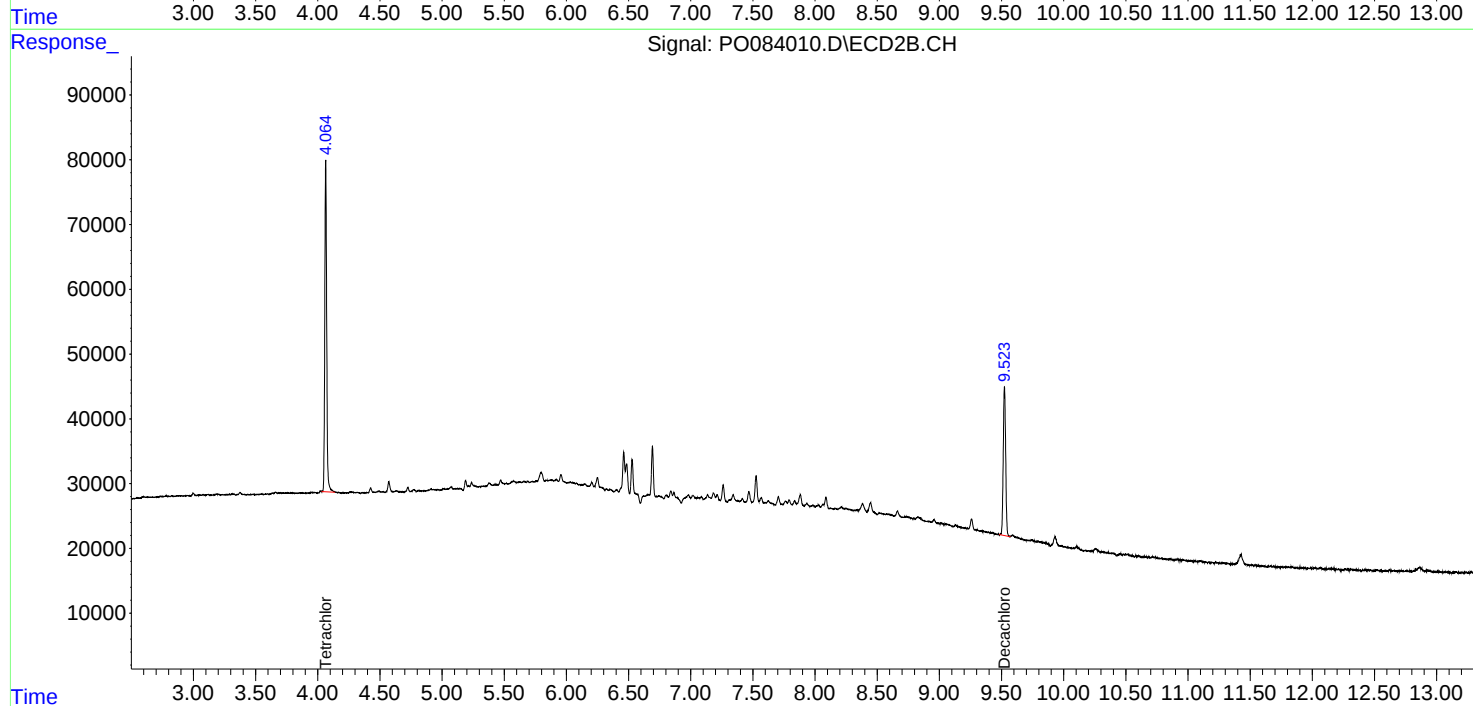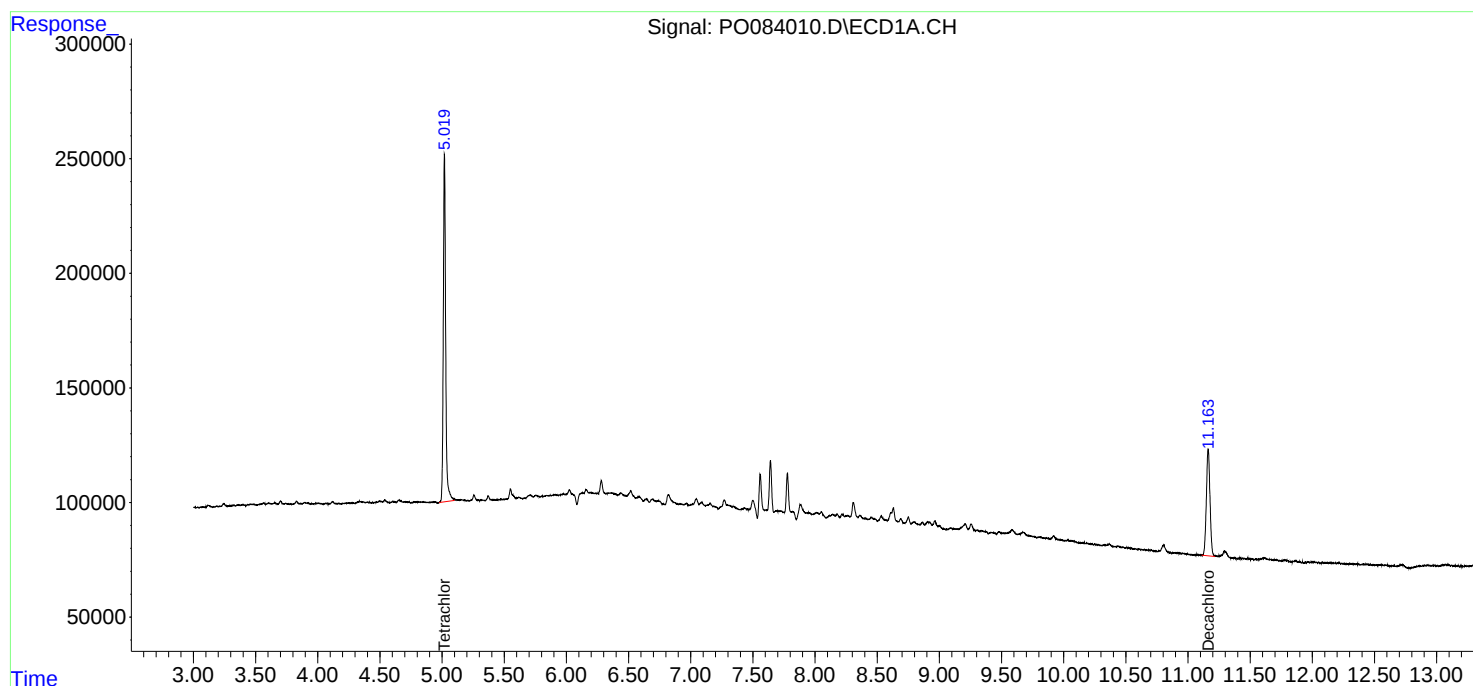


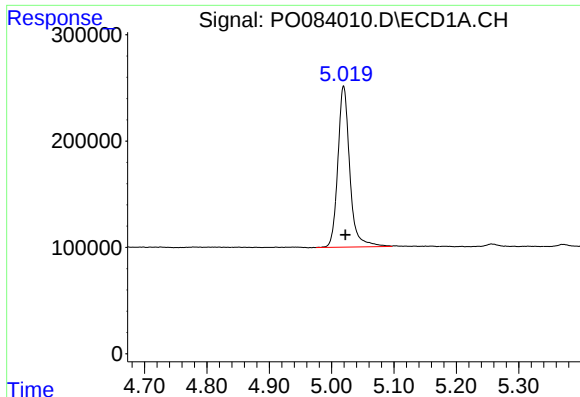

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 2011788
Conc: 22.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-1

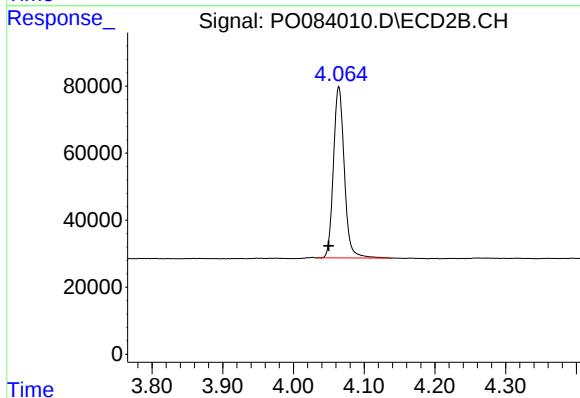


#1 Tetrachloro-m-xylene

R.T.: 4.064 min
Delta R.T.: 0.014 min
Response: 548206
Conc: 23.97 ng/ml

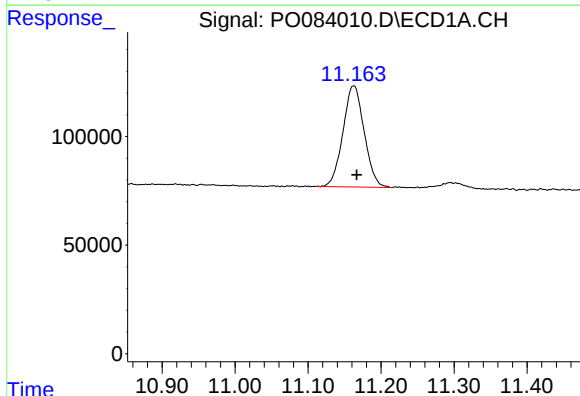

#2 Decachlorobiphenyl

R.T.: 11.163 min
Delta R.T.: -0.004 min
Response: 941934
Conc: 23.78 ng/ml

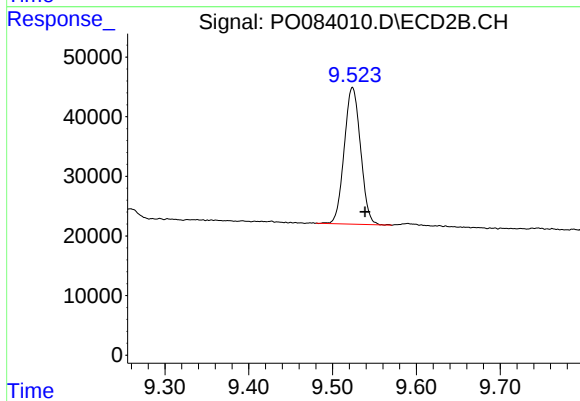

#2 Decachlorobiphenyl

R.T.: 9.524 min
Delta R.T.: -0.015 min
Response: 310057
Conc: 21.25 ng/ml