

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
 Data File : P0084024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2022 00:47
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 10:01:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 17:57:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.018	4.067	1781665	488811	20.261	21.373
2) SA Decachlor...	11.161	9.518	897030	278596	22.648	19.097

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010422\
Data File : PO084024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2022 00:47
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 10:01:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

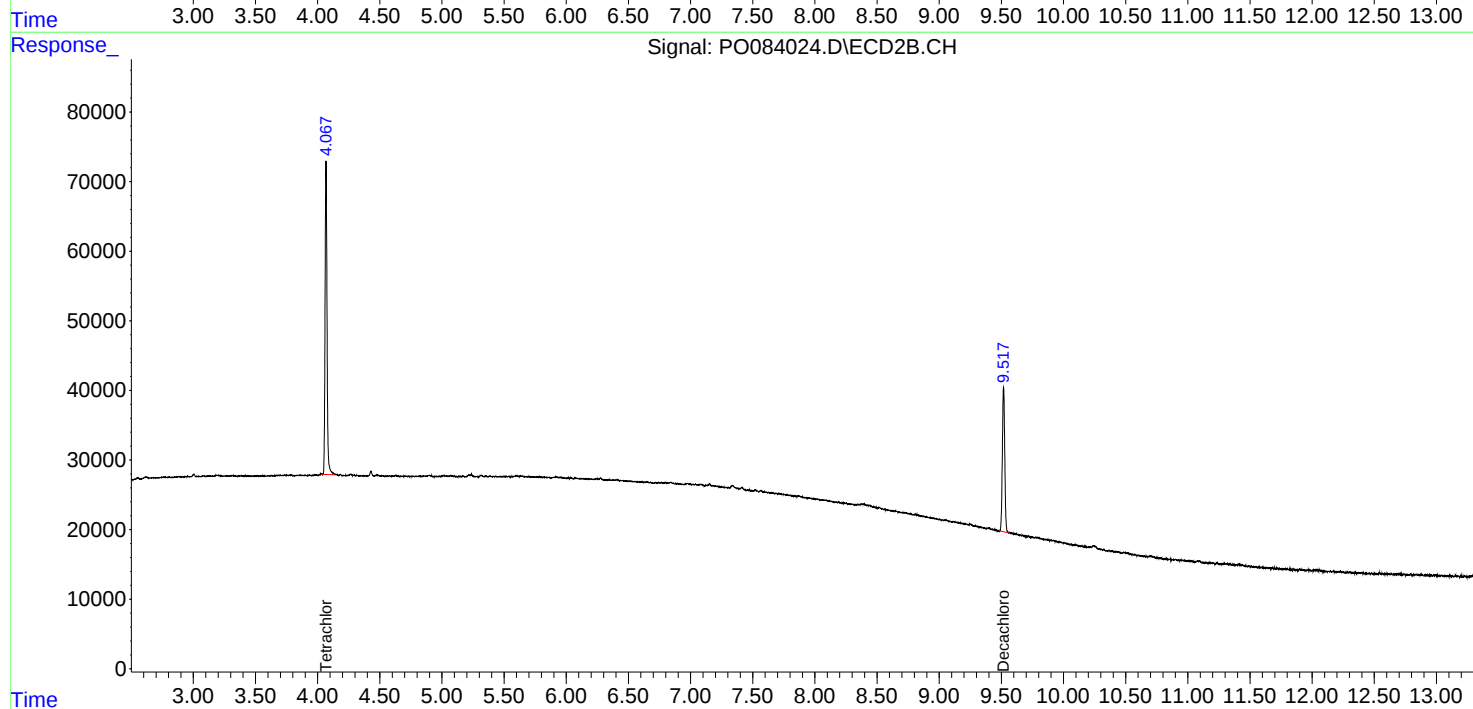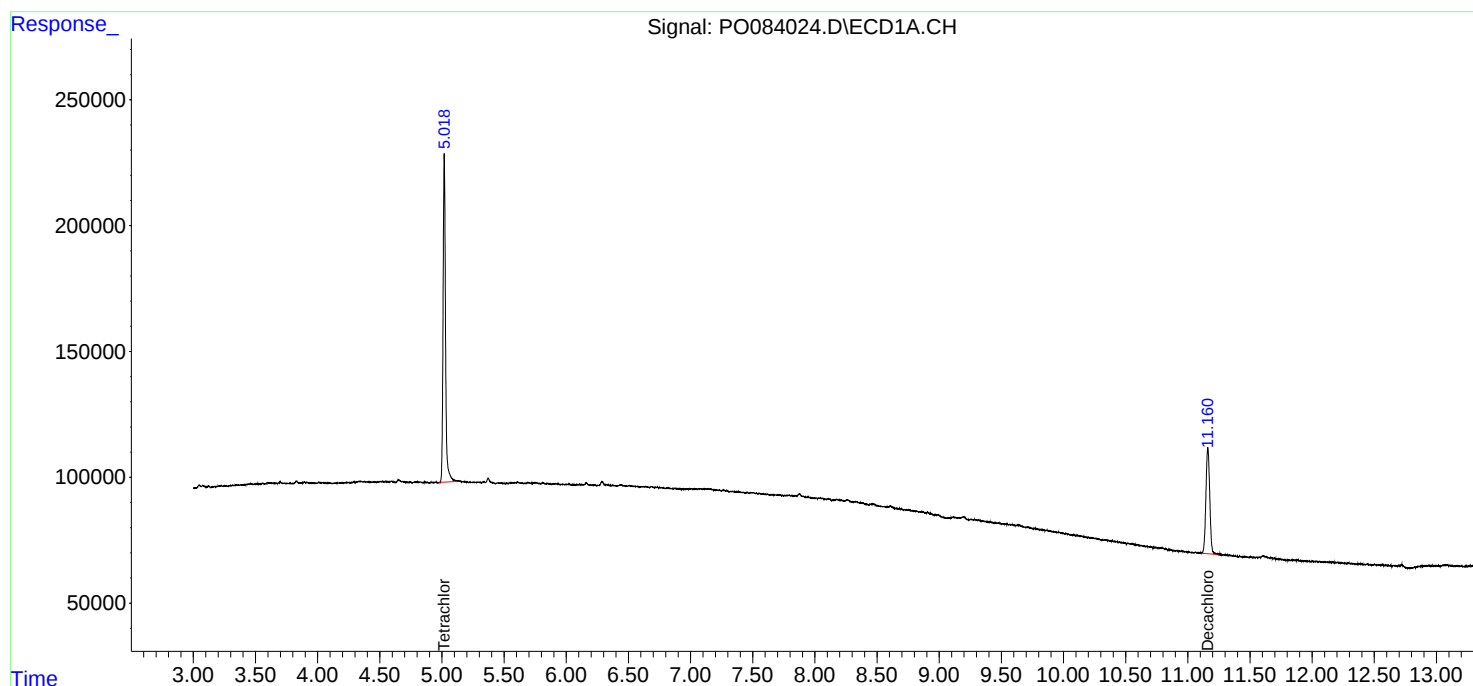


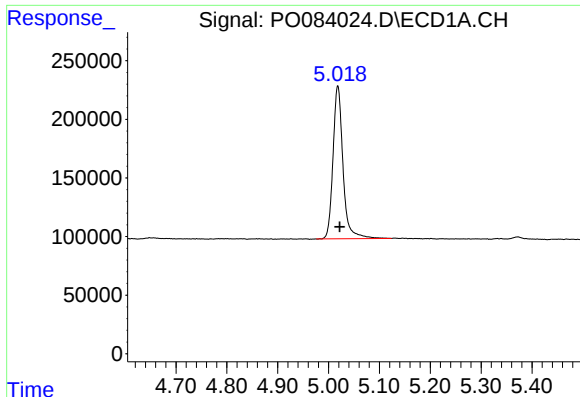

#1 Tetrachloro-m-xylene


R.T.: 5.018 min
Delta R.T.: -0.004 min
Response: 1781665
Conc: 20.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

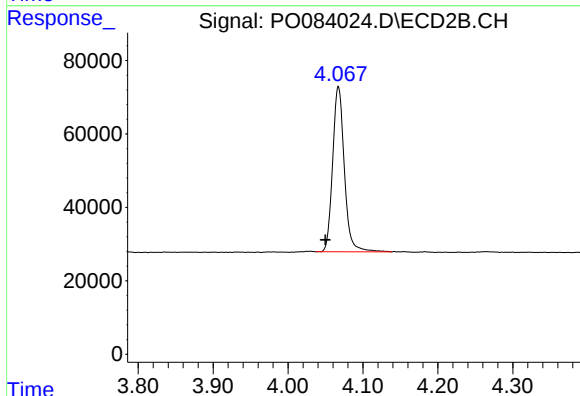


#1 Tetrachloro-m-xylene

R.T.: 4.067 min
Delta R.T.: 0.017 min
Response: 488811
Conc: 21.37 ng/ml

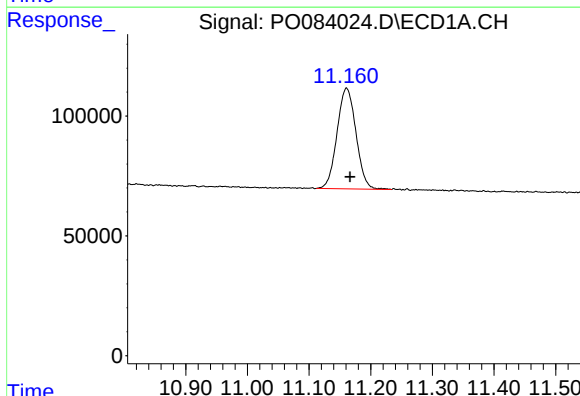

#2 Decachlorobiphenyl

R.T.: 11.161 min
Delta R.T.: -0.006 min
Response: 897030
Conc: 22.65 ng/ml

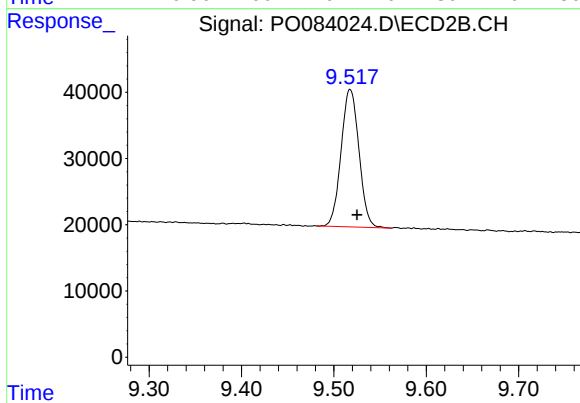

#2 Decachlorobiphenyl

R.T.: 9.518 min
Delta R.T.: -0.007 min
Response: 278596
Conc: 19.10 ng/ml