

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
 Data File : P0084047.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2022 7:57
 Operator : AJ\MA
 Sample : M5334-05 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-78-A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
 Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 11:57:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 17:57:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.109	139070	46442	1.582m	2.031 #
2) SA Decachlor...	11.167	9.559	101299	21309	2.558	1.461m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010422\
Data File : PO084047.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2022 7:57
Operator : AJ\MA
Sample : M5334-05 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEC-2021-78-A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 11:57:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

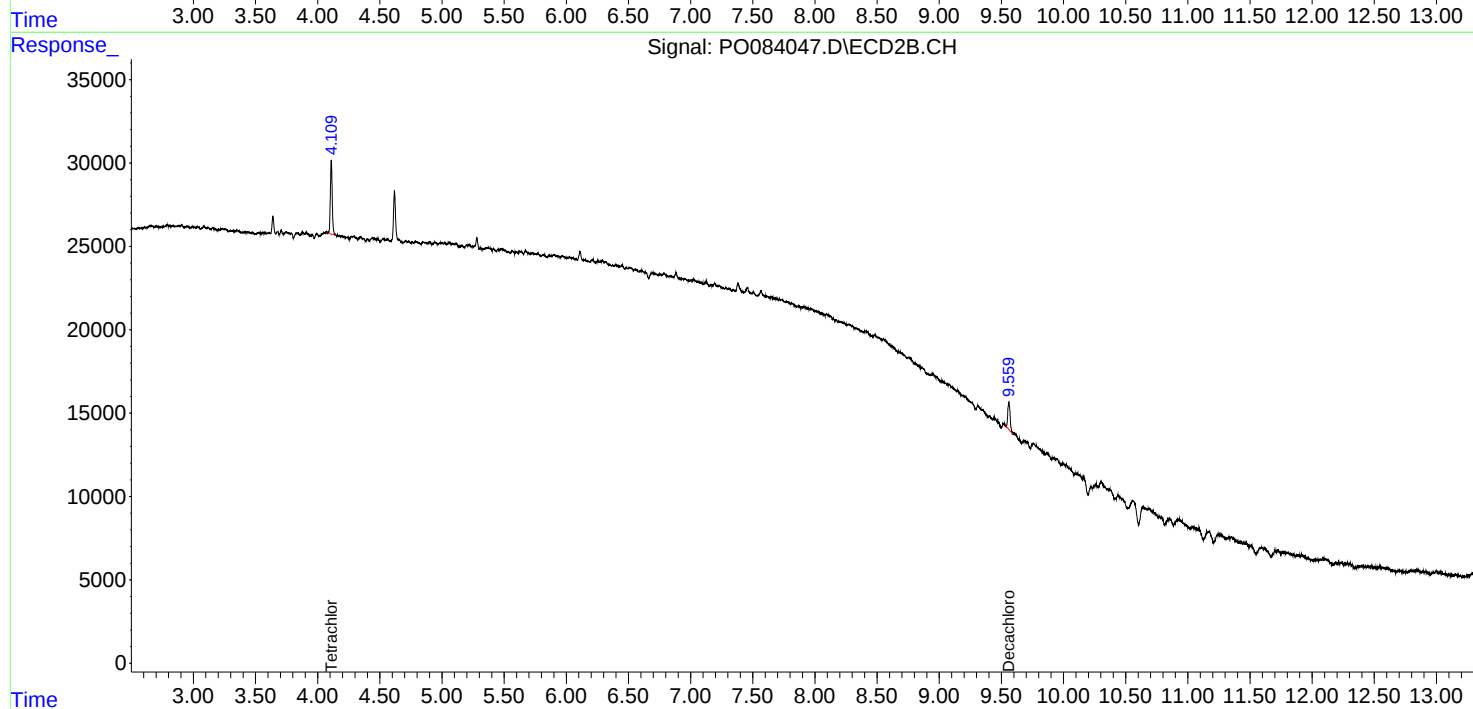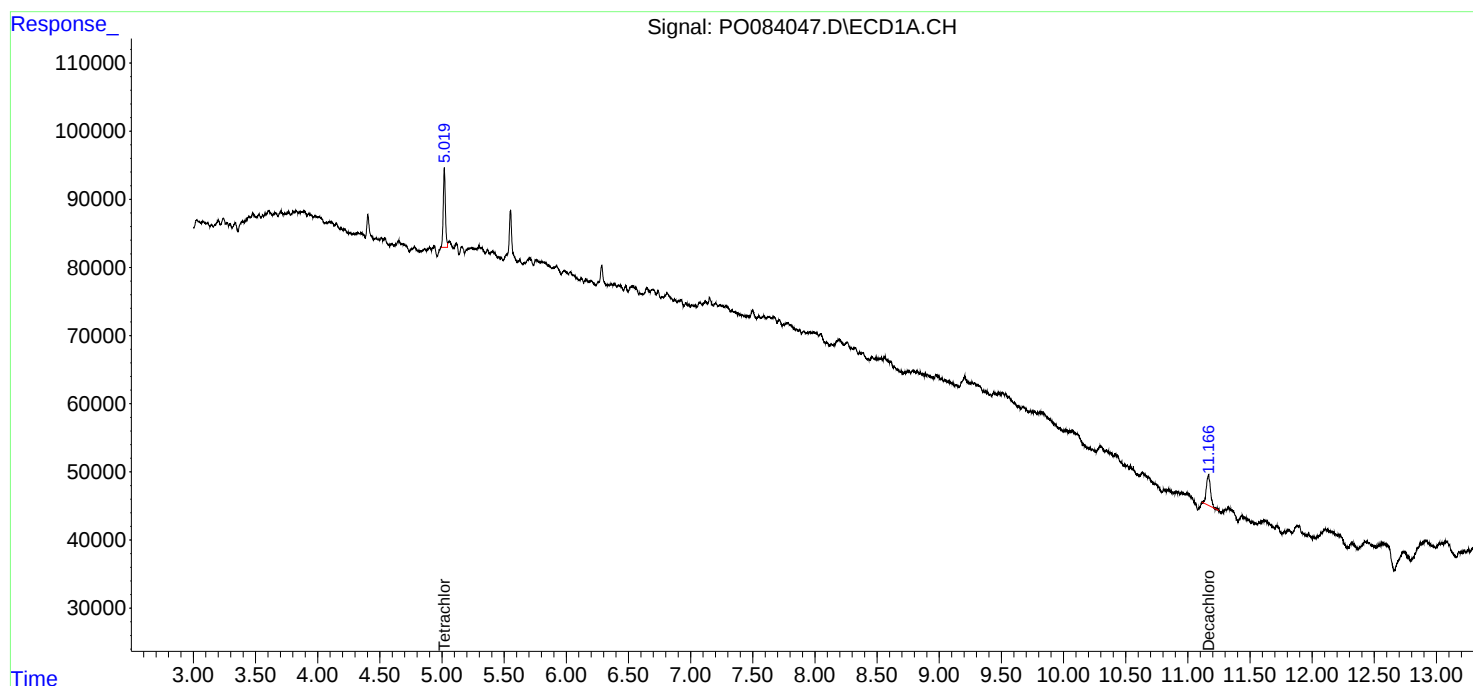

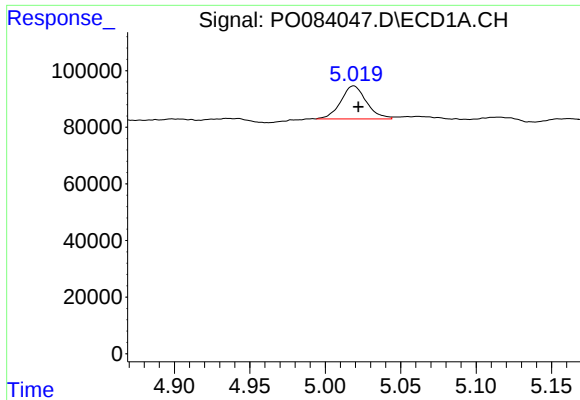


#1 Tetrachloro-m-xylene

R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 139070
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-78-A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

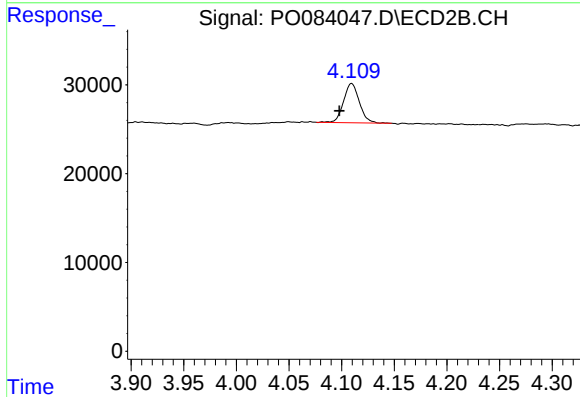


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.011 min
Response: 46442
Conc: 2.03 ng/ml

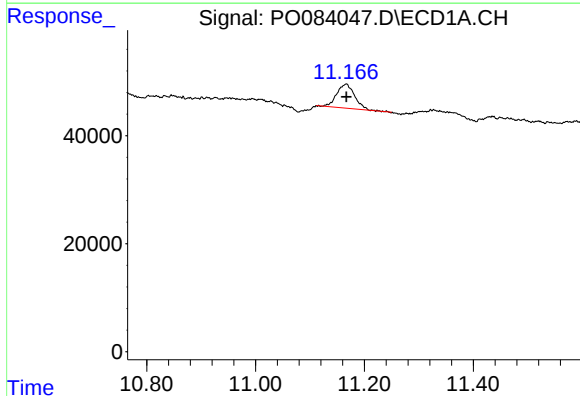

#2 Decachlorobiphenyl

R.T.: 11.167 min
Delta R.T.: 0.000 min
Response: 101299
Conc: 2.56 ng/ml

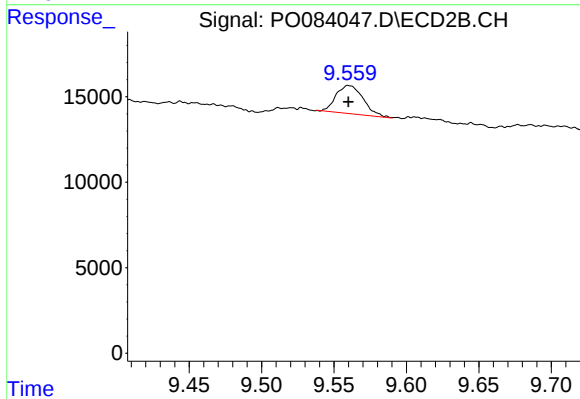

#2 Decachlorobiphenyl

R.T.: 9.559 min
Delta R.T.: 0.000 min
Response: 21309
Conc: 1.46 ng/ml m