

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
 Data File : P0084048.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2022 8:14
 Operator : AJ\MA
 Sample : M5334-06 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-78-B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
 Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 11:54:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 17:57:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.018	4.109	123402	44229	1.403m	1.934 #
2) SA Decachlor...	11.165	9.560	121427	22306	3.066	1.529m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010422\
Data File : PO084048.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2022 8:14
Operator : AJ\MA
Sample : M5334-06 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEC-2021-78-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 11:54:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

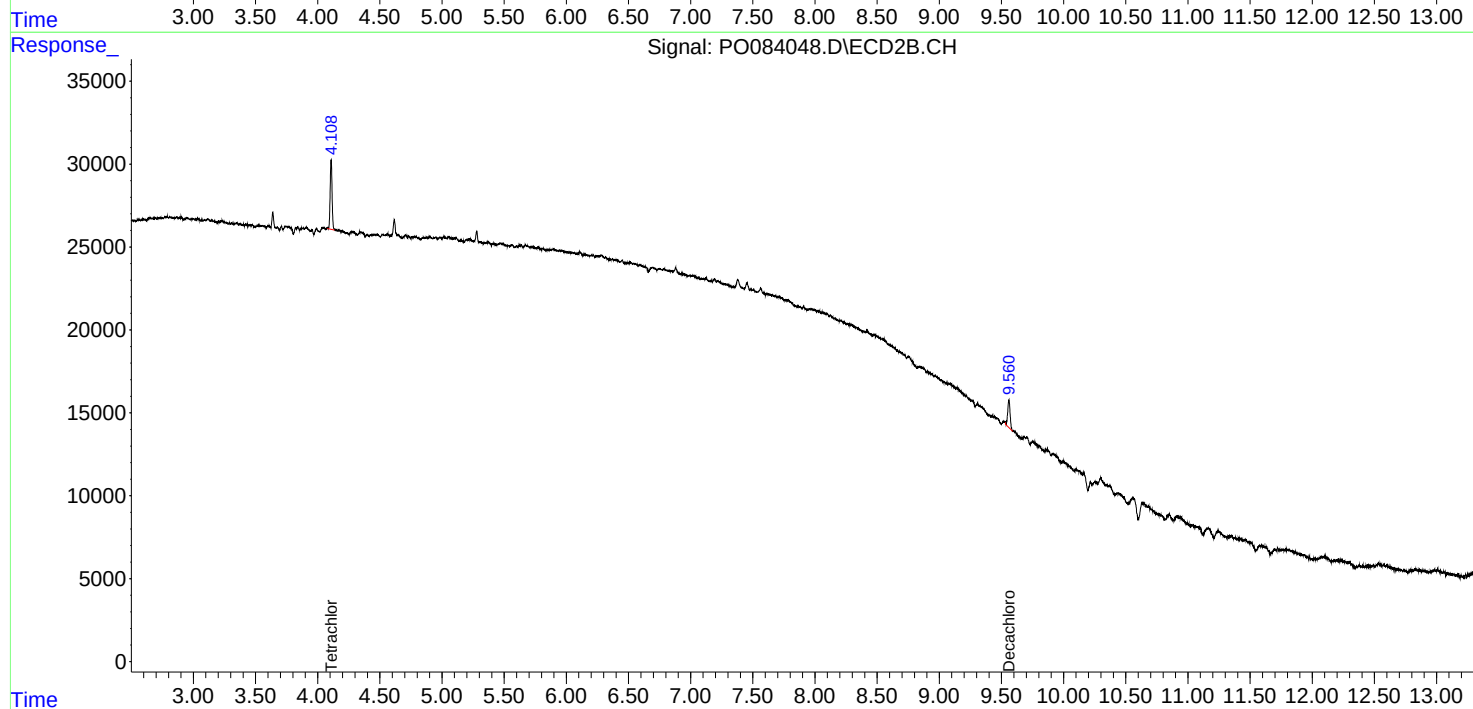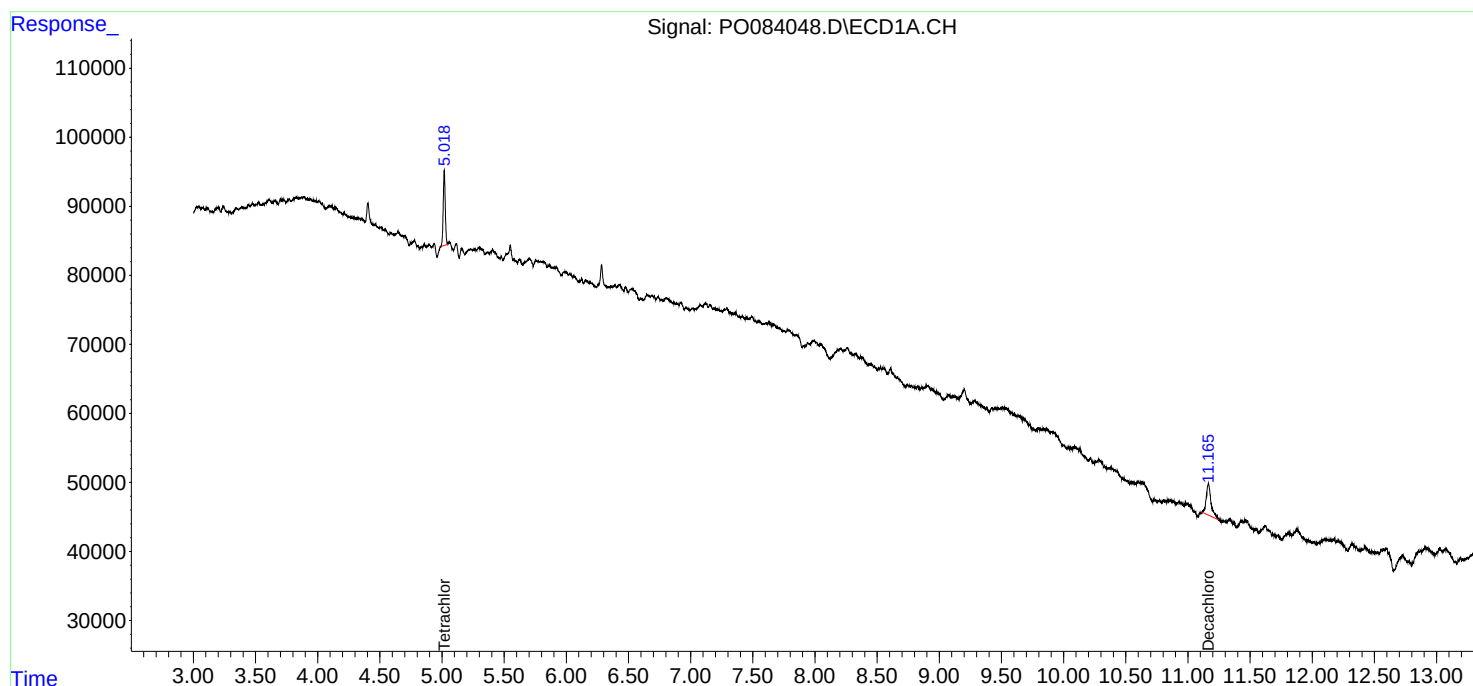

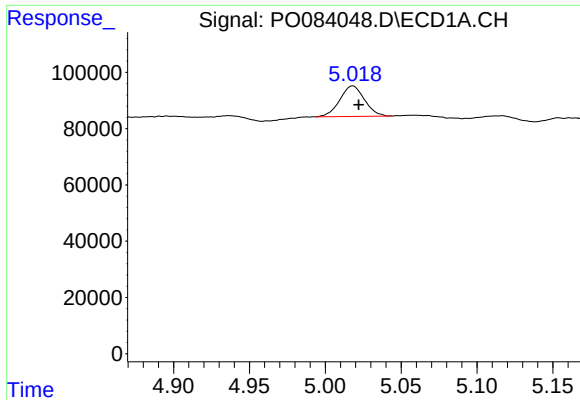


#1 Tetrachloro-m-xylene

R.T.: 5.018 min
Delta R.T.: -0.004 min
Response: 123402
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-78-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

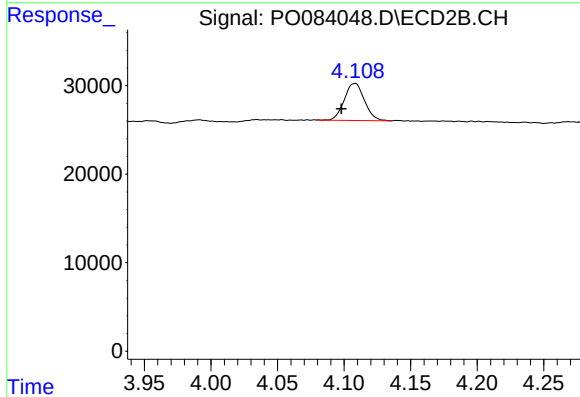


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.011 min
Response: 44229
Conc: 1.93 ng/ml

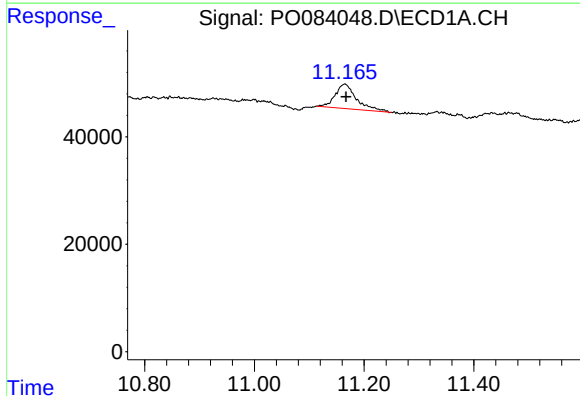

#2 Decachlorobiphenyl

R.T.: 11.165 min
Delta R.T.: -0.002 min
Response: 121427
Conc: 3.07 ng/ml

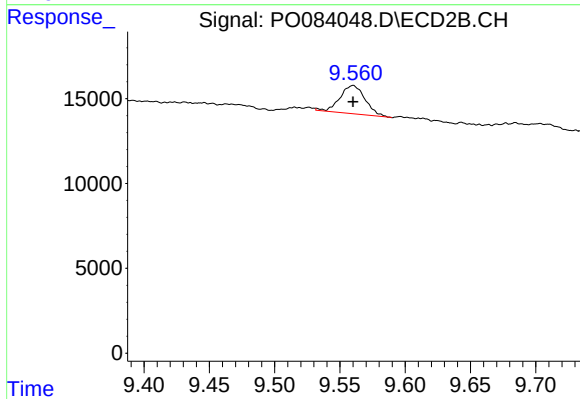

#2 Decachlorobiphenyl

R.T.: 9.560 min
Delta R.T.: 0.000 min
Response: 22306
Conc: 1.53 ng/ml m