

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
 Data File : P0084049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2022 8:31
 Operator : AJ\MA
 Sample : M5334-07 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-79-B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
 Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 00:50:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 04 17:57:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.109	140746	45373	1.601	1.984
2) SA Decachlor...	11.166	9.561	98796	25684	2.494	1.761m#
Target Compounds						
26) L6 AR-1254-1	7.267	6.291	115170	46673	40.318	38.510
27) L6 AR-1254-2	7.499	6.454	191096	48110	44.161	45.994
28) L6 AR-1254-3	7.881	6.883	154987	63939	35.338m	38.552m
29) L6 AR-1254-4	8.178	7.126	119241	36954	38.138m	36.024
30) L6 AR-1254-5	8.613	7.564	104661	51775	34.573	37.456

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010422\
Data File : P0084049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2022 8:31
Operator : AJ\MA
Sample : M5334-07 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 00:50:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 04 17:57:57 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

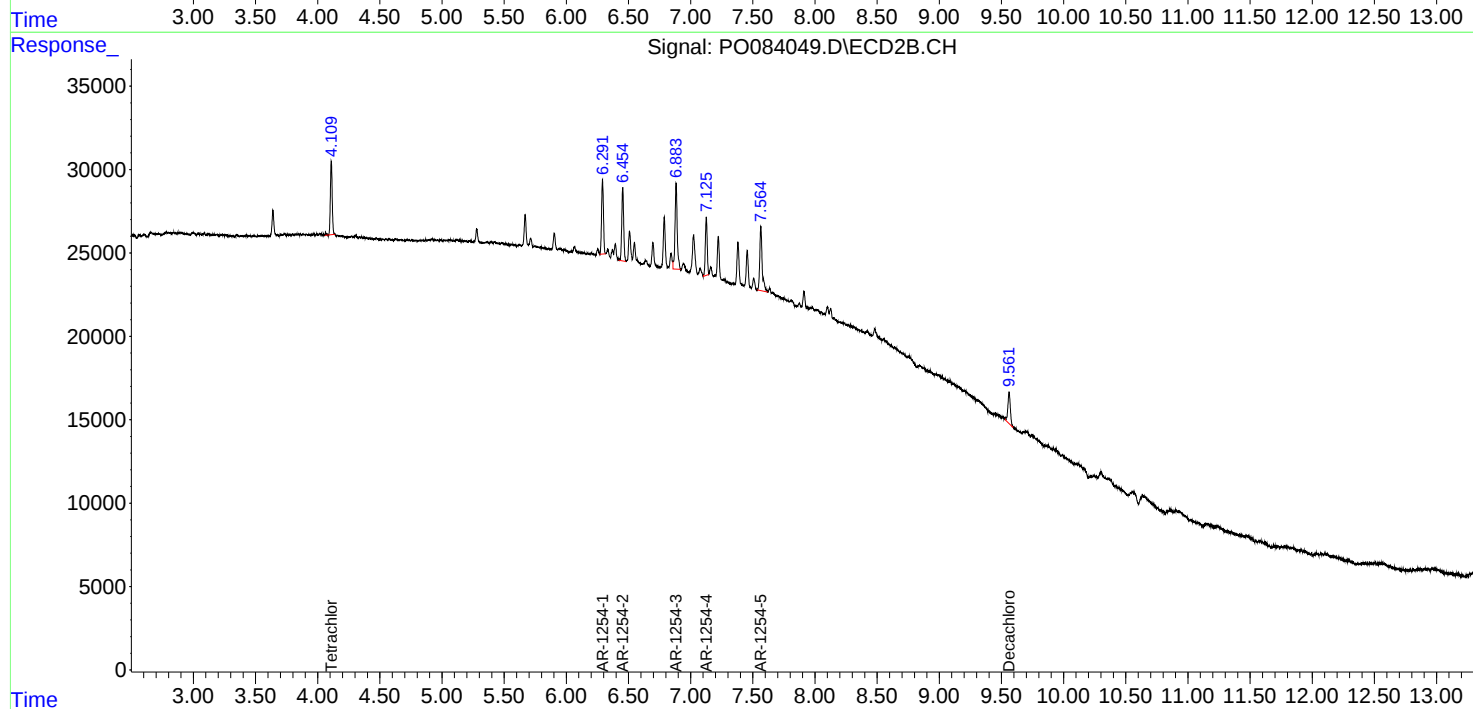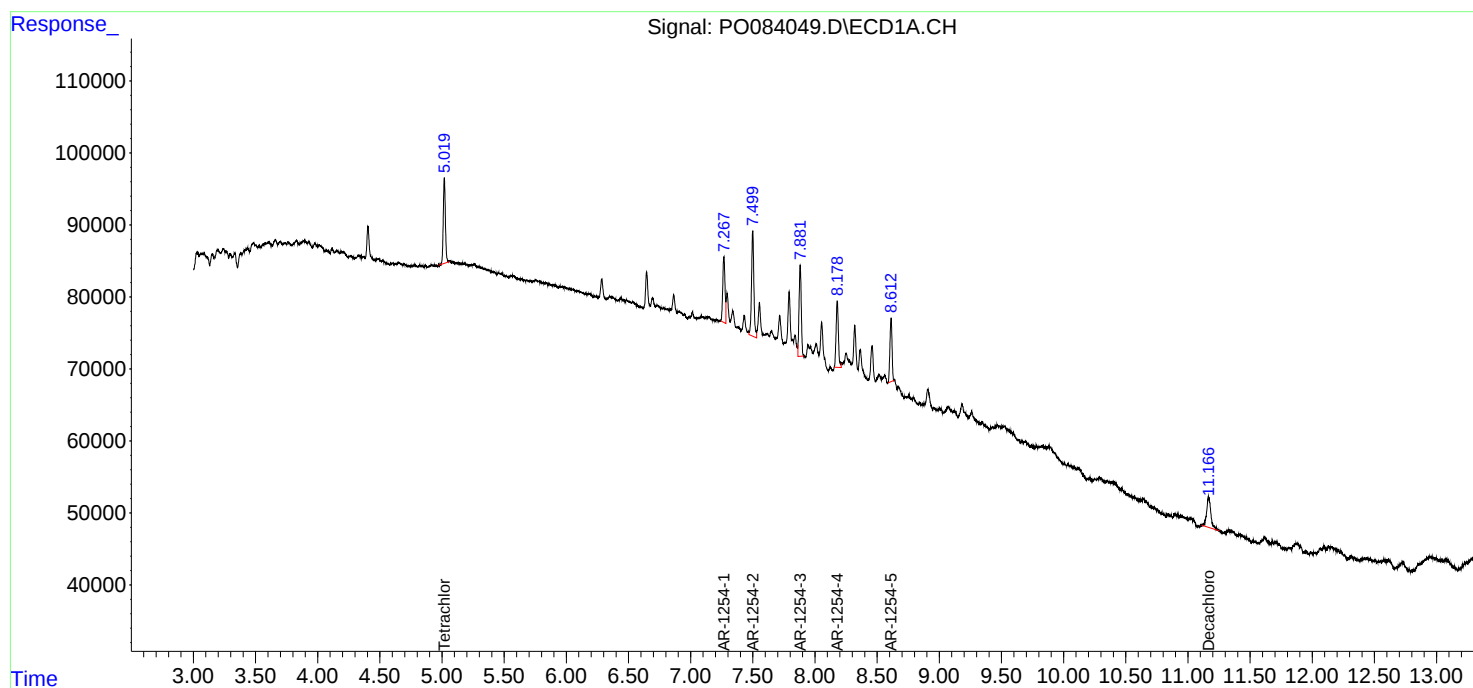

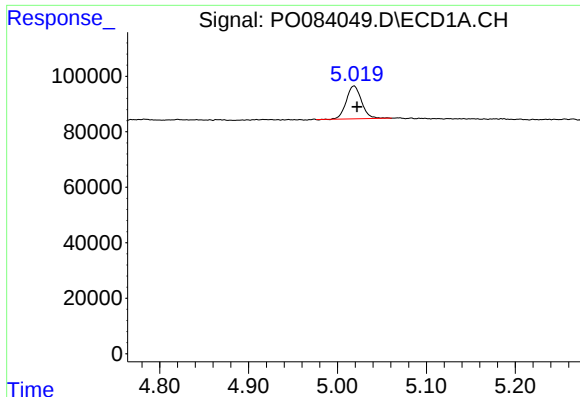


#1 Tetrachloro-m-xylene

R.T.: 5.019 min
Delta R.T.: -0.003 min
Response: 140746
Conc: 1.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

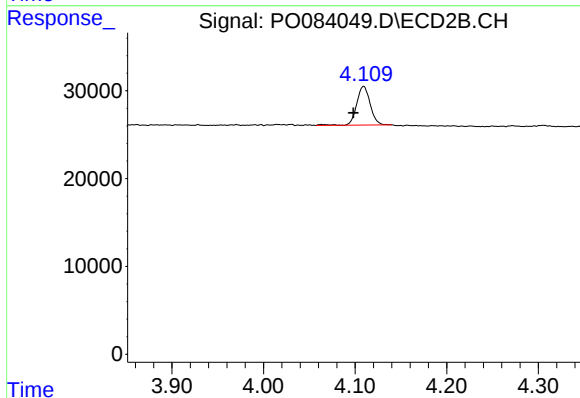


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.011 min
Response: 45373
Conc: 1.98 ng/ml

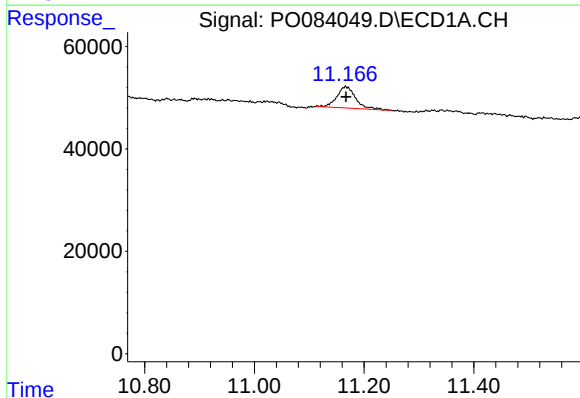


#2 Decachlorobiphenyl

R.T.: 11.166 min
Delta R.T.: 0.000 min
Response: 98796
Conc: 2.49 ng/ml

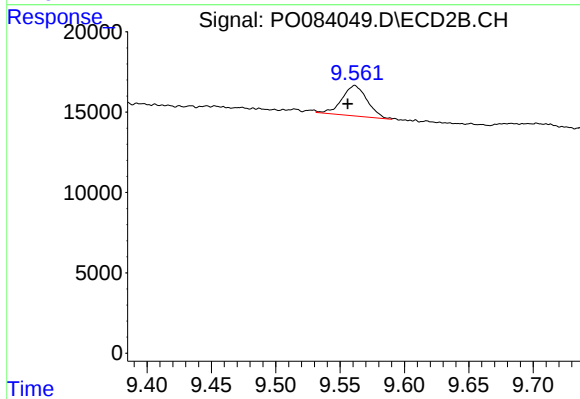

#2 Decachlorobiphenyl

R.T.: 9.561 min
Delta R.T.: 0.005 min
Response: 25684
Conc: 1.76 ng/ml m

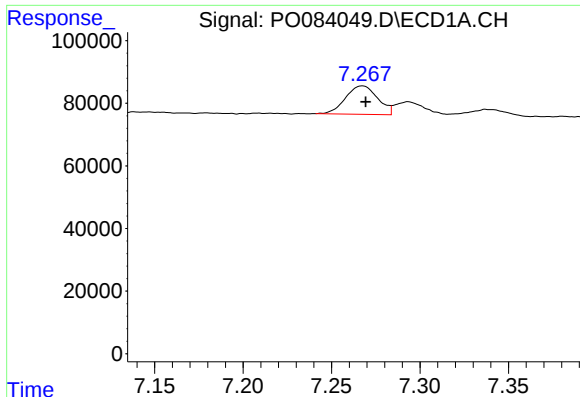


#26 AR-1254-1

R.T.: 7.267 min
Delta R.T.: -0.002 min
Response: 115170
Conc: 40.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

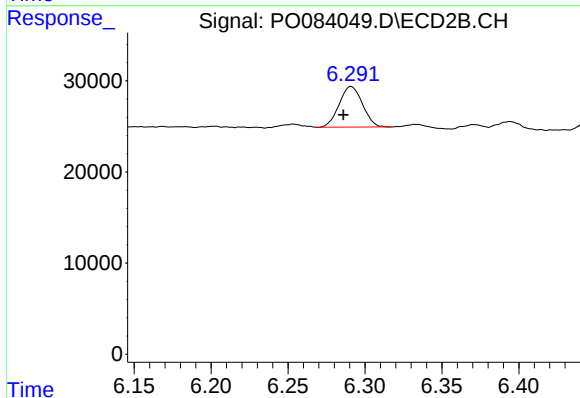


#26 AR-1254-1

R.T.: 6.291 min
Delta R.T.: 0.005 min
Response: 46673
Conc: 38.51 ng/ml

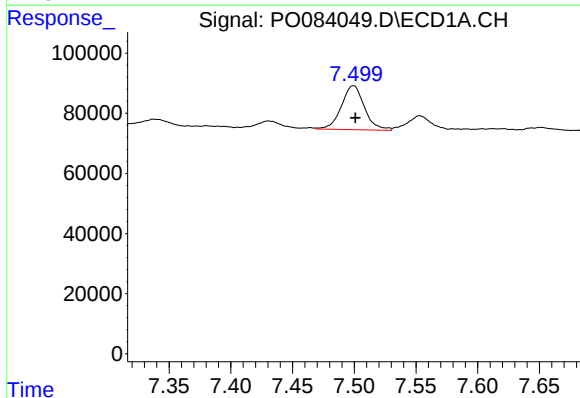


#27 AR-1254-2

R.T.: 7.499 min
Delta R.T.: -0.002 min
Response: 191096
Conc: 44.16 ng/ml

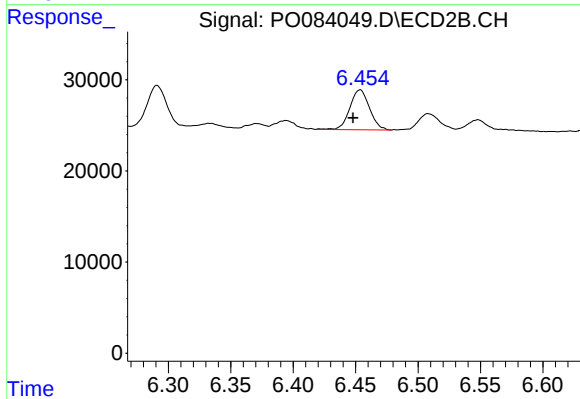

#27 AR-1254-2

R.T.: 6.454 min
Delta R.T.: 0.006 min
Response: 48110
Conc: 45.99 ng/ml

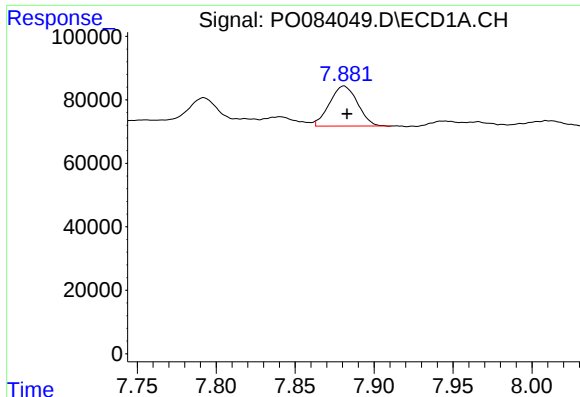


#28 AR-1254-3

R.T.: 7.881 min
Delta R.T.: -0.002 min
Response: 154987
Conc: 35.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

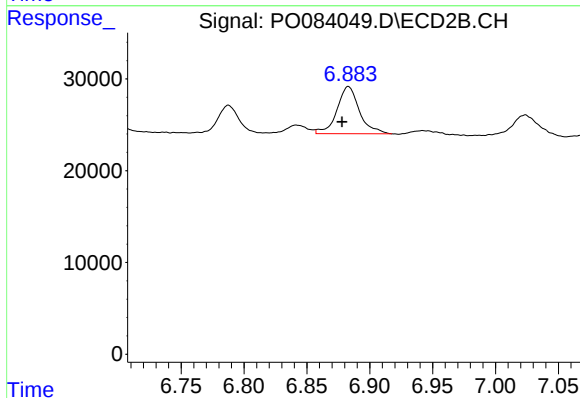


#28 AR-1254-3

R.T.: 6.883 min
Delta R.T.: 0.005 min
Response: 63939
Conc: 38.55 ng/ml m

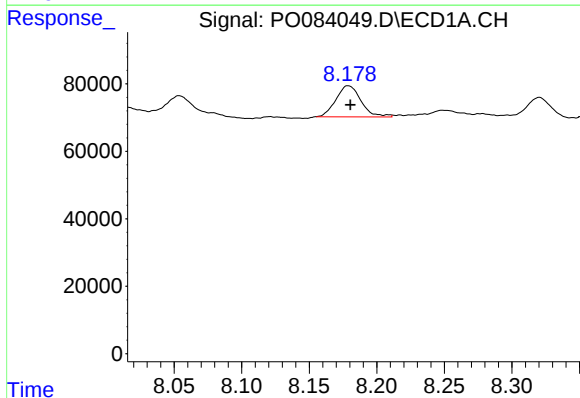


#29 AR-1254-4

R.T.: 8.178 min
Delta R.T.: -0.002 min
Response: 119241
Conc: 38.14 ng/ml m

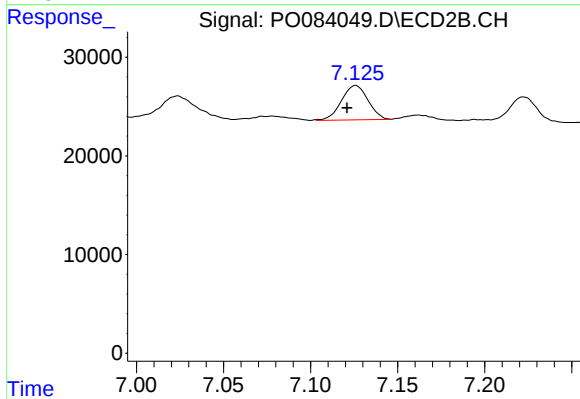

#29 AR-1254-4

R.T.: 7.126 min
Delta R.T.: 0.005 min
Response: 36954
Conc: 36.02 ng/ml

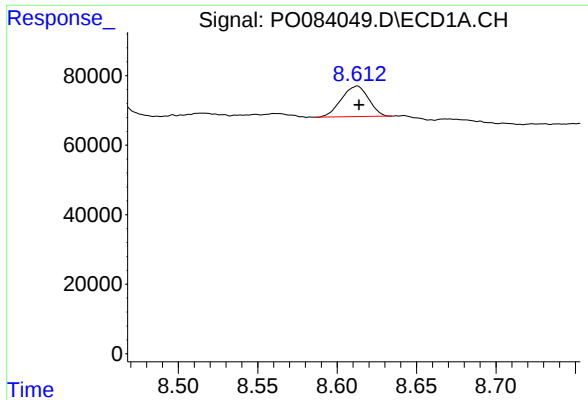


#30 AR-1254-5

R.T.: 8.613 min
Delta R.T.: -0.001 min
Response: 104661
Conc: 34.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-79-B

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

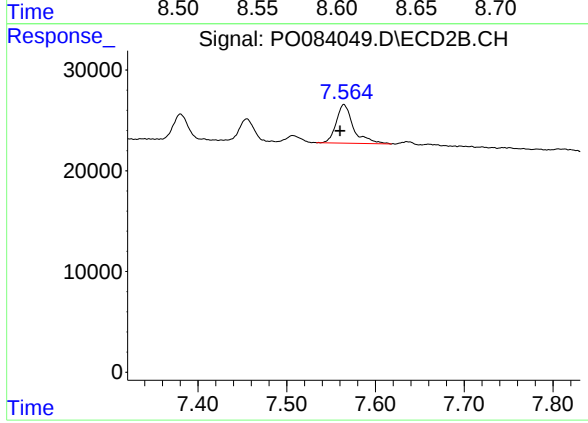

#30 AR-1254-5

R.T.: 7.564 min
Delta R.T.: 0.004 min
Response: 51775
Conc: 37.46 ng/ml