

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010521\
 Data File : P0074392.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2021 17:41
 Operator : DD\AJ
 Sample : M1010-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MT

Manual Integrations
 APPROVED

Ankita
 1/6/2021 9:44:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 02:49:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	3.989	233687	407390	2.432m	7.648m#
2) SA Decachlor...	10.957	9.246	176275	273386	1.896m	5.252 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010521\
Data File : P0074392.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2021 17:41
Operator : DD\AJ
Sample : M1010-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MT


Manual Integrations
APPROVED

Ankita
1/6/2021 9:44:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 02:49:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

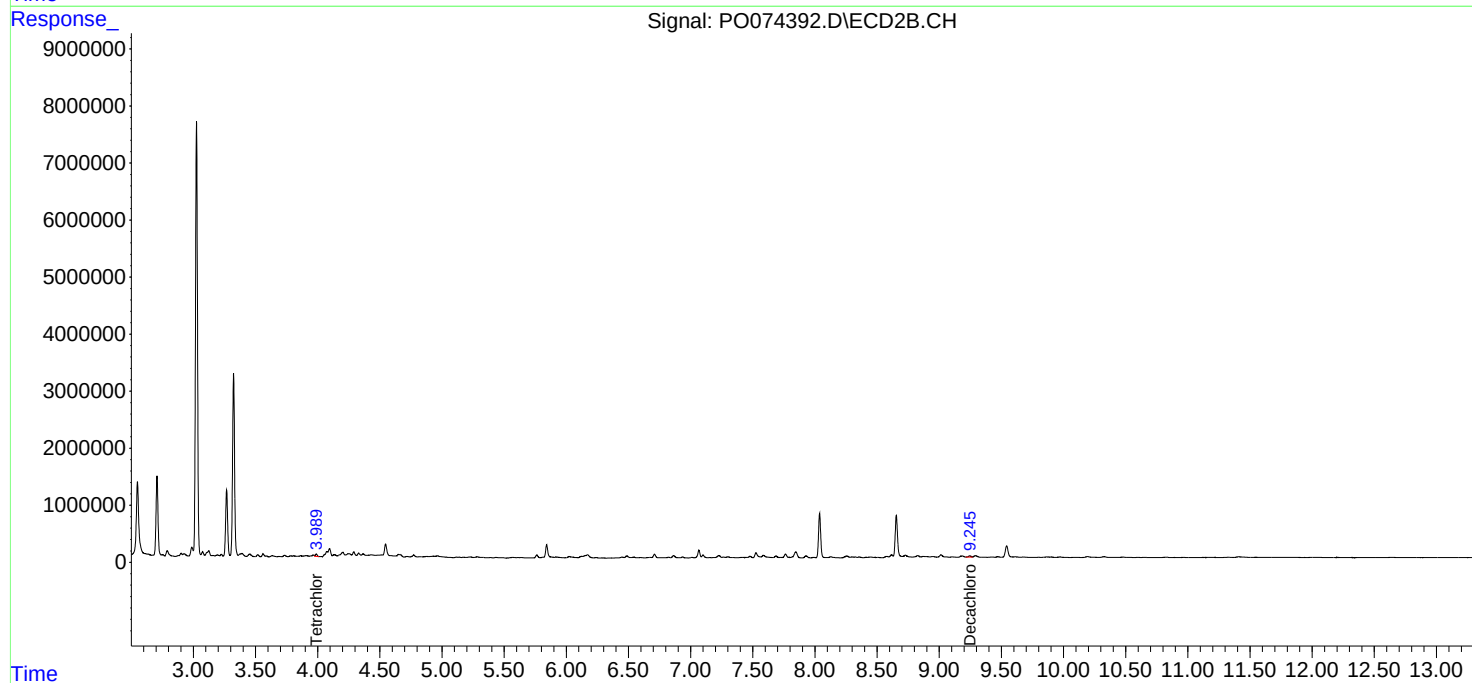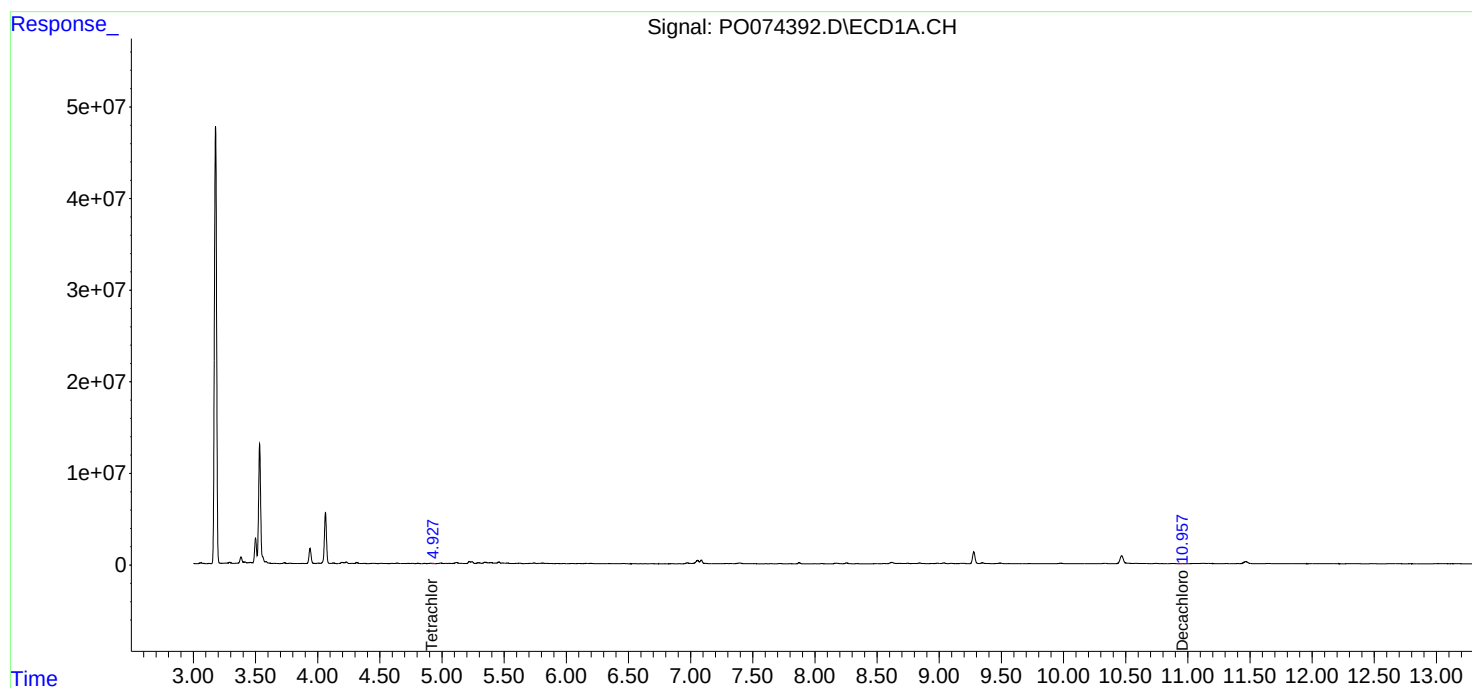

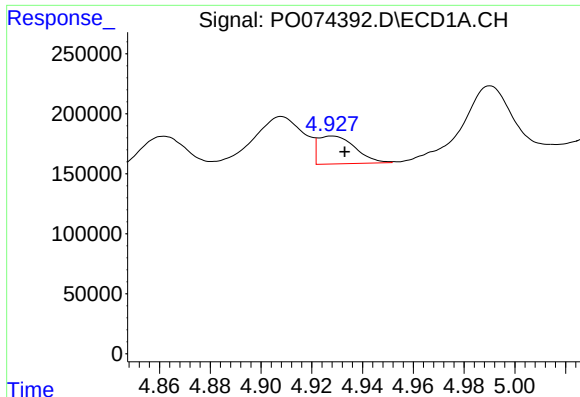


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.006 min
Response: 233687
Conc: 2.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MT


Manual Integrations
APPROVED

Ankita
1/6/2021 9:44:13 AM

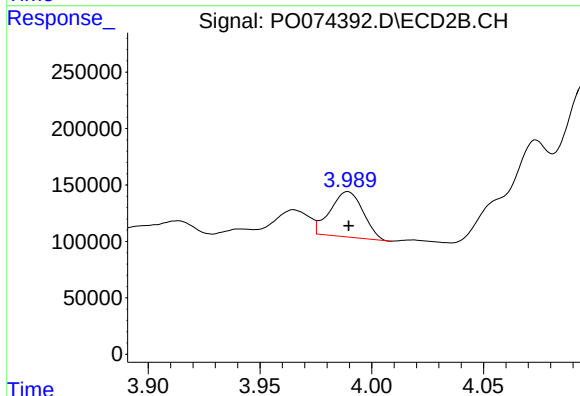


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 407390
Conc: 7.65 ng/ml m

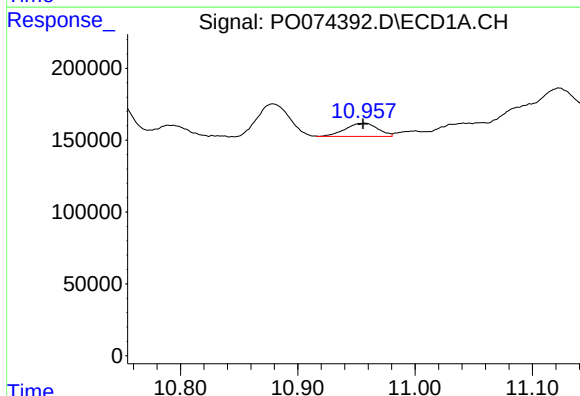

#2 Decachlorobiphenyl

R.T.: 10.957 min
Delta R.T.: 0.000 min
Response: 176275
Conc: 1.90 ng/ml m

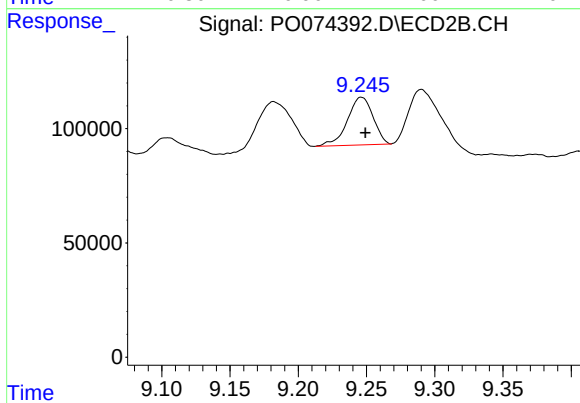

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: -0.003 min
Response: 273386
Conc: 5.25 ng/ml